

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
 Data File : BM019868.D
 Acq On : 10 Apr 2019 17:50
 Operator : JU/SJ
 Sample : K2303-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF885

Quant Time: Apr 11 04:00:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 03:09:11 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/12/2019 5:18:09 PM

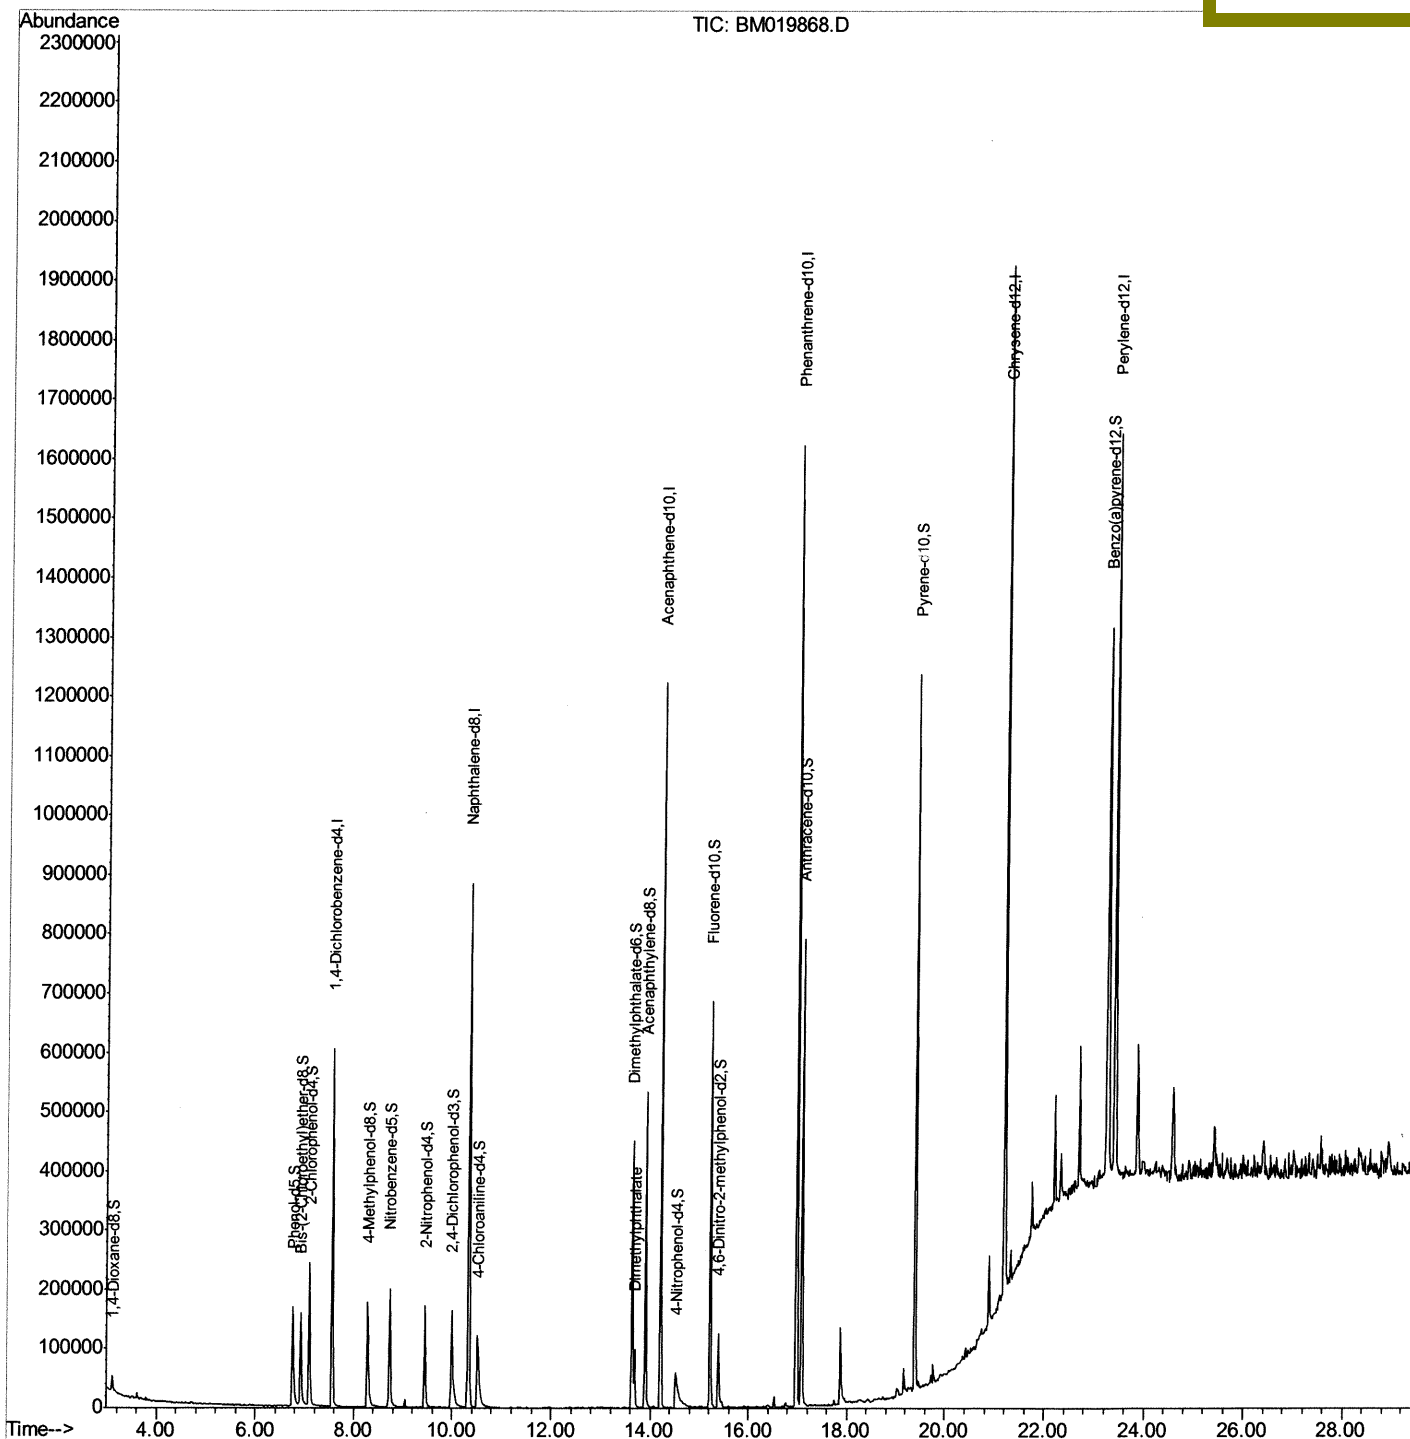

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
 Data File : BM019868.D
 Acq On : 10 Apr 2019 17:50
 Operator : JU/SJ
 Sample : K2303-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF885

Quant Time: Apr 11 03:23:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 03:09:11 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/12/2019 5:18:09 PM

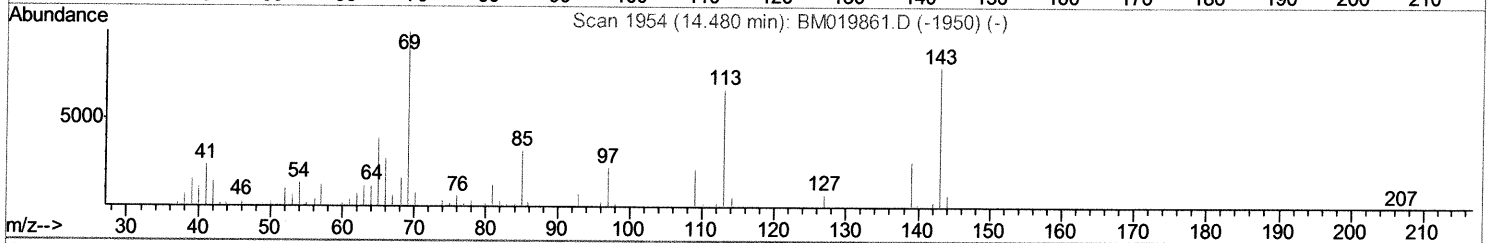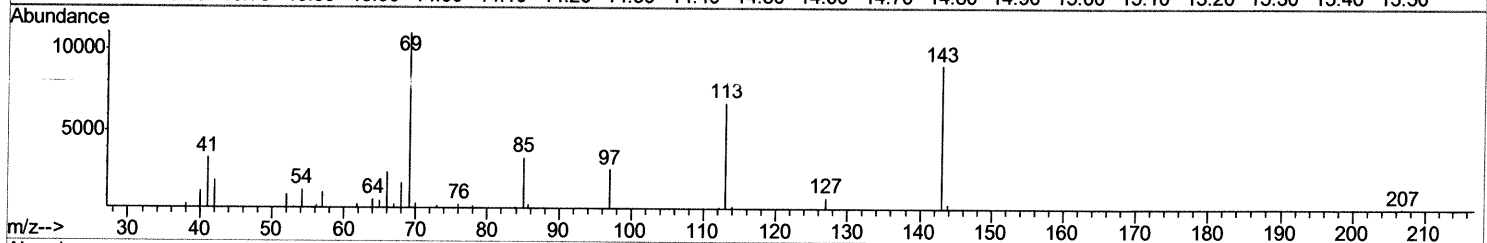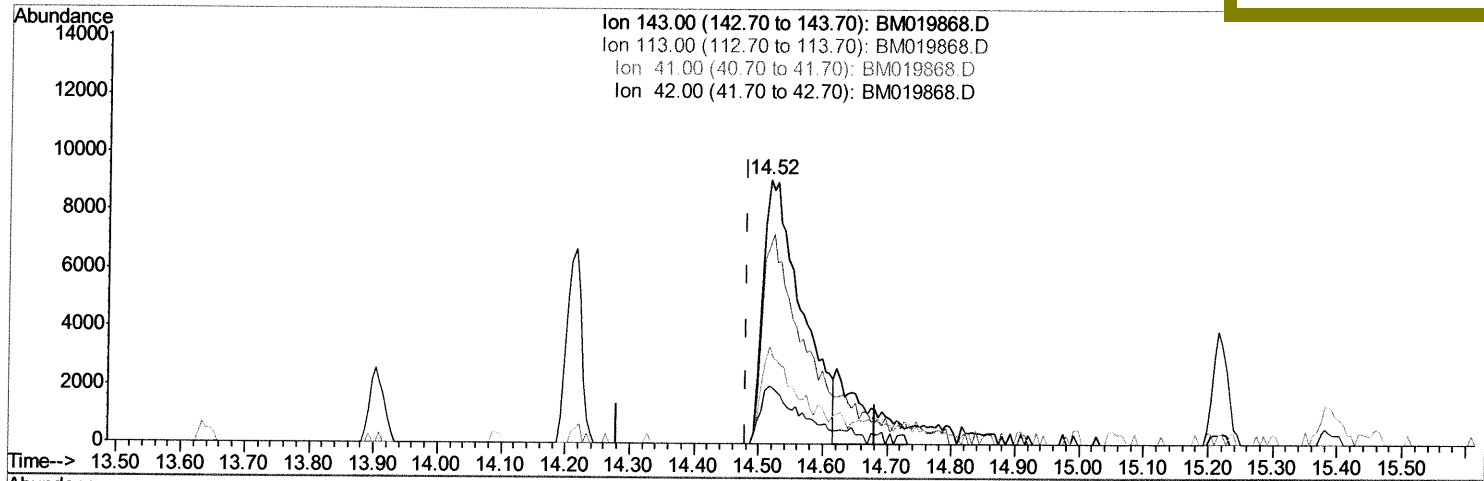

TIC: BM019868.D

(52) 4-Nitrophenol-d4 (S)

14.515min (+0.035) 7.51ng/ul

response 38205

Ion	Exp%	Act%
143.00	100	100
113.00	77.10	74.89
41.00	32.60	37.00
42.00	22.30	21.93

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
 Data File : BM019868.D
 Acq On : 10 Apr 2019 17:50
 Operator : JU/SJ
 Sample : K2303-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF885

Quant Time: Apr 11 03:23:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 03:09:11 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/12/2019 5:18:09 PM

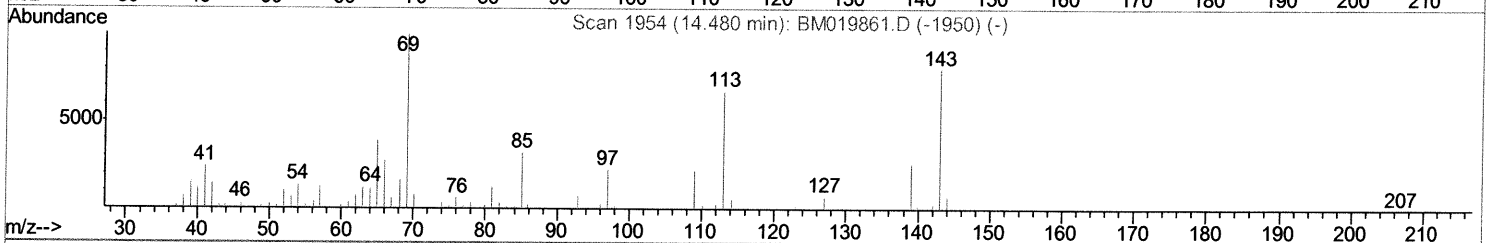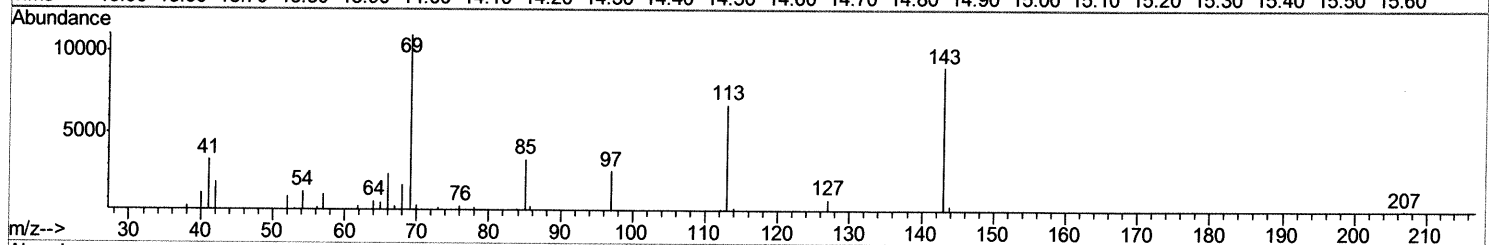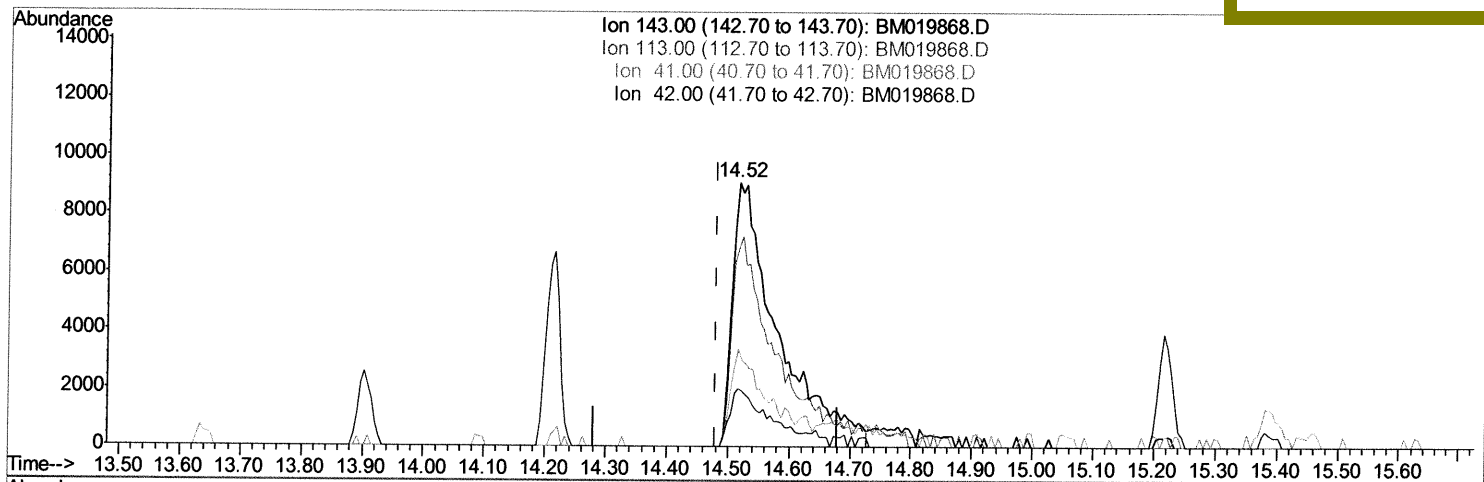

TIC: BM019868.D

(52) 4-Nitrophenol-d4 (S)

14.515min (+0.035) 9.21ng/ul m

response 46846

Ion	Exp%	Act%
143.00	100	100
113.00	77.10	74.89
41.00	32.60	37.00
42.00	22.30	21.93

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
 Data File : BM019868.D
 Acq On : 10 Apr 2019 17:50
 Operator : JU/SJ
 Sample : K2303-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF885

Quant Time: Apr 11 04:00:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 03:09:11 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/12/2019 5:18:09 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	165335	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	717399	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	402215	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	888710	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	784328	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	831786	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	17807	4.22	ng/uL	0.00
5) Phenol-d5	6.75	99	141391	9.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	94809	9.62	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	119813	10.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	90654	8.20	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	55069	10.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.44	143	63874	11.21	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	99969	9.30	ng/ul	0.01
29) 4-Chloroaniline-d4	10.51	131	120552	9.34	ng/ul	0.01
44) Dimethylphthalate-d6	13.64	166	339697	10.47	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	381068	9.39	ng/ul	0.00
52) 4-Nitrophenol-d4	14.52	143	46846m	9.21	ng/ul	0.04
58) Fluorene-d10	15.22	176	284441	10.17	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	34513	5.87	ng/ul	0.00
71) Anthracene-d10	17.07	188	460887	10.81	ng/ul	0.00
79) Pyrene-d10	19.39	212	572435	15.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.25	264	588407	13.34	ng/ul	0.00

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.69	163	66393	2.039	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed