
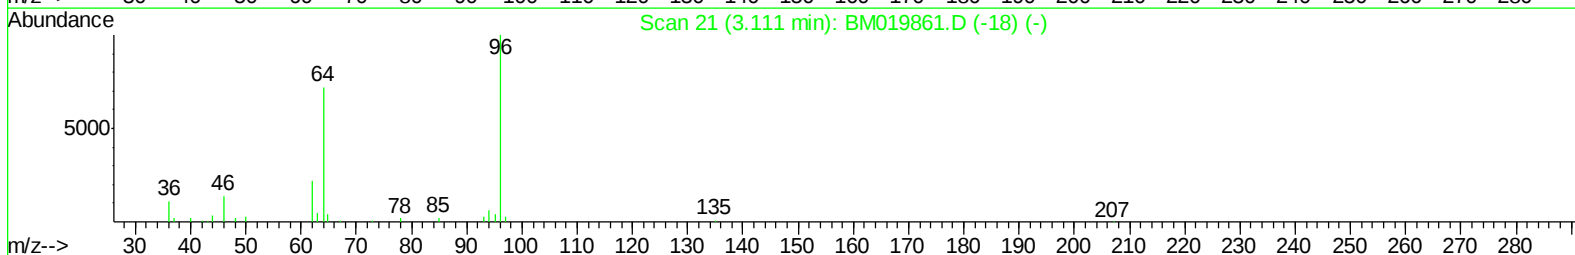
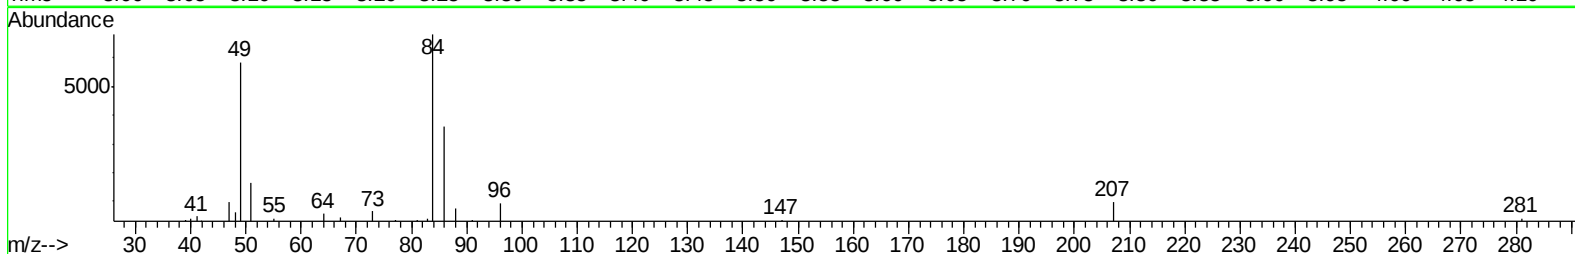


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019877.D
Acq On : 11 Apr 2019 00:00
Operator : JU/SJ
Sample : K2255-19DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 11 03:24:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 03:09:11 2019
Response via : Initial Calibration

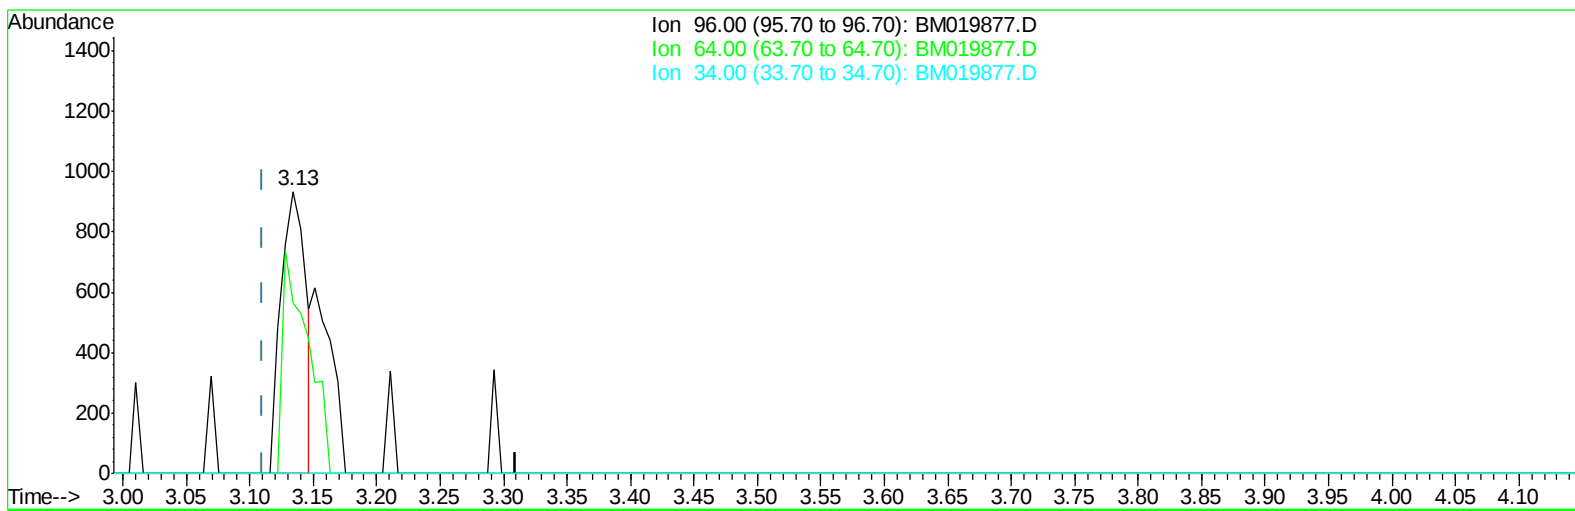

TIC: BM019877.D

(3) 1,4-Dioxane-d8 (S)




3.134min (+0.024) 0.39ng/uL

response 1245

Ion	Exp%	Act%
96.00	100	100
64.00	74.00	60.56
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019877.D
Acq On : 11 Apr 2019 00:00
Operator : JU/SJ
Sample : K2255-19DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 11 03:24:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 03:09:11 2019
Response via : Initial Calibration

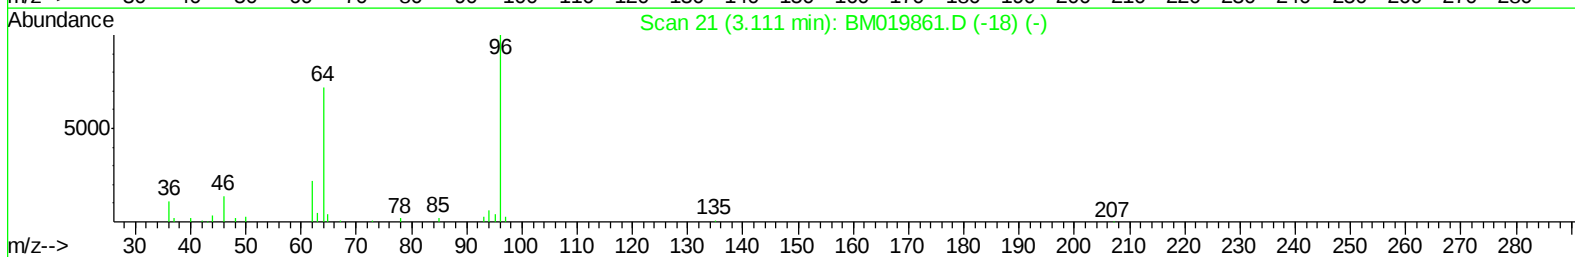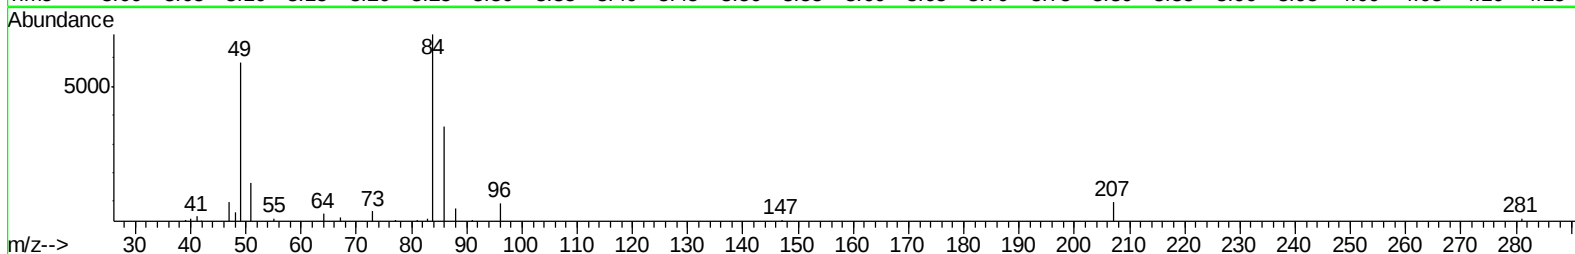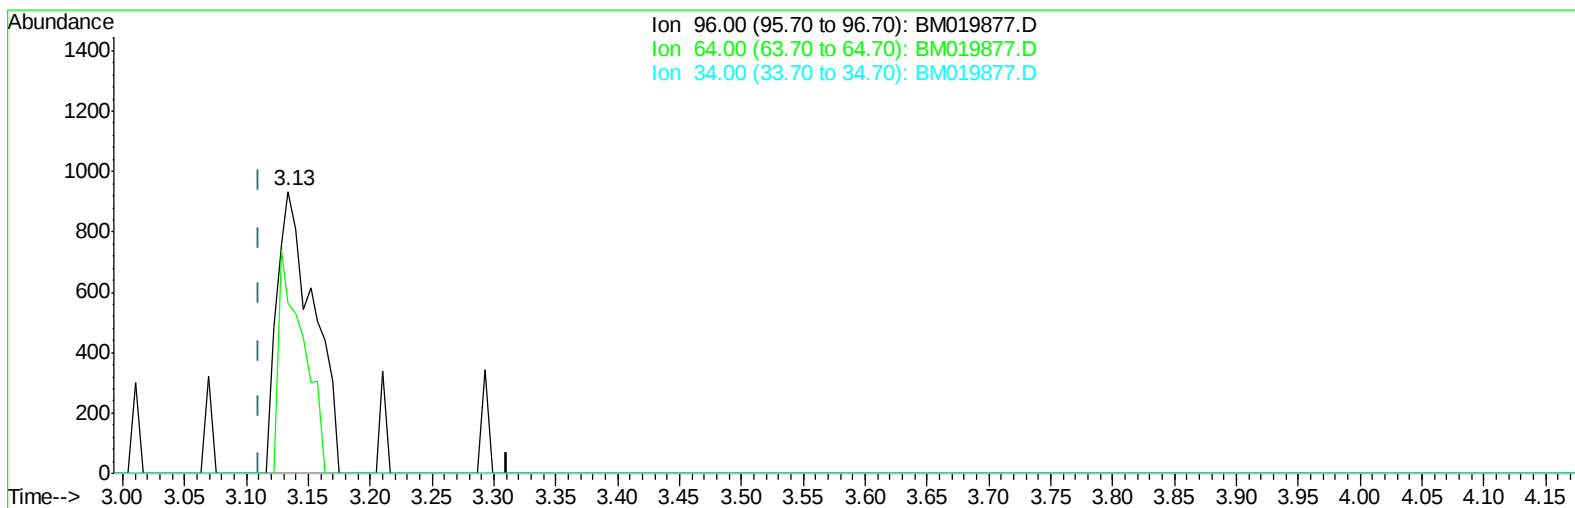

TIC: BM019877.D

(3) 1,4-Dioxane-d8 (S)




3.134min (+0.024) 0.59ng/uL m

response 1904

Ion	Exp%	Act%
96.00	100	100
64.00	74.00	60.56
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019877.D
Acq On : 11 Apr 2019 00:00
Operator : JU/SJ
Sample : K2255-19DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 11 03:24:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 03:09:11 2019
Response via : Initial Calibration

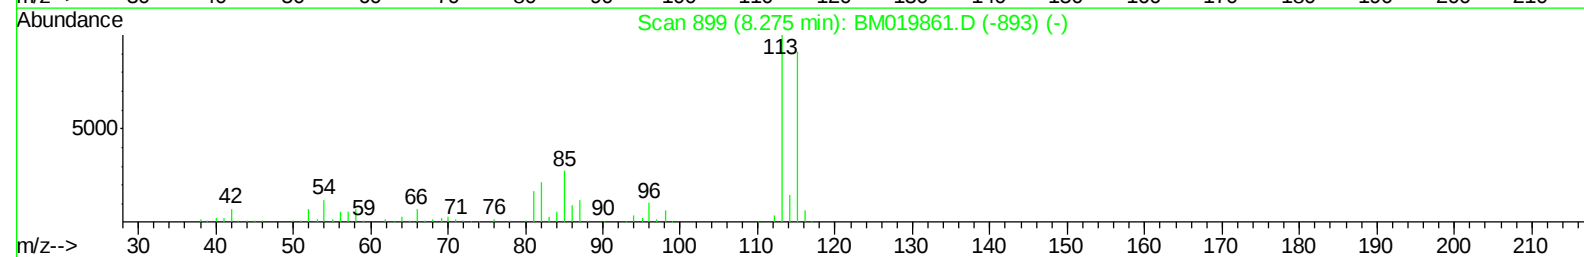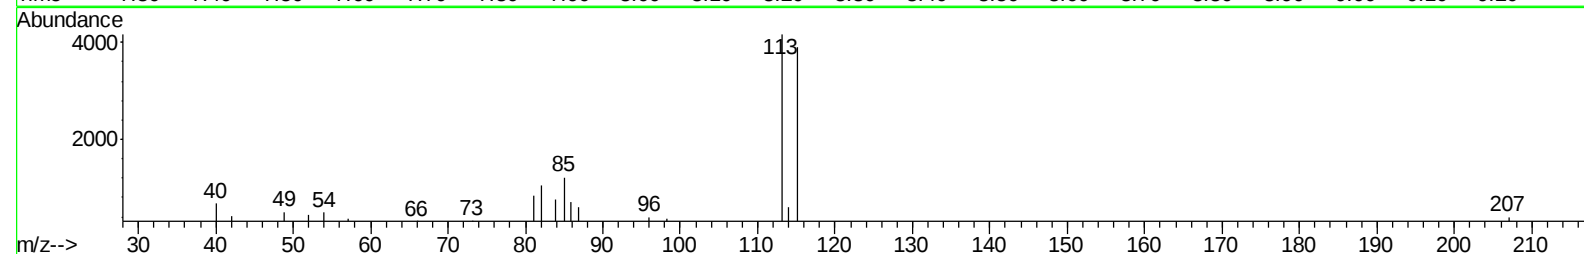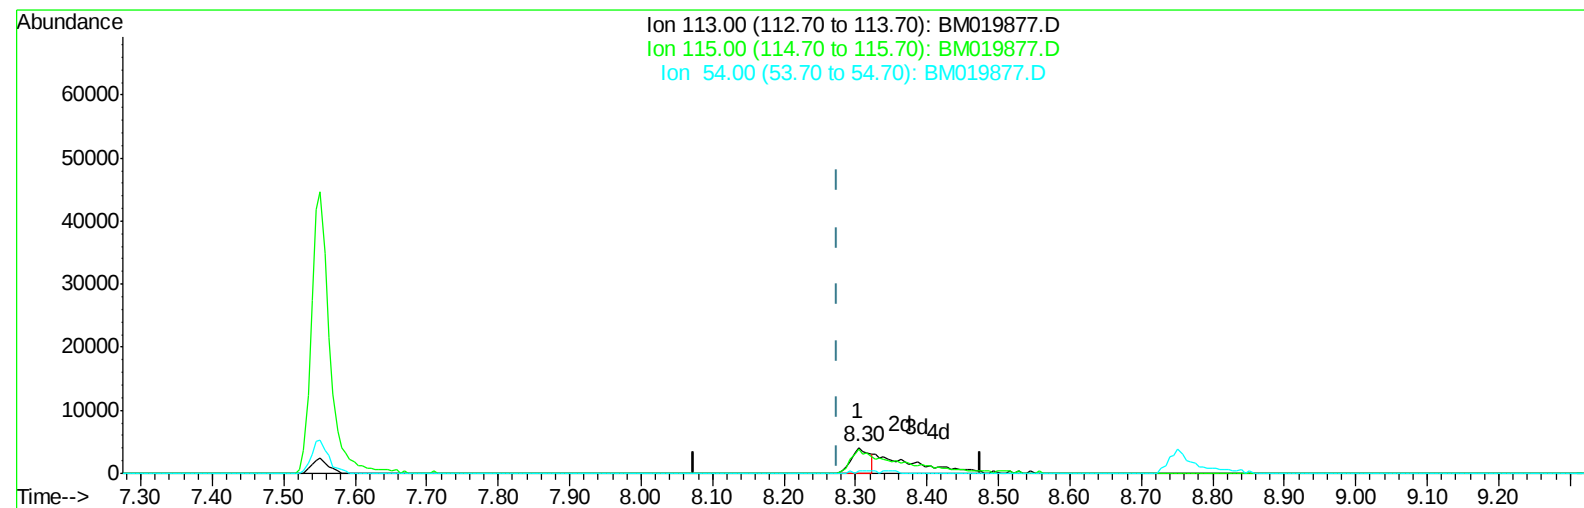

TIC: BM019877.D

(13) 4-Methylphenol-d8 (S)




8.304min (+0.029) 0.86ng/ul

response 7240

Ion	Exp%	Act%
113.00	100	100
115.00	89.70	93.97
54.00	13.30	11.62
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019877.D
Acq On : 11 Apr 2019 00:00
Operator : JU/SJ
Sample : K2255-19DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 11 03:24:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 03:09:11 2019
Response via : Initial Calibration

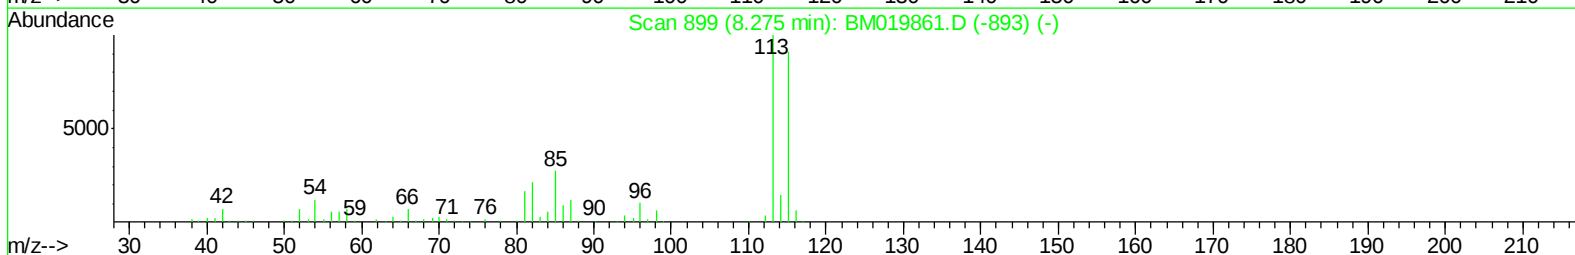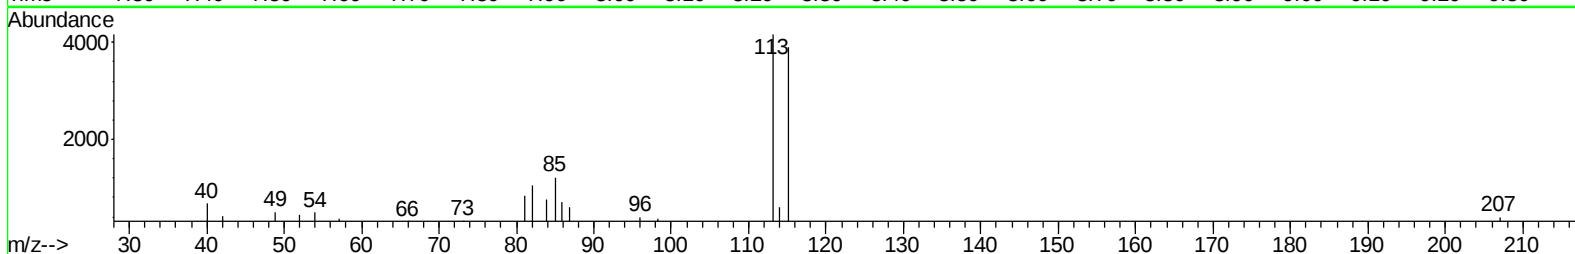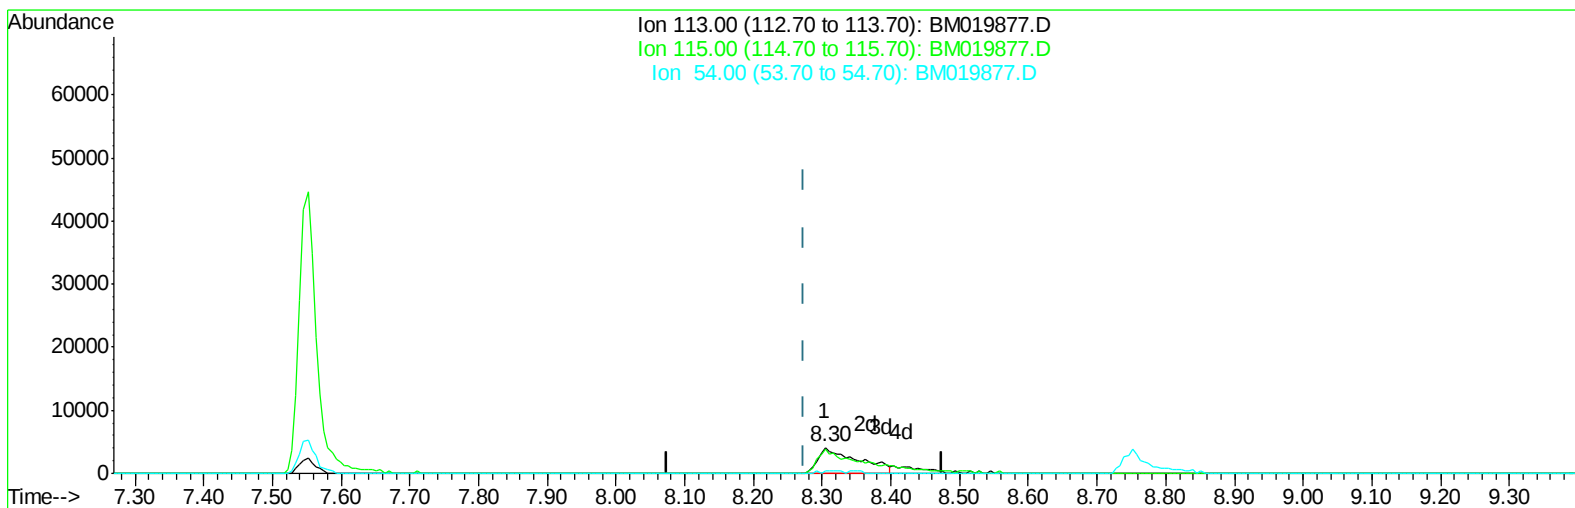

TIC: BM019877.D

(13) 4-Methylphenol-d8 (S)




8.304min (+0.029) 1.93ng/ul m

response 16233

Ion	Exp%	Act%
113.00	100	100
115.00	89.70	93.97
54.00	13.30	11.62
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019877.D
Acq On : 11 Apr 2019 00:00
Operator : JU/SJ
Sample : K2255-19DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 11 03:24:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 03:09:11 2019
Response via : Initial Calibration

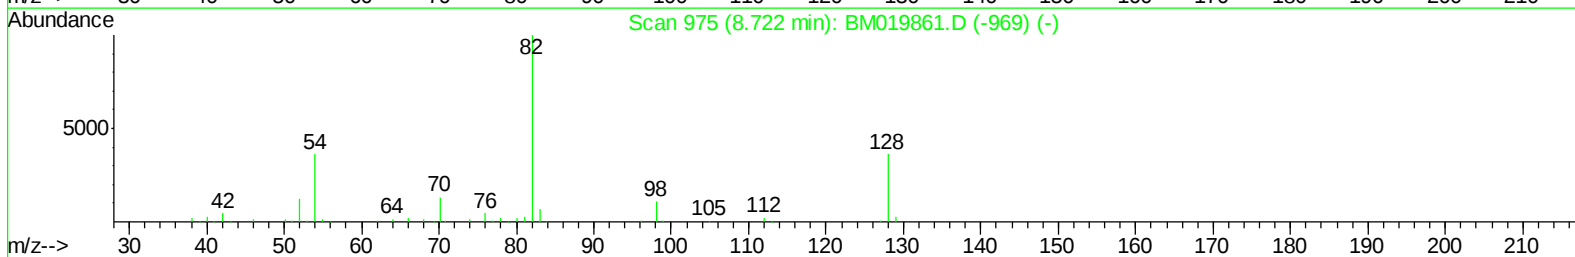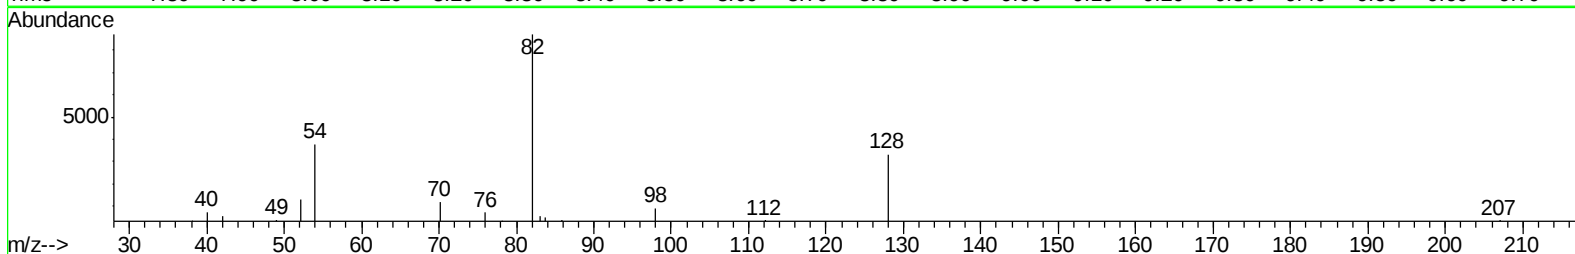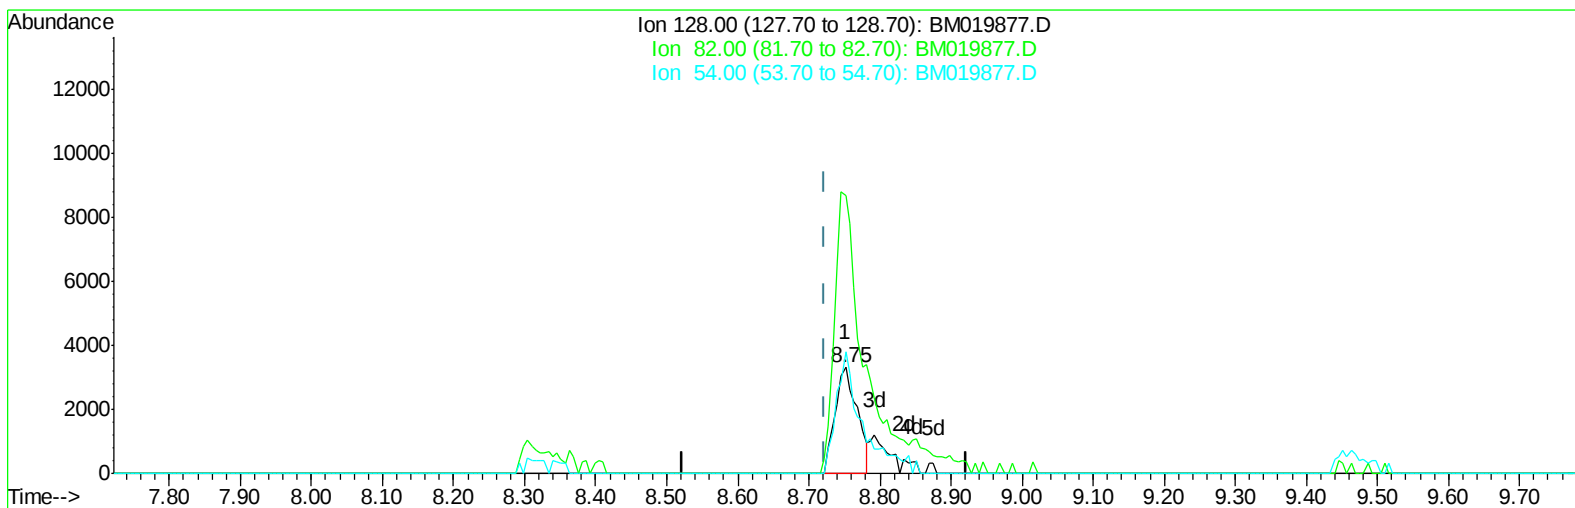

TIC: BM019877.D

(19) Nitrobenzene-d5 (S)




8.751min (+0.029) 1.96ng/ul

response 7080

Ion	Exp%	Act%
128.00	100	100
82.00	244.60	262.36
54.00	108.20	114.17
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019877.D
Acq On : 11 Apr 2019 00:00
Operator : JU/SJ
Sample : K2255-19DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 11 03:24:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 03:09:11 2019
Response via : Initial Calibration

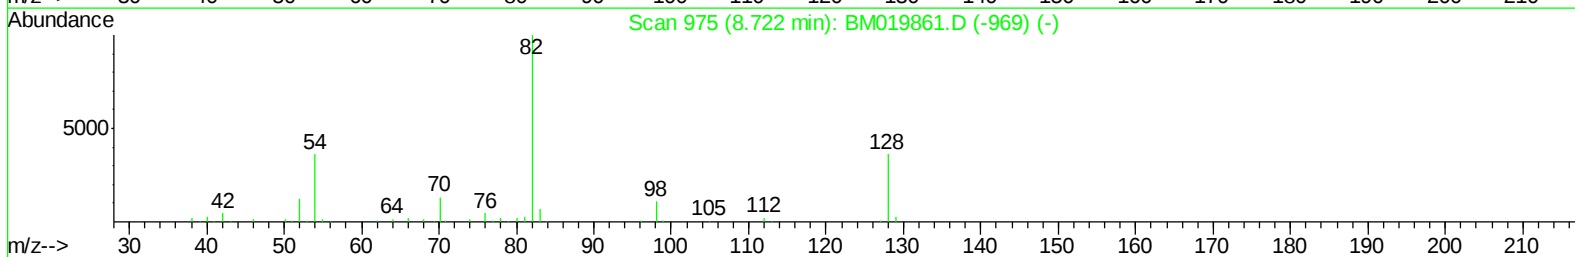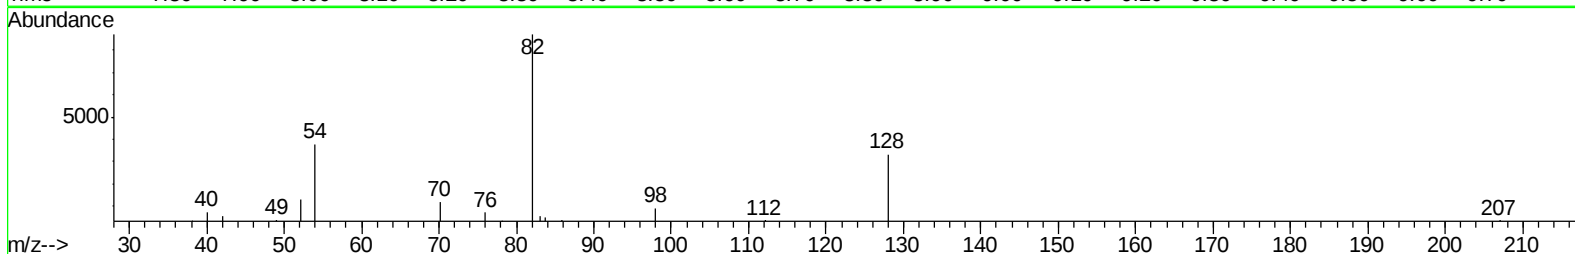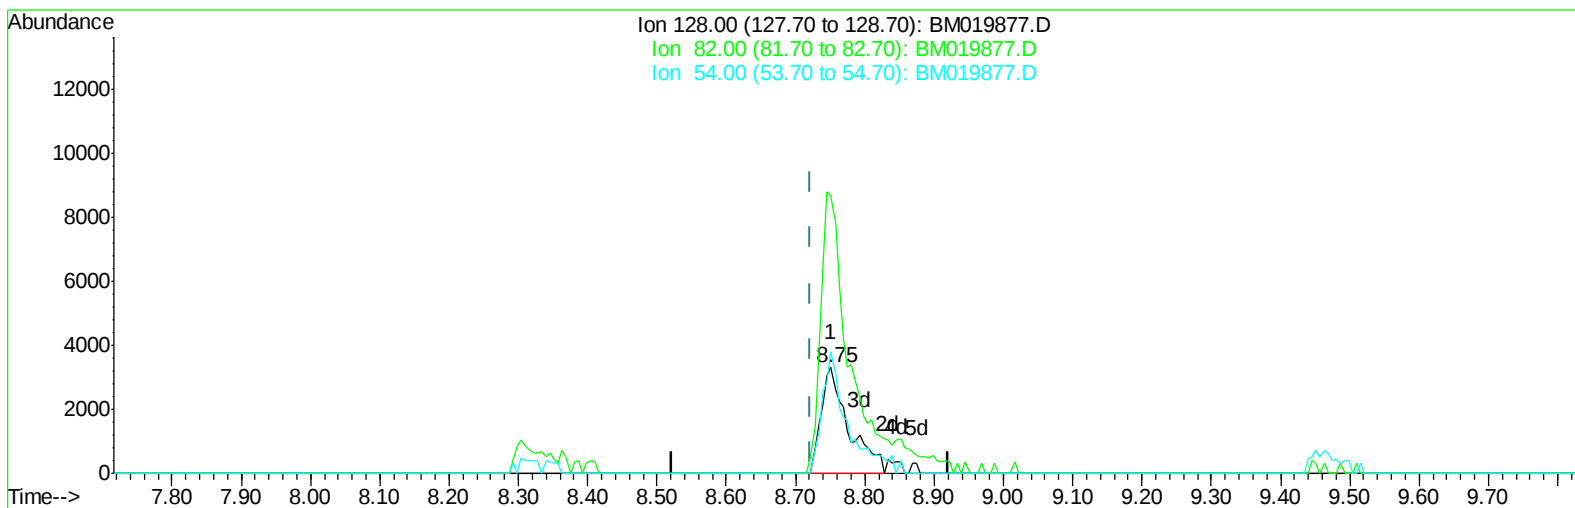

TIC: BM019877.D

(19) Nitrobenzene-d5 (S)




8.751min (+0.029) 2.52ng/ul m

response 9102

Ion	Exp%	Act%
128.00	100	100
82.00	244.60	262.36
54.00	108.20	114.17
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019877.D
Acq On : 11 Apr 2019 00:00
Operator : JU/SJ
Sample : K2255-19DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 11 03:24:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 03:09:11 2019
Response via : Initial Calibration

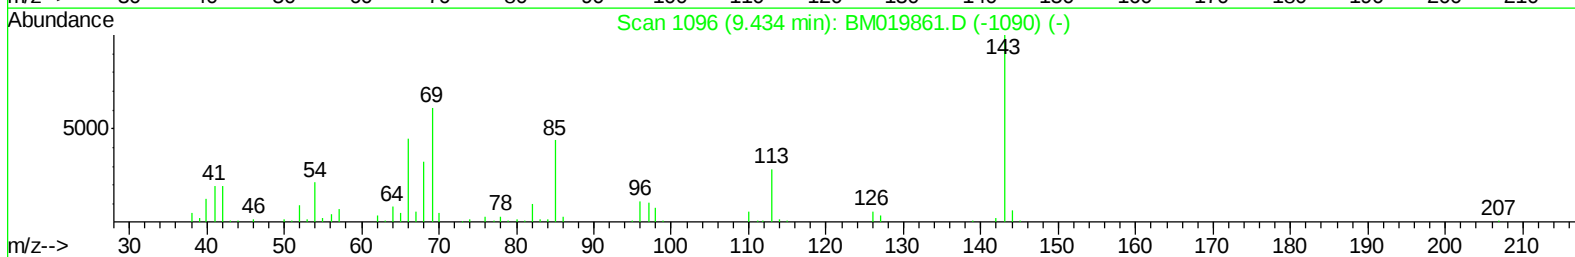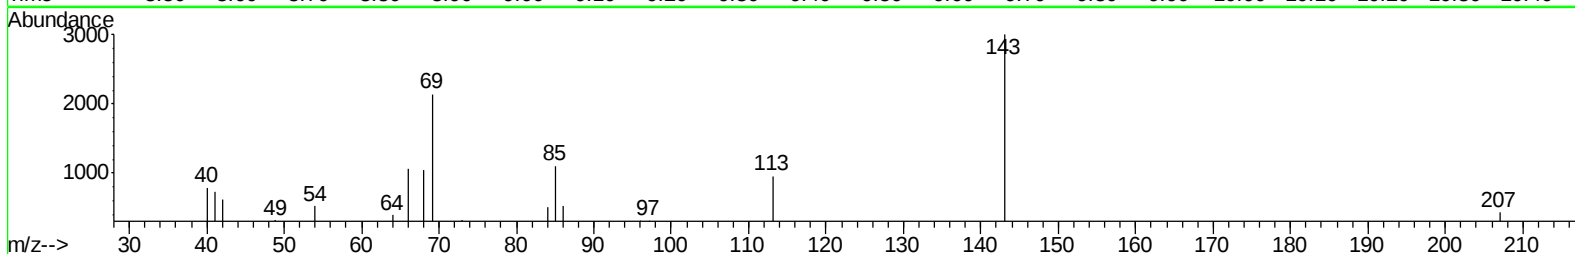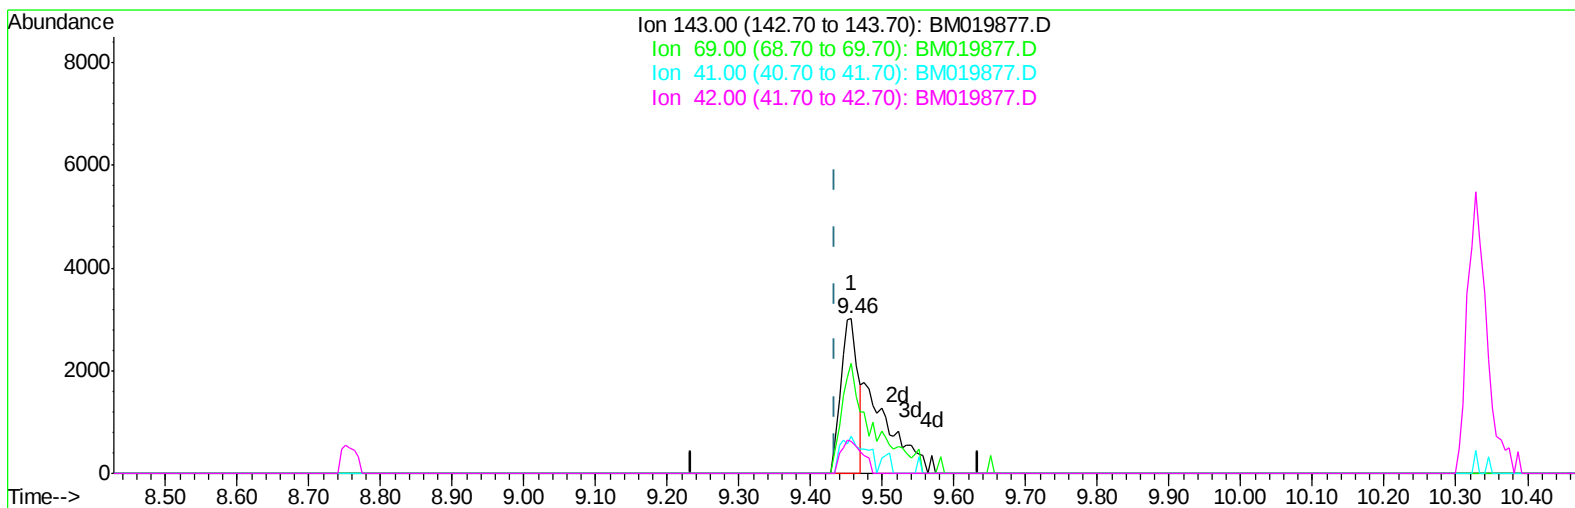

TIC: BM019877.D

(22) 2-Nitrophenol-d4 (S)




9.457min (+0.024) 1.24ng/ul

response 4977

Ion	Exp%	Act%
143.00	100	100
69.00	47.30	71.20#
41.00	18.80	24.04#
42.00	17.80	20.49

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019877.D
Acq On : 11 Apr 2019 00:00
Operator : JU/SJ
Sample : K2255-19DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 11 03:24:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 03:09:11 2019
Response via : Initial Calibration

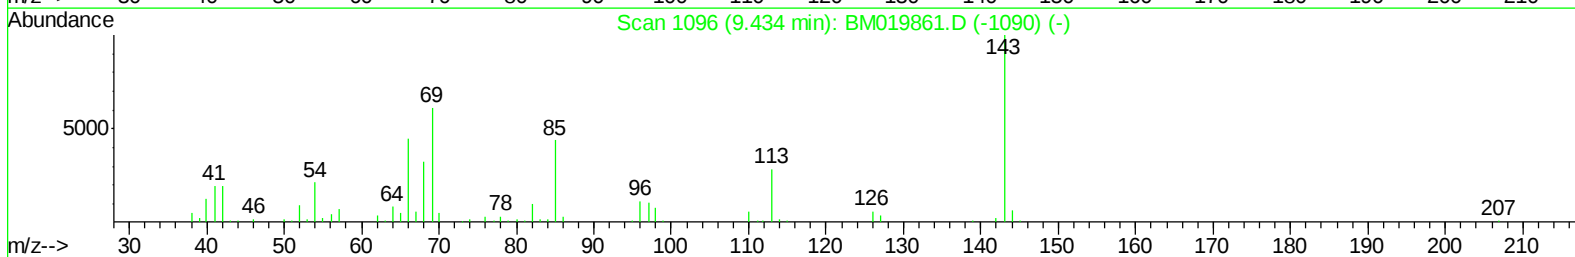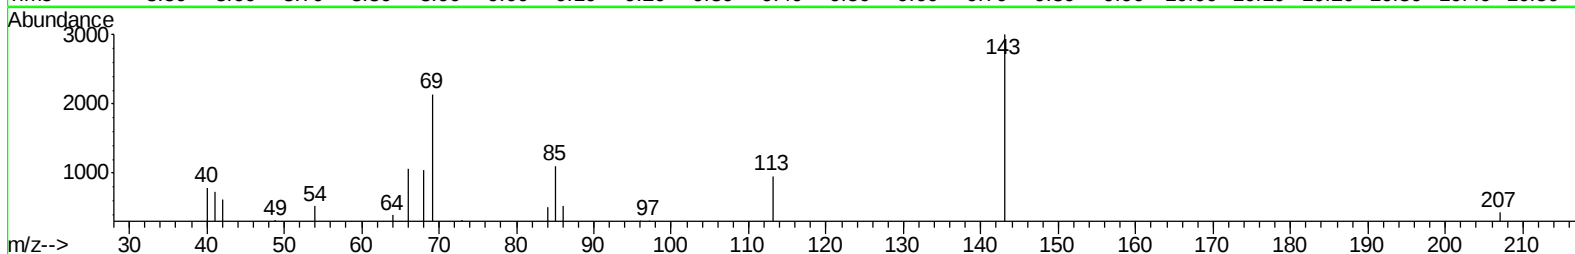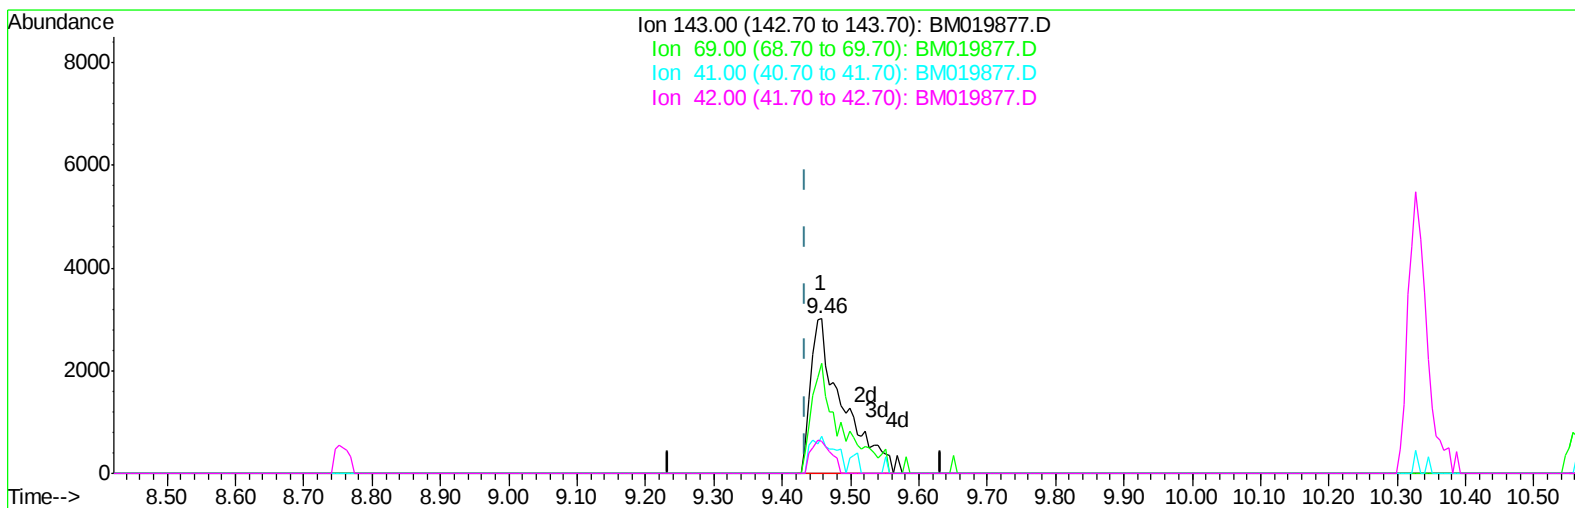




TIC: BM019877.D

(22) 2-Nitrophenol-d4 (S)
9.457min (+0.024) 2.41ng/ul m
response 9681

Ion	Exp%	Act%
143.00	100	100
69.00	47.30	71.20#
41.00	18.80	24.04#
42.00	17.80	20.49

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019877.D
Acq On : 11 Apr 2019 00:00
Operator : JU/SJ
Sample : K2255-19DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 11 03:24:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 03:09:11 2019
Response via : Initial Calibration

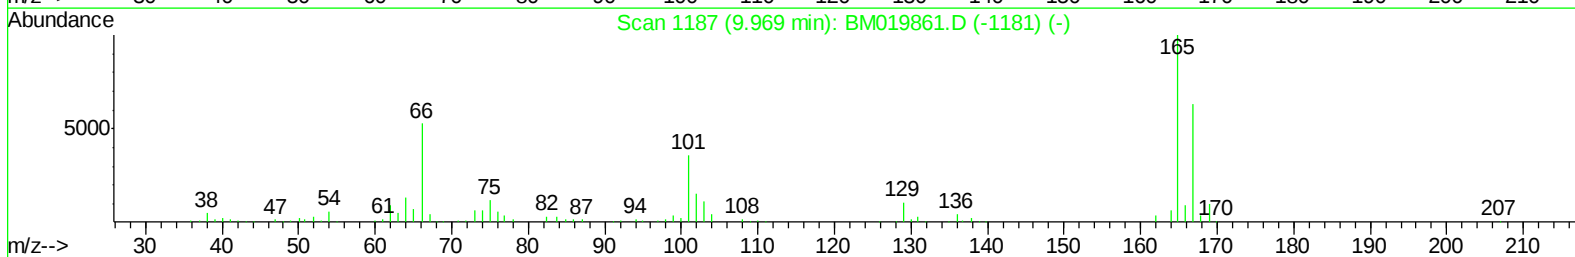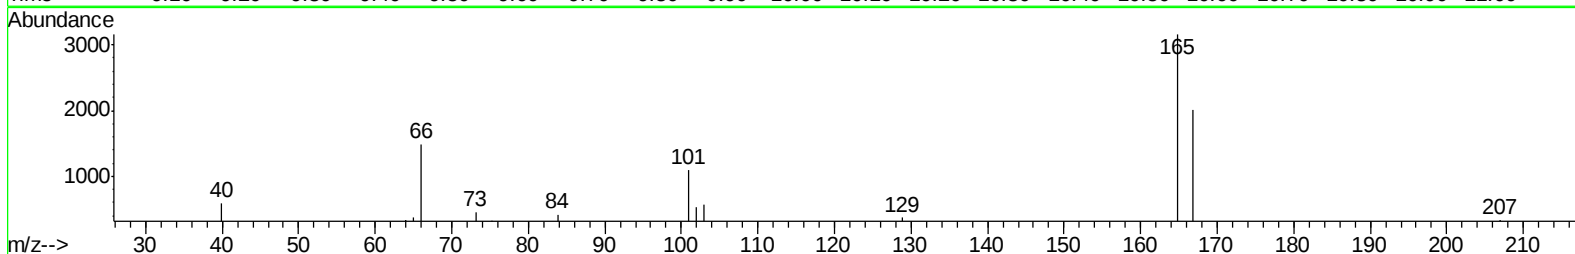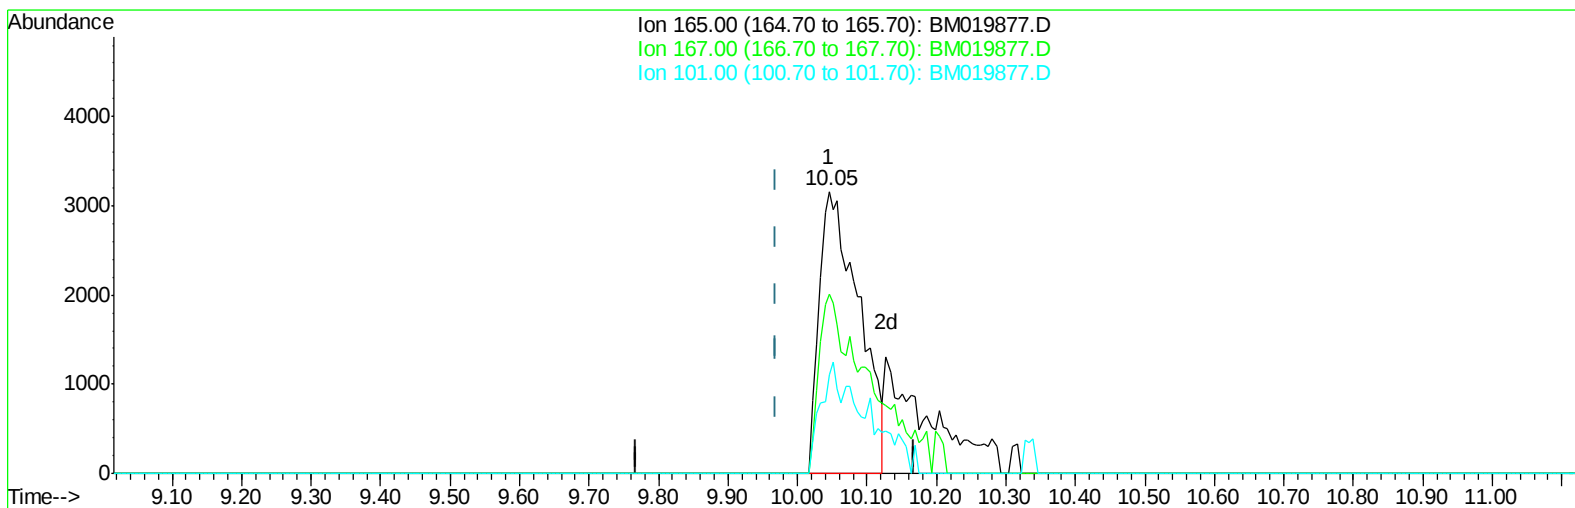

TIC: BM019877.D

(26) 2,4-Dichlorophenol-d3 (S)




10.045min (+0.076) 1.66ng/ul

response 12558

Ion	Exp%	Act%
165.00	100	100
167.00	69.50	63.54
101.00	31.20	34.94
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019877.D
Acq On : 11 Apr 2019 00:00
Operator : JU/SJ
Sample : K2255-19DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 11 03:24:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 03:09:11 2019
Response via : Initial Calibration

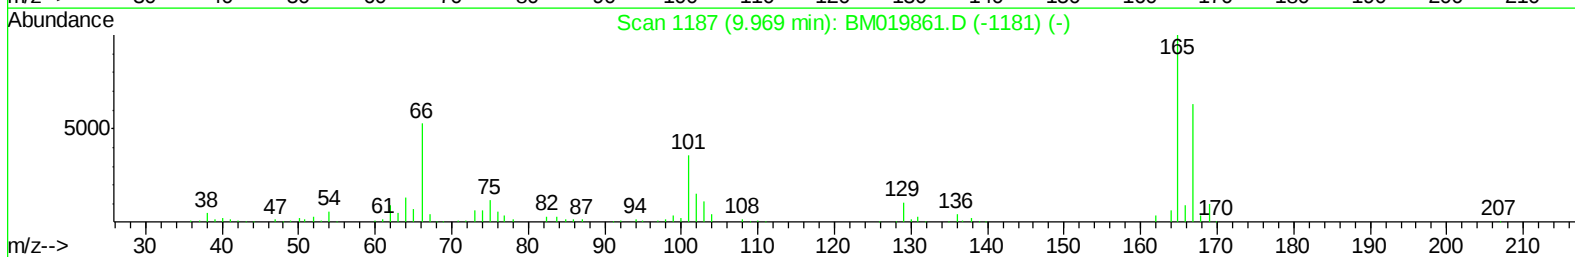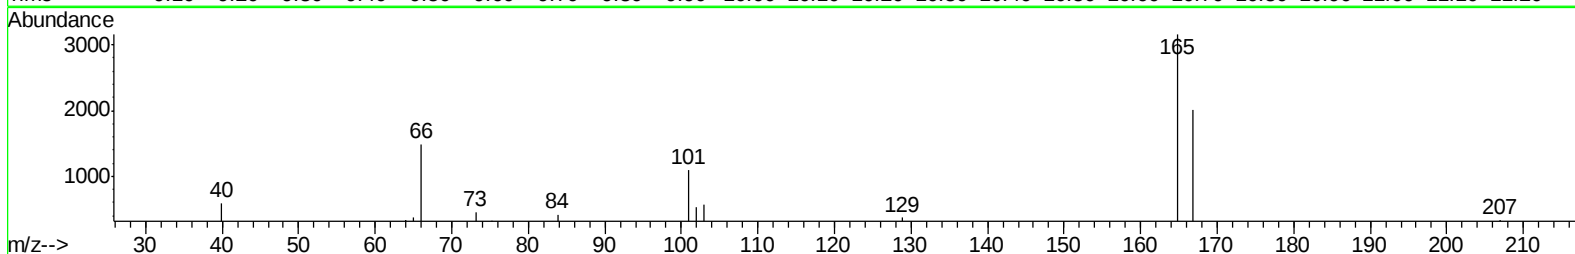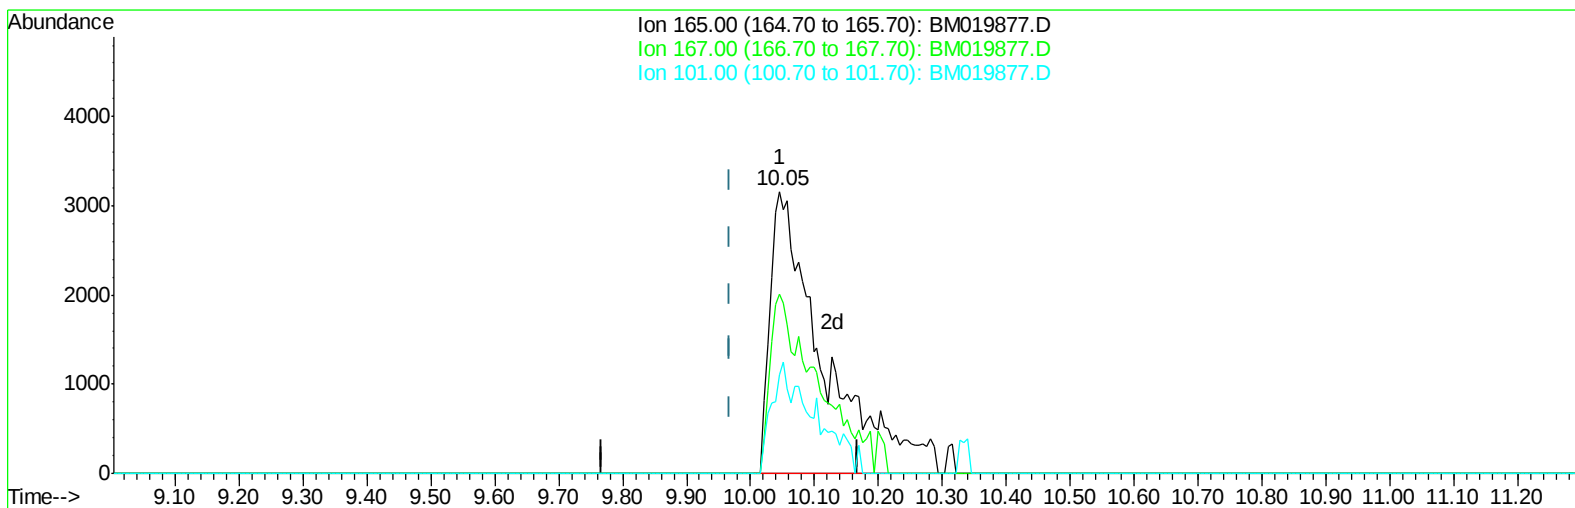

TIC: BM019877.D

(26) 2,4-Dichlorophenol-d3 (S)




10.045min (+0.076) 2.41ng/ul m

response 18275

Ion	Exp%	Act%
165.00	100	100
167.00	69.50	63.54
101.00	31.20	34.94
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019877.D
Acq On : 11 Apr 2019 00:00
Operator : JU/SJ
Sample : K2255-19DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 11 03:24:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 03:09:11 2019
Response via : Initial Calibration

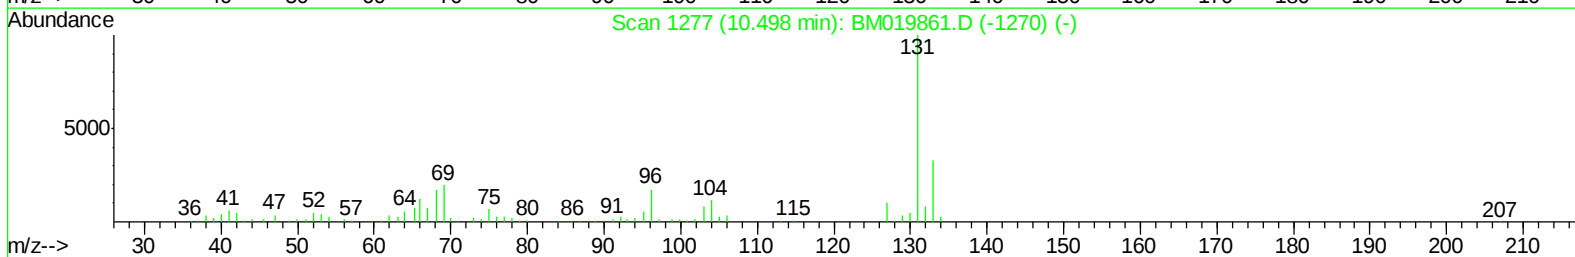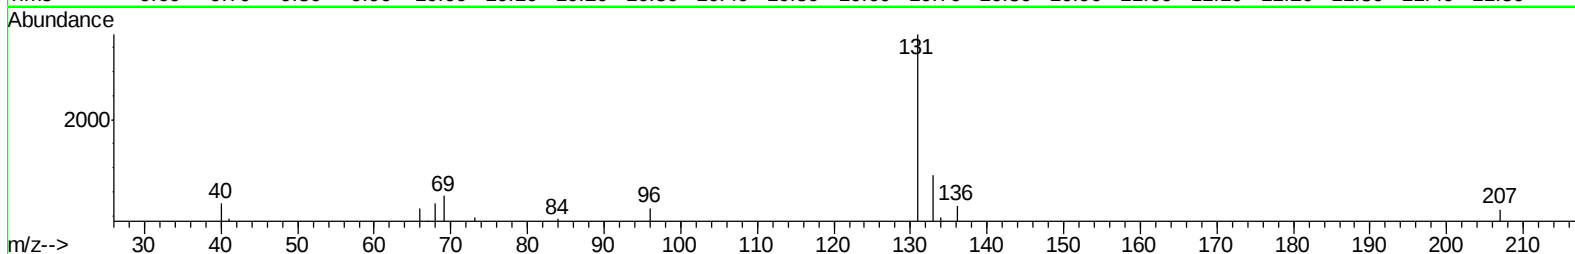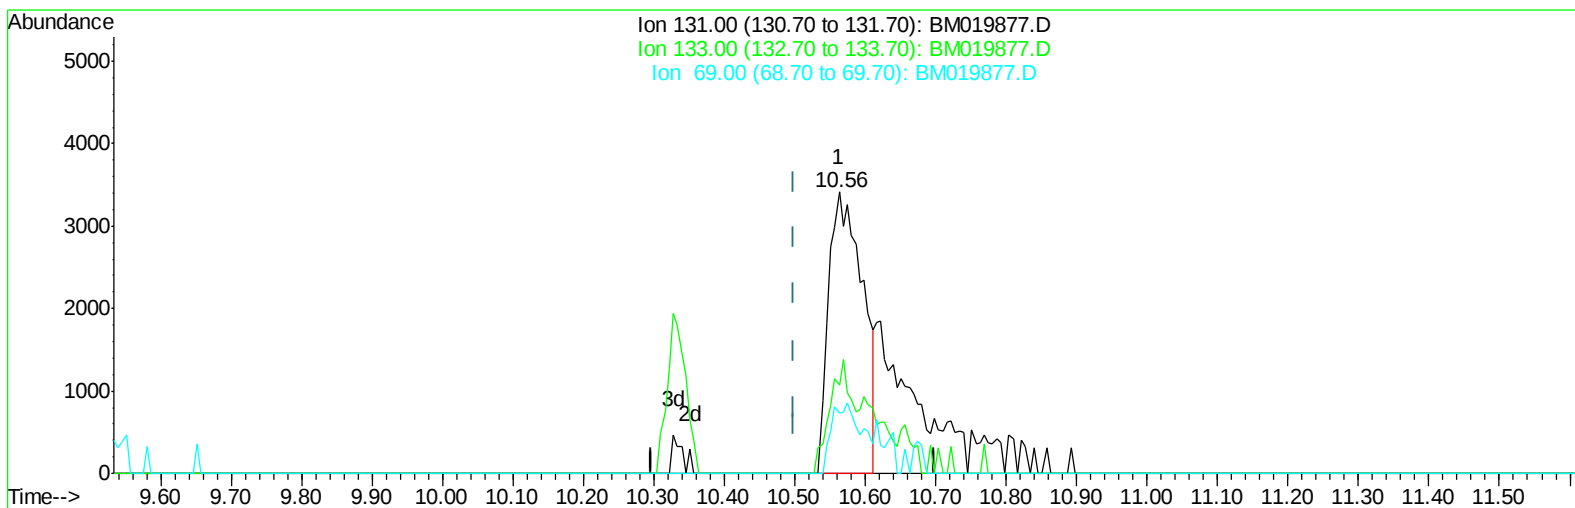




TIC: BM019877.D

(29) 4-Chloroaniline-d4 (S)
10.563min (+0.065) 1.25ng/ul
response 11337

Ion	Exp%	Act%
131.00	100	100
133.00	33.90	31.38
69.00	18.60	21.34
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019877.D
Acq On : 11 Apr 2019 00:00
Operator : JU/SJ
Sample : K2255-19DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 11 03:24:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 03:09:11 2019
Response via : Initial Calibration

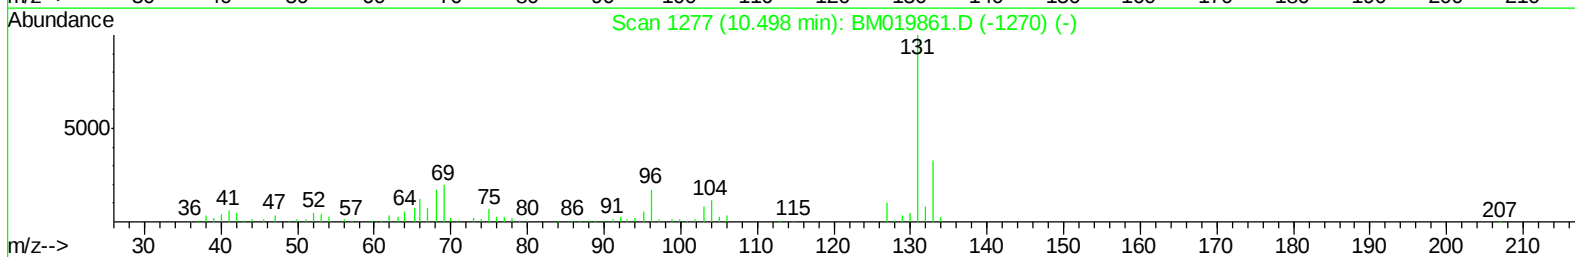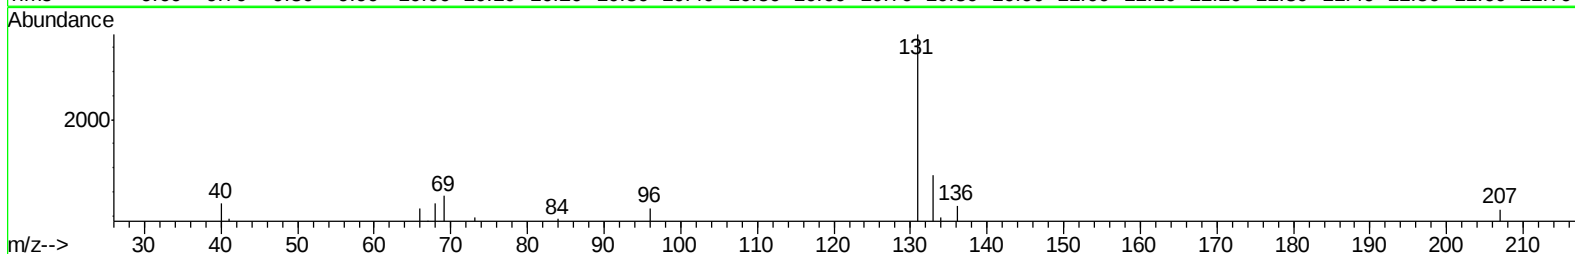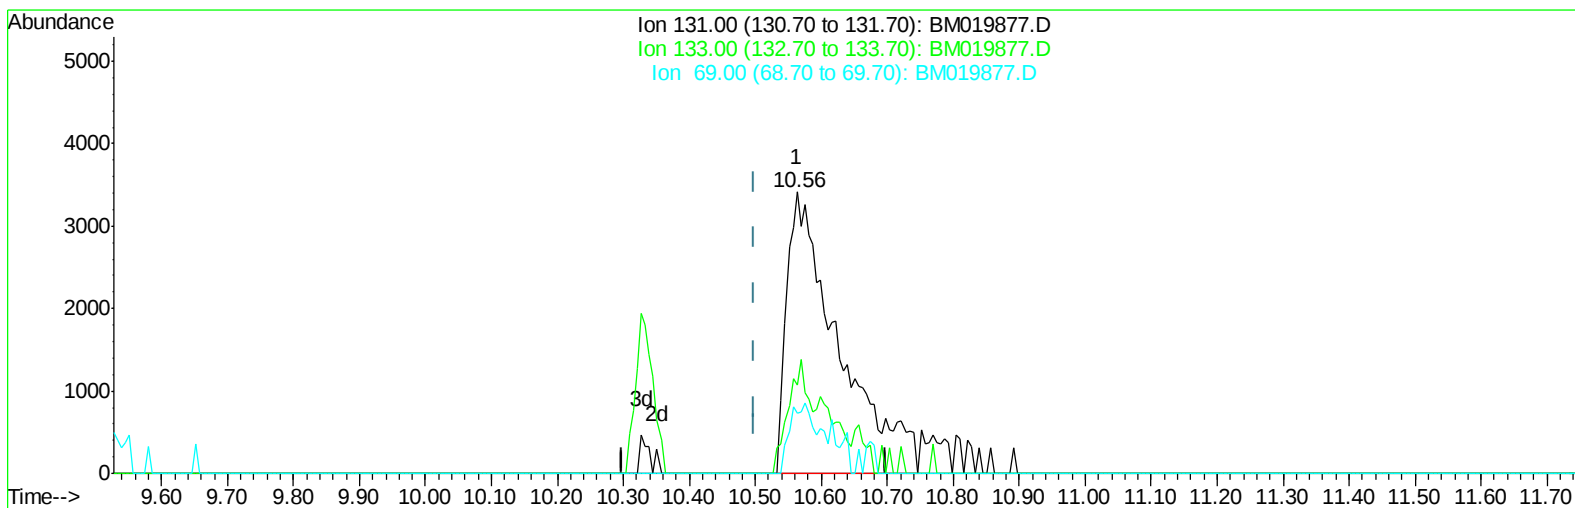

TIC: BM019877.D

(29) 4-Chloroaniline-d4 (S)




10.563min (+0.065) 2.02ng/ul m

response 18402

Ion	Exp%	Act%
131.00	100	100
133.00	33.90	31.38
69.00	18.60	21.34
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019877.D
Acq On : 11 Apr 2019 00:00
Operator : JU/SJ
Sample : K2255-19DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 11 03:24:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 03:09:11 2019
Response via : Initial Calibration

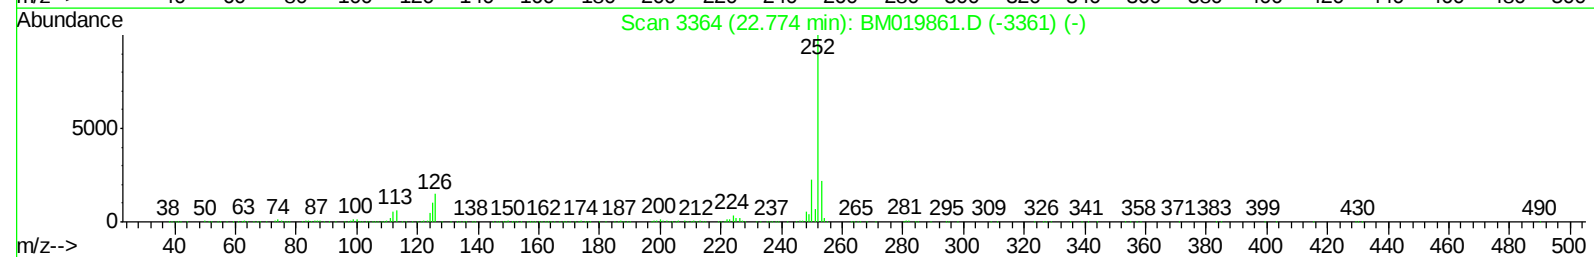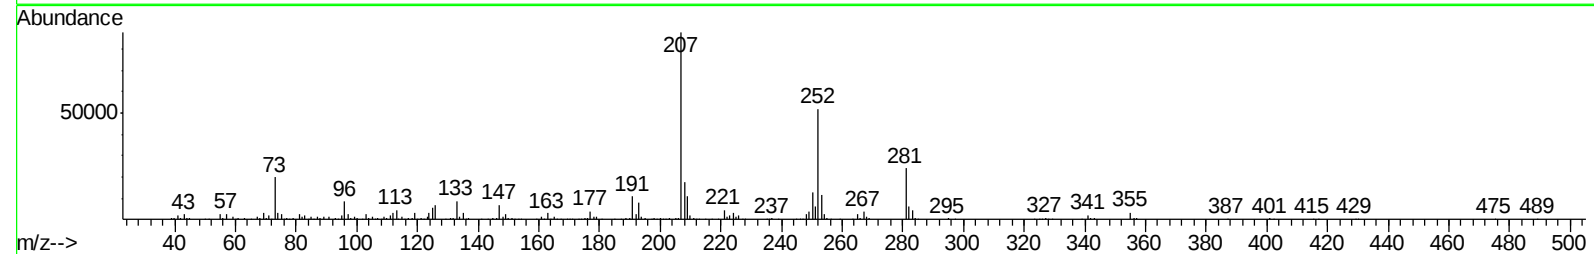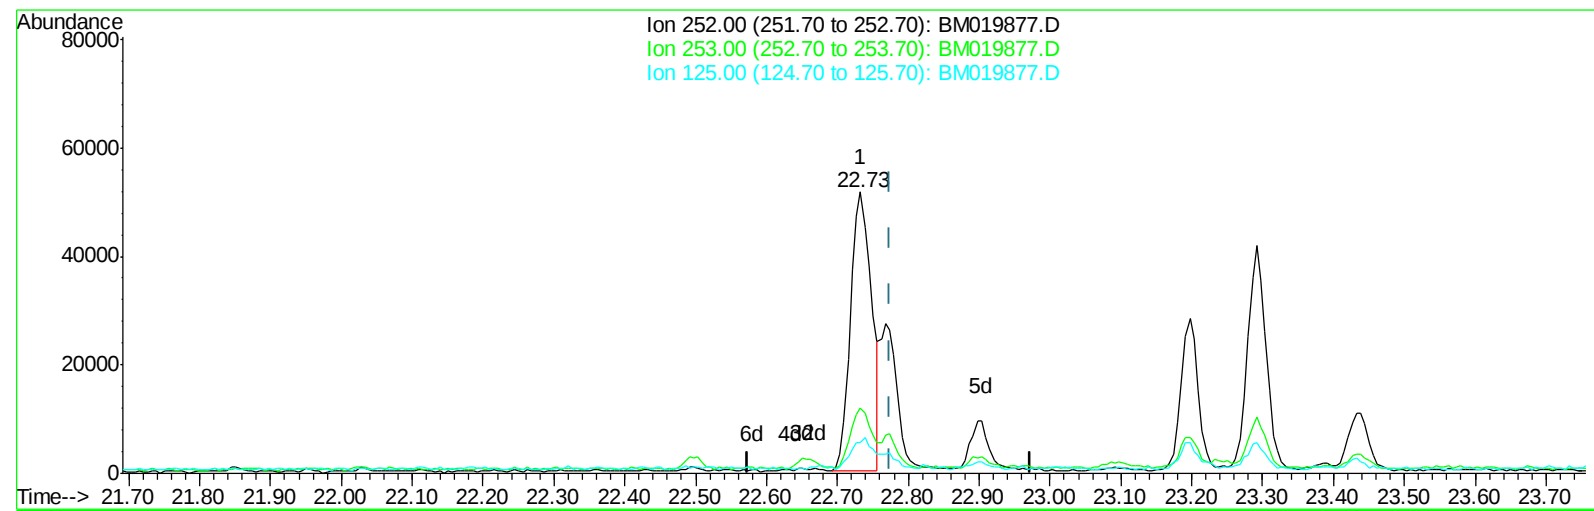




TIC: BM019877.D

(89) Benzo(k)fluoranthene
22.733min (-0.041) 2.98ng/ul
response 107372

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	23.05
125.00	6.70	10.91#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019877.D
Acq On : 11 Apr 2019 00:00
Operator : JU/SJ
Sample : K2255-19DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 11 03:24:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 03:09:11 2019
Response via : Initial Calibration

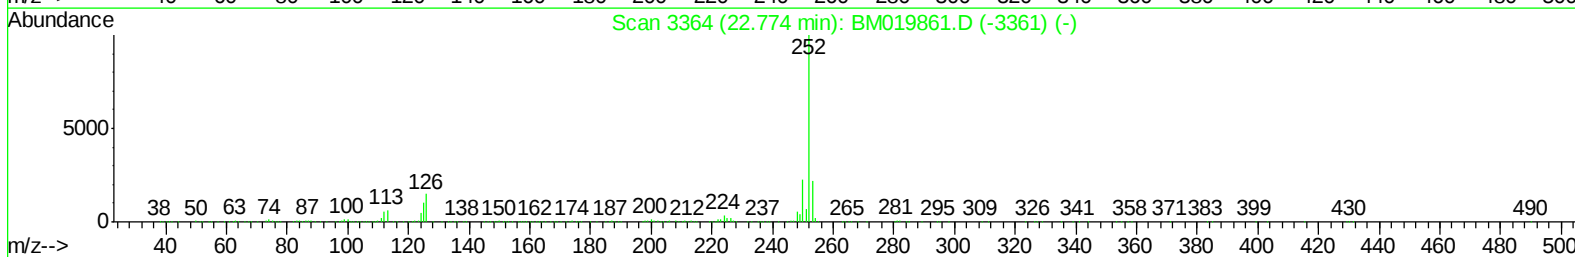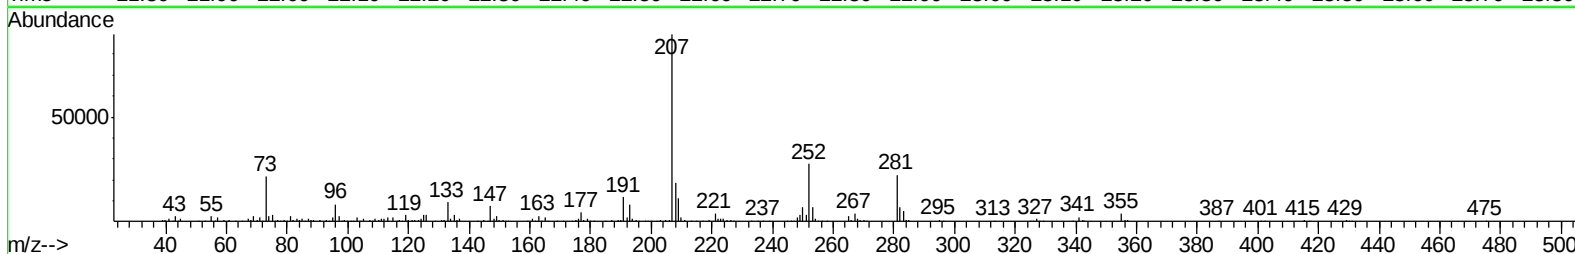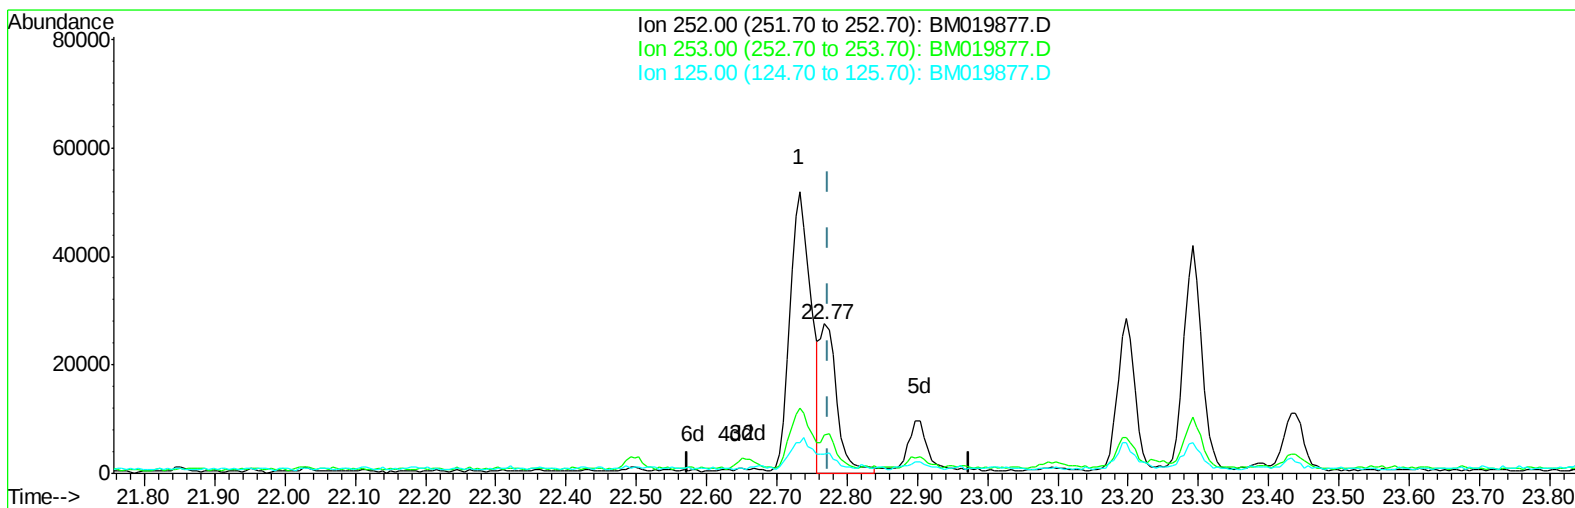

TIC: BM019877.D

(89) Benzo(k)fluoranthene

22.768min (-0.006) 1.31ng/ul m

response 47247

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	26.12#
125.00	6.70	12.74#
0.00	0.00	0.00