

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
 Data File : BM019870.D
 Acq On : 10 Apr 2019 19:04
 Operator : JU/SJ
 Sample : K2303-20
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF8B3

Manual Integrations
 APPROVED

Sohil
 4/12/2019 5:18:15 PM

Quant Time: Apr 11 04:04:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 03:09:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	173362	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	757147	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.21	164	415952	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	898742	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	855353	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	921998	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	17842	4.03	ng/uL	0.00
5) Phenol-d5	6.75	99	131795	8.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	93992	9.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	114376	9.78	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	77537	6.69	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	52769	9.77	ng/ul	0.00
22) 2-Nitrophenol-d4	9.44	143	59268	9.86	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	88582	7.81	ng/ul	0.01
29) 4-Chloroaniline-d4	10.51	131	116333	8.54	ng/ul	0.01
44) Dimethylphthalate-d6	13.64	166	341180	10.17	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	391814	9.34	ng/ul	0.00
52) 4-Nitrophenol-d4	14.52	143	34351m	6.53	ng/ul	0.04
58) Fluorene-d10	15.22	176	286327	9.90	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	30484	5.13	ng/ul	0.01
71) Anthracene-d10	17.07	188	420629	9.75	ng/ul	0.00
79) Pyrene-d10	19.39	212	452117	11.44	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.25	264	464842	9.51	ng/ul	0.00

Target Compounds					Qvalue
45) Dimethylphthalate	13.69	163	76930	2.285 ng/ul#	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019870.D
Acq On : 10 Apr 2019 19:04
Operator : JU/SJ
Sample : K2303-20
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BF8B3

Manual Integrations
APPROVED

Sohil
4/12/2019 5:18:15 PM

Quant Time: Apr 11 04:04:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 03:09:11 2019
Response via : Initial Calibration

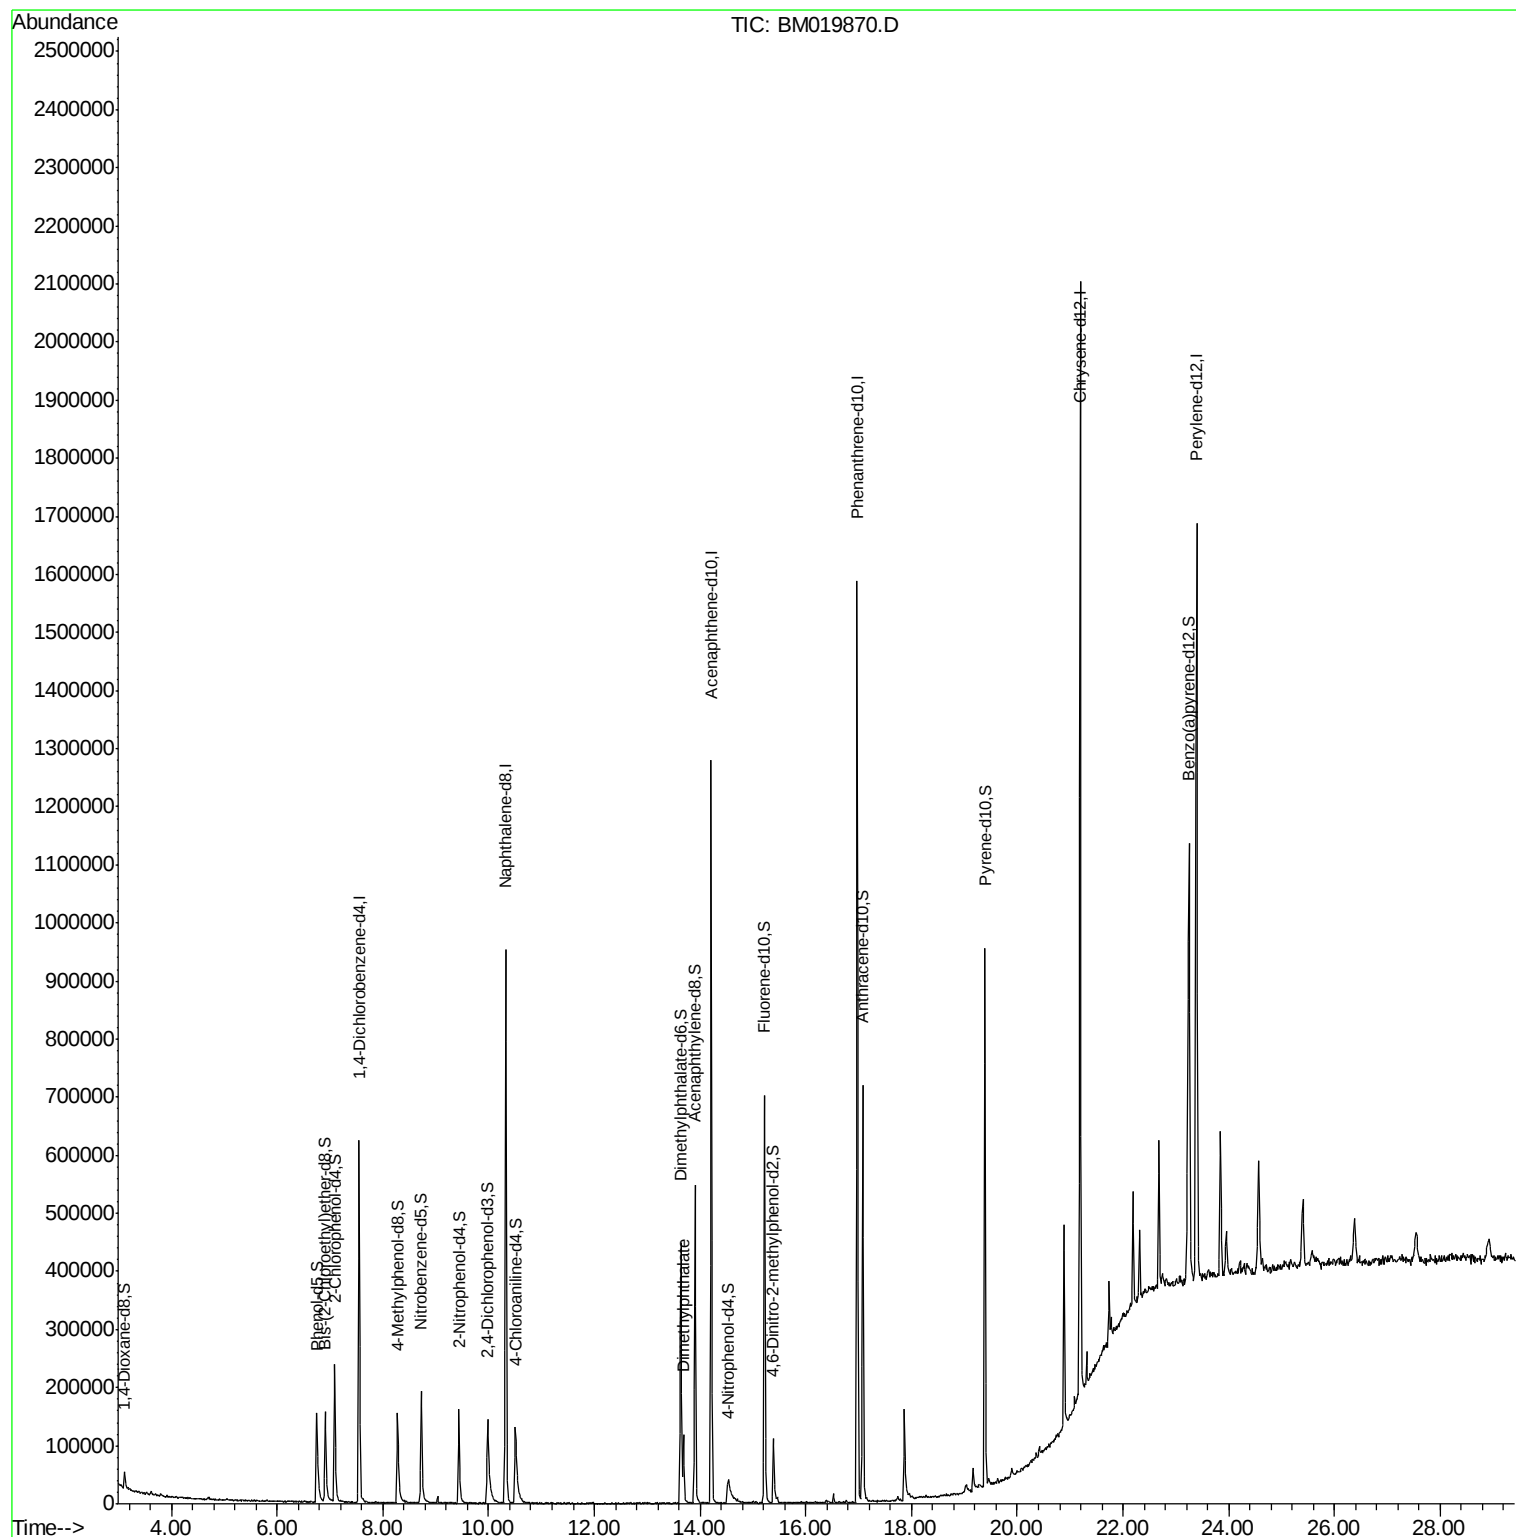

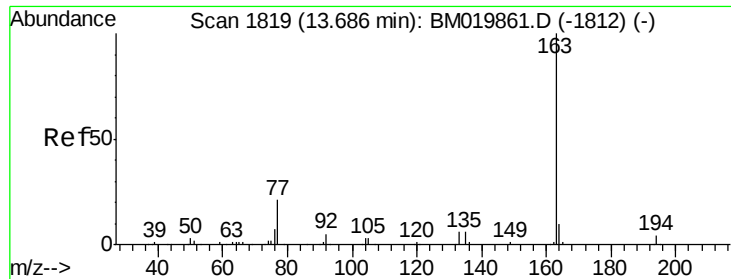

#45
 Dimethylphthalate
 Concen: 2.285 ng/ul
 RT: 13.69 min Scan# 1819
 Delta R.T. 0.00 min
 Lab File: BM019870.D
 Acq: 10 Apr 2019 19:04

Instrument :
 BNA_M
 ClientSampleId :
 BF8B3

Tgt Ion	Ratio	Resp Lower	Upper
163	100		
194	3.6	4.0	6.0#
164	10.3	8.4	12.6

Manual Integrations
 APPROVED

Sohil
 4/12/2019 5:18:15 PM

