

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
 Data File : BM019885.D
 Acq On : 11 Apr 2019 04:55
 Operator : JU/SJ
 Sample : K2303-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF896

Manual Integrations
 APPROVED

Sohil
 4/12/2019 5:19:01 PM

Quant Time: Apr 11 06:02:38 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 03:09:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	163940	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	633856	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	308530	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	583332	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	639774	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	780226	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	26376	6.30	ng/uL	0.00
5) Phenol-d5	6.75	99	187760	12.86	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	141016	14.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	169441	15.31	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	107521	9.81	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	77001	17.03	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	84078	16.71	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	131290	13.83	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	51436	4.51	ng/ul	0.02
44) Dimethylphthalate-d6	13.63	166	416925	16.75	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	498084	16.00	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	35463m	9.09	ng/ul	0.05
58) Fluorene-d10	15.22	176	330874	15.43	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	10608	2.75	ng/ul	0.01
71) Anthracene-d10	17.08	188	447338	15.98	ng/ul	0.00
79) Pyrene-d10	19.39	212	454475	15.38	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	572023	13.83	ng/ul	0.00

Target Compounds

					Qvalue
45) Dimethylphthalate	13.69	163	101707	4.072 ng/ul#	97
84) Bis(2-ethylhexyl)phthalate	21.09	149	25651	1.161 ng/ul#	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019885.D
Acq On : 11 Apr 2019 04:55
Operator : JU/SJ
Sample : K2303-01
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BF896

Manual Integrations
APPROVED

Sohil
4/12/2019 5:19:01 PM

Quant Time: Apr 11 06:02:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 03:09:11 2019
Response via : Initial Calibration

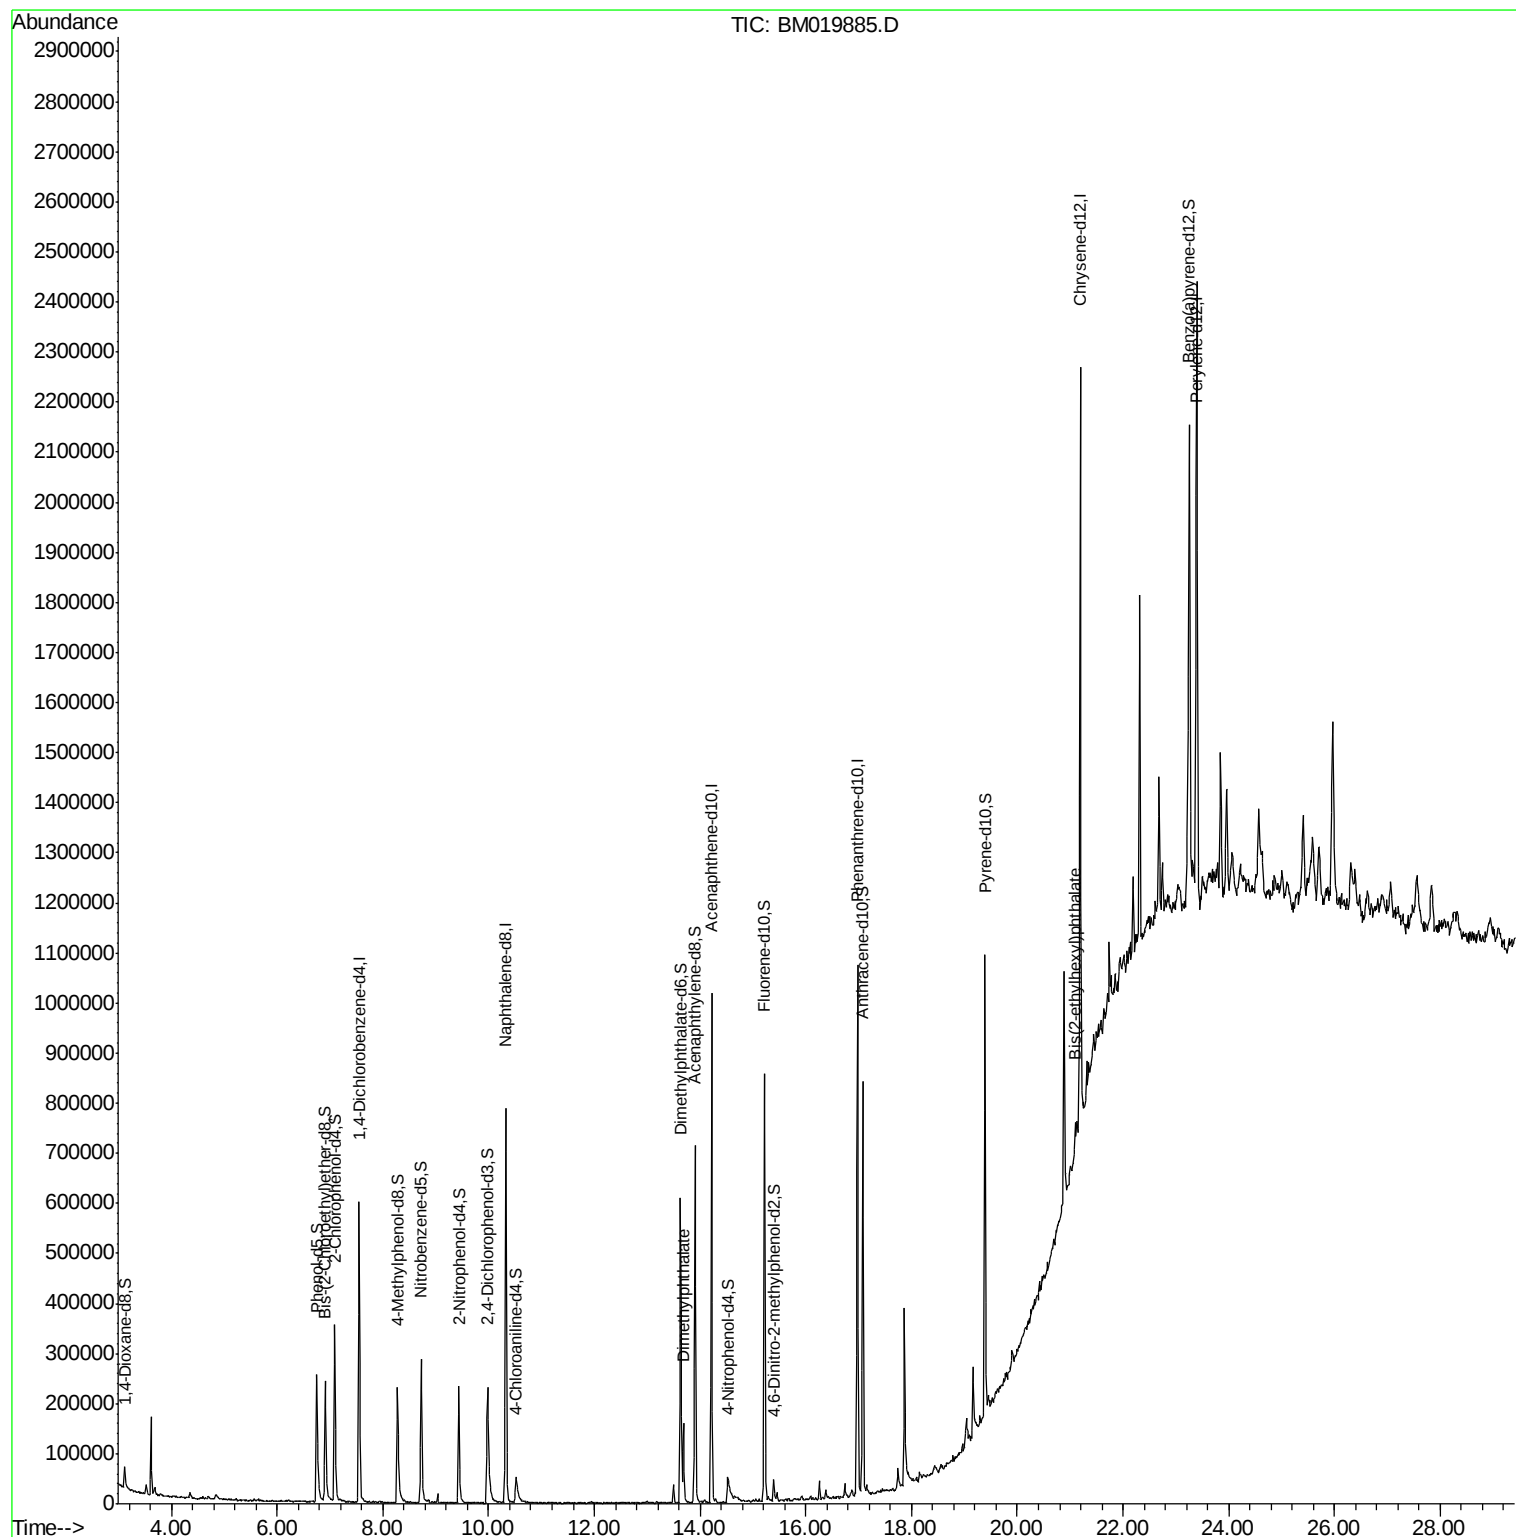

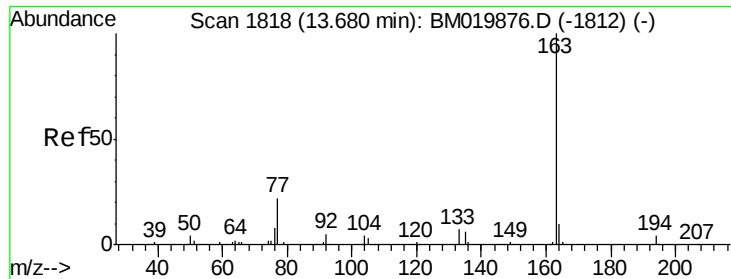





#45
Dimethylphthalate
Concen: 4.072 ng/ul
RT: 13.69 min Scan# 1819
Delta R.T. -0.00 min
Lab File: BM019885.D
Acq: 11 Apr 2019 04:55

Instrument :
BNA_M
ClientSampleId :
BF896

Tgt Ion	Ratio	Resp	Lower	Upper
163	100	101707		
194	3.5	4.0	6.0#	
164	9.9	8.4	12.6	

Manual Integrations
APPROVED

Sohil
4/12/2019 5:19:01 PM

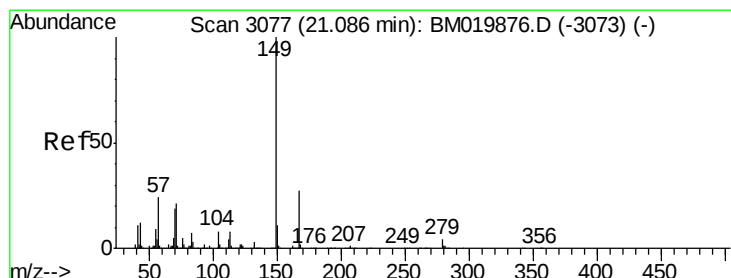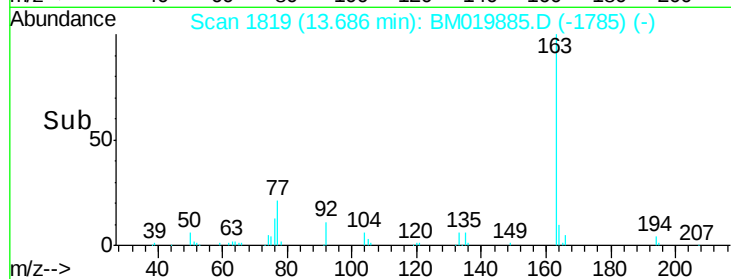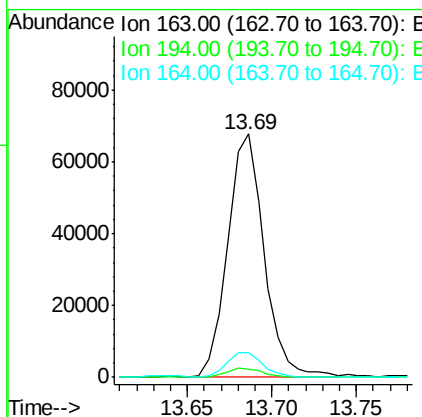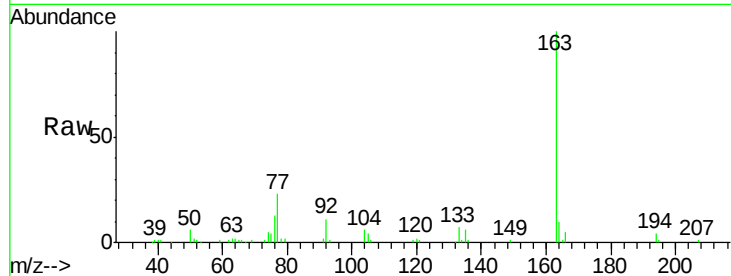

#84
Bis(2-ethylhexyl)phthalate
Concen: 1.161 ng/ul
RT: 21.09 min Scan# 3078
Delta R.T. -0.00 min
Lab File: BM019885.D
Acq: 11 Apr 2019 04:55

Tgt Ion	Ratio	Resp	Lower	Upper
149	100	25651		
167	28.0	23.0	34.6	
279	8.9	4.3	6.5#	

