

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
 Data File : BM019889.D
 Acq On : 11 Apr 2019 07:21
 Operator : JU/SJ
 Sample : K2303-04
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF899

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	18	22	30	rBV	39350	60970	3.05%	0.328%
2	3.622	105	108	115	rVB2	9261	13278	0.66%	0.071%
3	4.704	288	292	299	rVB4	5106	10690	0.53%	0.057%
4	5.457	417	420	422	rVB4	2086	2247	0.11%	0.012%
5	6.398	576	580	583	rVB2	1607	2453	0.12%	0.013%
6	6.757	635	641	657	rVV	182323	411551	20.56%	2.211%
7	6.910	662	667	679	rBV	173960	324433	16.21%	1.743%
8	7.092	692	698	717	rVV	274498	483369	24.15%	2.597%
9	7.210	717	718	722	rVB4	2082	2154	0.11%	0.012%
10	7.304	731	734	737	rVB3	1606	2179	0.11%	0.012%
11	7.551	769	776	786	rBV	527869	839740	41.95%	4.512%
12	8.281	894	900	920	rBV	185401	397779	19.87%	2.137%
13	8.416	920	923	926	rVB4	2806	3893	0.19%	0.021%
14	8.728	969	976	995	rBV	206200	415255	20.75%	2.231%
15	9.033	1024	1028	1034	rVB2	12806	17400	0.87%	0.093%
16	9.139	1043	1046	1051	rVB2	1255	2060	0.10%	0.011%
17	9.439	1091	1097	1115	rVB	158445	314093	15.69%	1.688%
18	9.980	1183	1189	1210	rBV	173935	461449	23.05%	2.480%
19	10.327	1241	1248	1260	rBV	635056	1076199	53.77%	5.783%
20	10.510	1272	1279	1300	rBV	139278	402497	20.11%	2.163%
21	10.651	1300	1303	1309	rVB4	3152	5889	0.29%	0.032%
22	11.945	1520	1523	1527	rBV	2784	3886	0.19%	0.021%
23	13.639	1805	1811	1816	rBV	453711	681431	34.04%	3.662%
24	13.686	1816	1819	1831	rVB	93307	137146	6.85%	0.737%
25	13.910	1850	1857	1869	rBV	549583	827462	41.34%	4.446%
26	14.092	1886	1888	1890	rVB2	3889	3532	0.18%	0.019%
27	14.215	1903	1909	1921	rBV2	827014	1245626	62.23%	6.693%
28	14.539	1958	1964	1980	rBV3	36549	151082	7.55%	0.812%
29	14.657	1981	1984	1991	rVB4	8396	15805	0.79%	0.085%
30	14.757	1998	2001	2004	rVB4	2097	2091	0.10%	0.011%
31	14.998	2037	2042	2046	rBV4	2864	5003	0.25%	0.027%
32	15.057	2046	2052	2056	rVV4	4487	8826	0.44%	0.047%
33	15.110	2059	2061	2066	rVB	1407	2323	0.12%	0.012%
34	15.221	2074	2080	2095	rBV	659526	1014974	50.71%	5.454%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
 Data File : BM019889.D
 Acq On : 11 Apr 2019 07:21
 Operator : JU/SJ
 Sample : K2303-04
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF899

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Title : SVOA CALIBRATION

35	15.327	2095	2098	2101	rVB3	1884	2287	0.11%	0.012%
36	15.404	2109	2111	2114	rBV2	5511	6067	0.30%	0.033%
37	15.457	2116	2120	2127	rVB2	6406	9631	0.48%	0.052%
38	15.651	2152	2153	2158	rBV2	2116	2479	0.12%	0.013%
39	15.774	2172	2174	2176	rBV2	1910	2090	0.10%	0.011%
40	15.915	2194	2198	2199	rBV4	4654	5640	0.28%	0.030%
41	16.009	2210	2214	2216	rBV3	2723	2536	0.13%	0.014%
42	16.039	2216	2219	2224	rVB2	2094	3113	0.16%	0.017%
43	16.086	2224	2227	2228	rBV	1910	2230	0.11%	0.012%
44	16.115	2228	2232	2237	rVV2	2170	3953	0.20%	0.021%
45	16.174	2239	2242	2246	rVB3	1973	2712	0.14%	0.015%
46	16.251	2253	2255	2257	rBV2	2864	2714	0.14%	0.015%
47	16.392	2276	2279	2285	rVB4	3182	3881	0.19%	0.021%
48	16.521	2298	2301	2306	rVB3	12840	16100	0.80%	0.087%
49	16.680	2326	2328	2330	rBV2	2574	2779	0.14%	0.015%
50	16.709	2330	2333	2338	rVB3	4848	6981	0.35%	0.038%
51	16.762	2338	2342	2343	rBV2	5409	6042	0.30%	0.032%
52	16.780	2343	2345	2348	rVB3	4988	4753	0.24%	0.026%
53	16.827	2350	2353	2355	rVB3	2592	2817	0.14%	0.015%
54	16.868	2355	2360	2361	rBV4	3441	4947	0.25%	0.027%
55	16.939	2369	2372	2373	rBV3	3916	2962	0.15%	0.016%
56	16.980	2373	2379	2390	rBV	982196	1368166	68.35%	7.352%
57	17.080	2390	2396	2406	rVV	706662	999152	49.92%	5.369%
58	17.245	2423	2424	2427	rBV2	2192	2562	0.13%	0.014%
59	17.292	2431	2432	2434	rBV2	3193	2292	0.11%	0.012%
60	17.327	2434	2438	2440	rBV3	5266	7857	0.39%	0.042%
61	17.356	2440	2443	2446	rVV4	3769	5430	0.27%	0.029%
62	17.456	2458	2460	2462	rVB3	4090	3550	0.18%	0.019%
63	17.868	2526	2530	2540	rBV2	74390	125721	6.28%	0.676%
64	18.145	2575	2577	2580	rBV4	4805	6085	0.30%	0.033%
65	18.245	2588	2594	2599	rBV9	9735	22751	1.14%	0.122%
66	18.286	2599	2601	2602	rVB2	4061	2911	0.15%	0.016%
67	19.162	2747	2750	2757	rBV4	37324	67023	3.35%	0.360%
68	19.392	2784	2789	2798	rBV	870016	1218442	60.87%	6.547%
69	19.721	2842	2845	2848	rBV2	59875	69316	3.46%	0.372%
70	19.756	2848	2851	2855	rVV	97318	108498	5.42%	0.583%
71	21.197	3091	3096	3101	rBV	1333312	1806909	90.27%	9.709%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019889.D
Acq On : 11 Apr 2019 07:21
Operator : JU/SJ
Sample : K2303-04
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF899

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Title : SVOA CALIBRATION

72	23.262	3444	3447	3457	rVB	796972	1346519	67.27%	7.235%
73	23.403	3466	3471	3479	rVB	1118629	2001568	100.00%	10.755%


Sum of corrected areas: 18610231

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019889.D
Acq On : 11 Apr 2019 07:21
Operator : JU/SJ
Sample : K2303-04
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF899

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

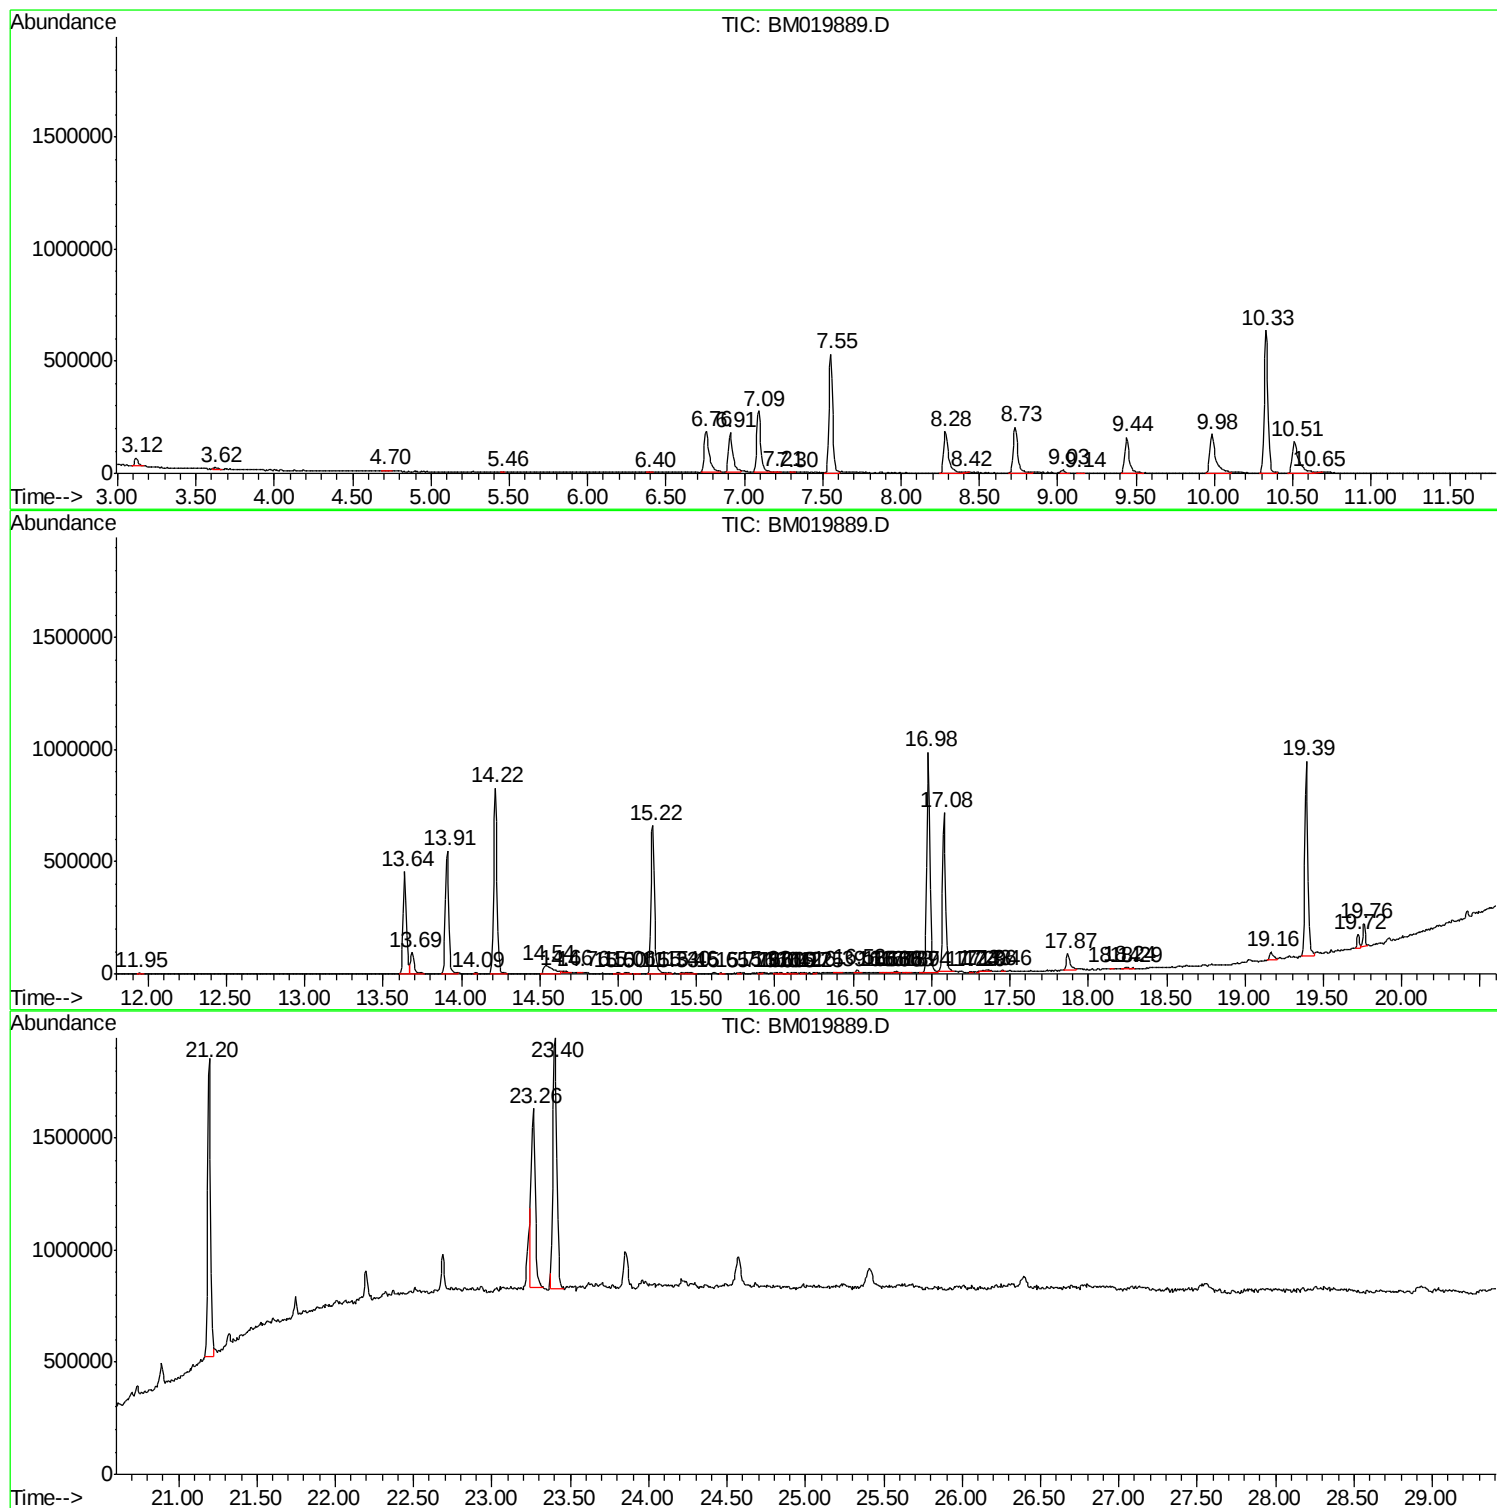

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019889.D
Acq On : 11 Apr 2019 07:21
Operator : JU/SJ
Sample : K2303-04
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF899

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041019\
Data File : BM019889.D
Acq On : 11 Apr 2019 07:21
Operator : JU/SJ
Sample : K2303-04
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF899

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc