
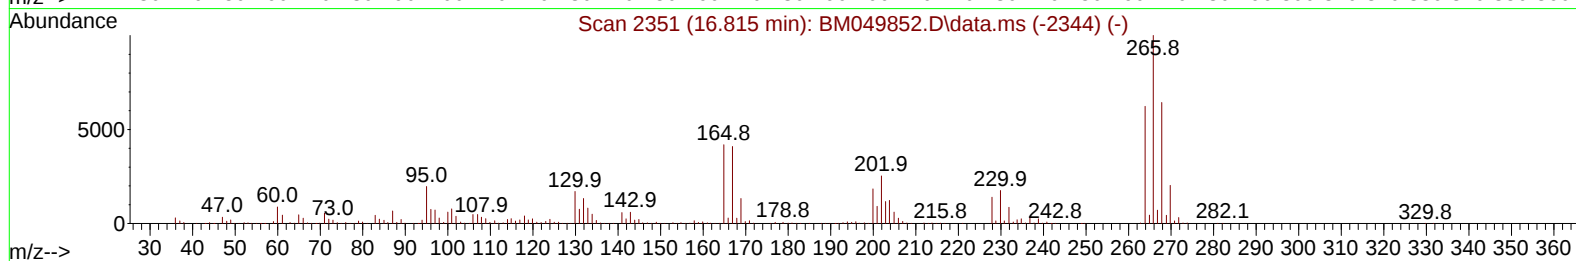
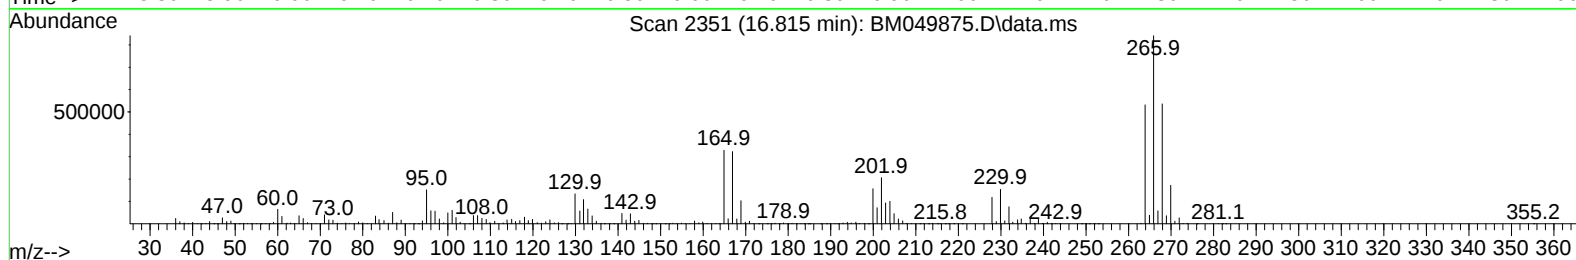


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041025\
Data File : BM049875.D
Acq On : 10 Apr 2025 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 12:01:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

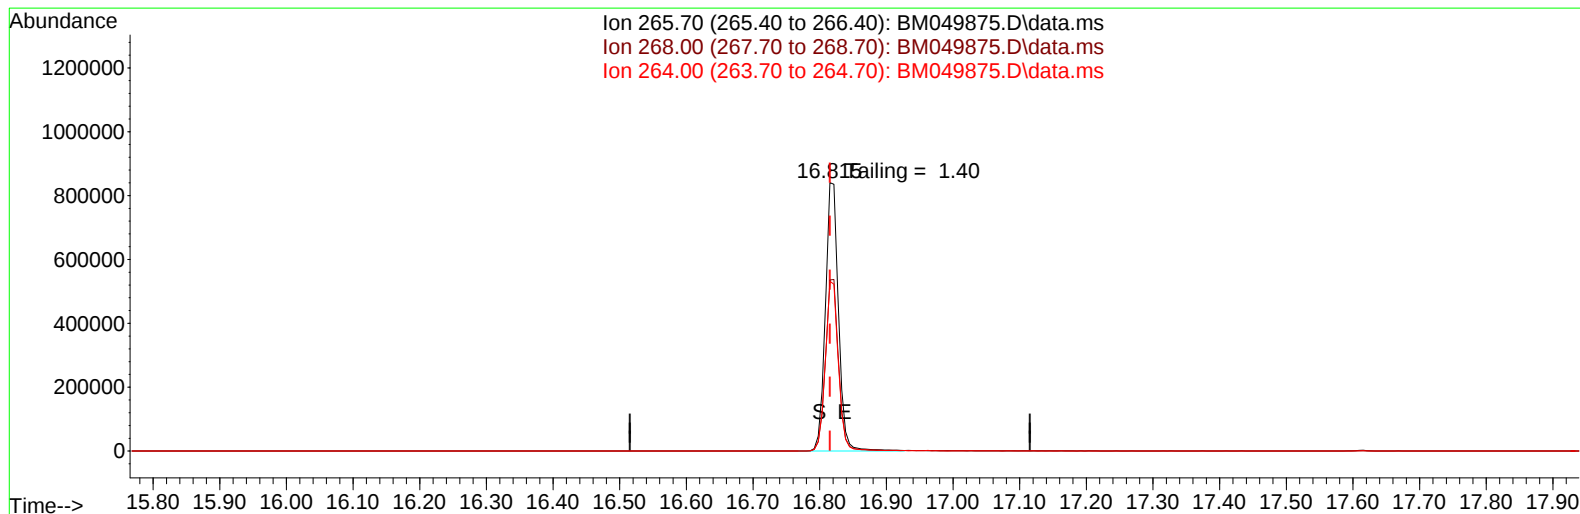

TIC: BM049875.D\data.ms

(70) Pentachlorophenol (C)




16.815min (-0.000) 211954.15 ng

response 1151118

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	63.75
264.00	62.30	63.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041025\
Data File : BM049875.D
Acq On : 10 Apr 2025 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 12:01:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

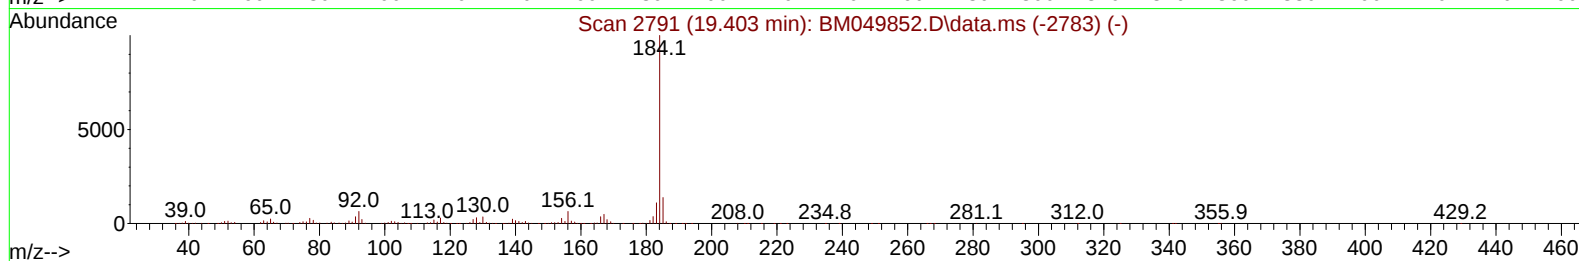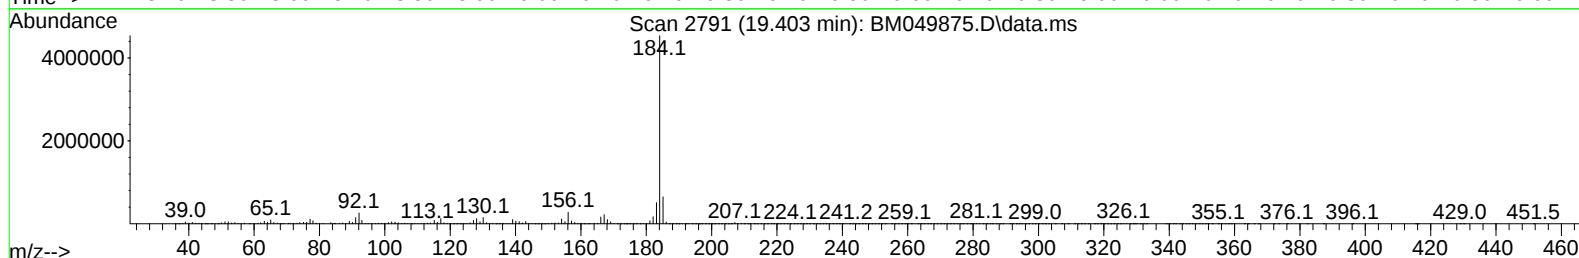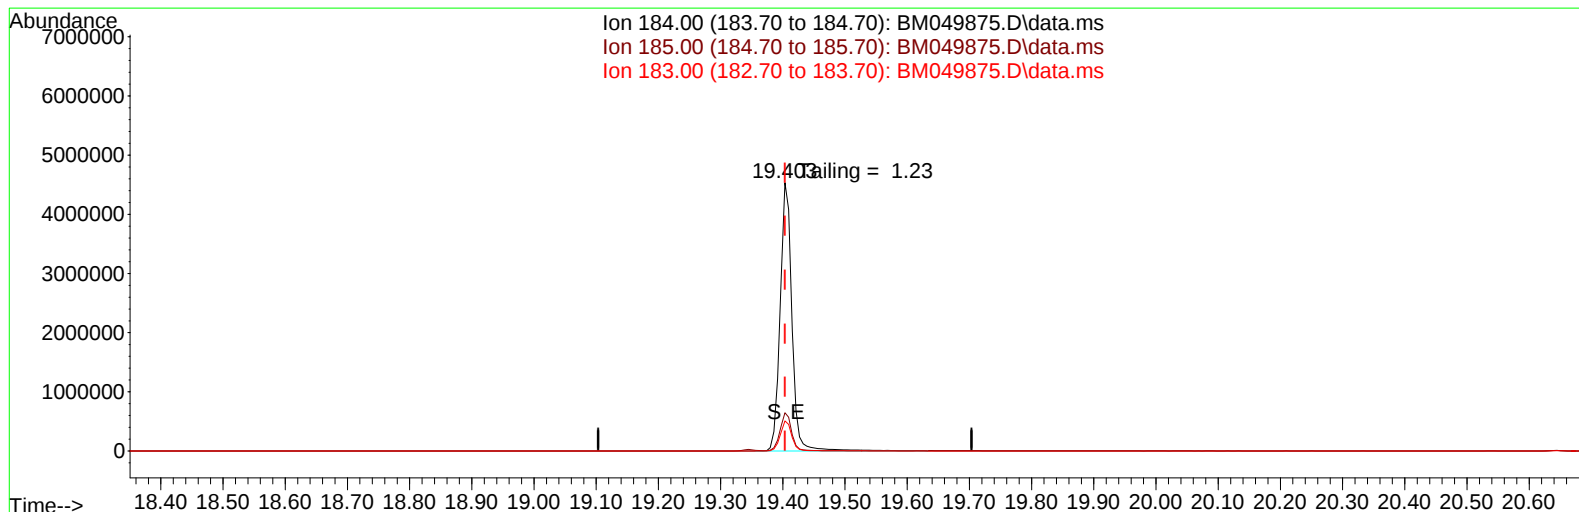

TIC: BM049875.D\data.ms

(77) Benzidine**19.403min (-0.000) 194071.13 ng****response 5998885**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.29
183.00	11.00	11.22
0.00	0.00	0.00