

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041025\
 Data File : BM049878.D
 Acq On : 10 Apr 2025 10:54
 Operator : RC/JU
 Sample : Q1753-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 WC-1

Quant Time: Apr 10 12:14:08 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 09 04:00:55 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	286951	20.000	ng	0.00
21) Naphthalene-d8	10.569	136	991689	20.000	ng	0.00
39) Acenaphthene-d10	14.421	164	665440	20.000	ng	0.00
64) Phenanthrene-d10	17.162	188	1396390	20.000	ng	0.00
76) Chrysene-d12	21.397	240	1346936	20.000	ng	0.00
86) Perylene-d12	24.391	264	1467562	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.363	112	1570706	92.949	ng	0.00
7) Phenol-d6	6.951	99	1975410	93.955	ng	0.00
23) Nitrobenzene-d5	8.934	82	1135457	63.758	ng	0.00
42) 2,4,6-Tribromophenol	15.910	330	997020	103.008	ng	0.00
45) 2-Fluorobiphenyl	13.039	172	3001475	61.163	ng	0.00
79) Terphenyl-d14	19.786	244	5150044	71.655	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041025\
Data File : BM049878.D
Acq On : 10 Apr 2025 10:54
Operator : RC/JU
Sample : Q1753-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-1


Quant Time: Apr 10 12:14:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

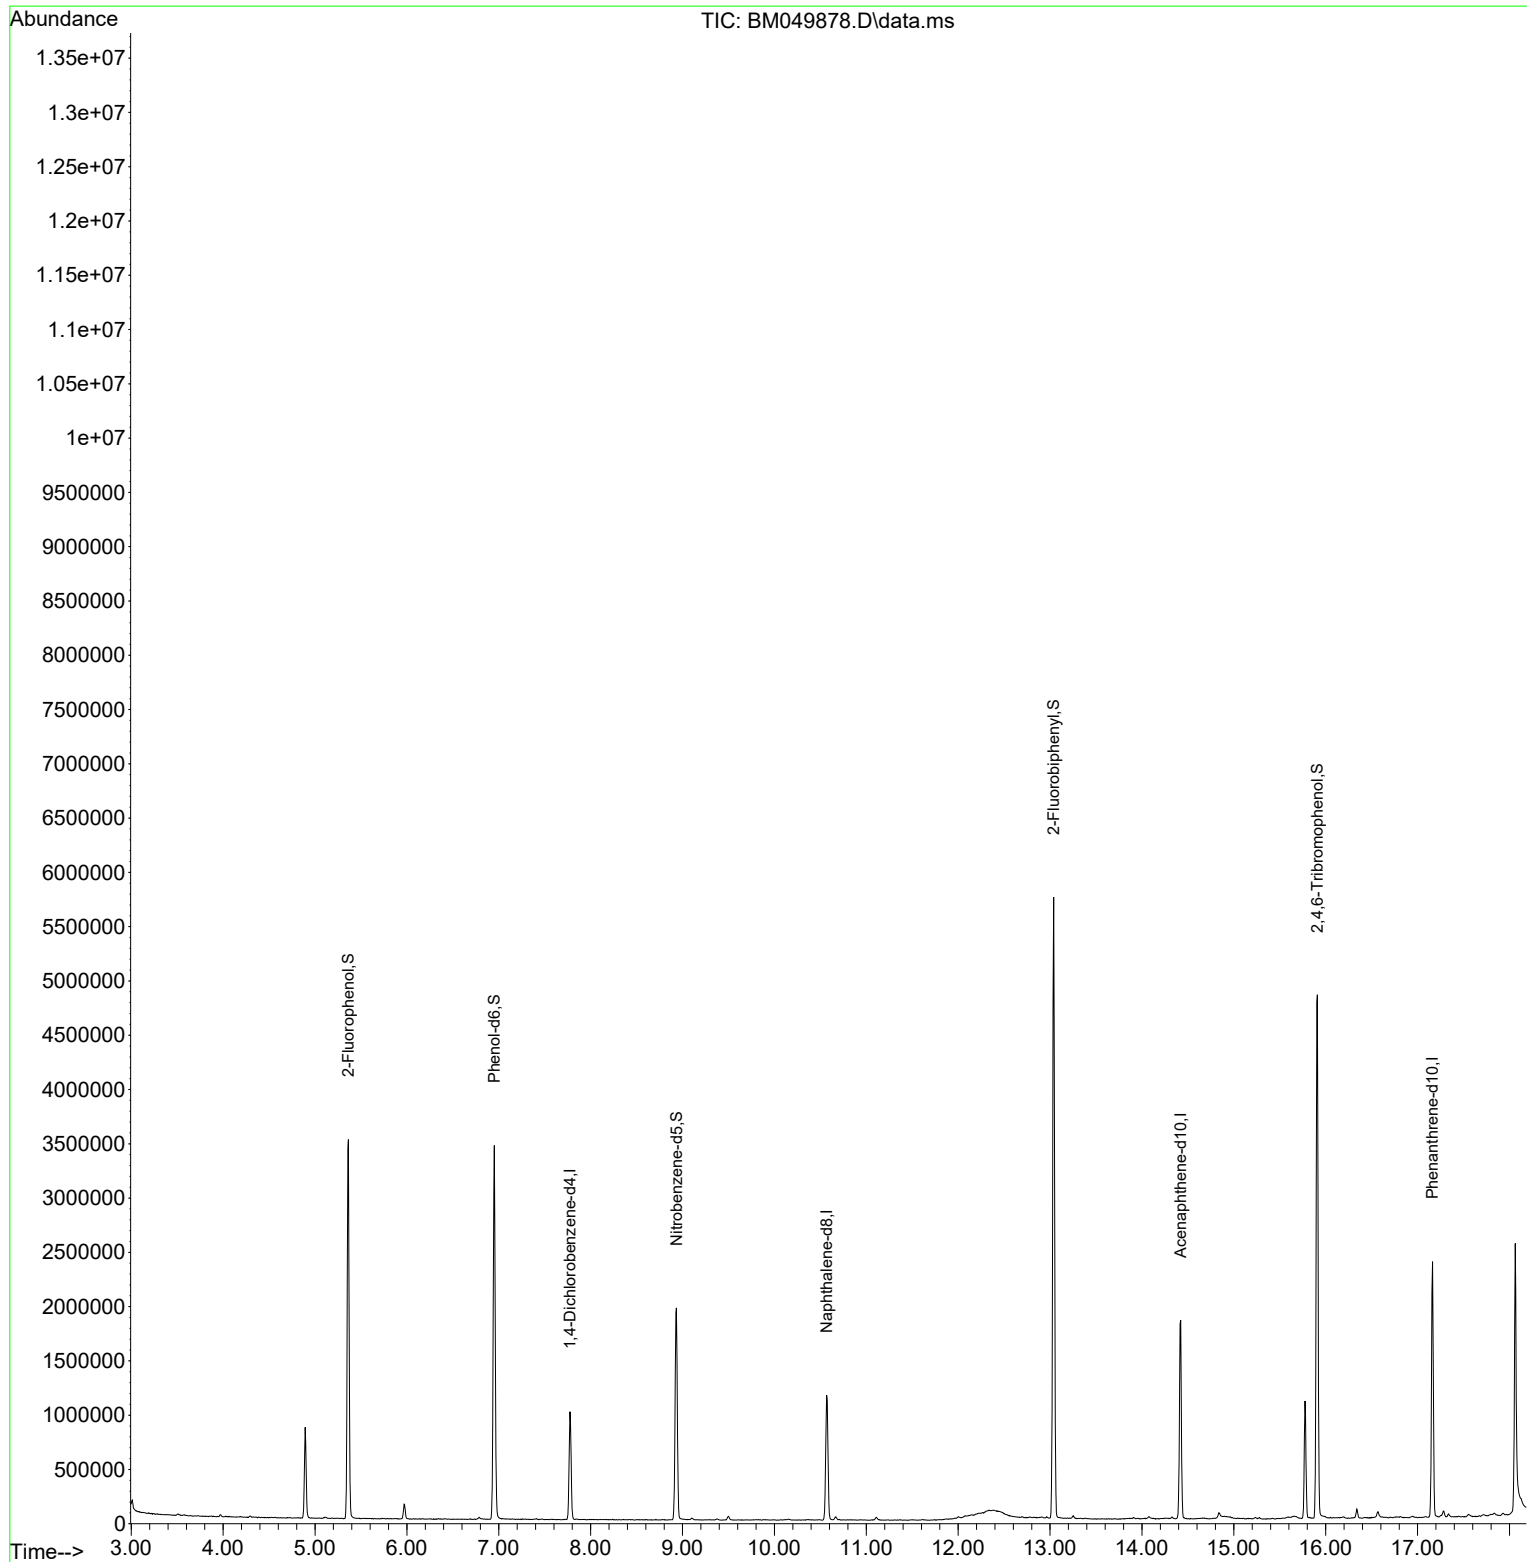

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041025\
Data File : BM049878.D
Acq On : 10 Apr 2025 10:54
Operator : RC/JU
Sample : Q1753-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-1

Quant Time: Apr 10 12:14:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration




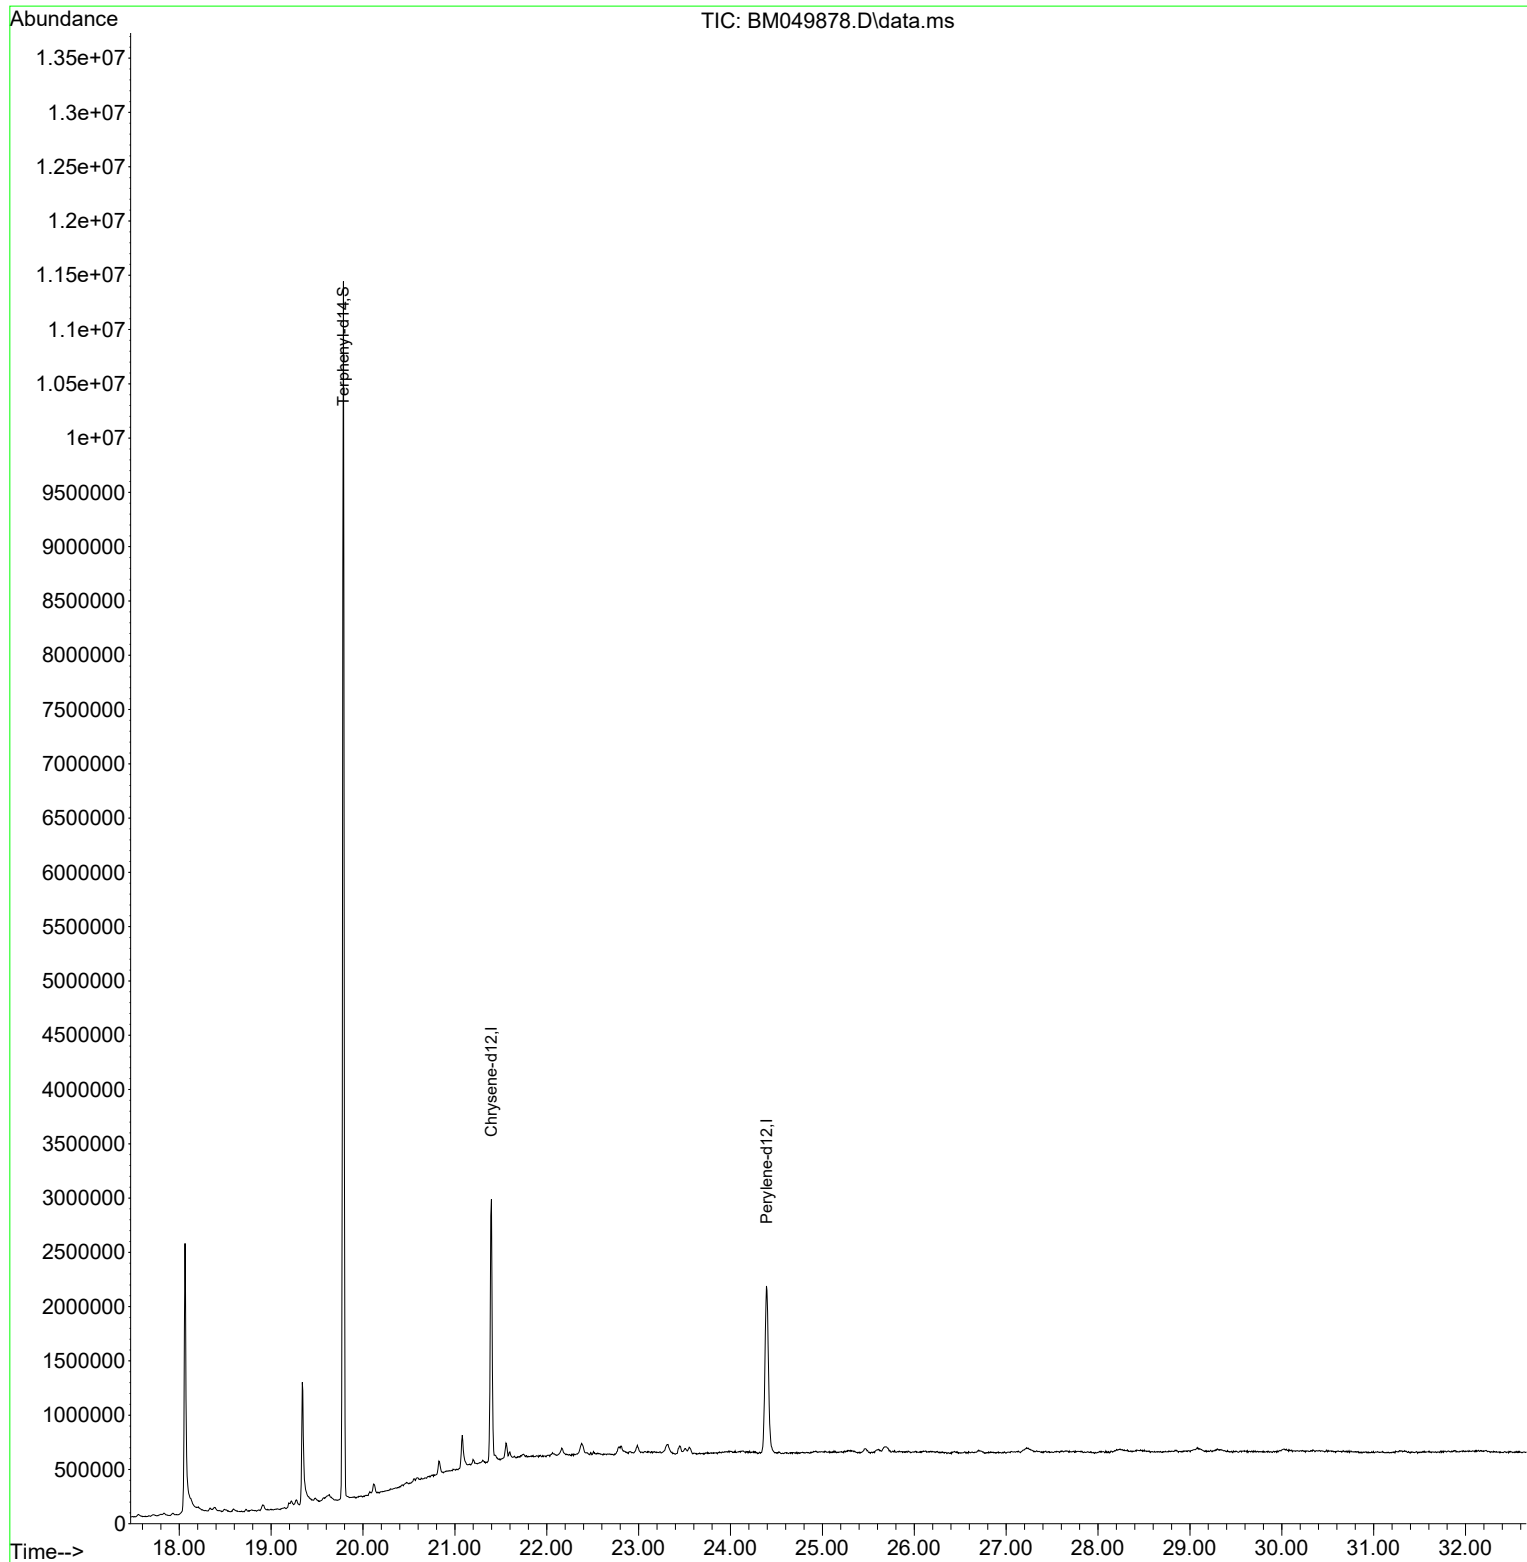




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.775 min Scan# 815
Delta R.T. -0.006 min
Lab File: BM049878.D
Acq: 10 Apr 2025 10:54




Instrument :
BNA_M
ClientSampleId :
WC-1

Tgt Ion:152 Resp: 286951
Ion Ratio Lower Upper
152 100
150 149.6 124.3 186.5
115 50.2 41.1 61.7

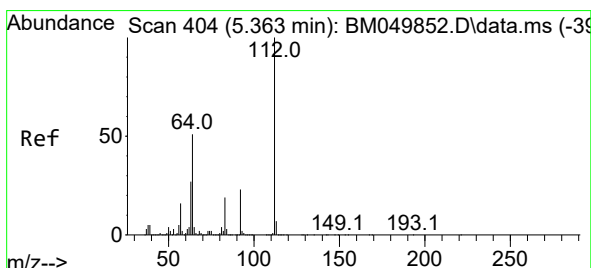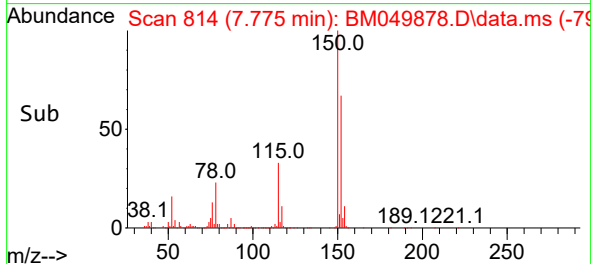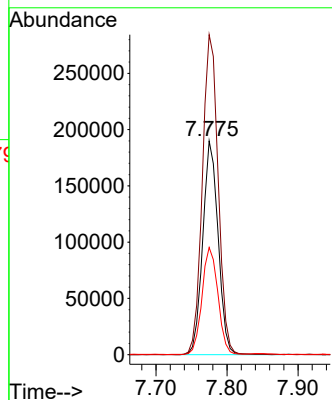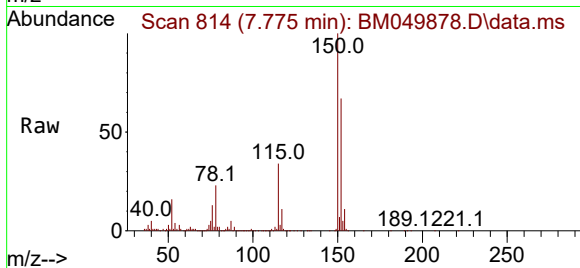

#5
2-Fluorophenol
Concen: 92.949 ng
RT: 5.363 min Scan# 404
Delta R.T. 0.000 min
Lab File: BM049878.D
Acq: 10 Apr 2025 10:54

Tgt Ion:112 Resp: 1570706
Ion Ratio Lower Upper
112 100
64 51.4 41.0 61.6
63 26.6 21.5 32.3

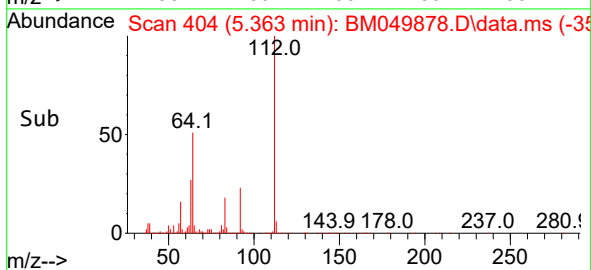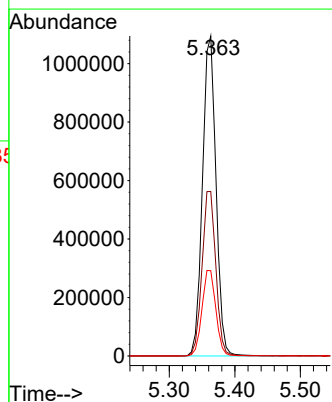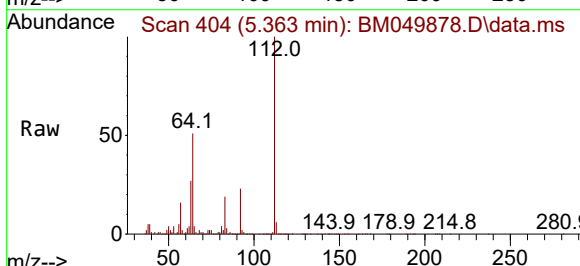







#7
Phenol-d6
Concen: 93.955 ng
RT: 6.951 min Scan# 61
Delta R.T. 0.000 min
Lab File: BM049878.D
Acq: 10 Apr 2025 10:54

Instrument :
BNA_M
ClientSampleId :
WC-1

Tgt Ion: 99 Resp: 1975410




Ion	Ratio	Lower	Upper
99	100		
42	15.3	12.1	18.1
71	31.1	24.9	37.3

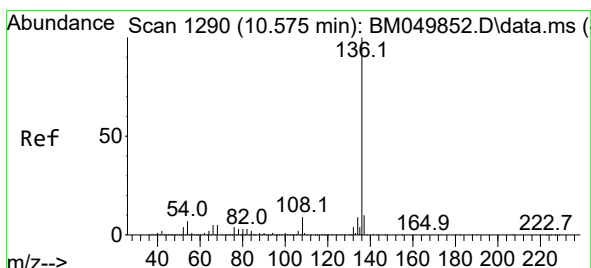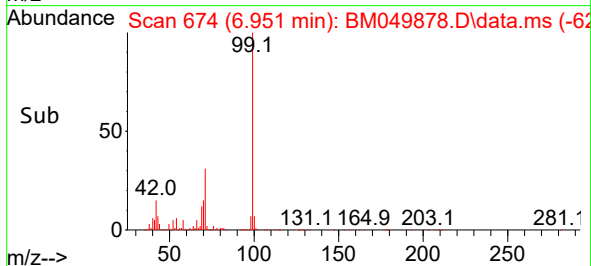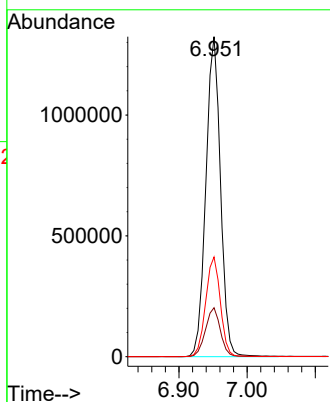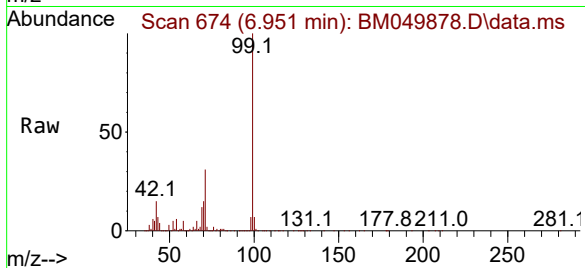


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.569 min Scan# 1289
Delta R.T. -0.006 min
Lab File: BM049878.D
Acq: 10 Apr 2025 10:54

Tgt Ion: 136 Resp: 991689

Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.4	12.6
54	6.5	5.3	7.9
68	5.4	4.3	6.5


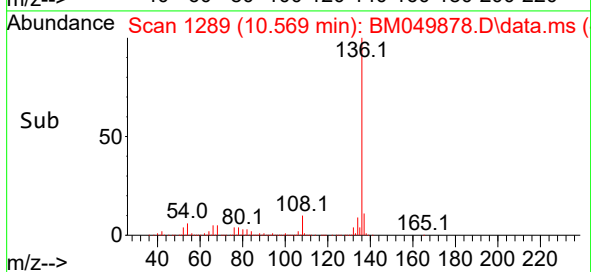
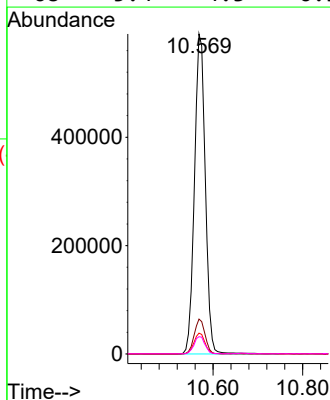
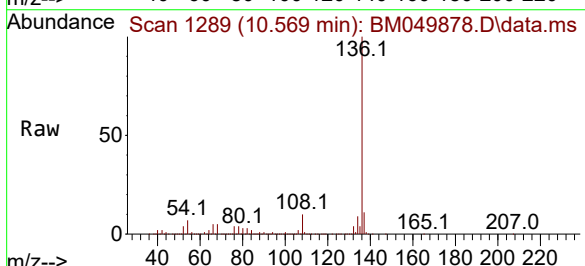


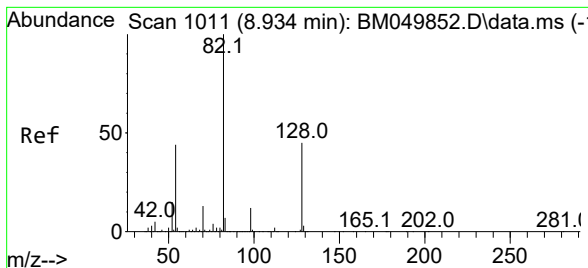

#23
Nitrobenzene-d5
Concen: 63.758 ng
RT: 8.934 min Scan# 1011
Delta R.T. 0.000 min
Lab File: BM049878.D
Acq: 10 Apr 2025 10:54




Instrument :
BNA_M
ClientSampleId :
WC-1


Tgt Ion: 82 Resp: 1135457
Ion Ratio Lower Upper
82 100
128 45.9 36.2 54.2
54 43.8 35.0 52.6

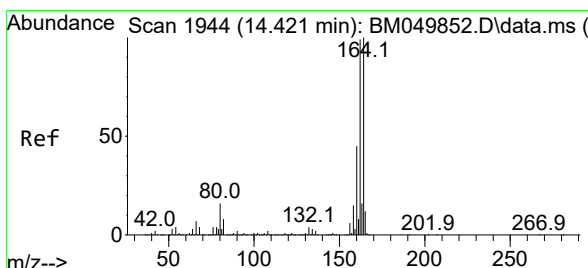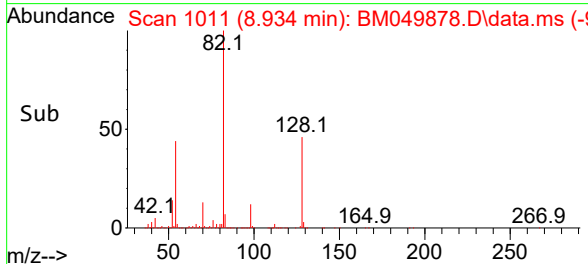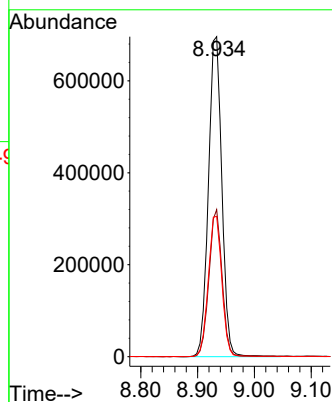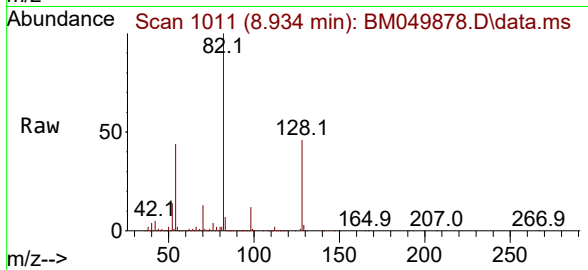

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.421 min Scan# 1944
Delta R.T. 0.000 min
Lab File: BM049878.D
Acq: 10 Apr 2025 10:54

Tgt Ion:164 Resp: 665440
Ion Ratio Lower Upper
164 100
162 99.5 79.4 119.0
160 44.4 36.2 54.2


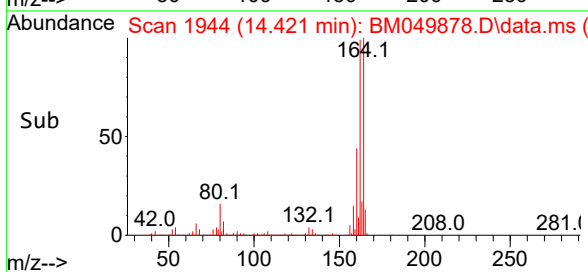
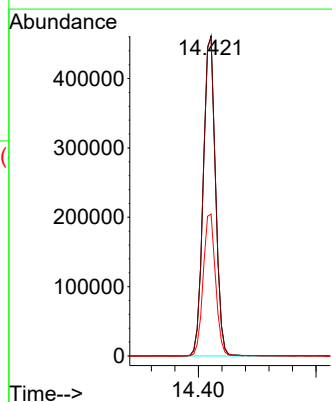
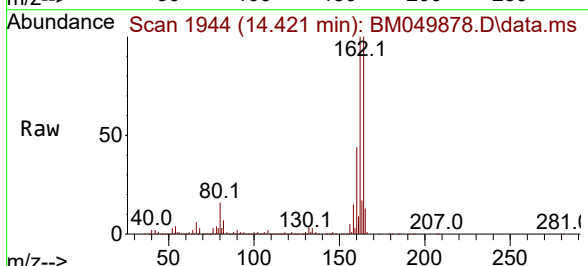


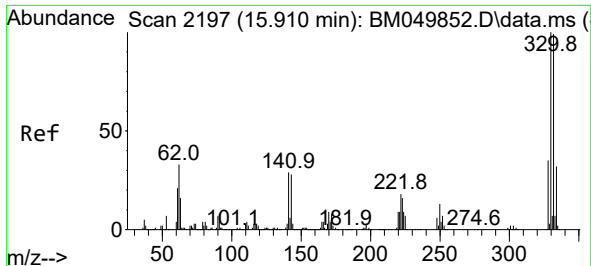

#42
 2,4,6-Tribromophenol
 Concen: 103.008 ng
 RT: 15.910 min Scan# 2197
 Delta R.T. 0.000 min
 Lab File: BM049878.D
 Acq: 10 Apr 2025 10:54




Instrument :
 BNA_M
 ClientSampleId :
 WC-1


Tgt Ion:330 Resp: 997020
 Ion Ratio Lower Upper
 330 100
 332 96.7 78.0 117.0
 141 28.0 23.5 35.3

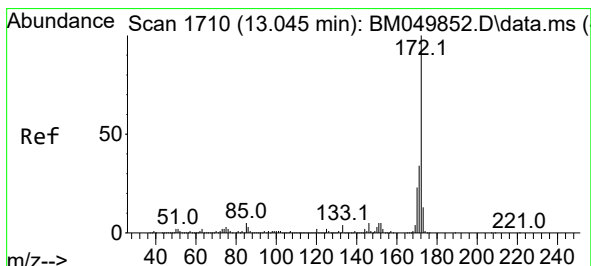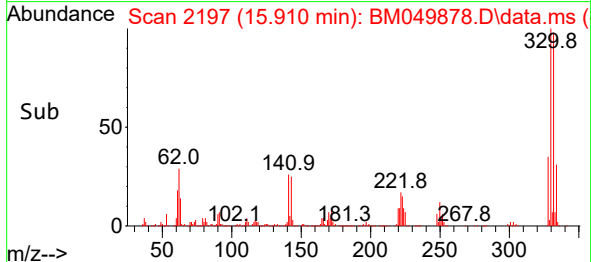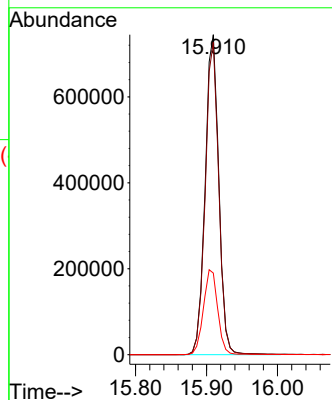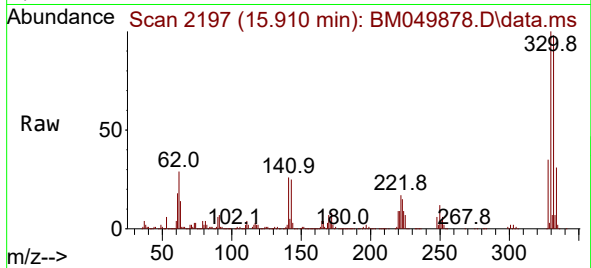

#45
 2-Fluorobiphenyl
 Concen: 61.163 ng
 RT: 13.039 min Scan# 1709
 Delta R.T. -0.006 min
 Lab File: BM049878.D
 Acq: 10 Apr 2025 10:54

Tgt Ion:172 Resp: 3001475
 Ion Ratio Lower Upper
 172 100
 171 34.8 27.4 41.2
 170 23.1 18.6 28.0

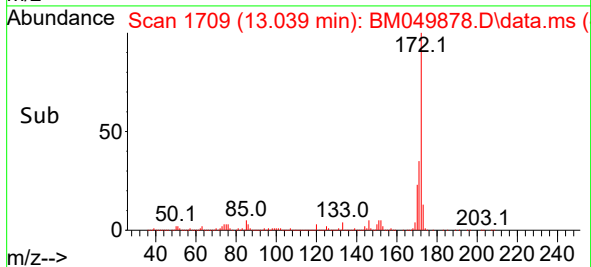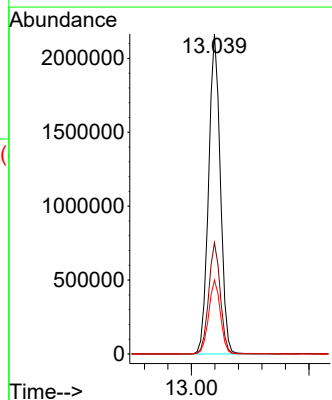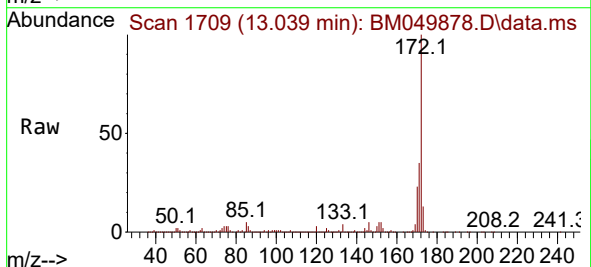

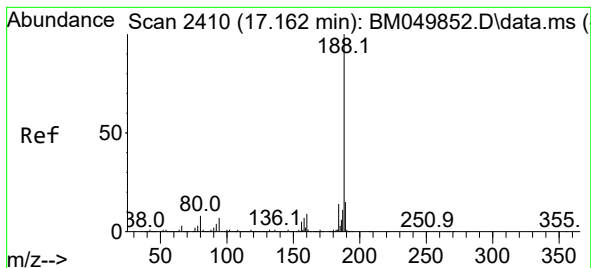

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.162 min Scan# 2410

Delta R.T. 0.000 min

Lab File: BM049878.D

Acq: 10 Apr 2025 10:54

Instrument :

BNA_M

ClientSampleId :

WC-1





Tgt Ion:188 Resp: 1396390

Ion Ratio Lower Upper

188 100

94 7.1 5.8 8.6

80 7.5 6.4 9.6

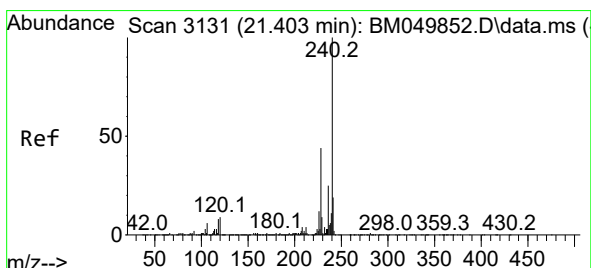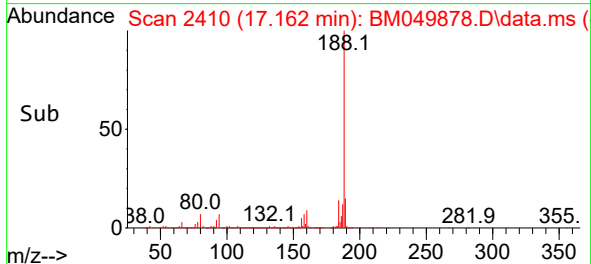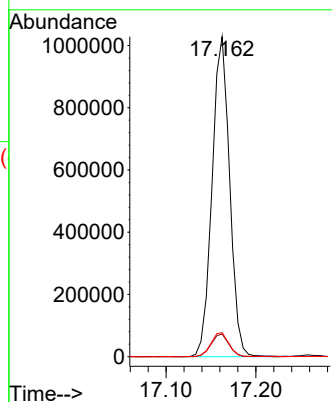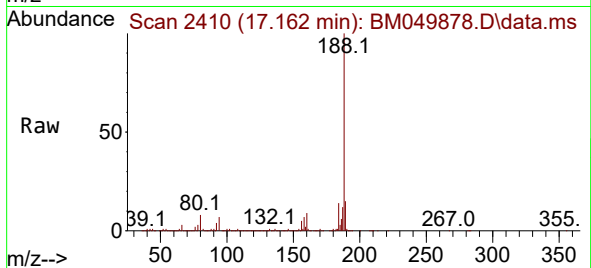

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.397 min Scan# 3130

Delta R.T. -0.006 min

Lab File: BM049878.D

Acq: 10 Apr 2025 10:54




Tgt Ion:240 Resp: 1346936


Ion Ratio Lower Upper

240 100

120 8.2 6.9 10.3

236 25.6 20.4 30.6


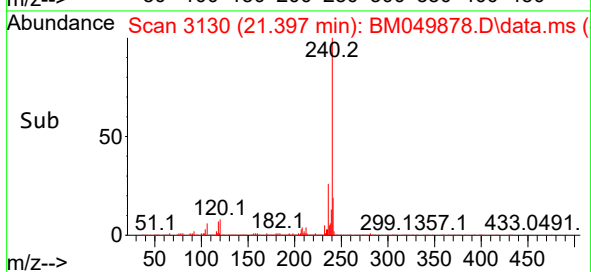
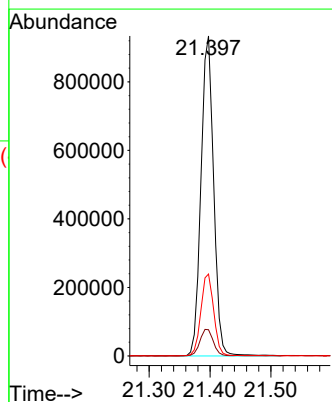
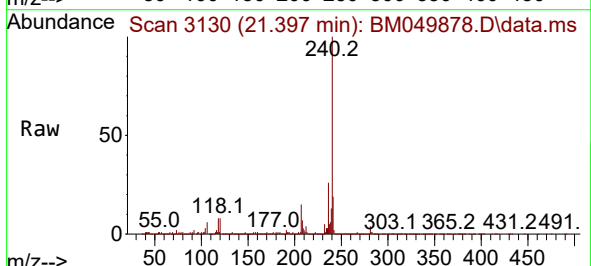


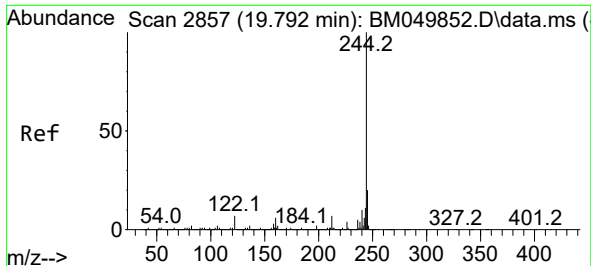

#79
Terphenyl-d14
Concen: 71.655 ng
RT: 19.786 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM049878.D
Acq: 10 Apr 2025 10:54

Instrument :
BNA_M
ClientSampleId :
WC-1

Tgt Ion:244 Resp: 5150044
Ion Ratio Lower Upper
244 100
212 7.0 5.5 8.3
122 7.1 5.4 8.0

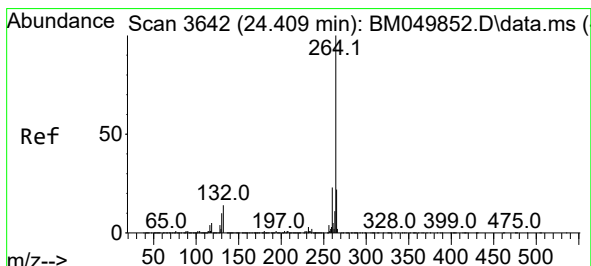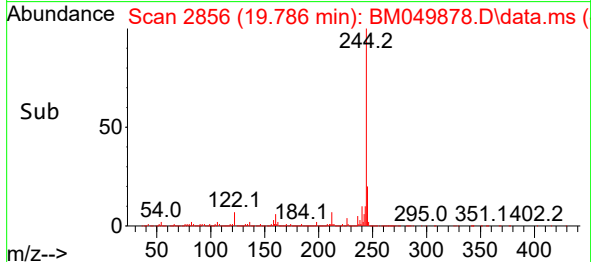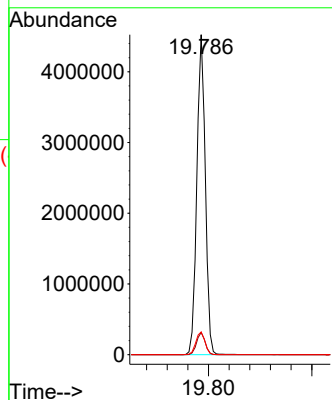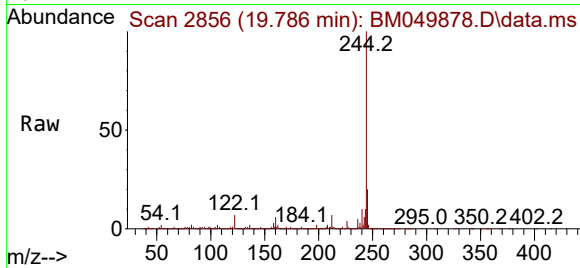

#86
Perylene-d12
Concen: 20.000 ng
RT: 24.391 min Scan# 3639
Delta R.T. -0.018 min
Lab File: BM049878.D
Acq: 10 Apr 2025 10:54

Tgt Ion:264 Resp: 1467562
Ion Ratio Lower Upper
264 100
260 23.4 18.6 28.0
265 22.2 17.8 26.8

