

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041119\
 Data File : BM019900.D
 Acq On : 11 Apr 2019 18:53
 Operator : JU/SJ
 Sample : K2304-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF895

Quant Time: Apr 12 04:19:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 12 04:12:05 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	120910	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	478724	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	254176	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	544489	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	596161	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	699593	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.10	96	16563	5.36	ng/uL	0.00
5) Phenol-d5	6.74	99	127439	11.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	95399	13.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.08	132	112205	13.75	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	88492	10.95	ng/ul	0.01
19) Nitrobenzene-d5	8.72	128	49363	14.45	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	57991	15.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	90403	12.61	ng/ul	0.02
29) 4-Chloroaniline-d4	10.50	131	88544	10.28	ng/ul	0.02
44) Dimethylphthalate-d6	13.63	166	301087	14.68	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	360145	14.04	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	5571	1.73	ng/ul	0.05
58) Fluorene-d10	15.21	176	258194	14.61	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	25250	7.01	ng/ul	0.01
71) Anthracene-d10	17.07	188	376926	14.43	ng/ul	0.00
79) Pyrene-d10	19.38	212	397105	14.42	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.24	264	469706	12.66	ng/ul	0.00


Target Compounds					Qvalue
45) Dimethylphthalate	13.68	163	71320	3.466 ng/ul#	98




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041119\
Data File : BM019900.D
Acq On : 11 Apr 2019 18:53
Operator : JU/SJ
Sample : K2304-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF895

Quant Time: Apr 12 04:19:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 12 04:12:05 2019
Response via : Initial Calibration

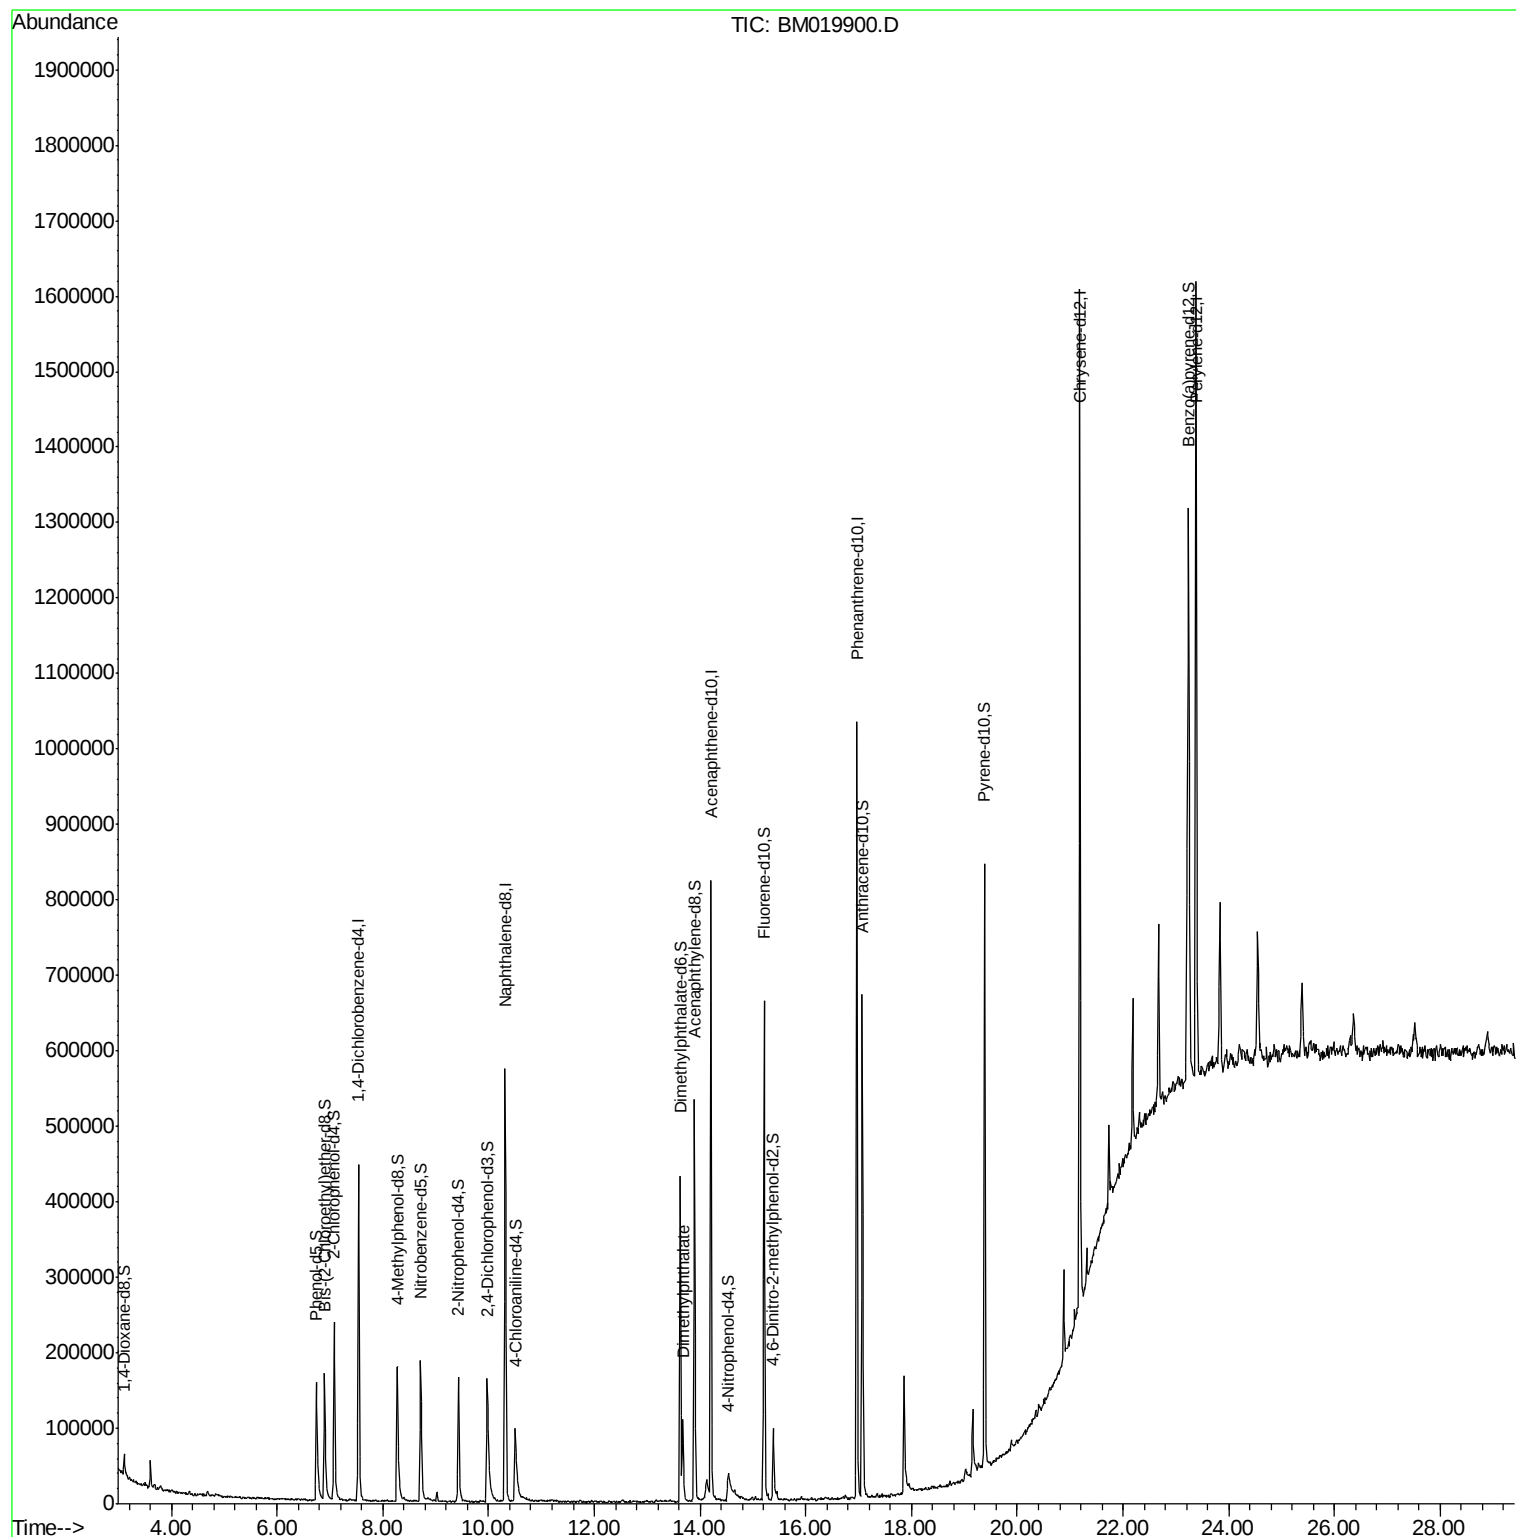

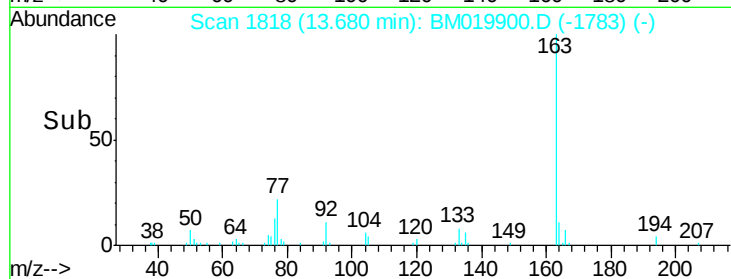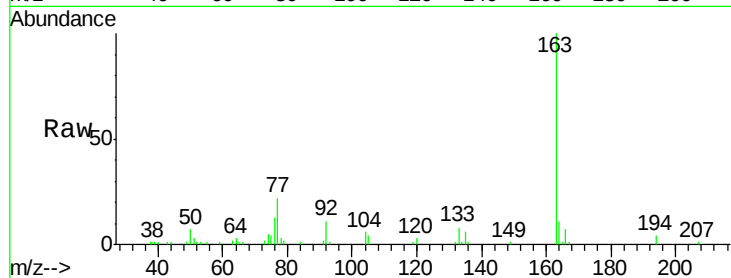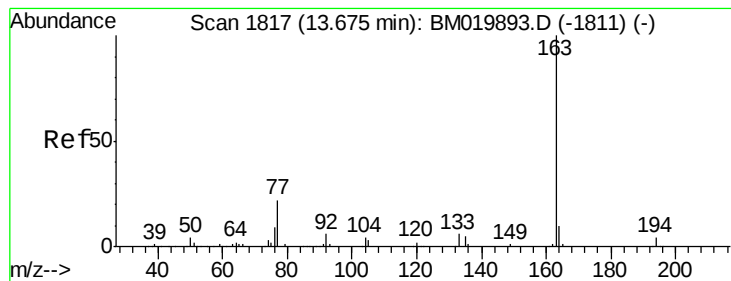

#45

Dimethylphthalate

Concen: 3.466 ng/ul

RT: 13.68 min Scan# 1818

Delta R.T. 0.01 min

Lab File: BM019900.D

Acq: 11 Apr 2019 18:53

Instrument :

BNA_M

ClientSampleId :

BF895

Tgt Ion:163 Resp: 71320

Ion Ratio Lower Upper

163 100

194 3.7 4.0 6.0#

164 11.0 8.4 12.6

