


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041119\
Data File : BM019900.D
Acq On : 11 Apr 2019 18:53
Operator : JU/SJ
Sample : K2304-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Apr 12 05:34:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 12 04:12:05 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BF895

Manual Integrations
APPROVED

Sohil
4/12/2019 5:21:03 PM

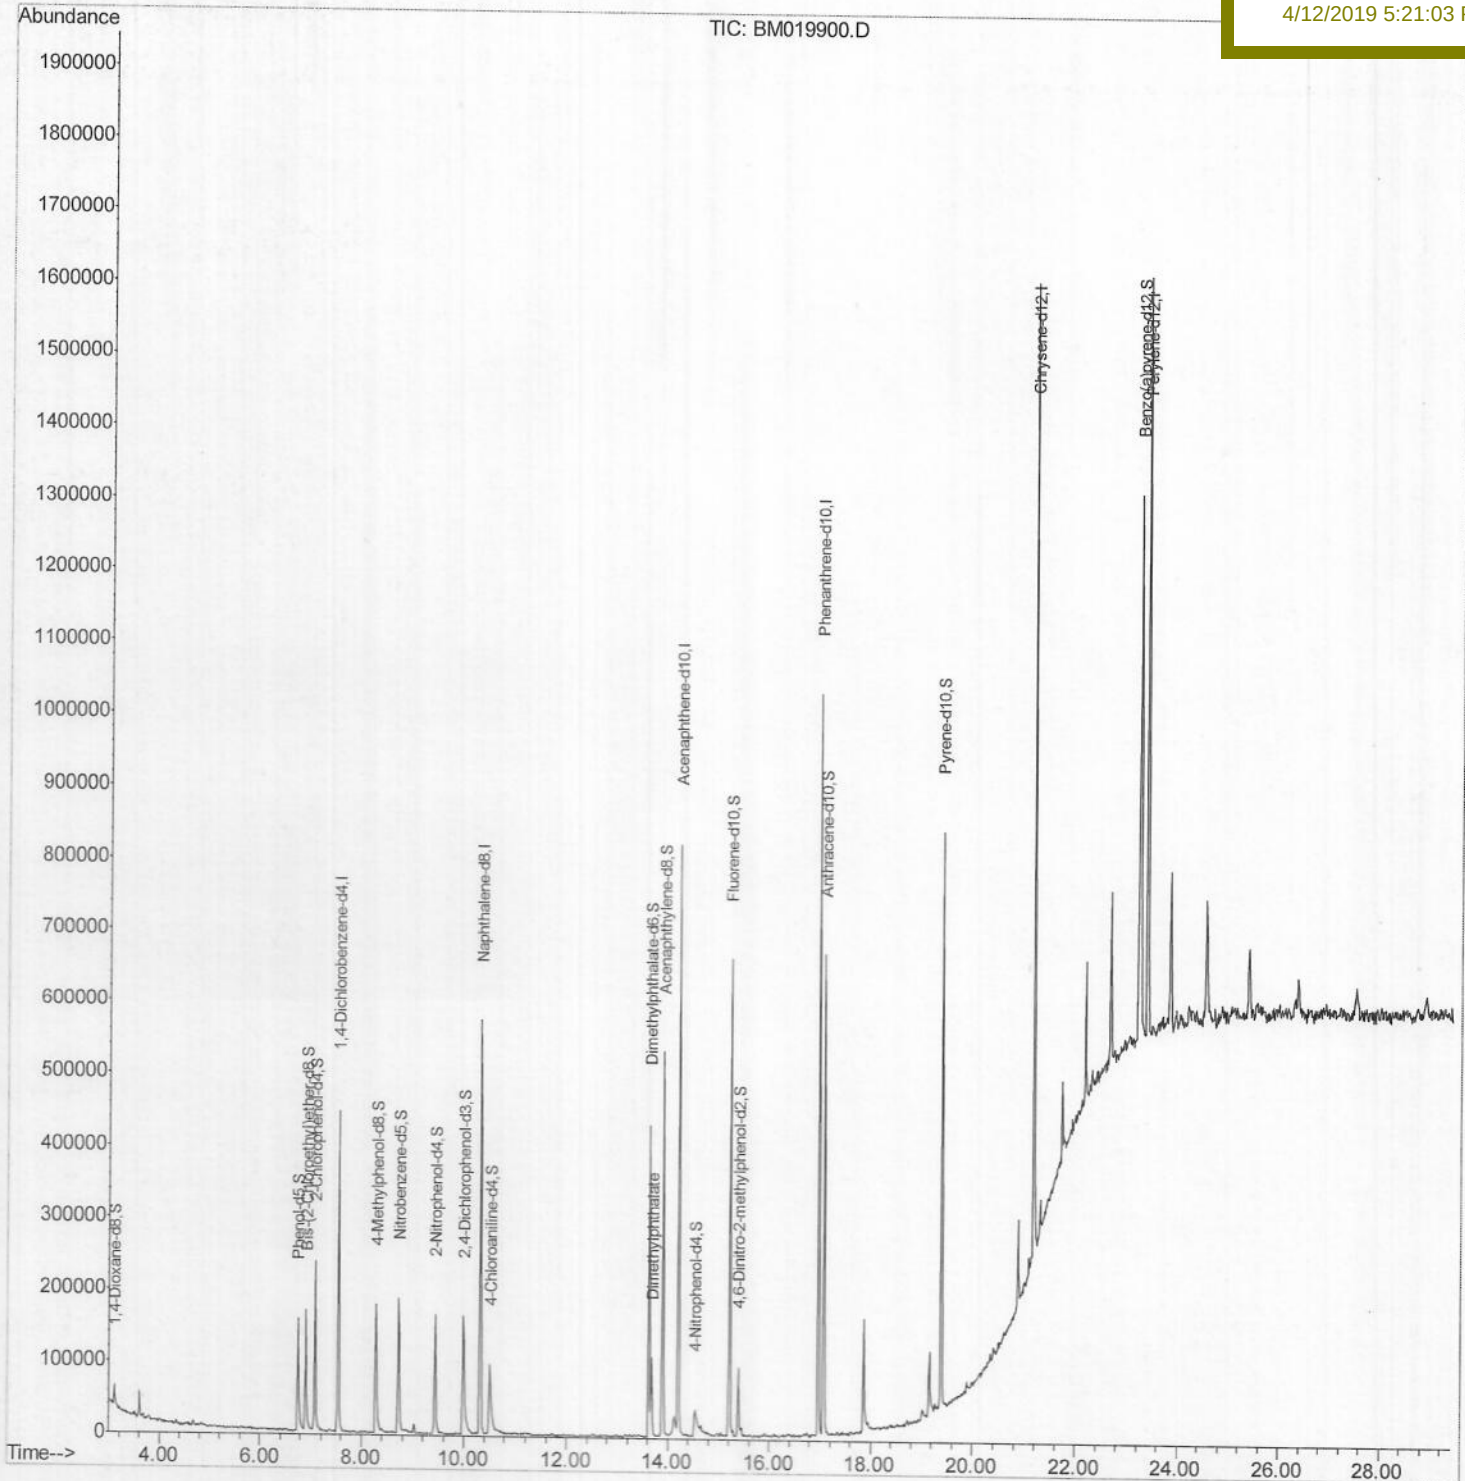

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041119\

Data File : BM019900.D

Acq On : 11 Apr 2019 18:53

Operator : JU/SJ

Sample : K2304-11

Misc :

ALS Vial : 9 Sample Multiplier: 1

Quant Time: Apr 12 04:19:40 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Fri Apr 12 04:12:05 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




BF895

Manual Integrations

APPROVED

Sohil

4/12/2019 5:21:03 PM

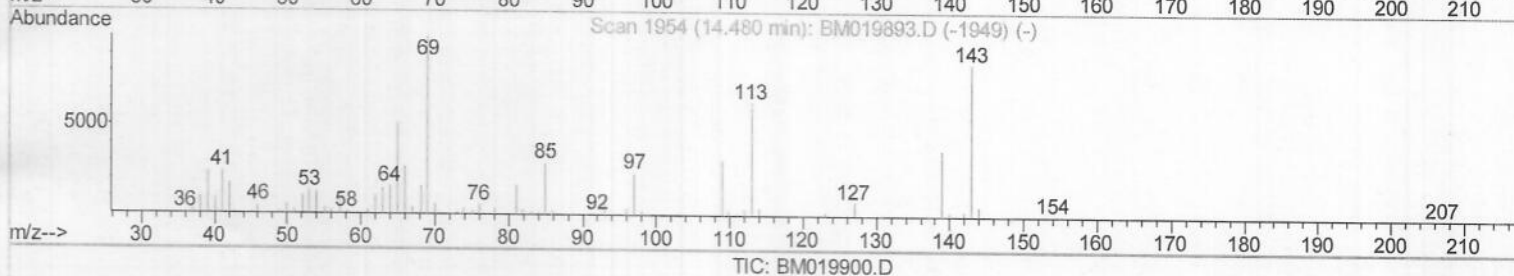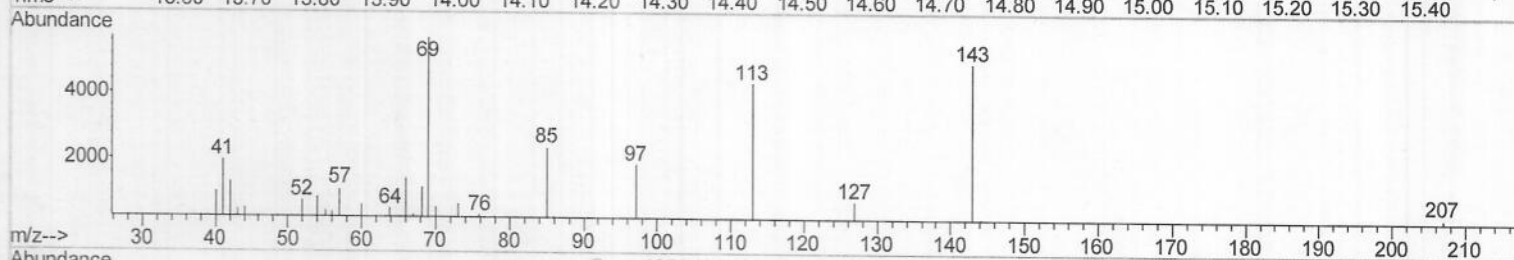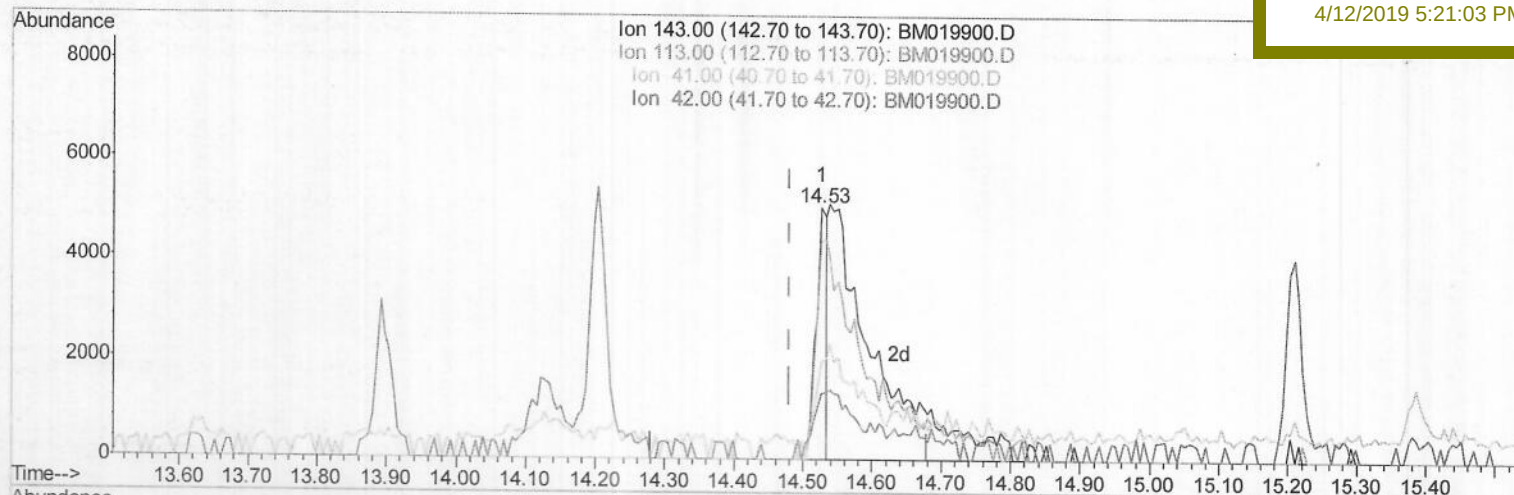

(52) 4-Nitrophenol-d4 (S)

14.527min (+0.047) 1.73ng/ul

response 5571

Ion	Exp%	Act%
143.00	100	100
113.00	77.10	86.92
41.00	32.60	38.91
42.00	22.30	26.54

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041119\

Data File : BM019900.D

Acq On : 11 Apr 2019 18:53

Operator : JU/SJ

Sample : K2304-11

Misc :

ALS Vial : 9 Sample Multiplier: 1

Quant Time: Apr 12 04:19:40 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Fri Apr 12 04:12:05 2019

Response via : Initial Calibration

Instrument :

BNA_M




ClientSampleId :

BF895

Manual Integrations
APPROVED

Sohil

4/12/2019 5:21:03 PM

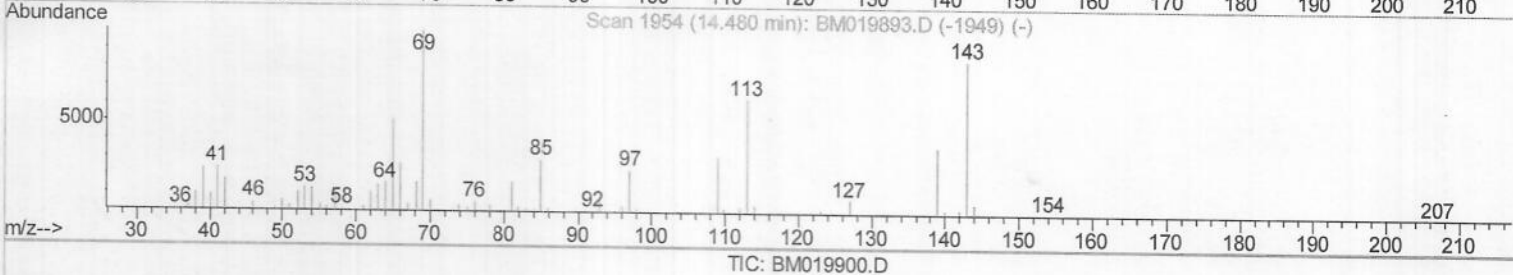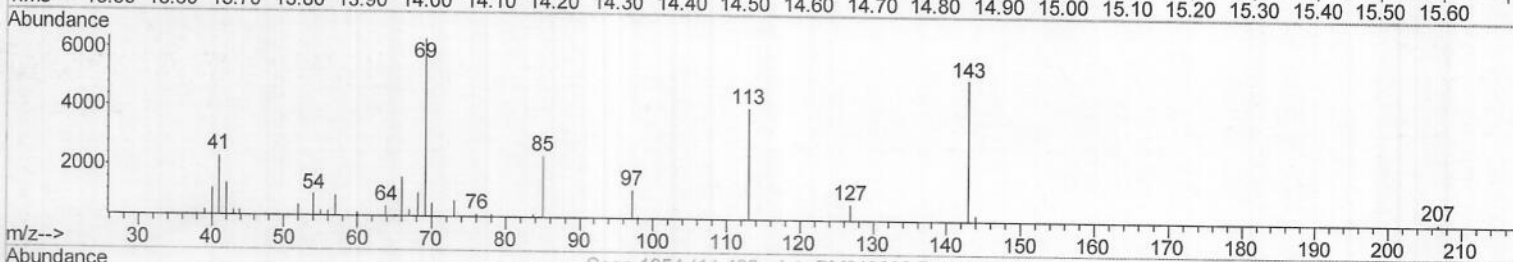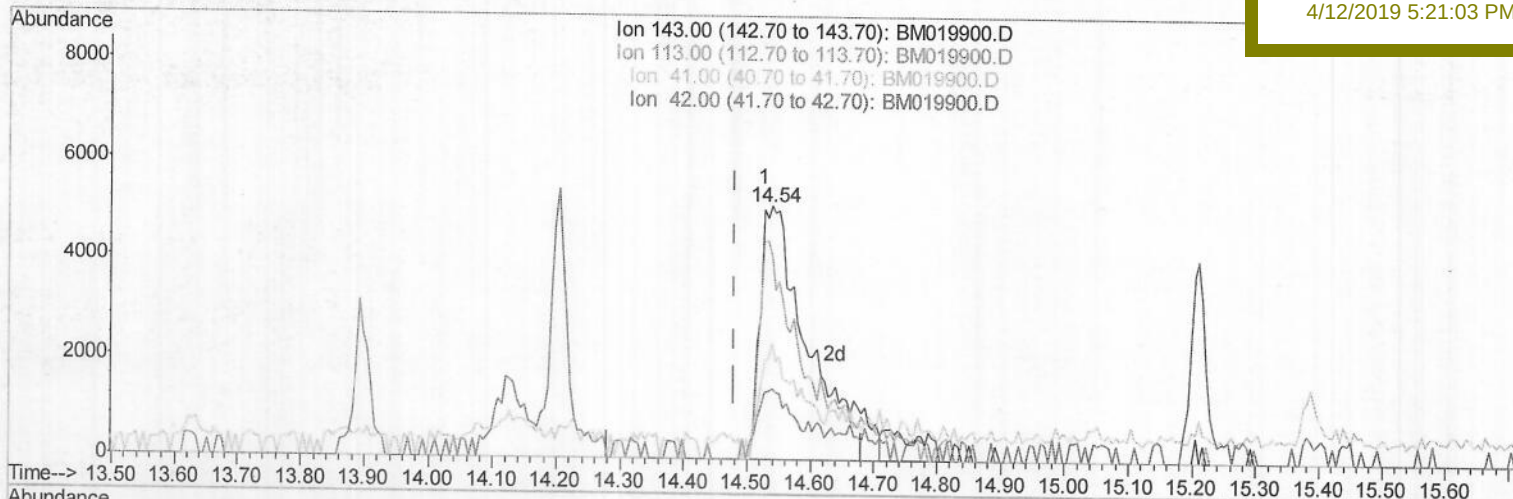

TIC: BM019900.D

(52) 4-Nitrophenol-d4 (S)

14.539min (+0.059) 8.55ng/ul m

response 27492

Ion	Exp%	Act%
143.00	100	100
113.00	77.10	80.13
41.00	32.60	45.65#
42.00	22.30	27.67#

S7
04/12/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041119\
 Data File : BM019900.D
 Acq On : 11 Apr 2019 18:53
 Operator : JU/SJ
 Sample : K2304-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Quant Time: Apr 12 05:34:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 12 04:12:05 2019
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 BF895

Manual Integrations
 APPROVED

Sohil
 4/12/2019 5:21:03 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	120910	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	478724	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	254176	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	544489	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	596161	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	699593	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.10	96	16563	5.36	ng/uL	0.00
5) Phenol-d5	6.74	99	127439	11.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	95399	13.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.08	132	112205	13.75	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	88492	10.95	ng/ul	0.01
19) Nitrobenzene-d5	8.72	128	49363	14.45	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	57991	15.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	90403	12.61	ng/ul	0.02
29) 4-Chloroaniline-d4	10.50	131	88544	10.28	ng/ul	0.02
44) Dimethylphthalate-d6	13.63	166	301087	14.68	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	360145	14.04	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	27492m	8.55	ng/ul	0.06
58) Fluorene-d10	15.21	176	258194	14.61	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	25250	7.01	ng/ul	0.01
71) Anthracene-d10	17.07	188	376926	14.43	ng/ul	0.00
79) Pyrene-d10	19.38	212	397105	14.42	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.24	264	469706	12.66	ng/ul	0.00

Target Compounds					Qvalue
45) Dimethylphthalate	13.68	163	71320	3.466 ng/ul#	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ
 04/12/19