




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045143.D
Acq On : 11 Apr 2024 20:33
Operator : MA/JU
Sample : P1968-01 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E07R9

Manual IntegrationsAPPROVED

Quant Time: Apr 11 22:43:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/12/2024
Supervised By :mohammad ahmed 04/16/2024

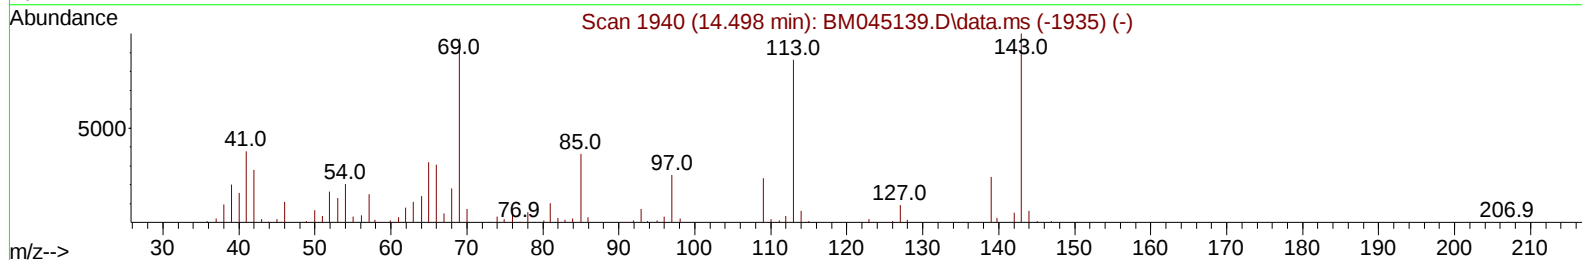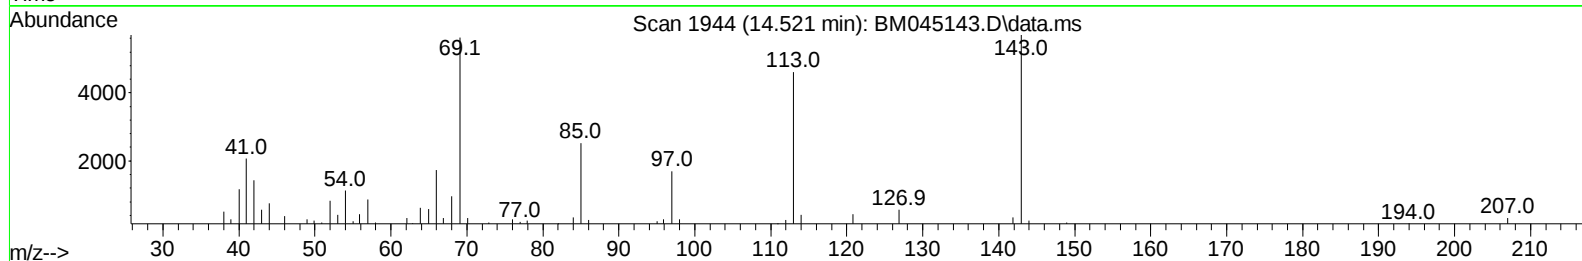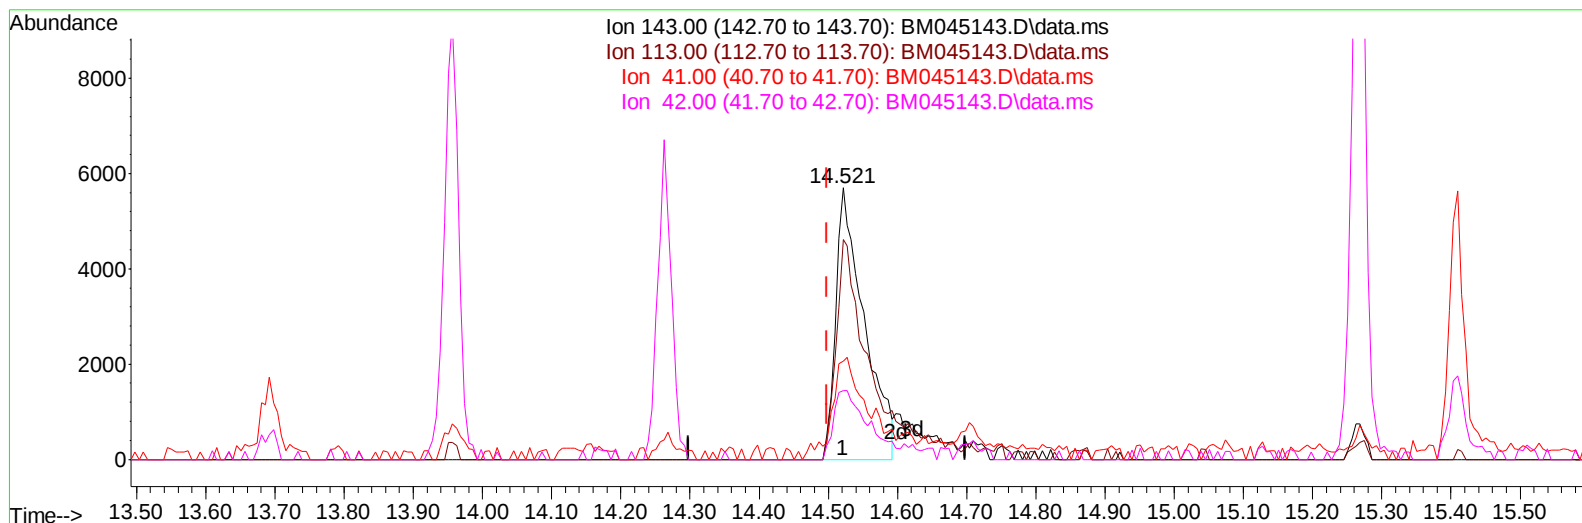

TIC: BM045143.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.521min (+ 0.024) 5.63 ng/u1

response 16173

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.80	80.96
41.00	36.50	36.27
42.00	23.30	25.27




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045143.D
Acq On : 11 Apr 2024 20:33
Operator : MA/JU
Sample : P1968-01 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E07R9

Manual IntegrationsAPPROVED

Quant Time: Apr 11 22:43:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/12/2024
Supervised By :mohammad ahmed 04/16/2024

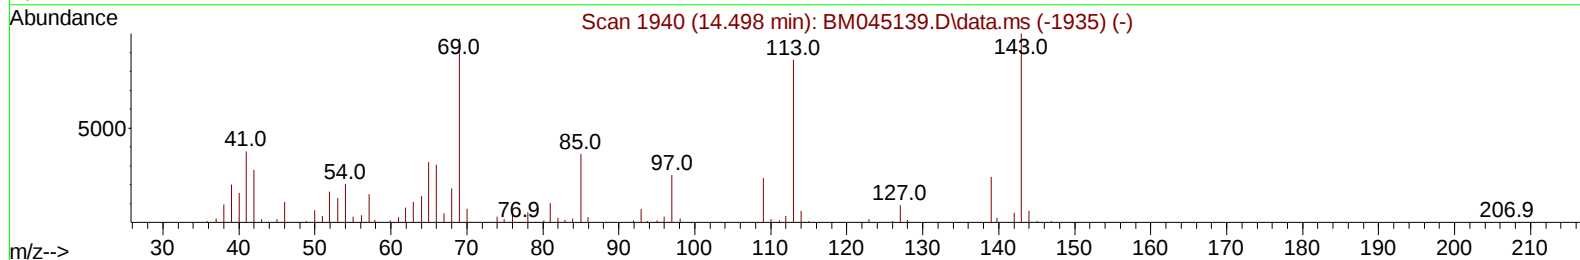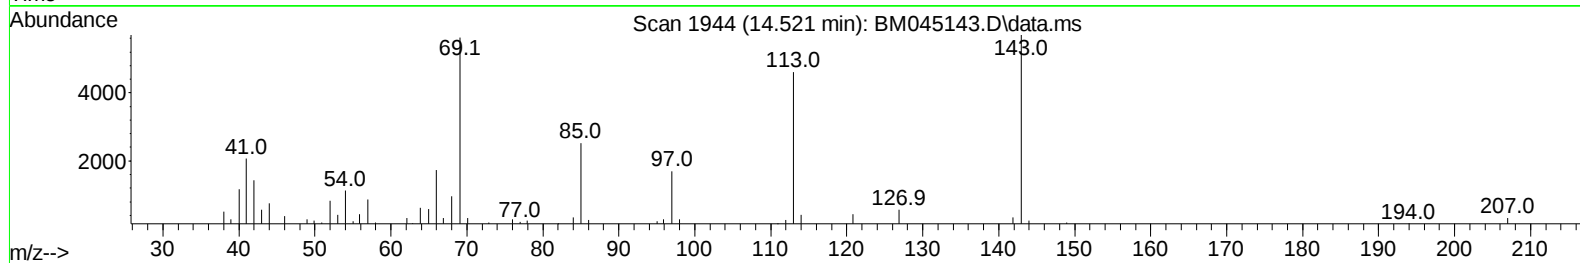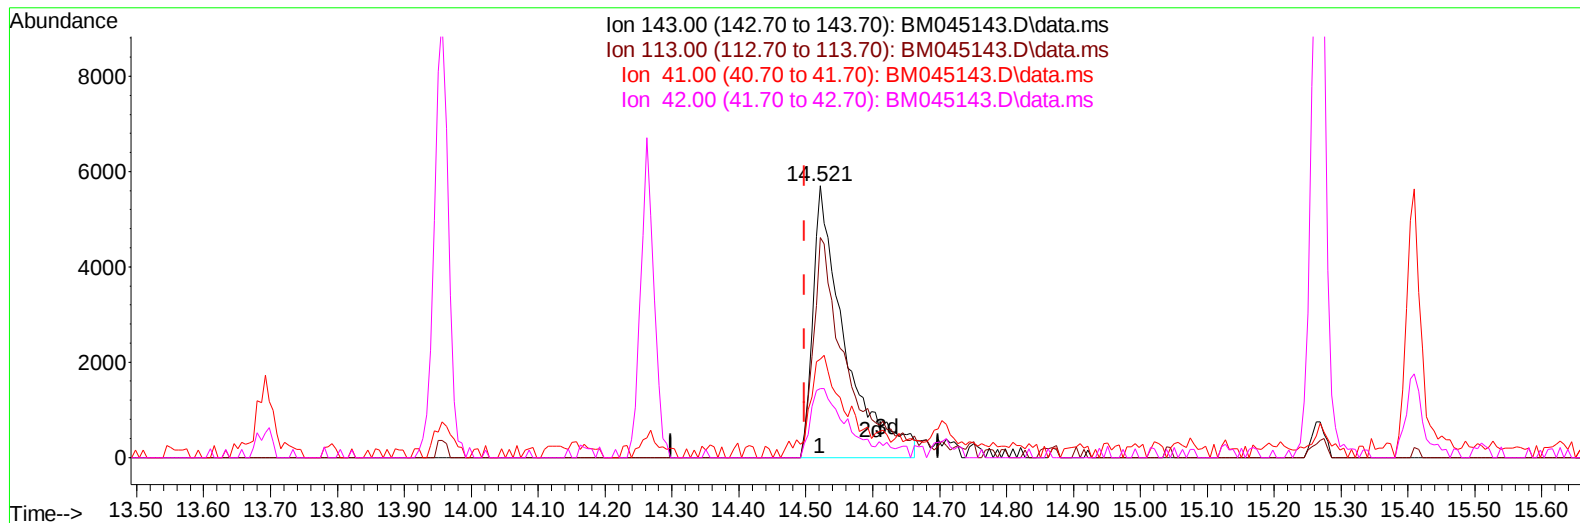

TIC: BM045143.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.521min (+ 0.024) 6.54 ng/ul m

response 18764

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.80	80.96
41.00	36.50	36.27
42.00	23.30	25.27

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045143.D
 Acq On : 11 Apr 2024 20:33
 Operator : MA/JU
 Sample : P1968-01 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E07R9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/12/2024
 Supervised By :mohammad ahmed 04/16/2024

Quant Time: Apr 11 22:50:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 18:54:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	66952	20.000	ng/ul	0.00
20) Naphthalene-d8	10.392	136	288141	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.263	164	197596	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.027	188	407654	20.000	ng/ul	0.00
79) Chrysene-d12	21.233	240	318813	20.000	ng/ul	0.00
88) Perylene-d12	23.450	264	328587	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.204	96	7948	4.433	ng/uL	0.00
4) Pyridine-d5	3.610	84	57379	11.768	ng/ul	0.00
7) Phenol-d5	6.804	99	48539	8.552	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	139526	41.260	ng/ul	0.00
11) 2-Chlorophenol-d4	7.151	132	139234	31.311	ng/ul	0.00
15) 4-Methylphenol-d8	8.328	113	92210	20.755	ng/ul	0.00
21) Nitrobenzene-d5	8.781	128	92407	41.751	ng/ul	0.00
24) 2-Nitrophenol-d4	9.492	143	97792	41.861	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.022	165	156920	36.636	ng/ul	0.00
31) 4-Chloroaniline-d4	10.551	131	206913	30.343	ng/ul	0.00
46) Dimethylphthalate-d6	13.692	166	638832	46.433	ng/ul	0.00
49) Acenaphthylene-d8	13.957	160	685743	42.191	ng/ul	0.00
54) 4-Nitrophenol-d4	14.521	143	18764m	6.535	ng/ul	0.02
60) Fluorene-d10	15.268	176	541878	44.179	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	86457	35.769	ng/ul	0.00
73) Anthracene-d10	17.127	188	866312	47.240	ng/ul	0.00
81) Pyrene-d10	19.433	212	994273	63.336	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.309	264	810648	50.572	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045143.D
Acq On : 11 Apr 2024 20:33
Operator : MA/JU
Sample : P1968-01 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E07R9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/12/2024
Supervised By :mohammad ahmed 04/16/2024

Quant Time: Apr 11 22:50:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

