




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045149.D
Acq On : 12 Apr 2024 00:11
Operator : MA/JU
Sample : P2013-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MC1

Manual IntegrationsAPPROVED

Quant Time: Apr 12 01:26:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

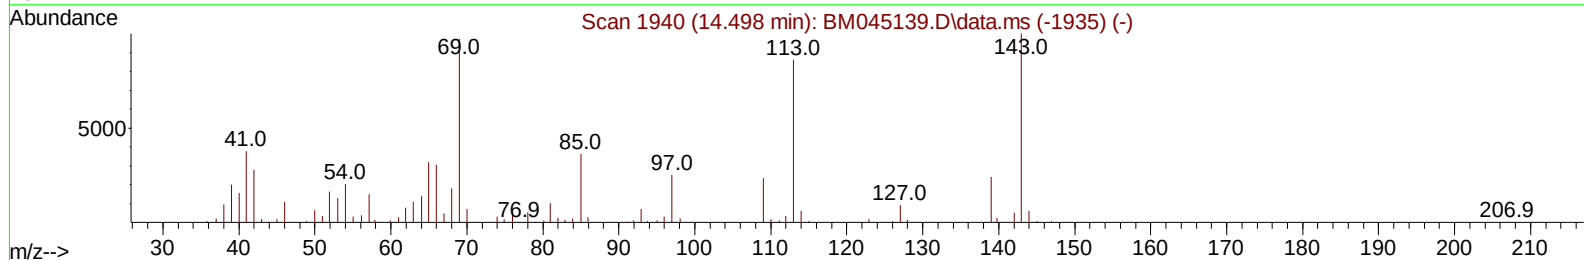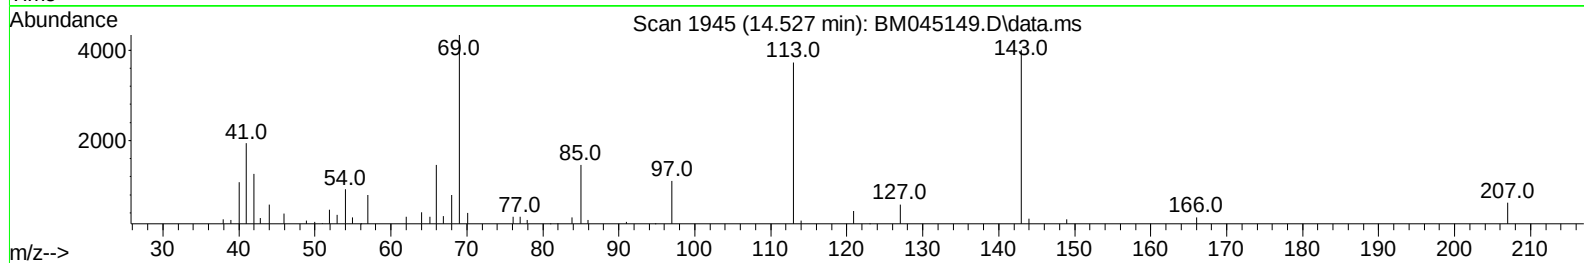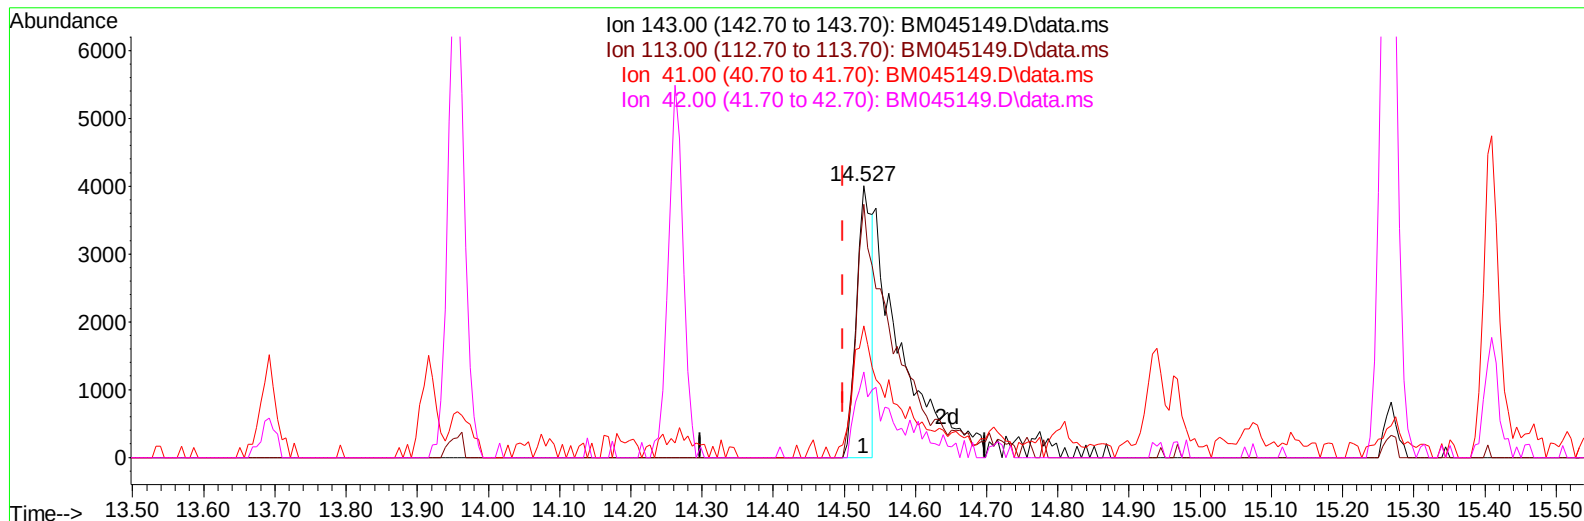

TIC: BM045149.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.527min (+ 0.029) 2.51 ng/ul

response 6073

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.80	93.16
41.00	36.50	48.35#
42.00	23.30	31.44#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045149.D
 Acq On : 12 Apr 2024 00:11
 Operator : MA/JU
 Sample : P2013-17
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MC1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/16/2024
 Supervised By :mohammad ahmed 04/16/2024

Quant Time: Apr 12 01:28:56 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 18:54:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	59136	20.000	ng/ul	0.00
20) Naphthalene-d8	10.386	136	249529	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.262	164	166753	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.021	188	347206	20.000	ng/ul	0.00
79) Chrysene-d12	21.233	240	304535	20.000	ng/ul	0.00
88) Perylene-d12	23.450	264	320134	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.204	96	6880	4.344	ng/uL	0.00
4) Pyridine-d5	3.610	84	45447	10.553	ng/ul	0.00
7) Phenol-d5	6.804	99	42824	8.542	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	121512	40.682	ng/ul	0.00
11) 2-Chlorophenol-d4	7.151	132	124473	31.692	ng/ul	0.00
15) 4-Methylphenol-d8	8.328	113	82055	20.911	ng/ul	0.00
21) Nitrobenzene-d5	8.780	128	83625	43.630	ng/ul	0.00
24) 2-Nitrophenol-d4	9.492	143	86026	42.523	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.022	165	139553	37.623	ng/ul	0.00
31) 4-Chloroaniline-d4	10.551	131	190164	32.202	ng/ul	0.00
46) Dimethylphthalate-d6	13.692	166	563266	48.513	ng/ul	0.00
49) Acenaphthylene-d8	13.957	160	609911	44.466	ng/ul	0.00
54) 4-Nitrophenol-d4	14.527	143	15663m	6.464	ng/ul	0.03
60) Fluorene-d10	15.268	176	475702	45.957	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.409	200	75966	36.901	ng/ul	0.00
73) Anthracene-d10	17.121	188	776857	49.737	ng/ul	0.00
81) Pyrene-d10	19.427	212	907346	60.509	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.309	264	818939	52.439	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045149.D
Acq On : 12 Apr 2024 00:11
Operator : MA/JU
Sample : P2013-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MC1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

Quant Time: Apr 12 01:28:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

