




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045162.D
Acq On : 12 Apr 2024 08:40
Operator : MA/JU
Sample : P2014-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME1

Manual IntegrationsAPPROVED

Quant Time: Apr 12 10:59:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

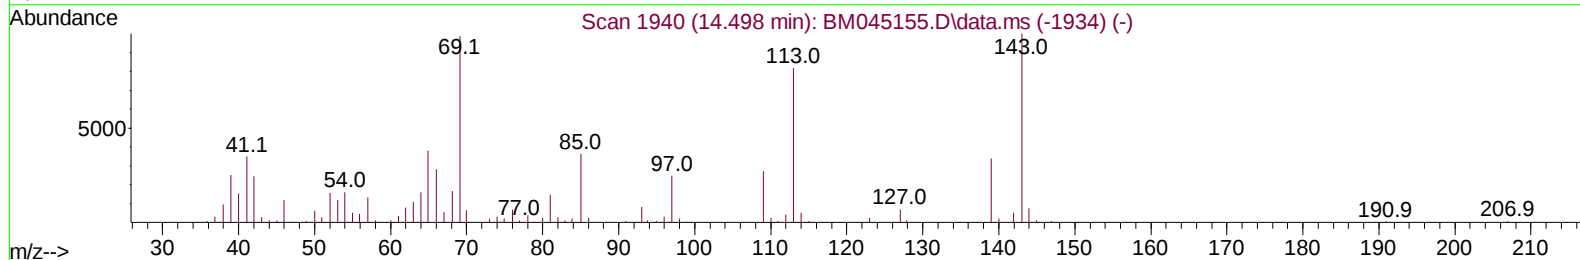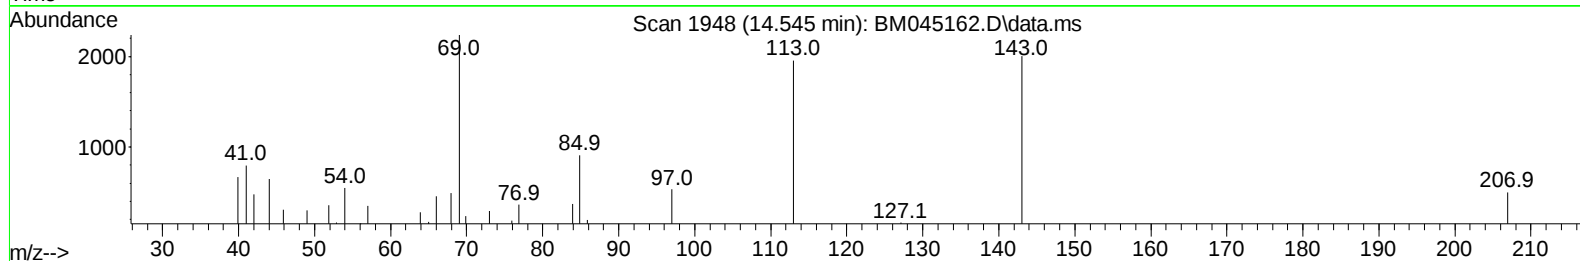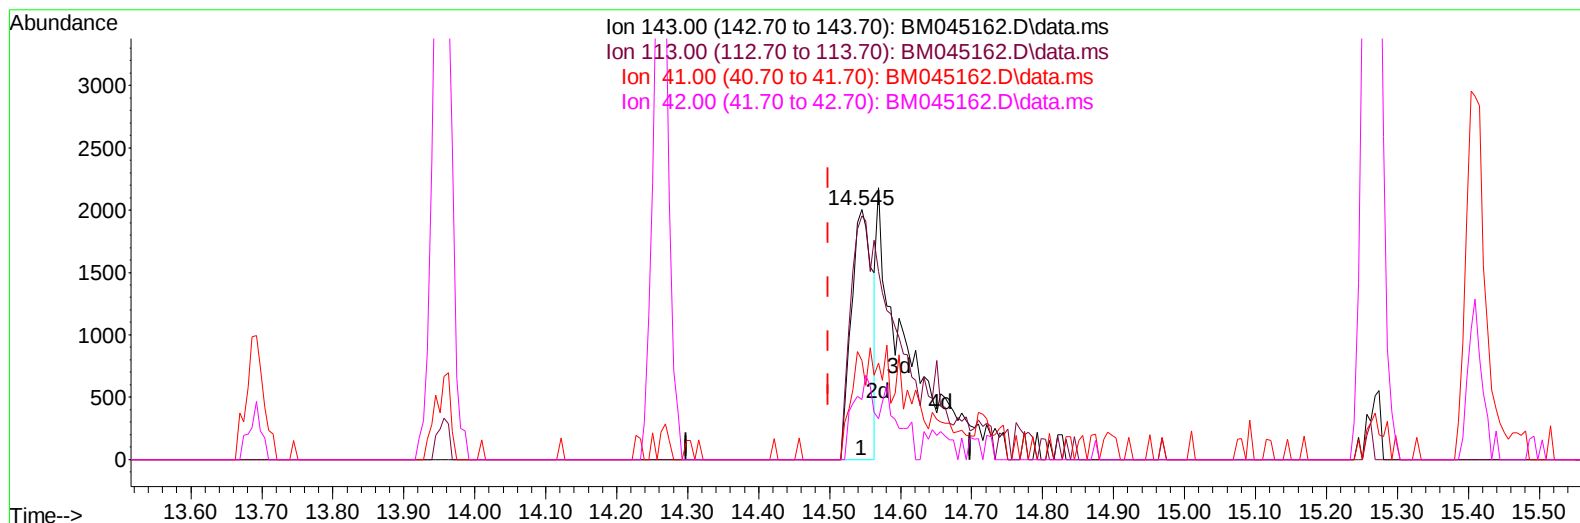

TIC: BM045162.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.545min (+ 0.047) 1.71 ng/u1

response 4067

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.80	97.51#
41.00	36.50	39.70
42.00	23.30	23.94




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045162.D
Acq On : 12 Apr 2024 08:40
Operator : MA/JU
Sample : P2014-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME1

Manual IntegrationsAPPROVED

Quant Time: Apr 12 10:59:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

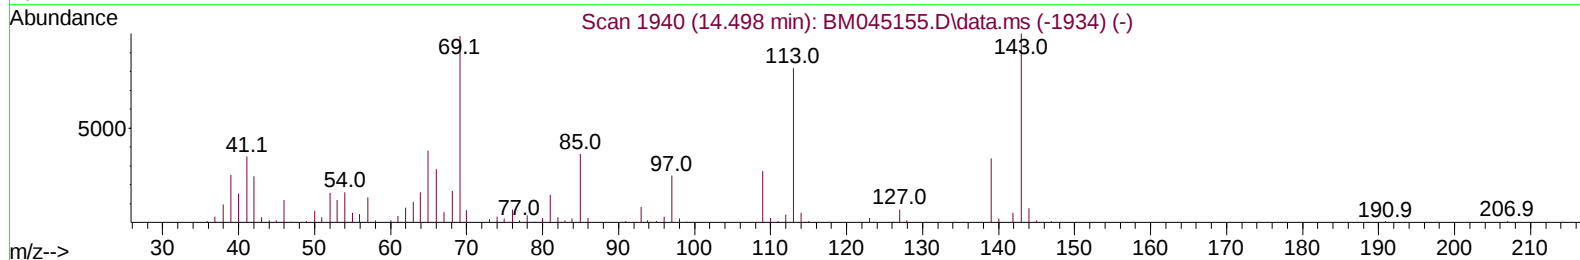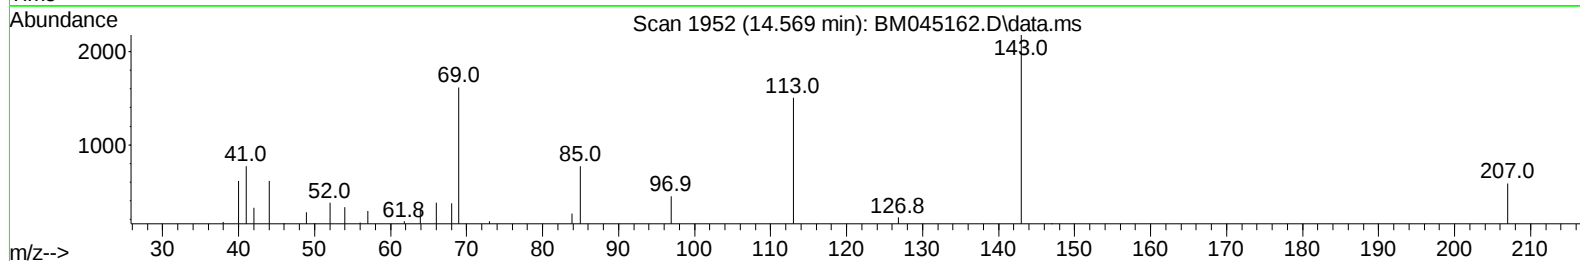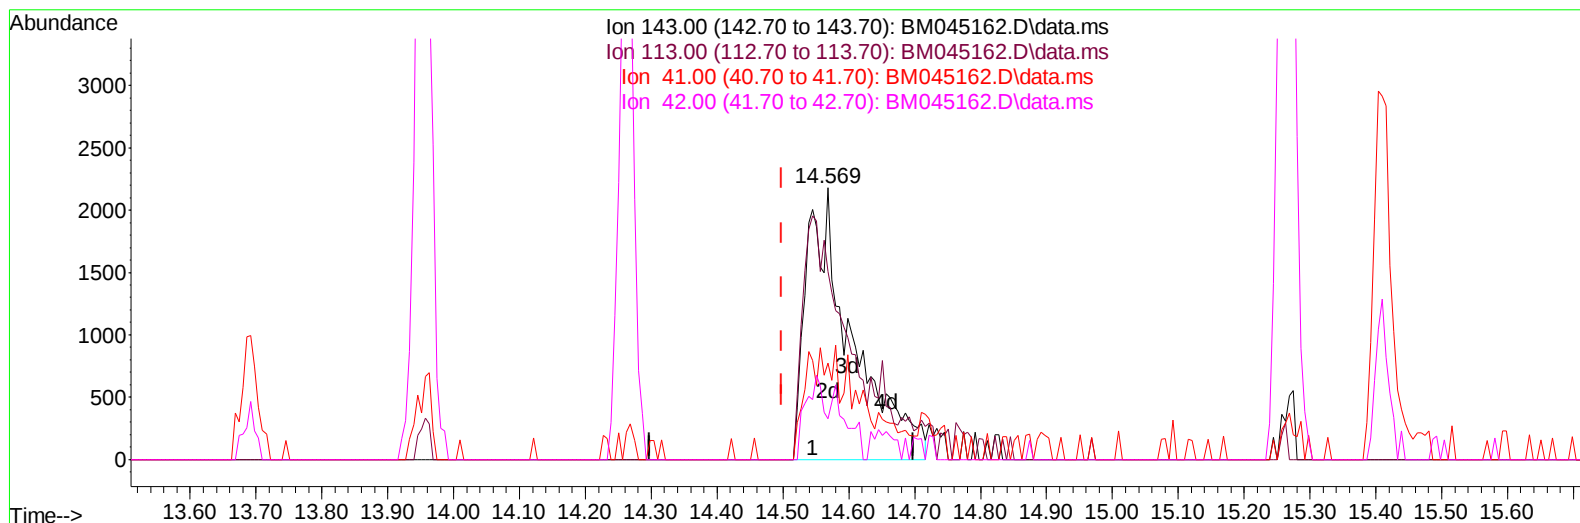

TIC: BM045162.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.569min (+ 0.071) 4.42 ng/ul m

response 10477

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.80	69.16
41.00	36.50	35.52
42.00	23.30	15.01#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045162.D
 Acq On : 12 Apr 2024 08:40
 Operator : MA/JU
 Sample : P2014-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0ME1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/16/2024
 Supervised By :mohammad ahmed 04/16/2024

Quant Time: Apr 12 11:01:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 18:54:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	58076	20.000	ng/ul	0.00
20) Naphthalene-d8	10.386	136	247054	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.263	164	163304	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.021	188	323304	20.000	ng/ul	0.00
79) Chrysene-d12	21.233	240	245716	20.000	ng/ul	0.00
88) Perylene-d12	23.450	264	289472	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.210	96	6078	3.908	ng/uL	0.00
4) Pyridine-d5	3.610	84	33683	7.964	ng/ul	0.00
7) Phenol-d5	6.804	99	32923	6.687	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	103511	35.288	ng/ul	0.00
11) 2-Chlorophenol-d4	7.151	132	104492	27.090	ng/ul	0.00
15) 4-Methylphenol-d8	8.328	113	66032	17.134	ng/ul	0.00
21) Nitrobenzene-d5	8.781	128	70416	37.106	ng/ul	0.00
24) 2-Nitrophenol-d4	9.492	143	72166	36.029	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.022	165	116976	31.853	ng/ul	0.00
31) 4-Chloroaniline-d4	10.551	131	163343	27.937	ng/ul	0.00
46) Dimethylphthalate-d6	13.692	166	470140	41.348	ng/ul	0.00
49) Acenaphthylene-d8	13.957	160	528560	39.349	ng/ul	0.00
54) 4-Nitrophenol-d4	14.569	143	10477m	4.415	ng/ul	0.07
60) Fluorene-d10	15.263	176	404161	39.870	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	58737	30.641	ng/ul	0.00
73) Anthracene-d10	17.121	188	653189	44.912	ng/ul	0.00
81) Pyrene-d10	19.427	212	707524	58.478	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.309	264	644300	45.626	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045162.D
Acq On : 12 Apr 2024 08:40
Operator : MA/JU
Sample : P2014-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

Quant Time: Apr 12 11:01:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

