




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045163.D
Acq On : 12 Apr 2024 09:16
Operator : MA/JU
Sample : P2014-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME2

Manual IntegrationsAPPROVED

Quant Time: Apr 12 11:05:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

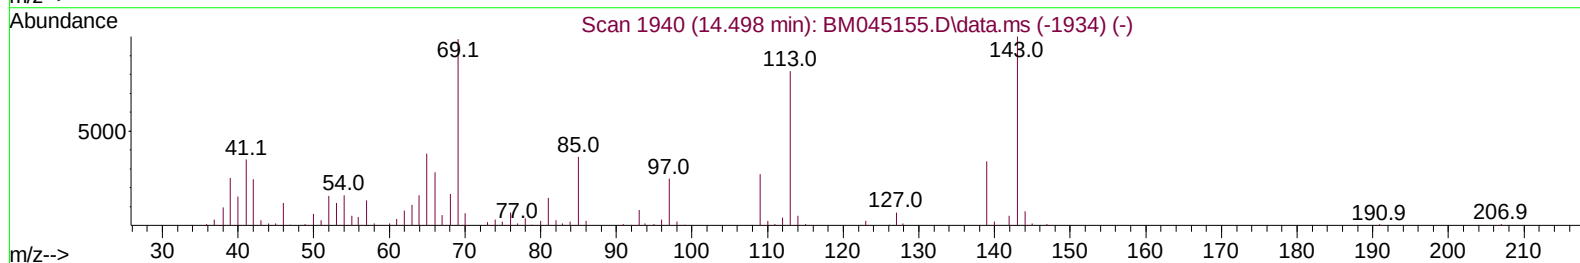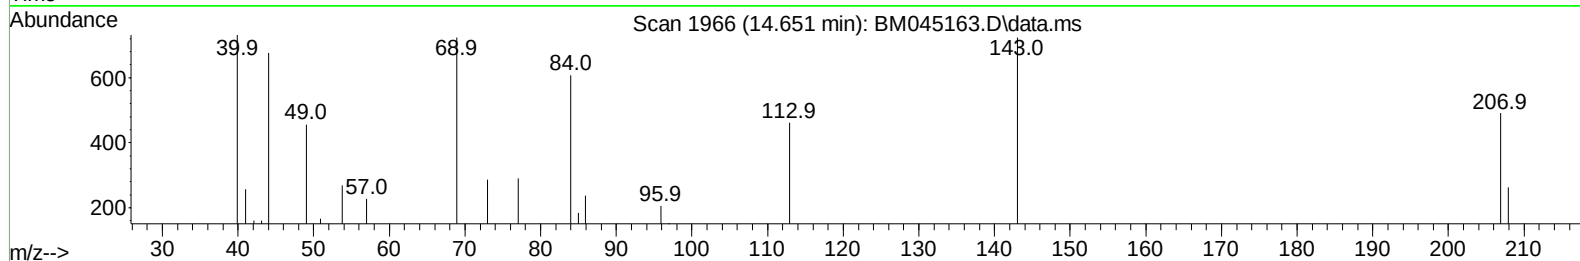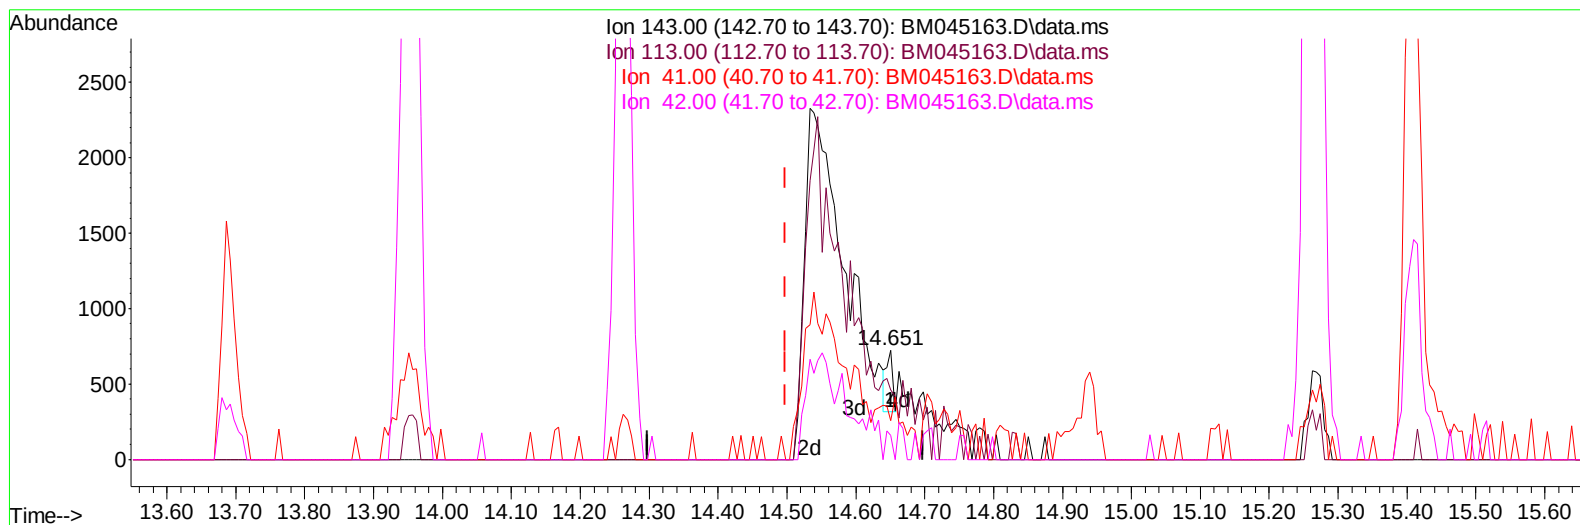

TIC: BM045163.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.651min (+ 0.153) 0.10 ng/ul

response 248

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.80	63.81
41.00	36.50	35.64
42.00	23.30	22.10




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045163.D
Acq On : 12 Apr 2024 09:16
Operator : MA/JU
Sample : P2014-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME2

Manual IntegrationsAPPROVED

Quant Time: Apr 12 11:05:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

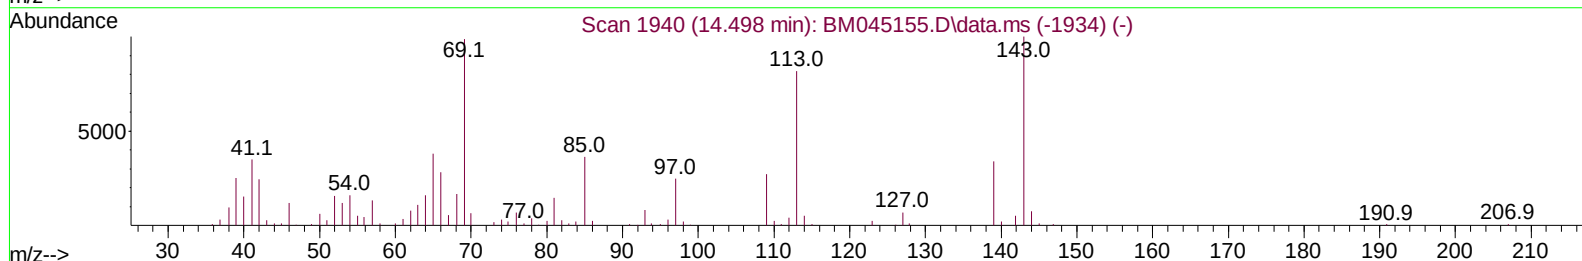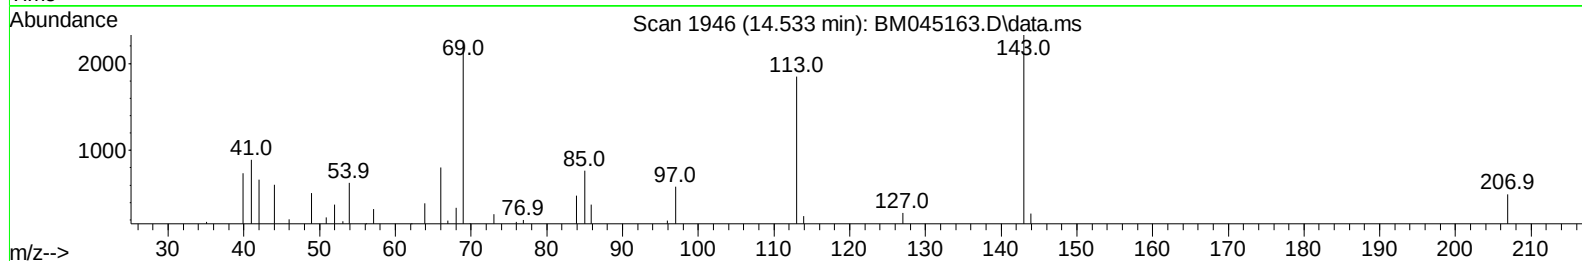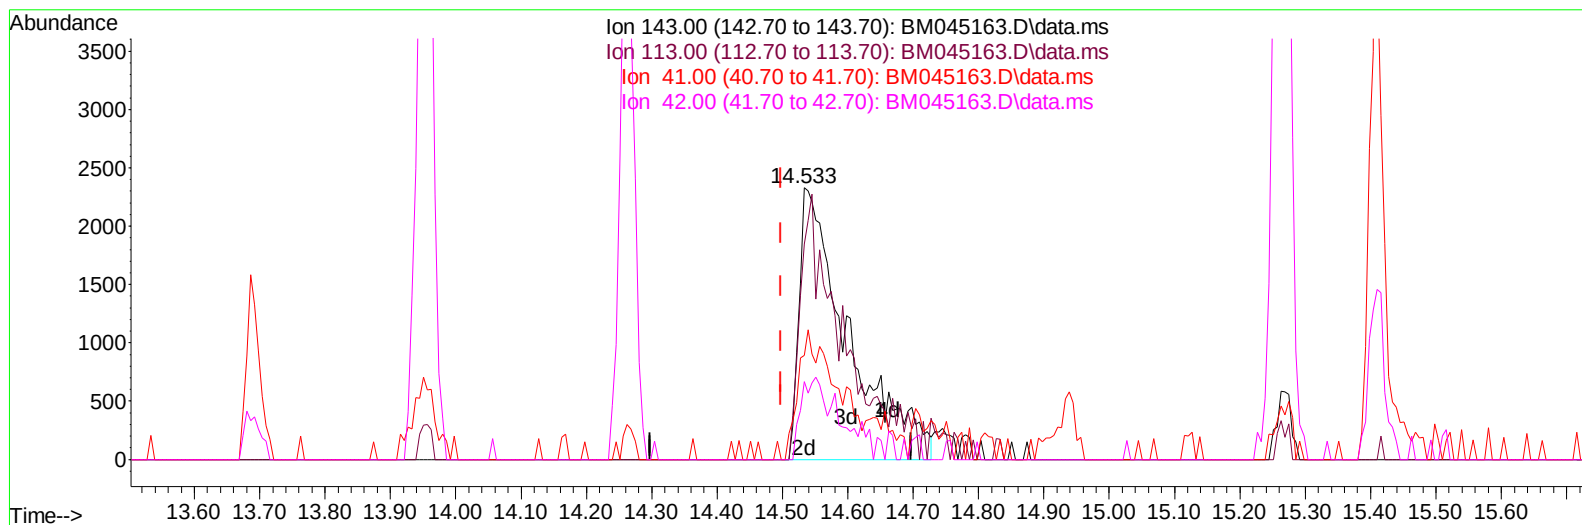

TIC: BM045163.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.533min (+ 0.035) 5.11 ng/ul m

response 12108

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.80	79.42
41.00	36.50	38.32
42.00	23.30	28.57#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045163.D
 Acq On : 12 Apr 2024 09:16
 Operator : MA/JU
 Sample : P2014-17
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0ME2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/16/2024
 Supervised By :mohammad ahmed 04/16/2024

Quant Time: Apr 12 11:06:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 18:54:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	56367	20.000	ng/ul	0.00
20) Naphthalene-d8	10.386	136	245977	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.263	164	163168	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.021	188	342774	20.000	ng/ul	0.00
79) Chrysene-d12	21.239	240	296697	20.000	ng/ul	0.00
88) Perylene-d12	23.450	264	325587	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.210	96	6478	4.292	ng/uL	0.00
4) Pyridine-d5	3.616	84	47444	11.558	ng/ul	0.01
7) Phenol-d5	6.804	99	37212	7.787	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.969	67	122935	43.181	ng/ul	0.00
11) 2-Chlorophenol-d4	7.151	132	121144	32.359	ng/ul	0.00
15) 4-Methylphenol-d8	8.328	113	74251	19.851	ng/ul	0.00
21) Nitrobenzene-d5	8.781	128	84419	44.680	ng/ul	0.00
24) 2-Nitrophenol-d4	9.486	143	84354	42.298	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.022	165	135159	36.965	ng/ul	0.00
31) 4-Chloroaniline-d4	10.545	131	182894	31.418	ng/ul	0.00
46) Dimethylphthalate-d6	13.692	166	563702	49.618	ng/ul	0.00
49) Acenaphthylene-d8	13.957	160	617701	46.023	ng/ul	0.00
54) 4-Nitrophenol-d4	14.533	143	12108m	5.107	ng/ul	0.04
60) Fluorene-d10	15.262	176	481669	47.556	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	72670	35.756	ng/ul	0.00
73) Anthracene-d10	17.121	188	775074	50.265	ng/ul	0.00
81) Pyrene-d10	19.433	212	892979	61.124	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.309	264	855592	53.868	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045163.D
Acq On : 12 Apr 2024 09:16
Operator : MA/JU
Sample : P2014-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

Quant Time: Apr 12 11:06:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

