




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045164.D
Acq On : 12 Apr 2024 09:53
Operator : MA/JU
Sample : P2014-18
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOME3

Manual IntegrationsAPPROVED

Quant Time: Apr 12 11:07:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

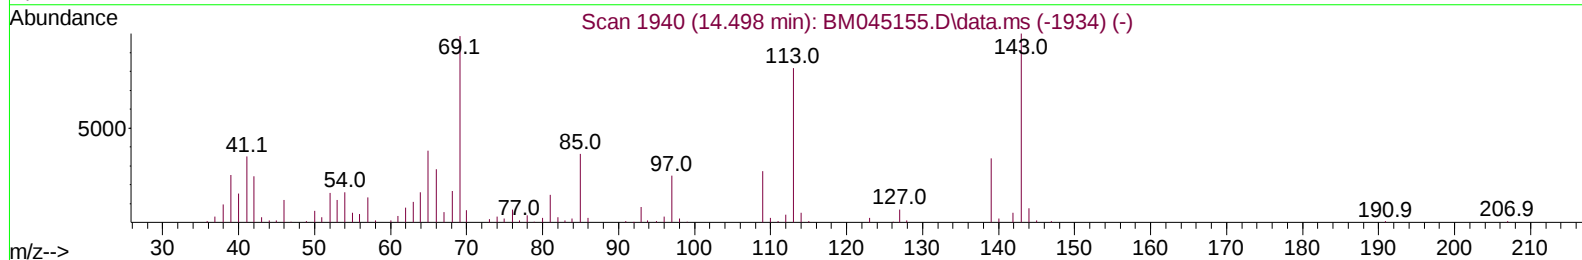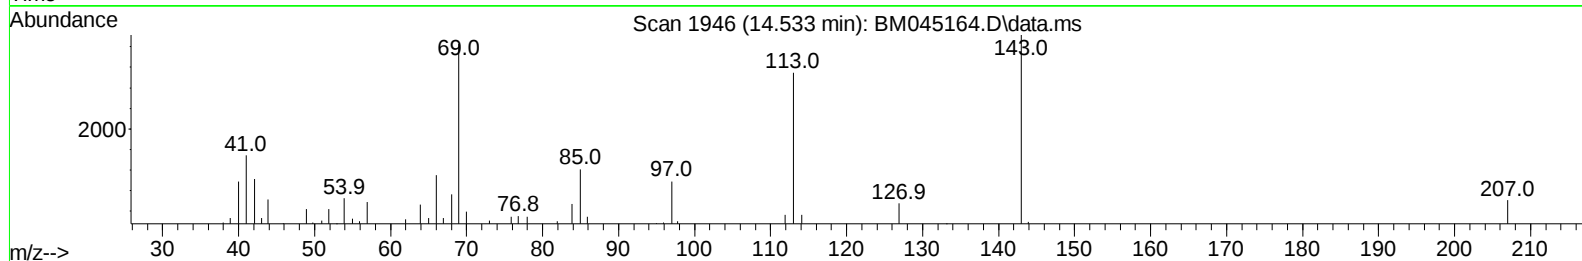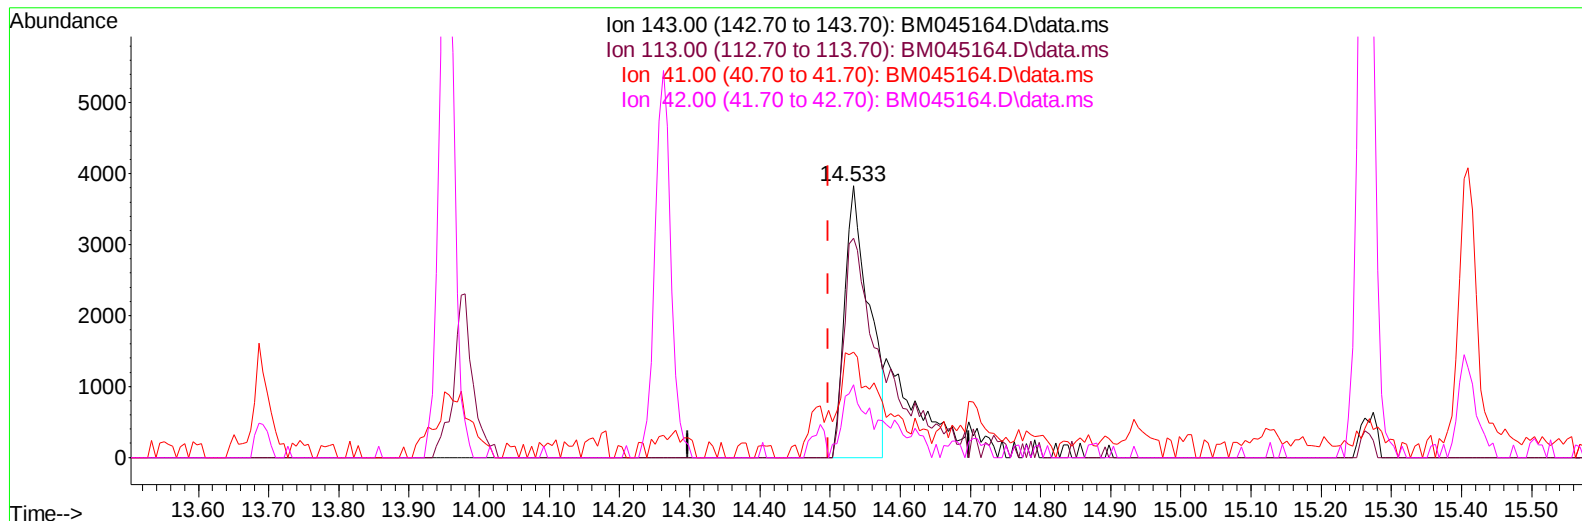

TIC: BM045164.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.533min (+ 0.035) 3.45 ng/ul

response 9292

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.80	80.64
41.00	36.50	38.77
42.00	23.30	26.72




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045164.D
Acq On : 12 Apr 2024 09:53
Operator : MA/JU
Sample : P2014-18
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME3

Manual IntegrationsAPPROVED

Quant Time: Apr 12 11:07:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

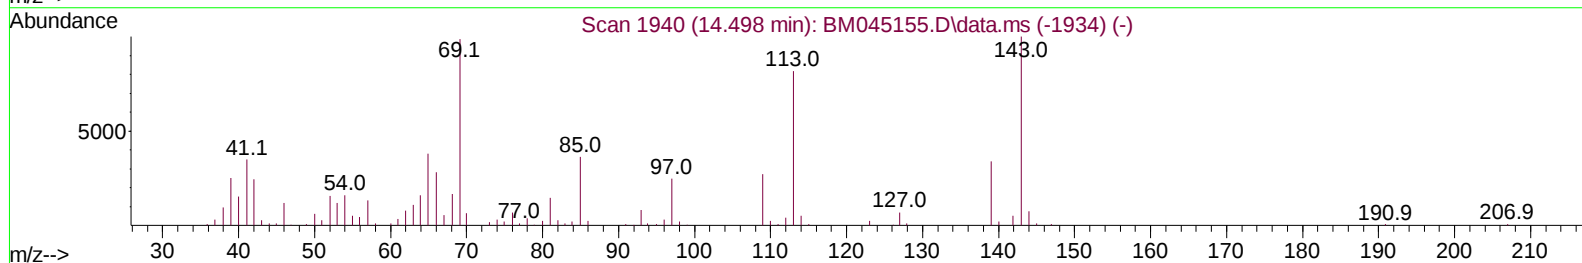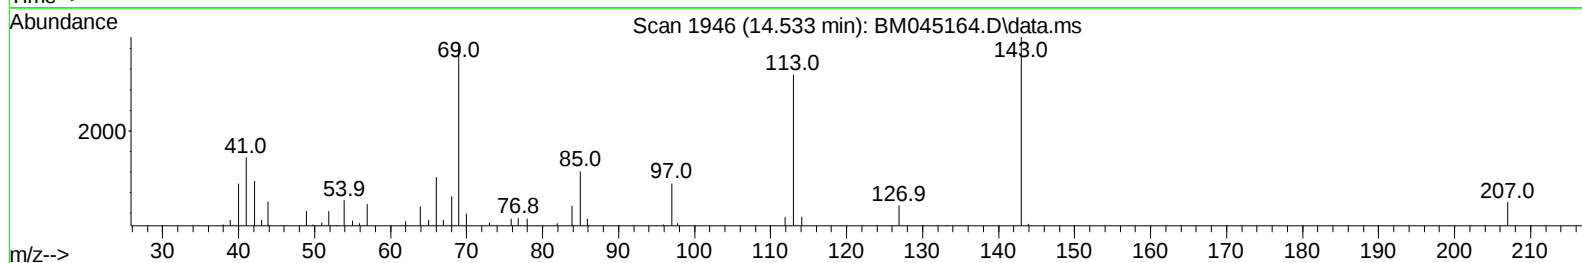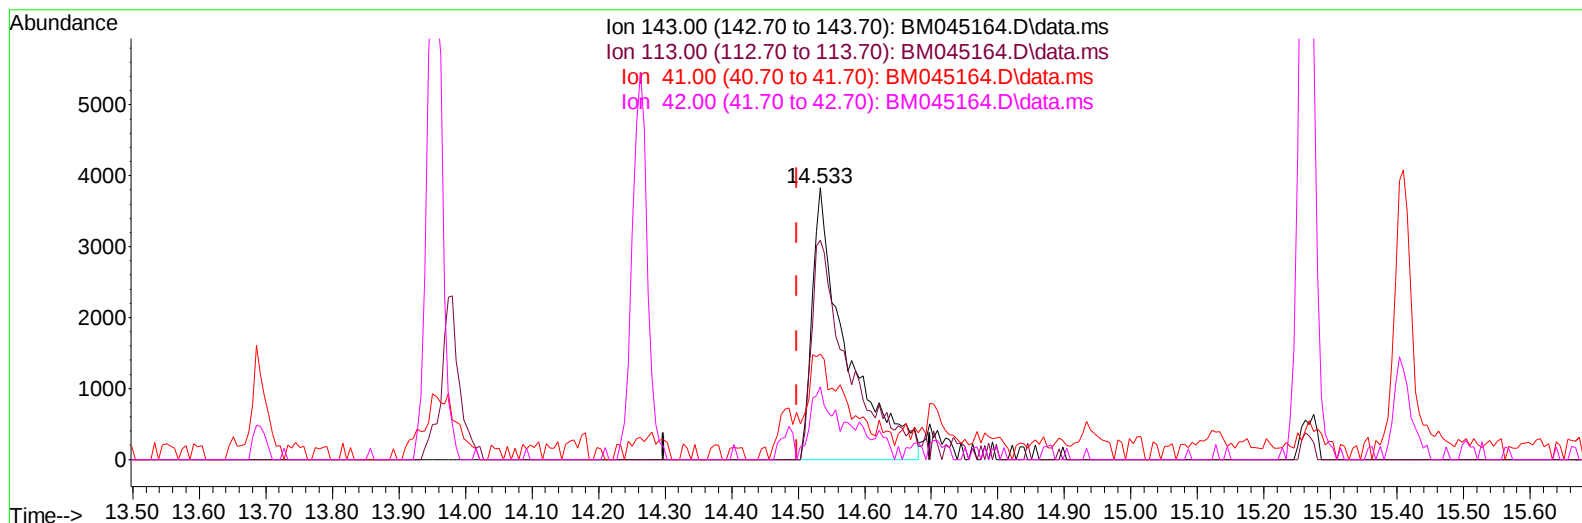

TIC: BM045164.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.533min (+ 0.035) 5.15 ng/ul m

response 13847

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.80	80.64
41.00	36.50	38.77
42.00	23.30	26.72

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045164.D
 Acq On : 12 Apr 2024 09:53
 Operator : MA/JU
 Sample : P2014-18
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0ME3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/16/2024
 Supervised By :mohammad ahmed 04/16/2024

Quant Time: Apr 12 11:09:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 18:54:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	63778	20.000	ng/ul	0.00
20) Naphthalene-d8	10.386	136	280572	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.263	164	185109	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.021	188	375384	20.000	ng/ul	0.00
79) Chrysene-d12	21.233	240	315765	20.000	ng/ul	0.00
88) Perylene-d12	23.450	264	334993	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.204	96	7147	4.185	ng/uL	0.00
4) Pyridine-d5	3.610	84	37011	7.969	ng/ul	0.00
7) Phenol-d5	6.804	99	42002	7.768	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.969	67	117120	36.358	ng/ul	0.00
11) 2-Chlorophenol-d4	7.151	132	121710	28.733	ng/ul	0.00
15) 4-Methylphenol-d8	8.328	113	84998	20.084	ng/ul	0.00
21) Nitrobenzene-d5	8.781	128	81133	37.646	ng/ul	0.00
24) 2-Nitrophenol-d4	9.492	143	83196	36.574	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.022	165	149568	35.862	ng/ul	0.00
31) 4-Chloroaniline-d4	10.545	131	200753	30.233	ng/ul	0.00
46) Dimethylphthalate-d6	13.692	166	555316	43.086	ng/ul	0.00
49) Acenaphthylene-d8	13.957	160	613106	40.266	ng/ul	0.00
54) 4-Nitrophenol-d4	14.533	143	13847m	5.148	ng/ul	0.04
60) Fluorene-d10	15.268	176	474125	41.262	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	69372	31.168	ng/ul	0.00
73) Anthracene-d10	17.121	188	743583	44.034	ng/ul	0.00
81) Pyrene-d10	19.427	212	864031	55.571	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.309	264	733823	44.904	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045164.D
Acq On : 12 Apr 2024 09:53
Operator : MA/JU
Sample : P2014-18
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

Quant Time: Apr 12 11:09:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

