




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045166.D
 Acq On : 12 Apr 2024 11:06
 Operator : MA/JU
 Sample : P2014-23
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOME6

Manual IntegrationsAPPROVED

Quant Time: Apr 12 11:36:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 18:54:49 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
 Supervised By :mohammad ahmed 04/16/2024

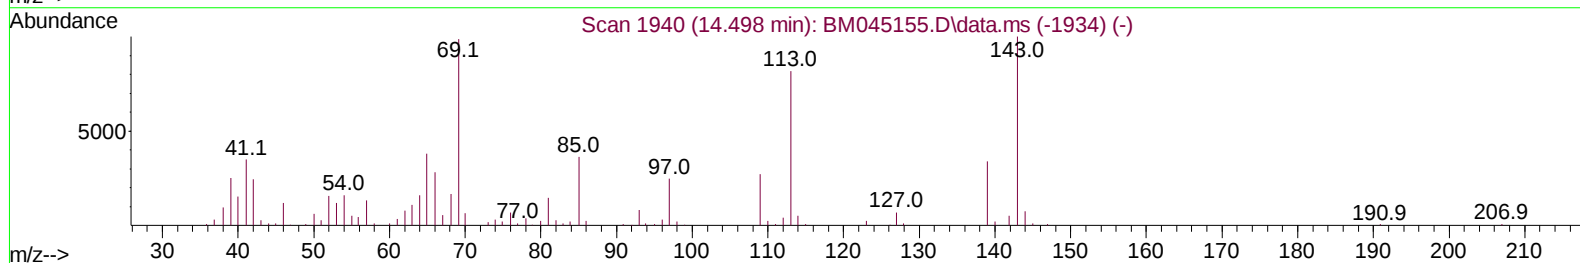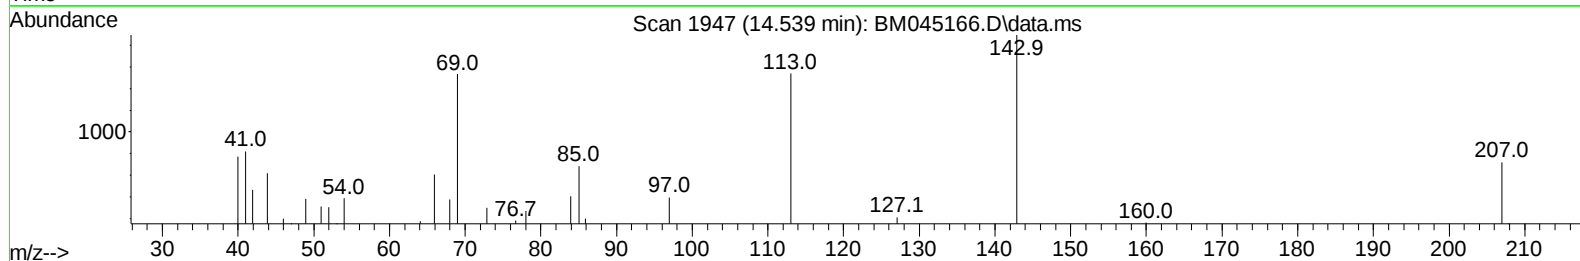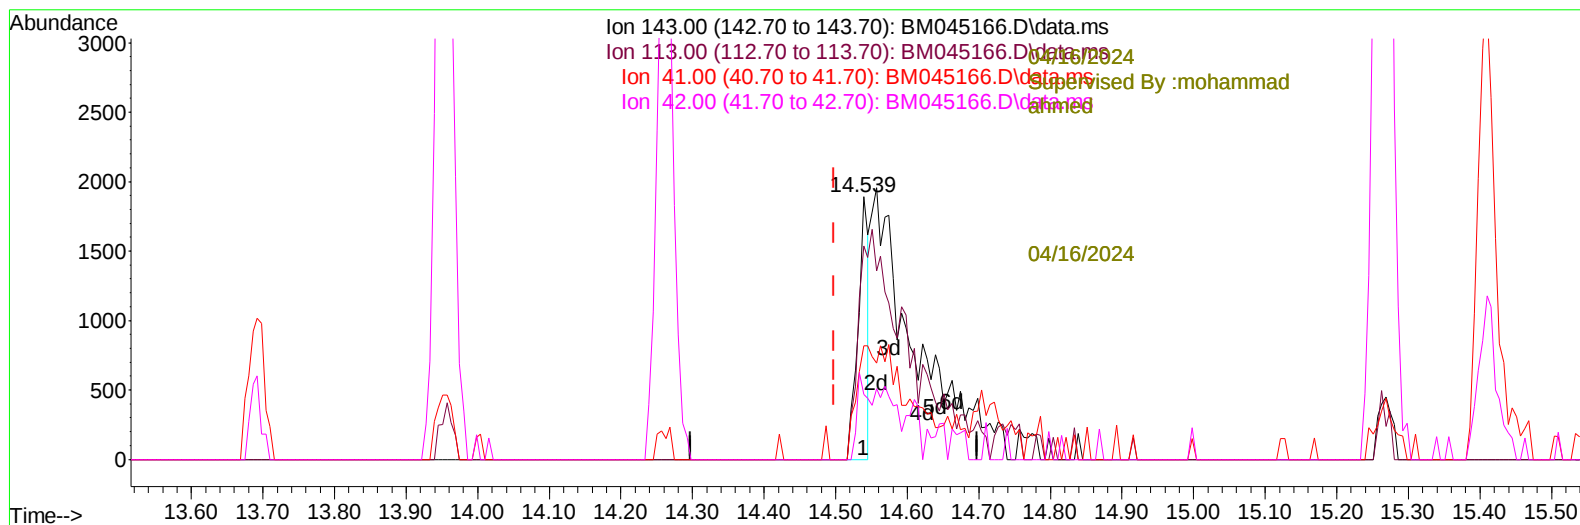

TIC: BM045166.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.539min (+ 0.041) 0.87 ng/u1

response 1968

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.80	81.30
41.00	36.50	43.32
42.00	23.30	24.62




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045166.D
Acq On : 12 Apr 2024 11:06
Operator : MA/JU
Sample : P2014-23
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOME6

Manual IntegrationsAPPROVED

Quant Time: Apr 12 11:36:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

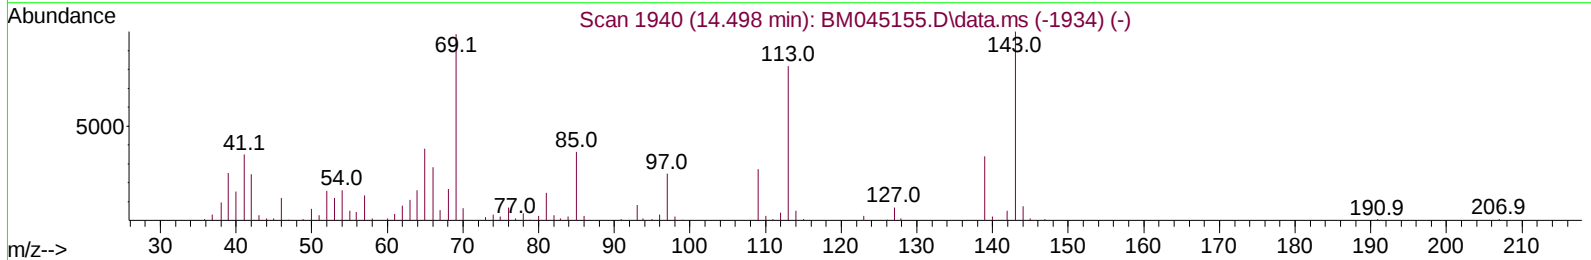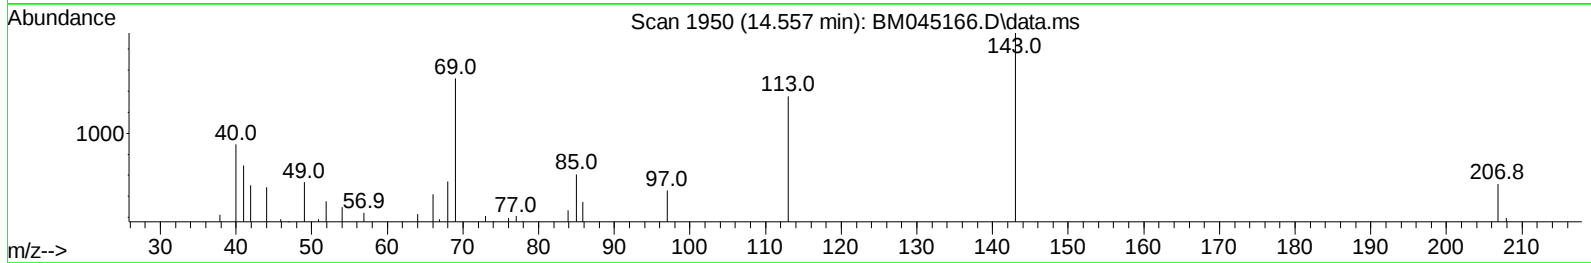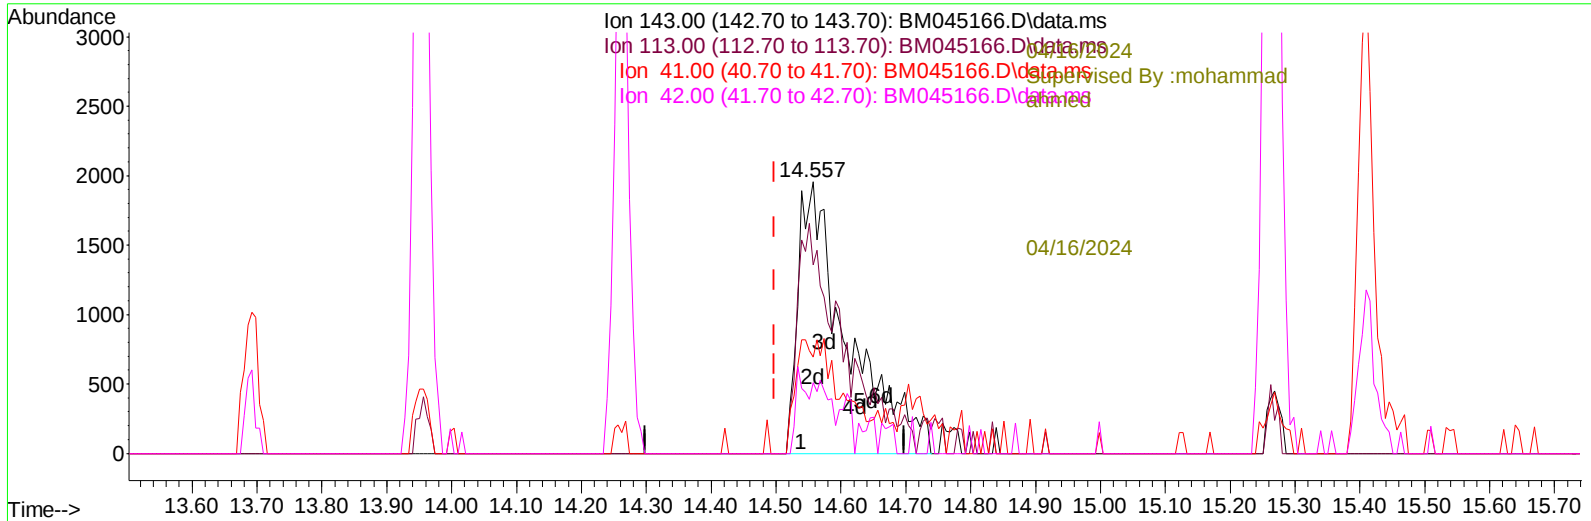

TIC: BM045166.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.557min (+ 0.059) 4.57 ng/ul m

response 10352

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.80	69.31
41.00	36.50	35.45
42.00	23.30	25.93

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045166.D
 Acq On : 12 Apr 2024 11:06
 Operator : MA/JU
 Sample : P2014-23
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0ME6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/16/2024
 Supervised By :mohammad ahmed 04/16/2024

Quant Time: Apr 12 11:37:15 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 18:54:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----04/16/2024						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	55894	20.000	ng/ul	0.00
20) Naphthalene-d8	10.386	136	237903	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.263	164	155943	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.021	188	323857	20.000	ng/ul	0.00
79) Chrysene-d12	21.239	240	278076	20.000	ng/ul	0.00
88) Perylene-d12	23.450	264	318934	20.000	ng/ul	0.00
-----04/16/2024						
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	5609	3.747	ng/uL	0.00
4) Pyridine-d5	3.616	84	27925	6.861	ng/ul	0.01
7) Phenol-d5	6.804	99	33020	6.969	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.969	67	107154	37.956	ng/ul	0.00
11) 2-Chlorophenol-d4	7.151	132	108032	29.101	ng/ul	0.00
15) 4-Methylphenol-d8	8.328	113	65554	17.674	ng/ul	0.00
21) Nitrobenzene-d5	8.781	128	72828	39.853	ng/ul	0.00
24) 2-Nitrophenol-d4	9.492	143	75181	38.978	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.016	165	111658	31.574	ng/ul	0.00
31) 4-Chloroaniline-d4	10.551	131	168322	29.896	ng/ul	0.00
46) Dimethylphthalate-d6	13.692	166	467715	43.076	ng/ul	0.00
49) Acenaphthylene-d8	13.951	160	532005	41.475	ng/ul	0.00
54) 4-Nitrophenol-d4	14.557	143	10352m	4.568	ng/ul	0.06
60) Fluorene-d10	15.269	176	406917	42.037	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	57862	30.133	ng/ul	0.00
73) Anthracene-d10	17.121	188	654654	44.935	ng/ul	0.00
81) Pyrene-d10	19.427	212	753756	55.049	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.309	264	717979	46.147	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045166.D
Acq On : 12 Apr 2024 11:06
Operator : MA/JU
Sample : P2014-23
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME6

Manual IntegrationsAPPROVED

Quant Time: Apr 12 11:37:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

