




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045175.D
Acq On : 12 Apr 2024 17:35
Operator : MA/JU
Sample : P2006-04
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0R63

Manual IntegrationsAPPROVED

Quant Time: Apr 12 19:03:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

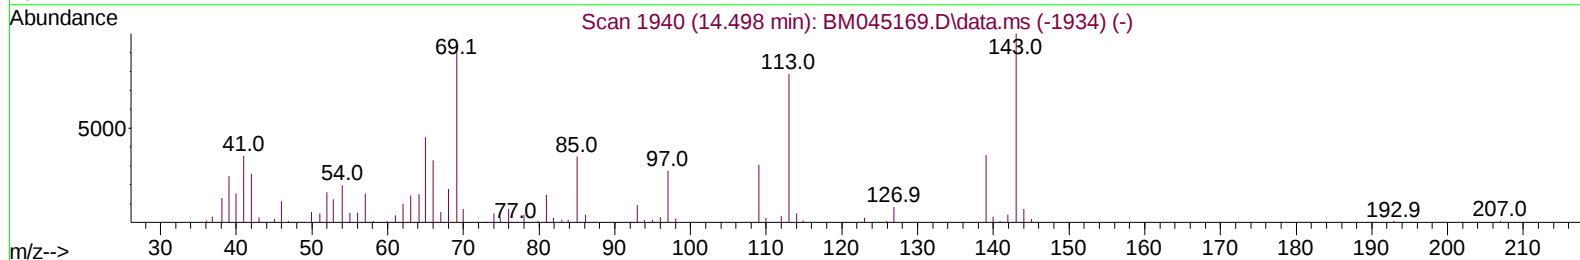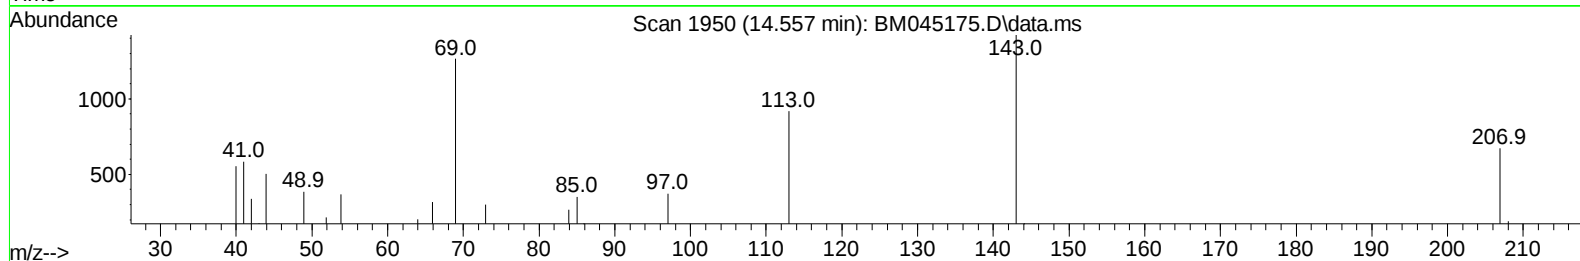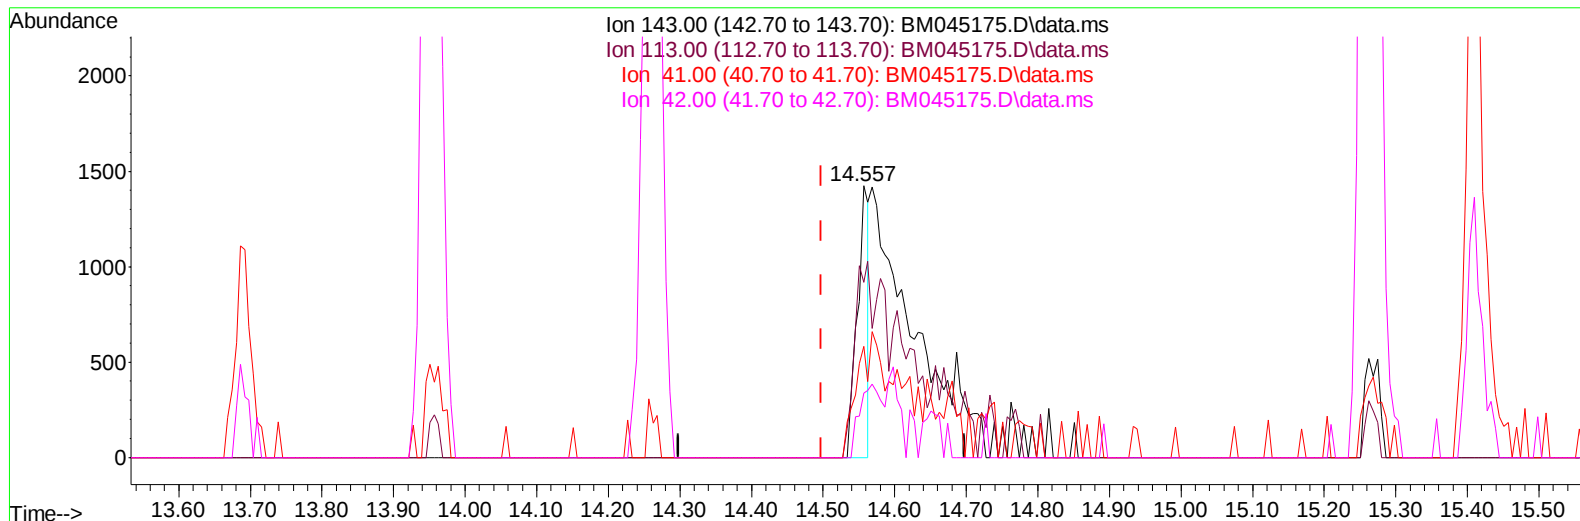

TIC: BM045175.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.557min (+ 0.059) 0.59 ng/u1

response 1620

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.80	64.44
41.00	36.50	41.04
42.00	23.30	23.82




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045175.D
Acq On : 12 Apr 2024 17:35
Operator : MA/JU
Sample : P2006-04
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0R63

Manual IntegrationsAPPROVED

Quant Time: Apr 12 19:03:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

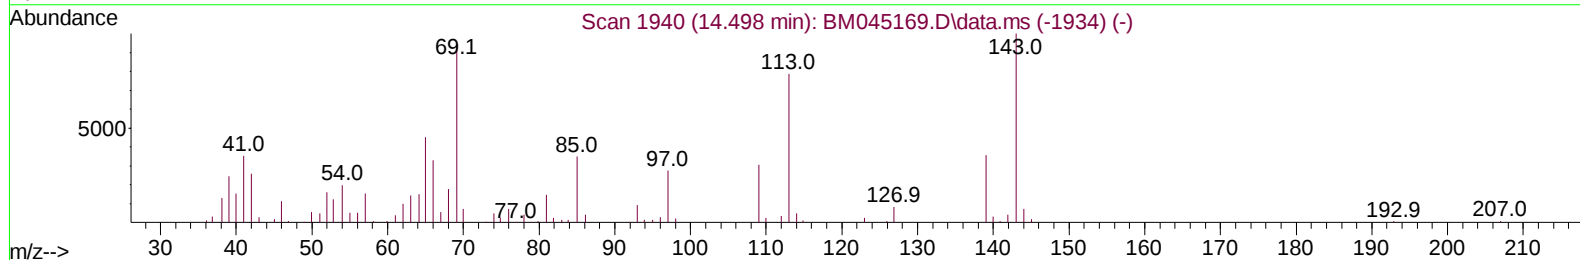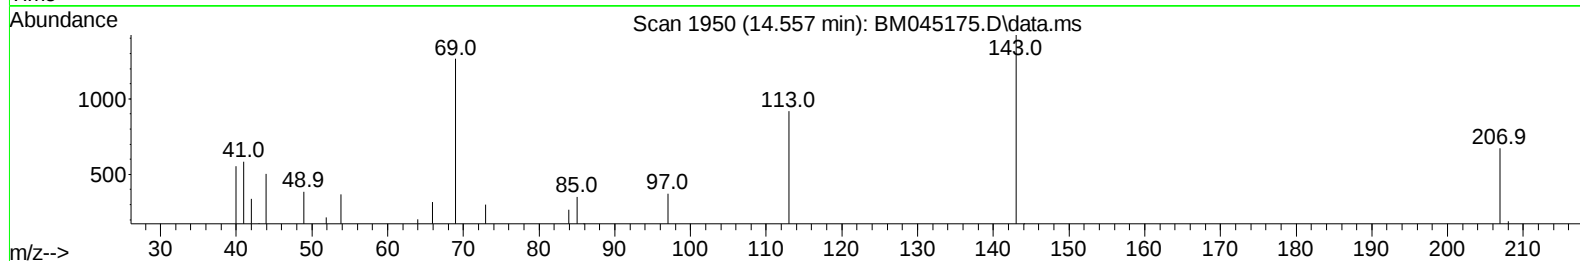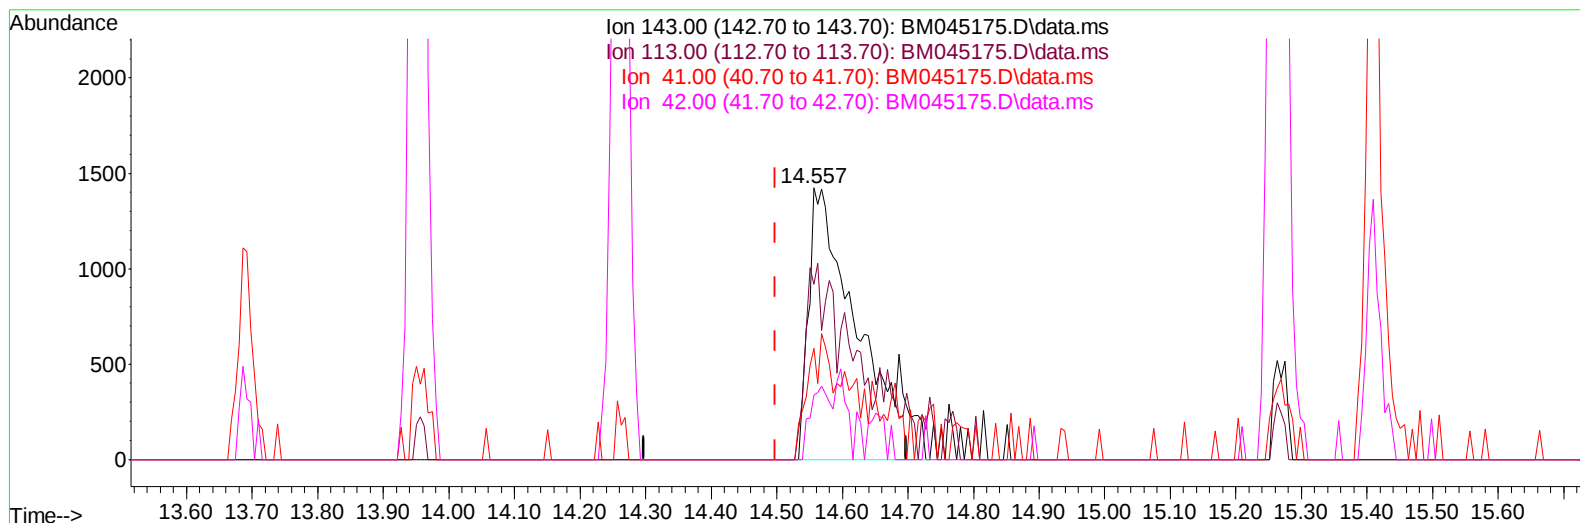

TIC: BM045175.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.557min (+ 0.059) 2.77 ng/ul m

response 7555

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.80	64.44
41.00	36.50	41.04
42.00	23.30	23.82

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045175.D
 Acq On : 12 Apr 2024 17:35
 Operator : MA/JU
 Sample : P2006-04
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MC0R63

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/16/2024
 Supervised By :mohammad ahmed 04/16/2024

Quant Time: Apr 12 19:03:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 18:54:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	72119	20.000	ng/ul	0.00
20) Naphthalene-d8	10.386	136	294250	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.263	164	187687	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.021	188	371728	20.000	ng/ul	0.00
79) Chrysene-d12	21.239	240	291546	20.000	ng/ul	0.00
88) Perylene-d12	23.450	264	305249	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	6723	3.481	ng/uL	0.00
4) Pyridine-d5	3.616	84	26554	5.056	ng/ul	0.01
7) Phenol-d5	6.804	99	25872	4.232	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.969	67	113943	31.281	ng/ul	0.00
11) 2-Chlorophenol-d4	7.151	132	104343	21.784	ng/ul	0.00
15) 4-Methylphenol-d8	8.328	113	56104	11.723	ng/ul	0.00
21) Nitrobenzene-d5	8.775	128	72653	32.144	ng/ul	0.00
24) 2-Nitrophenol-d4	9.486	143	74520	31.237	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.022	165	109970	25.142	ng/ul	0.00
31) 4-Chloroaniline-d4	10.545	131	162375	23.317	ng/ul	0.00
46) Dimethylphthalate-d6	13.692	166	490421	37.528	ng/ul	0.00
49) Acenaphthylene-d8	13.957	160	524295	33.961	ng/ul	0.00
54) 4-Nitrophenol-d4	14.557	143	7555m	2.770	ng/ul	0.06
60) Fluorene-d10	15.268	176	419354	35.994	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	59077	26.804	ng/ul	0.00
73) Anthracene-d10	17.121	188	699772	41.847	ng/ul	0.00
81) Pyrene-d10	19.427	212	778067	54.199	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.309	264	653190	43.865	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045175.D
Acq On : 12 Apr 2024 17:35
Operator : MA/JU
Sample : P2006-04
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0R63

Manual IntegrationsAPPROVED

Quant Time: Apr 12 19:03:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

