




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045180.D
Acq On : 12 Apr 2024 20:37
Operator : MA/JU
Sample : P2006-10
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0RE9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

Quant Time: Apr 12 22:37:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

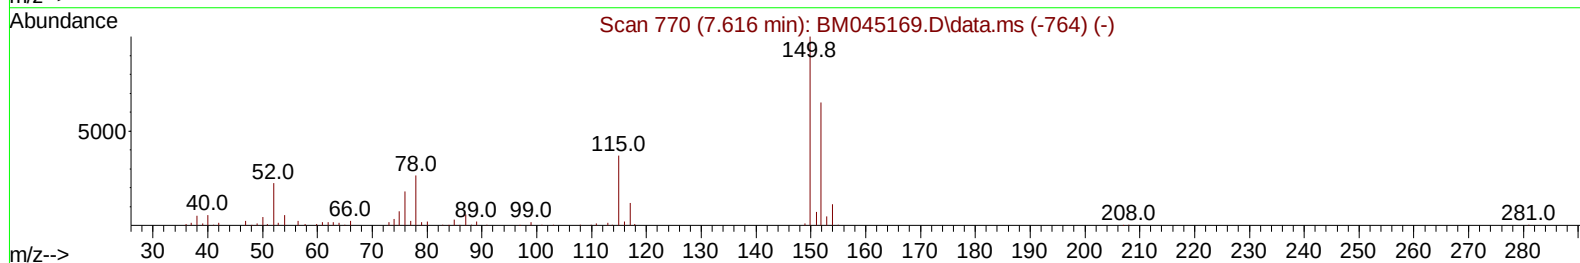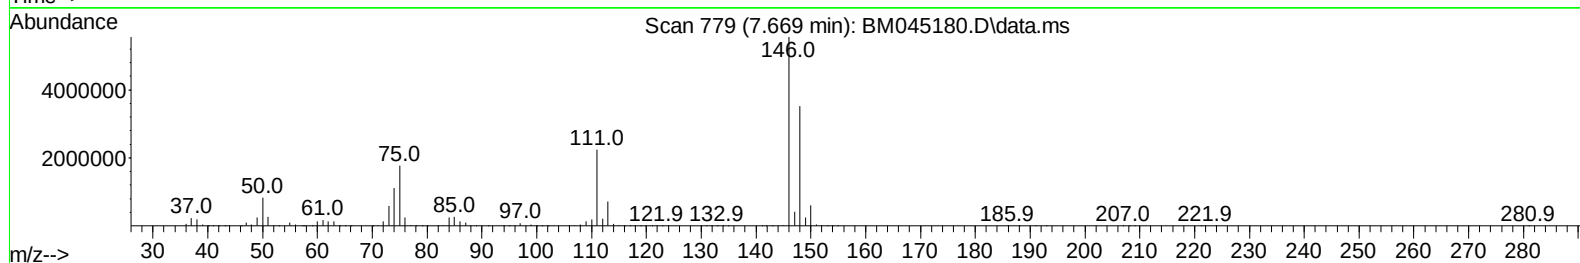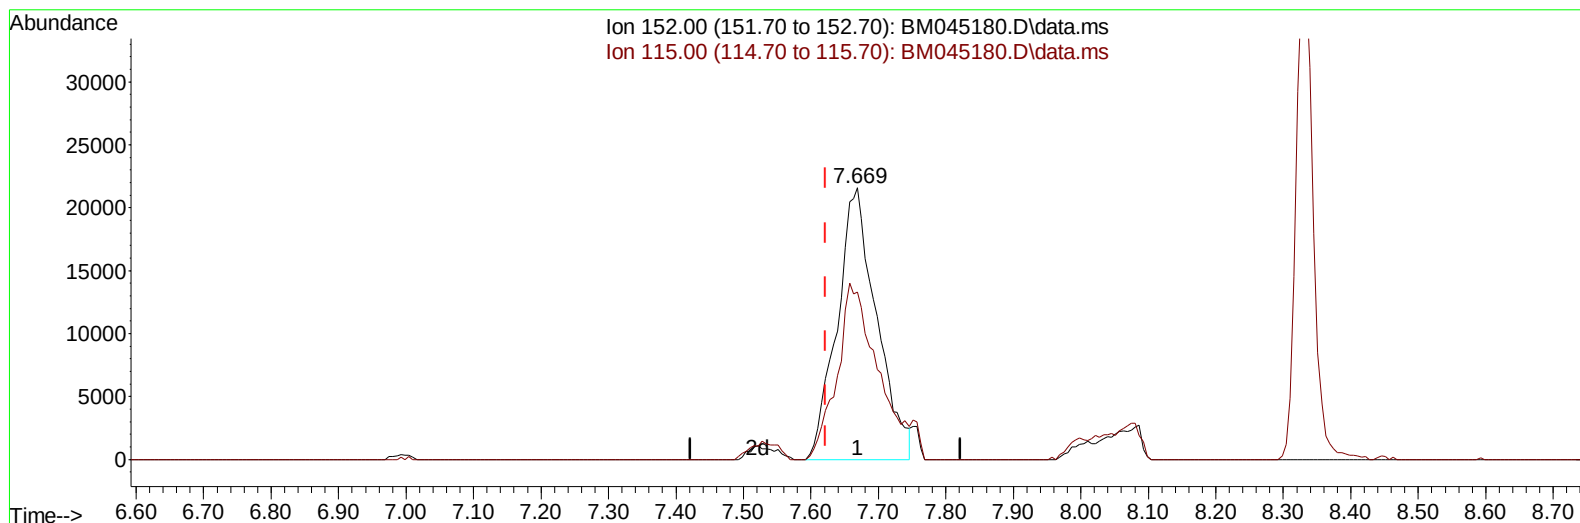

TIC: BM045180.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.669min (+ 0.047) 20.00 ng/ul

response 87308

Ion	Exp%	Act%
152.00	100.00	100.00
115.00	55.90	61.55
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045180.D
Acq On : 12 Apr 2024 20:37
Operator : MA/JU
Sample : P2006-10
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0RE9

Manual IntegrationsAPPROVED

Quant Time: Apr 12 22:37:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

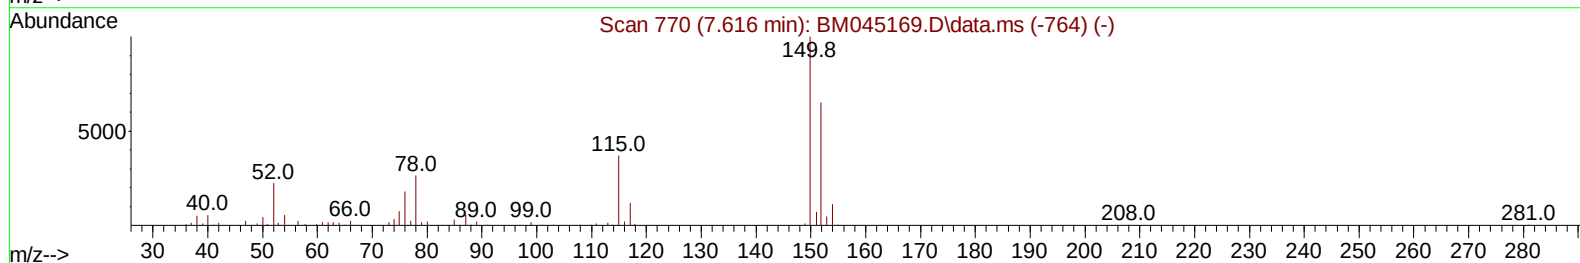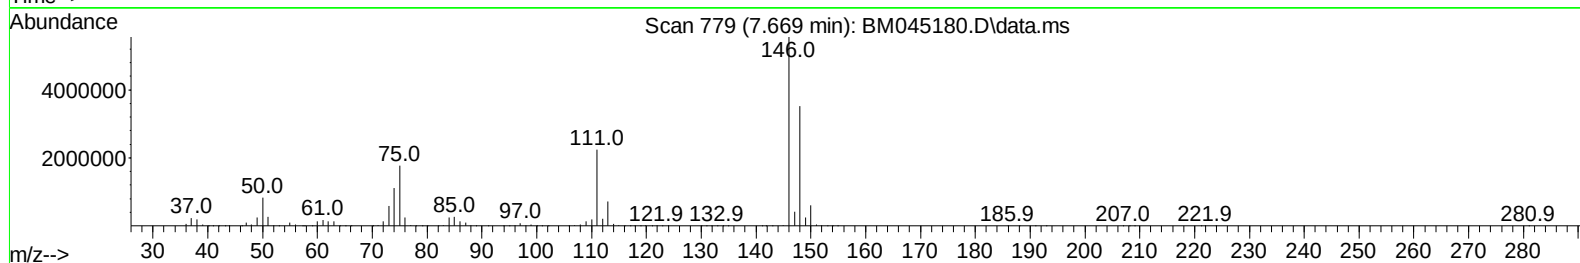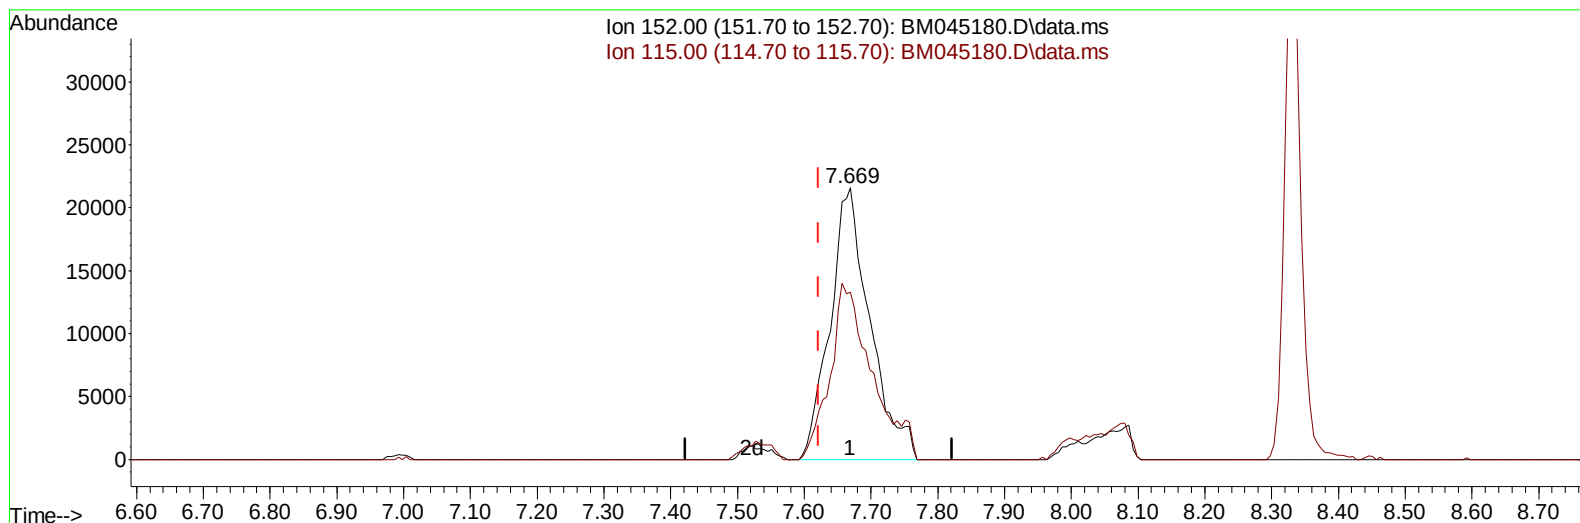

TIC: BM045180.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.669min (+ 0.047) 20.00 ng/ul m

response 89480

Ion	Exp%	Act%
152.00	100.00	100.00
115.00	55.90	61.55
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045180.D
 Acq On : 12 Apr 2024 20:37
 Operator : MA/JU
 Sample : P2006-10
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MCORE9

Manual IntegrationsAPPROVED

Quant Time: Apr 12 22:37:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 18:54:49 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
 Supervised By :mohammad ahmed 04/16/2024

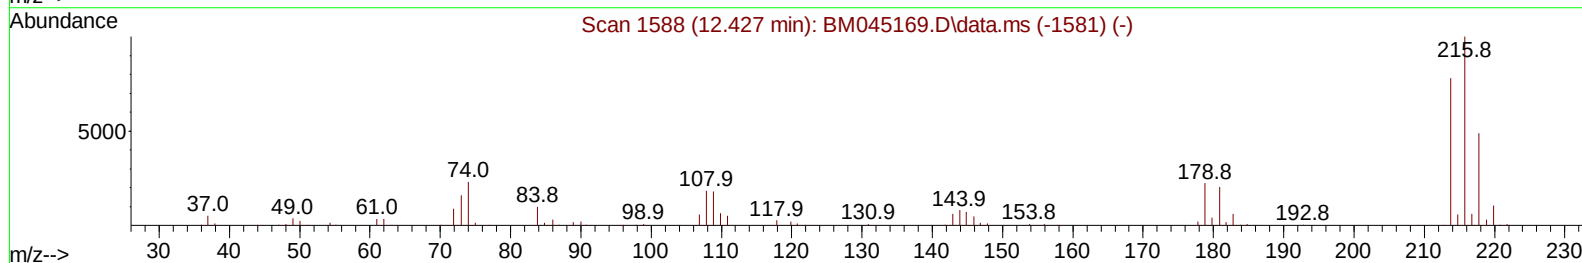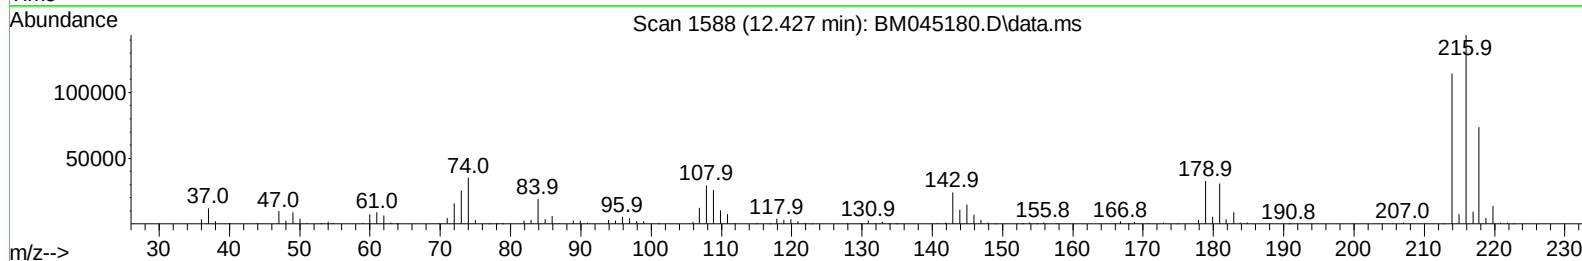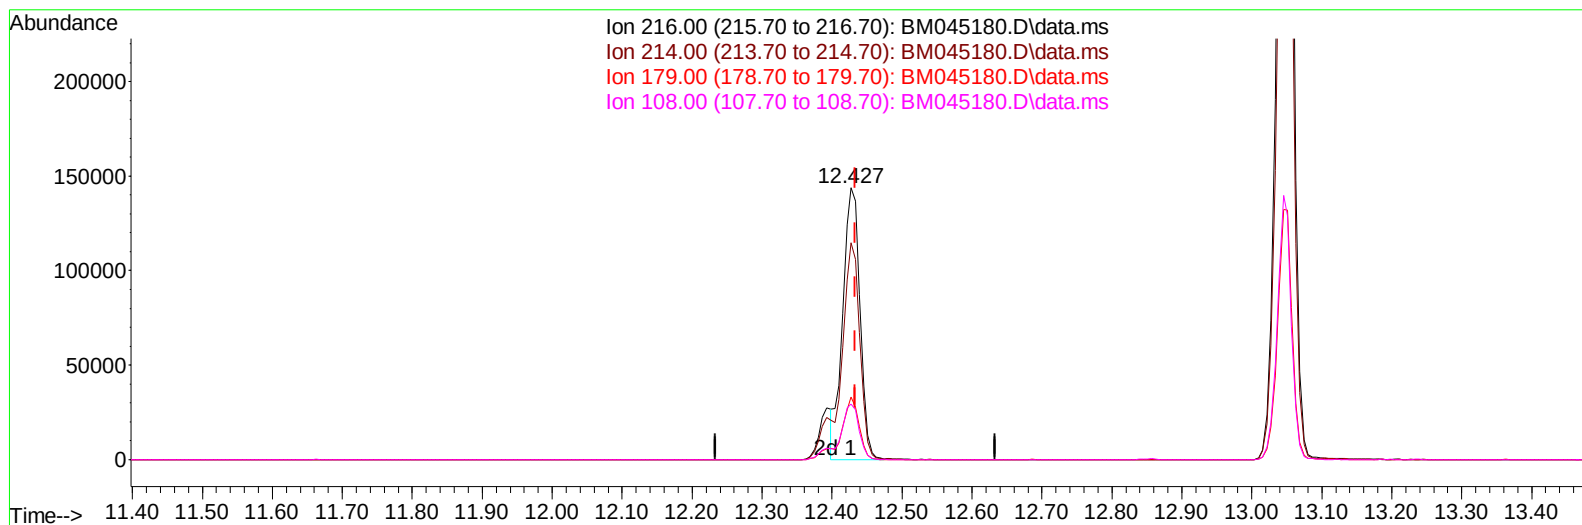

TIC: BM045180.D\data.ms

(39) 1,2,4,5-Tetrachlorobenzene

12.427min (-0.006) 50.12 ng/uI

response 244469

Ion	Exp%	Act%
216.00	100.00	100.00
214.00	79.40	79.82
179.00	20.80	22.92
108.00	18.70	20.48




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045180.D
 Acq On : 12 Apr 2024 20:37
 Operator : MA/JU
 Sample : P2006-10
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MC0RE9

Manual IntegrationsAPPROVED

Quant Time: Apr 12 22:37:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 18:54:49 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
 Supervised By :mohammad ahmed 04/16/2024

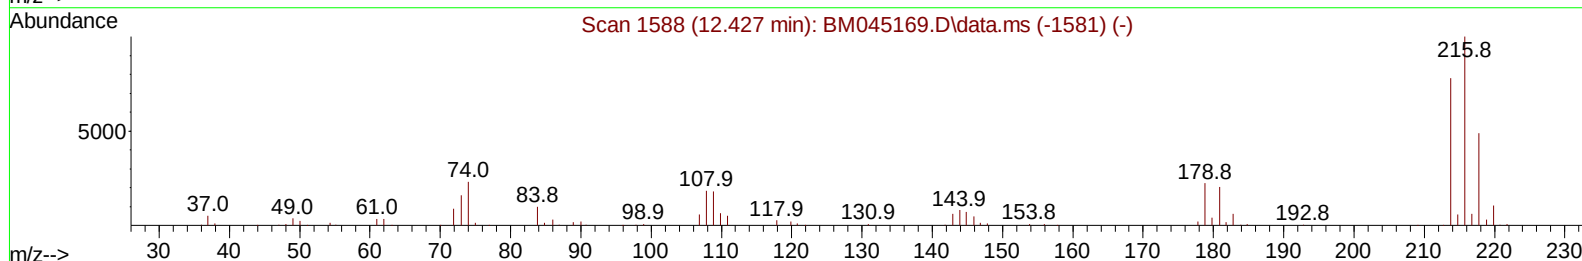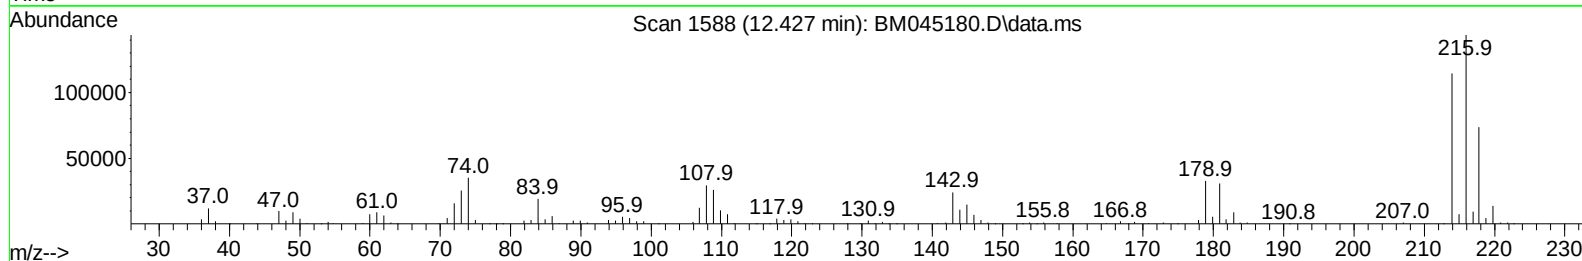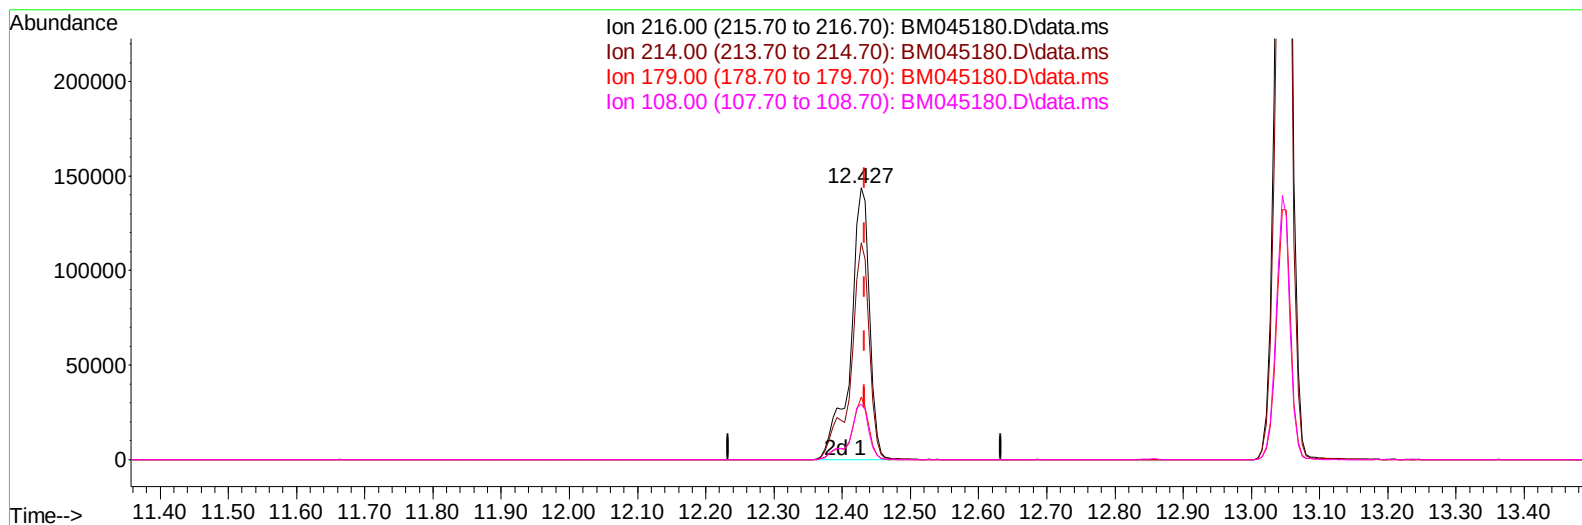

TIC: BM045180.D\data.ms

(39) 1,2,4,5-Tetrachlorobenzene

12.427min (-0.006) 57.05 ng/ul m

response 278299

Ion	Exp%	Act%
216.00	100.00	100.00
214.00	79.40	79.82
179.00	20.80	22.92
108.00	18.70	20.48




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045180.D
Acq On : 12 Apr 2024 20:37
Operator : MA/JU
Sample : P2006-10
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0RE9

Manual IntegrationsAPPROVED

Quant Time: Apr 12 22:46:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

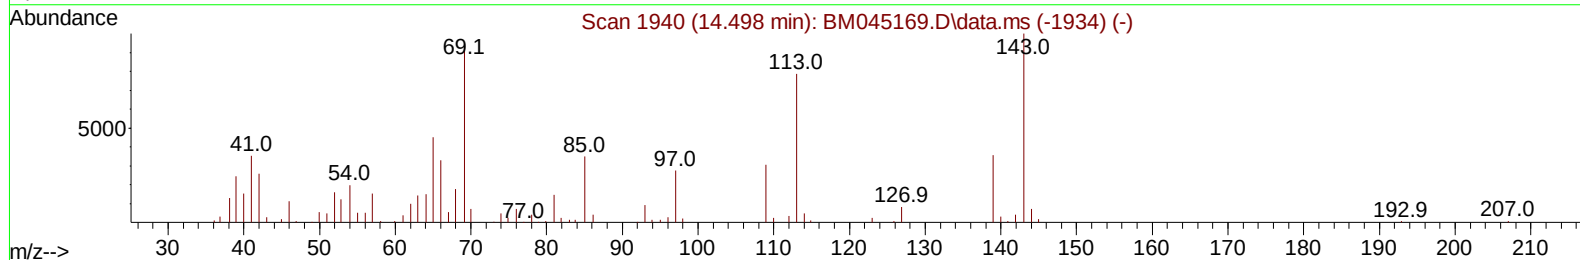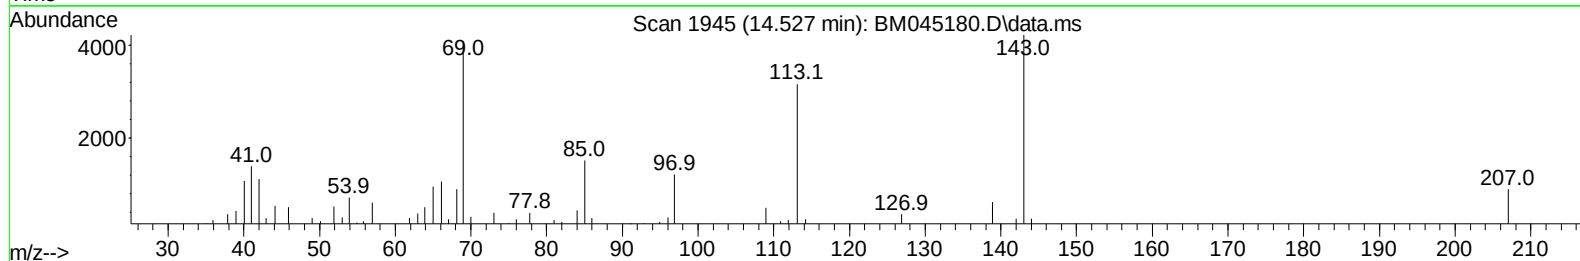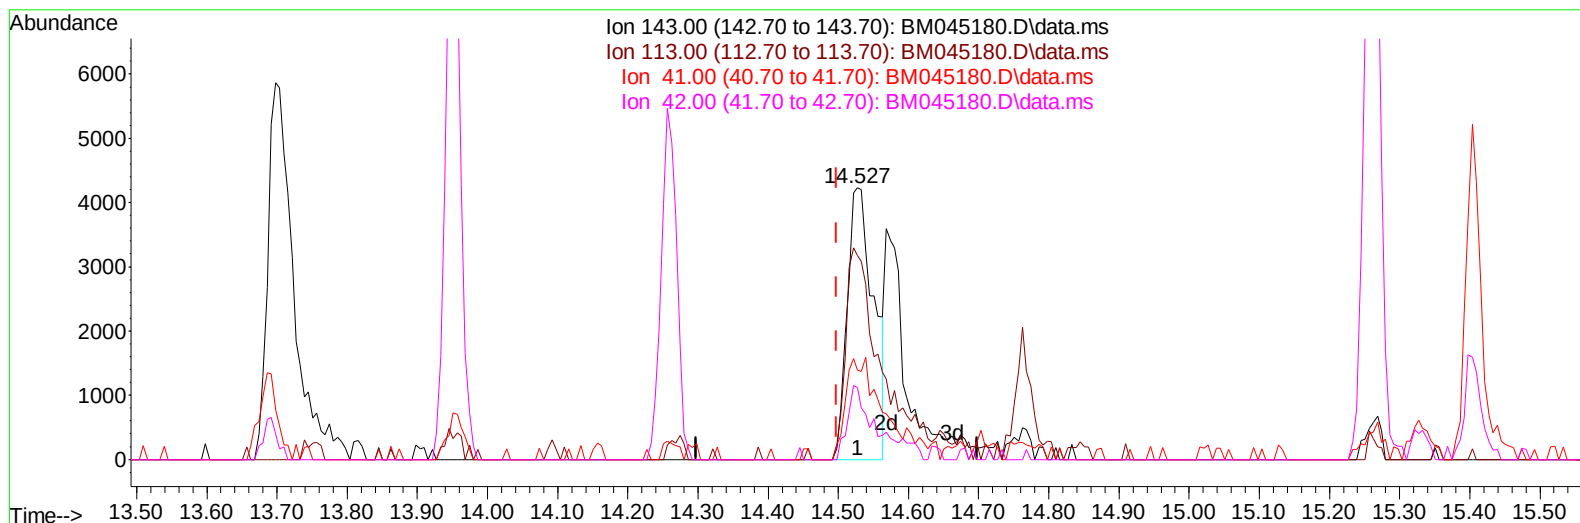

TIC: BM045180.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.527min (+ 0.029) 4.23 ng/ul

response 10968

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.80	74.99
41.00	36.50	32.93
42.00	23.30	26.43




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045180.D
Acq On : 12 Apr 2024 20:37
Operator : MA/JU
Sample : P2006-10
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0RE9

Manual IntegrationsAPPROVED

Quant Time: Apr 12 22:46:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

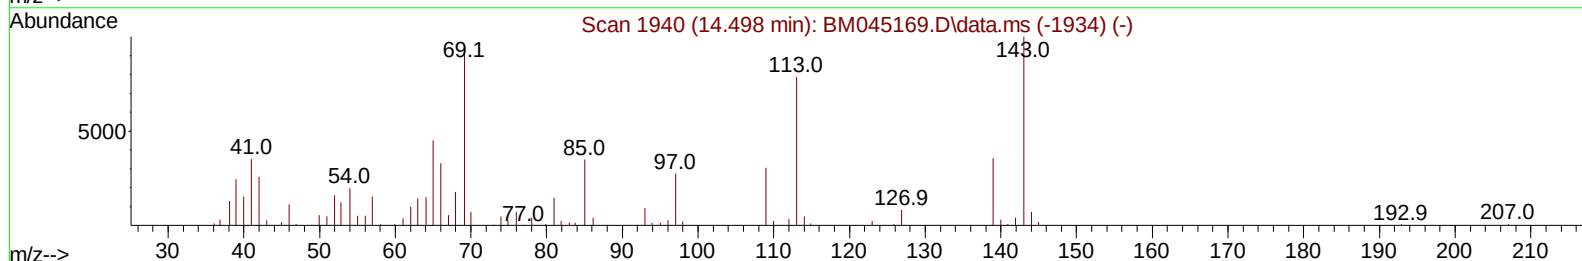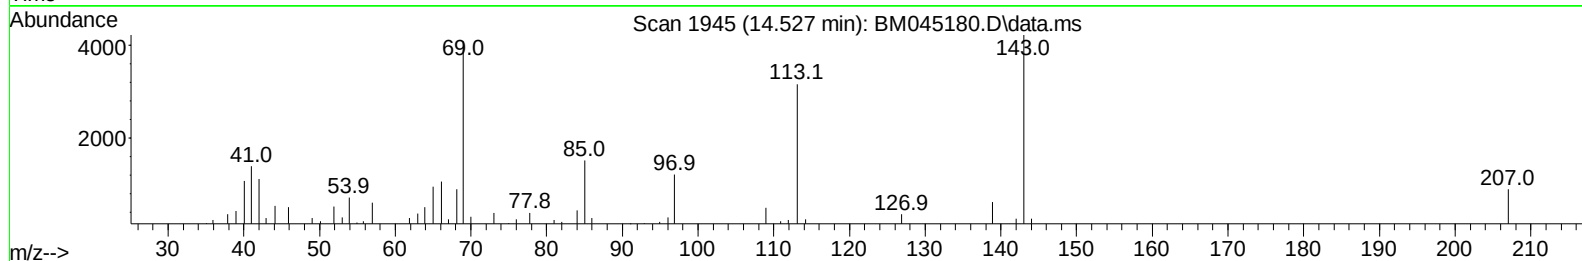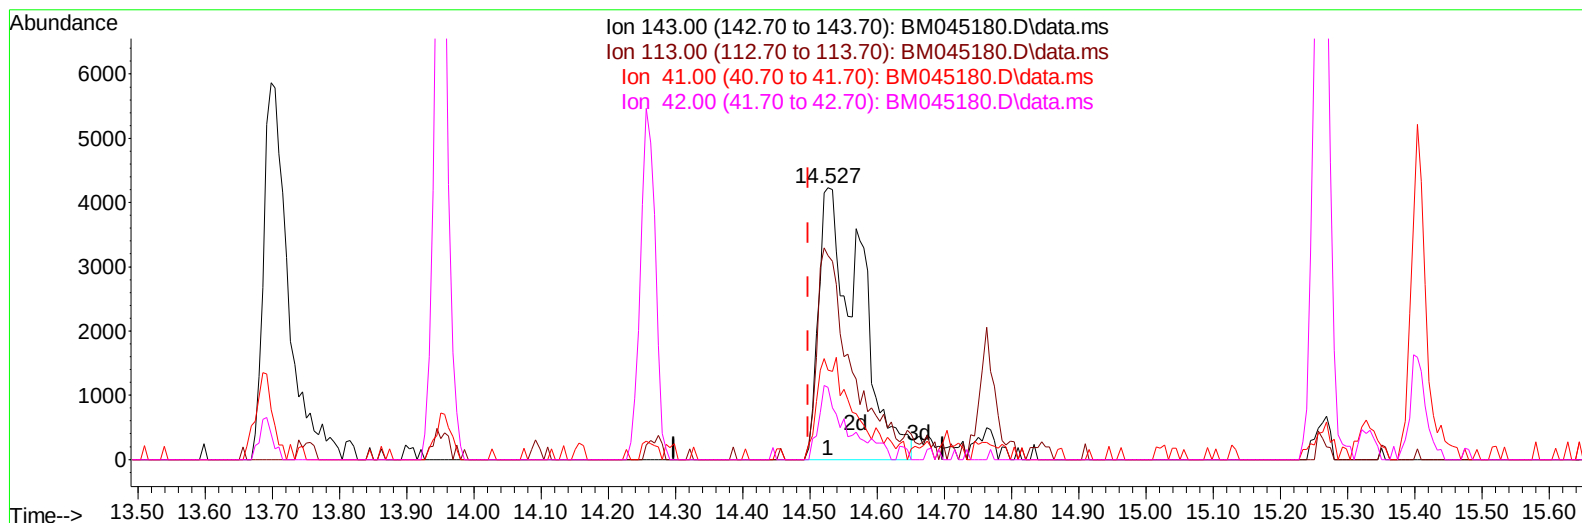

TIC: BM045180.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.527min (+ 0.029) 6.93 ng/ul m

response 17971

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.80	74.99
41.00	36.50	32.93
42.00	23.30	26.43

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045180.D
 Acq On : 12 Apr 2024 20:37
 Operator : MA/JU
 Sample : P2006-10
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MCORE9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/16/2024
 Supervised By :mohammad ahmed 04/16/2024

Quant Time: Apr 12 22:46:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 11 18:54:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.669	152	89480m	20.000	ng/ul	0.05
20) Naphthalene-d8	10.416	136	277144	20.000	ng/ul	# 0.02
38) Acenaphthene-d10	14.263	164	178363	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.021	188	369488	20.000	ng/ul	0.00
79) Chrysene-d12	21.233	240	346755	20.000	ng/ul	0.00
88) Perylene-d12	23.444	264	375353	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.210	96	7663	3.198	ng/uL	0.00
4) Pyridine-d5	3.616	84	49227	7.554	ng/ul	0.01
7) Phenol-d5	6.804	99	38695	5.101	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.992	67	139939	30.964	ng/ul	0.02
11) 2-Chlorophenol-d4	7.163	132	138738	23.345	ng/ul	0.01
15) 4-Methylphenol-d8	8.334	113	78138	13.160	ng/ul	0.00
21) Nitrobenzene-d5	8.786	128	92645	43.519	ng/ul	0.00
24) 2-Nitrophenol-d4	9.492	143	101215	45.046	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.028	165	151731	36.831	ng/ul	0.00
31) 4-Chloroaniline-d4	10.557	131	129897	19.804	ng/ul	0.00
46) Dimethylphthalate-d6	13.692	166	563991	45.414	ng/ul	0.00
49) Acenaphthylene-d8	13.951	160	659837	44.974	ng/ul	0.00
54) 4-Nitrophenol-d4	14.527	143	17971m	6.934	ng/ul	0.03
60) Fluorene-d10	15.262	176	482109	43.544	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.404	200	83302	38.024	ng/ul	0.00
73) Anthracene-d10	17.121	188	762061	45.848	ng/ul	0.00
81) Pyrene-d10	19.427	212	895711	52.460	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.303	264	871040	47.570	ng/ul	0.00
Target Compounds						
					Qvalue	
22) Nitrobenzene	8.833	77	1232731	236.022	ng/ul	97
25) 2-Nitrophenol	9.522	139	15014	6.020	ng/ul#	79
39) 1,2,4,5-Tetrachloroben...	12.427	216	278299m	57.053	ng/ul	
75) 1,2,3,4-Tetrachloroben...	13.051	216	848523	182.205	ng/uL	99
76) Pentachlorobenzene	14.574	250	32277	6.514	ng/uL	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045180.D
Acq On : 12 Apr 2024 20:37
Operator : MA/JU
Sample : P2006-10
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0RE9

Manual IntegrationsAPPROVED

Quant Time: Apr 12 22:46:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/16/2024

