

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045140.D
 Acq On : 11 Apr 2024 18:44
 Operator : MA/JU
 Sample : PB160160BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK160

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045140.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	17	20	26	rBV2	14863	20073	1.23%	0.121%
2	3.605	85	88	106	rBV	174670	317976	19.52%	1.923%
3	3.899	135	138	143	rVB5	4013	4995	0.31%	0.030%
4	4.057	161	165	166	rBV2	1540	1944	0.12%	0.012%
5	5.657	435	437	440	rVB4	1548	1649	0.10%	0.010%
6	6.640	599	604	606	rBV4	1148	1889	0.12%	0.011%
7	6.798	625	631	644	rBV	212534	394100	24.19%	2.383%
8	6.975	654	661	673	rVV	204147	329831	20.25%	1.994%
9	7.151	684	691	703	rVV	241982	417555	25.63%	2.525%
10	7.234	703	705	709	rVB4	1561	1693	0.10%	0.010%
11	7.616	763	770	781	rVB	198443	330729	20.30%	2.000%
12	8.057	840	845	852	rVB5	1098	2768	0.17%	0.017%
13	8.328	885	891	905	rVV	291825	500824	30.75%	3.028%
14	8.781	960	968	979	rBV	239942	407346	25.01%	2.463%
15	9.492	1083	1089	1098	rBV	205037	347689	21.35%	2.102%
16	9.886	1152	1156	1157	rVB4	1489	1715	0.11%	0.010%
17	10.022	1173	1179	1202	rBV	254480	496003	30.45%	2.999%
18	10.392	1234	1242	1249	rBV	281230	476247	29.24%	2.879%
19	10.551	1262	1269	1294	rBV	237713	542070	33.28%	3.277%
20	12.016	1513	1518	1519	rBV3	2996	3698	0.23%	0.022%
21	12.028	1519	1520	1525	rVB4	3431	2710	0.17%	0.016%
22	13.163	1710	1713	1718	rBV4	2486	3122	0.19%	0.019%
23	13.569	1779	1782	1786	rBV4	1030	1685	0.10%	0.010%
24	13.692	1797	1803	1818	rBV	629515	897786	55.12%	5.428%
25	13.957	1841	1848	1858	rBV	695208	1018836	62.55%	6.160%
26	14.263	1894	1900	1912	rVB	462084	696142	42.74%	4.209%
27	14.510	1936	1942	1958	rBV	128211	356905	21.91%	2.158%
28	14.863	1998	2002	2006	rBV3	1547	3096	0.19%	0.019%
29	15.268	2063	2071	2081	rBV	896271	1293101	79.39%	7.818%
30	15.410	2089	2095	2107	rBV	245245	375042	23.02%	2.268%
31	15.516	2111	2113	2118	rVB5	3389	3697	0.23%	0.022%
32	15.974	2186	2191	2192	rBV2	1075	1720	0.11%	0.010%
33	16.057	2202	2205	2208	rVB2	1786	2477	0.15%	0.015%
34	16.380	2256	2260	2265	rVB3	1310	2702	0.17%	0.016%
35	16.651	2303	2306	2309	rVB4	1289	1728	0.11%	0.010%
36	17.027	2363	2370	2379	rBV	591921	845839	51.93%	5.114%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045140.D
 Acq On : 11 Apr 2024 18:44
 Operator : MA/JU
 Sample : PB160160BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK160

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	17.127	2380	2387	2399	rVV	931787	1412995	86.75%	8.543%
38	17.457	2441	2443	2447	rBV5	1487	2049	0.13%	0.012%
39	17.833	2505	2507	2512	rVB4	1312	2013	0.12%	0.012%
40	17.898	2517	2518	2521	rBV2	1456	1632	0.10%	0.010%
41	17.939	2521	2525	2532	rBV6	14321	25624	1.57%	0.155%
42	18.015	2537	2538	2541	rVV2	2180	2013	0.12%	0.012%
43	18.057	2543	2545	2548	rVB4	1722	1839	0.11%	0.011%
44	18.268	2578	2581	2585	rBV5	2448	3650	0.22%	0.022%
45	18.998	2700	2705	2710	rVB3	8678	12438	0.76%	0.075%
46	19.068	2713	2717	2721	rBV2	7746	10447	0.64%	0.063%
47	19.239	2740	2746	2750	rBV9	11013	17914	1.10%	0.108%
48	19.433	2772	2779	2790	rBV	1163347	1628879	100.00%	9.849%
49	19.680	2816	2821	2824	rBV6	2754	6413	0.39%	0.039%
50	19.962	2867	2869	2871	rBV3	2466	2272	0.14%	0.014%
51	21.233	3080	3085	3094	rBV	608258	861862	52.91%	5.211%
52	23.309	3431	3438	3445	rBV2	849635	1542047	94.67%	9.324%
53	23.450	3456	3462	3478	rVB	454472	897853	55.12%	5.429%




Sum of corrected areas: 16539322

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045140.D
Acq On : 11 Apr 2024 18:44
Operator : MA/JU
Sample : PB160160BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK160

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

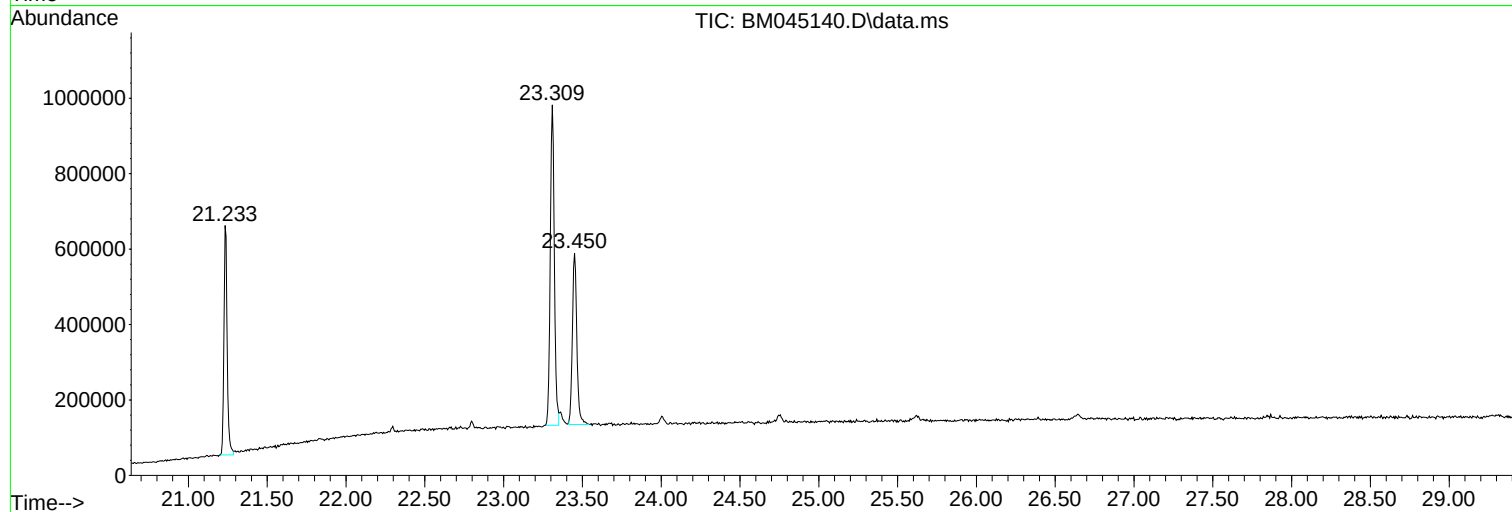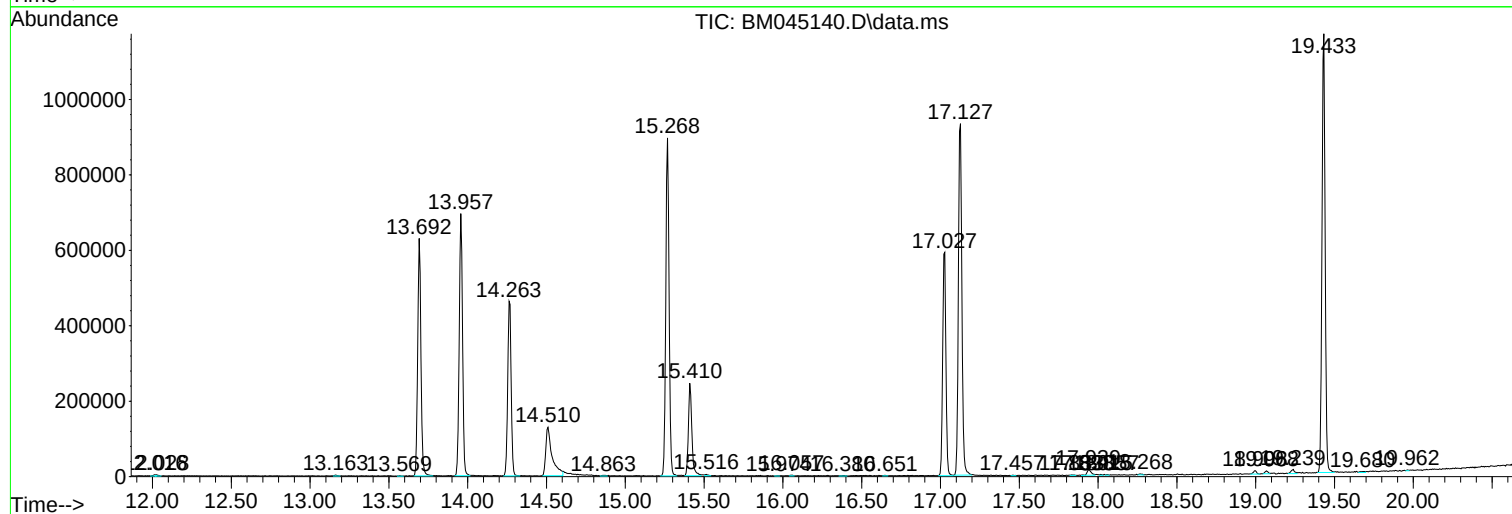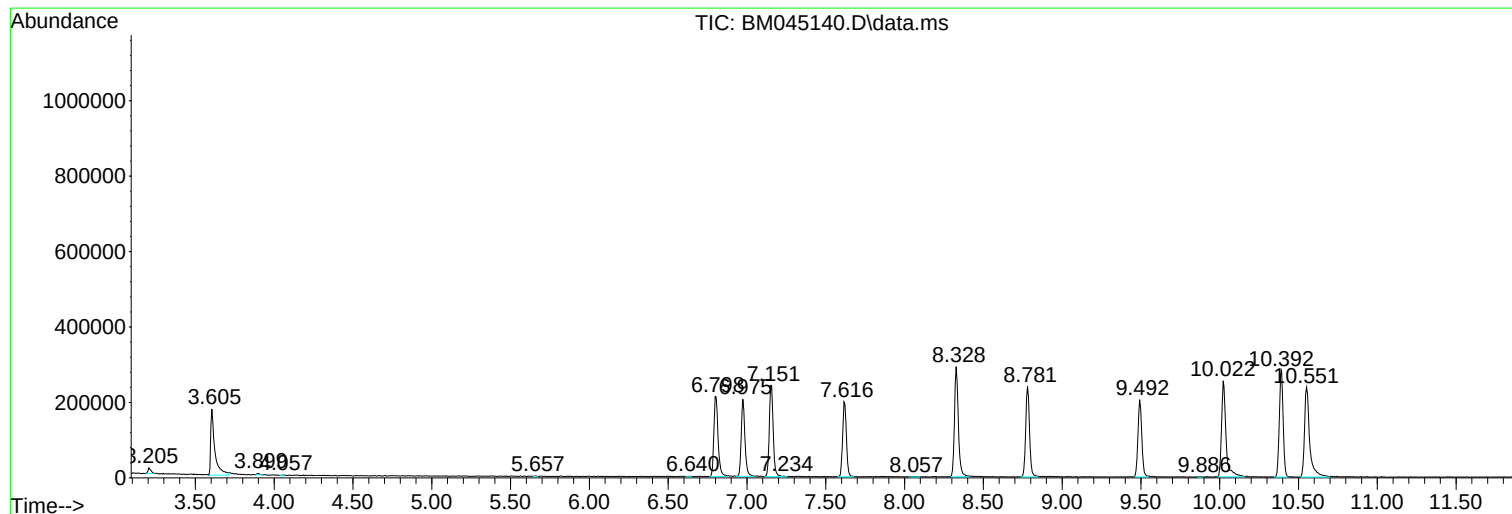

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045140.D
Acq On : 11 Apr 2024 18:44
Operator : MA/JU
Sample : PB160160BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK160

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045140.D
Acq On : 11 Apr 2024 18:44
Operator : MA/JU
Sample : PB160160BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK160

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc