

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045142.D
 Acq On : 11 Apr 2024 19:56
 Operator : MA/JU
 Sample : PB160097TB 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLEB097

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045142.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.204	17	20	28	rVB	19781	27544	1.30%	0.126%
2	3.604	85	88	115	rBV	241344	442274	20.84%	2.026%
3	3.893	135	137	141	rVB3	3236	3483	0.16%	0.016%
4	6.798	625	631	644	rBV	304847	538751	25.39%	2.468%
5	6.975	654	661	674	rBV	283230	445607	21.00%	2.042%
6	7.151	685	691	702	rBV	335880	556939	26.24%	2.552%
7	7.616	764	770	780	rBV	255985	418368	19.71%	1.917%
8	8.328	884	891	900	rBV	400489	682853	32.18%	3.129%
9	8.781	960	968	979	rBV	332398	556319	26.22%	2.549%
10	8.904	988	989	995	rVB5	1635	2301	0.11%	0.011%
11	9.492	1082	1089	1098	rBV	286085	480261	22.63%	2.200%
12	10.022	1171	1179	1197	rBV	368066	695891	32.79%	3.188%
13	10.392	1234	1242	1252	rVB	361486	609507	28.72%	2.793%
14	10.551	1261	1269	1293	rBV	358974	778456	36.68%	3.567%
15	12.022	1514	1519	1525	rBV4	4143	7079	0.33%	0.032%
16	13.157	1707	1712	1718	rVB4	5543	9534	0.45%	0.044%
17	13.692	1795	1803	1817	rBV	862362	1230978	58.01%	5.640%
18	13.957	1841	1848	1859	rBV2	975110	1413916	66.63%	6.478%
19	14.263	1894	1900	1908	rBV	614724	906244	42.71%	4.152%
20	14.498	1932	1940	1954	rBV	206041	496999	23.42%	2.277%
21	15.268	2064	2071	2085	rBV	1234340	1766637	83.25%	8.094%
22	15.410	2089	2095	2107	rVV	372253	542355	25.56%	2.485%
23	15.510	2109	2112	2119	rVB5	5119	8933	0.42%	0.041%
24	16.057	2200	2205	2209	rVB5	3344	4910	0.23%	0.022%
25	17.027	2363	2370	2380	rBV	742904	1069013	50.38%	4.898%
26	17.127	2380	2387	2402	rBV2	1268482	1922343	90.59%	8.808%
27	17.945	2523	2526	2533	rVV4	10292	17476	0.82%	0.080%
28	17.998	2533	2535	2540	rVB5	1536	2180	0.10%	0.010%
29	18.280	2576	2583	2585	rBV5	1689	2406	0.11%	0.011%
30	18.762	2663	2665	2670	rVV5	1516	2254	0.11%	0.010%
31	18.992	2701	2704	2709	rBV3	12575	17208	0.81%	0.079%
32	19.068	2714	2717	2723	rVV	9830	13361	0.63%	0.061%
33	19.239	2741	2746	2751	rBV5	6246	11442	0.54%	0.052%
34	19.433	2772	2779	2791	rBV	1557641	2122084	100.00%	9.723%
35	21.239	3080	3086	3097	rBV	715036	1028152	48.45%	4.711%
36	23.309	3431	3438	3453	rBV	1035812	1965343	92.61%	9.005%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045142.D
Acq On : 11 Apr 2024 19:56
Operator : MA/JU
Sample : PB160097TB 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLEB097

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

37	23.450	3456	3462	3474	rVB	535058	1026171	48.36%	4.702%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 21825572

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045142.D
Acq On : 11 Apr 2024 19:56
Operator : MA/JU
Sample : PB160097TB 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLEB097

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

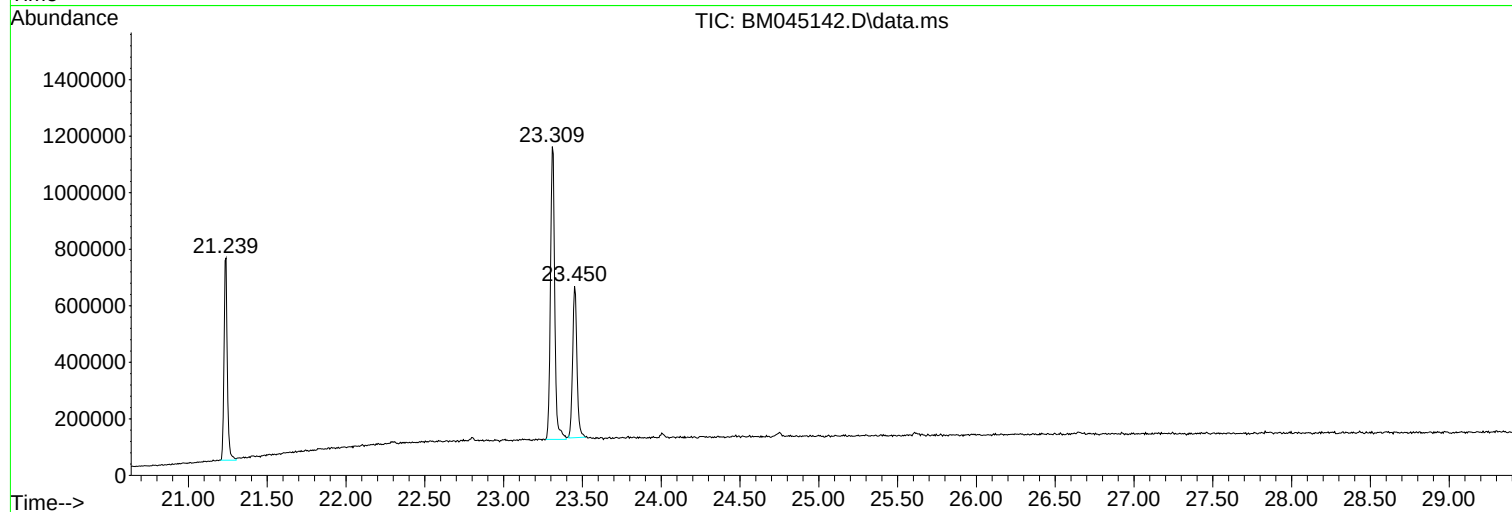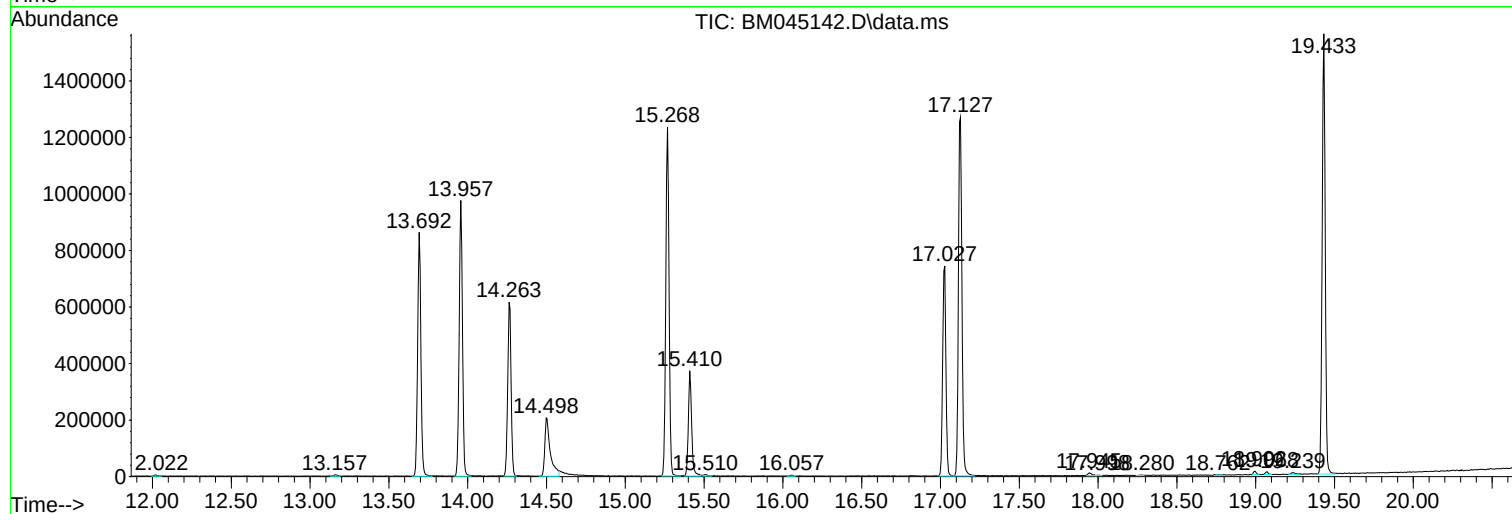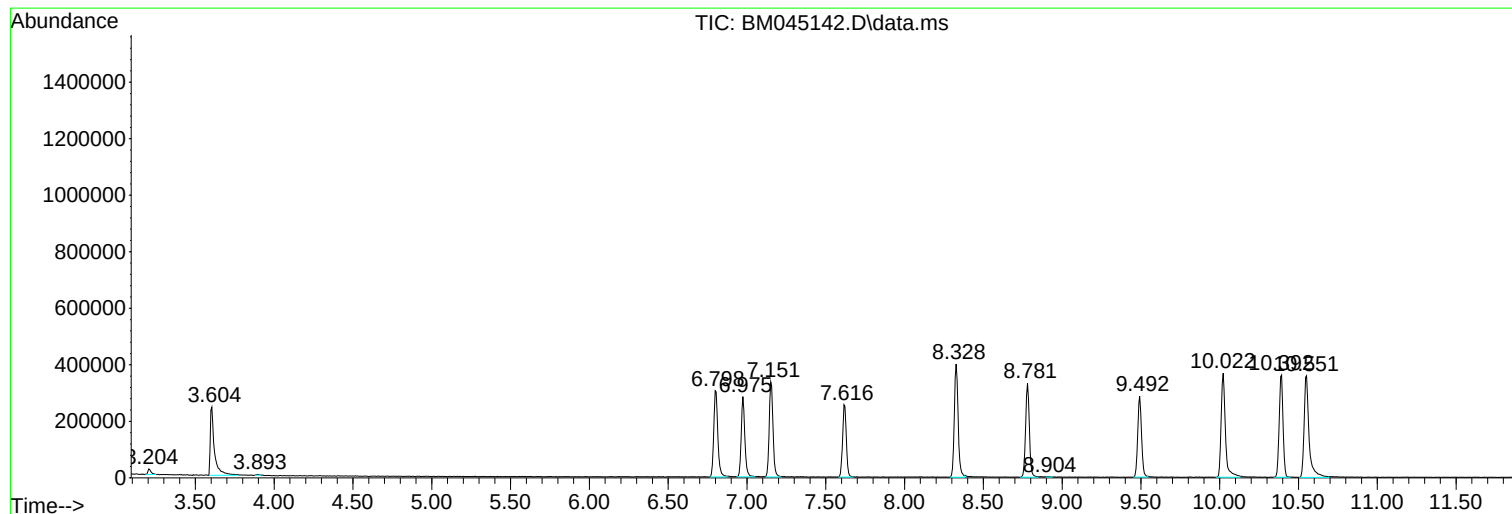

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045142.D
Acq On : 11 Apr 2024 19:56
Operator : MA/JU
Sample : PB160097TB 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLEB097

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045142.D
Acq On : 11 Apr 2024 19:56
Operator : MA/JU
Sample : PB160097TB 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLEB097

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------