

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045147.D
 Acq On : 11 Apr 2024 22:58
 Operator : MA/JU
 Sample : P2013-11
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOMB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045147.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	17	21	26	rVB	12615	17626	0.81%	0.088%
2	3.610	86	89	105	rBV	64589	128274	5.87%	0.639%
3	3.793	117	120	122	rBV3	2162	2413	0.11%	0.012%
4	3.899	135	138	142	rVB3	4021	5638	0.26%	0.028%
5	4.163	181	183	186	rVB4	2007	2274	0.10%	0.011%
6	5.016	323	328	330	rBV5	1448	2919	0.13%	0.015%
7	5.163	351	353	359	rVB7	2345	3606	0.16%	0.018%
8	5.298	370	376	378	rBV4	5661	8534	0.39%	0.043%
9	5.657	434	437	443	rVB6	3225	3834	0.18%	0.019%
10	6.722	614	618	623	rVB5	1891	3444	0.16%	0.017%
11	6.804	626	632	643	rVV	57258	120033	5.49%	0.598%
12	6.975	653	661	678	rBV	284961	470112	21.50%	2.343%
13	7.151	685	691	701	rBV	257154	433909	19.85%	2.162%
14	7.616	764	770	780	rBV	237555	388005	17.75%	1.933%
15	7.692	782	783	789	rVB5	1961	2571	0.12%	0.013%
16	8.328	884	891	905	rBV	203670	358955	16.42%	1.789%
17	8.781	961	968	982	rBV	347424	588572	26.92%	2.933%
18	9.139	1021	1029	1034	rBV5	4903	8355	0.38%	0.042%
19	9.492	1080	1089	1099	rBV	282690	483651	22.12%	2.410%
20	10.022	1172	1179	1200	rBV	354570	686325	31.39%	3.420%
21	10.251	1212	1218	1221	rBV6	2827	4968	0.23%	0.025%
22	10.386	1234	1241	1250	rBV	331817	574184	26.26%	2.861%
23	10.551	1260	1269	1286	rBV	262733	585490	26.78%	2.917%
24	12.010	1511	1517	1526	rBV5	6078	12528	0.57%	0.062%
25	12.116	1530	1535	1536	rBV3	1744	2225	0.10%	0.011%
26	13.080	1696	1699	1703	rBV5	2190	2389	0.11%	0.012%
27	13.163	1707	1713	1718	rVV3	5091	6967	0.32%	0.035%
28	13.692	1796	1803	1812	rBV	893775	1265985	57.91%	6.308%
29	13.792	1814	1820	1826	rVB3	10002	13616	0.62%	0.068%
30	13.957	1841	1848	1859	rBV	982225	1462731	66.91%	7.289%
31	14.263	1894	1900	1908	rBV	545273	807882	36.95%	4.026%
32	14.339	1908	1913	1926	rVV	39242	90637	4.15%	0.452%
33	14.421	1926	1927	1931	rVB4	3353	3069	0.14%	0.015%
34	14.533	1939	1946	1959	rBV4	25684	87000	3.98%	0.434%
35	14.639	1962	1964	1967	rVB3	2586	2348	0.11%	0.012%
36	14.704	1973	1975	1978	rBV3	1710	2340	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045147.D
Acq On : 11 Apr 2024 22:58
Operator : MA/JU
Sample : P2013-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOMB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

37	15.268	2064	2071	2081	rBV	1268544	1866743	85.39%	9.302%
38	15.410	2089	2095	2107	rBV	395557	578428	26.46%	2.882%
39	15.504	2108	2111	2119	rVB7	5565	10581	0.48%	0.053%
40	15.992	2191	2194	2197	rBV4	2046	3319	0.15%	0.017%
41	16.051	2202	2204	2208	rBV3	3919	4722	0.22%	0.024%
42	16.962	2355	2359	2363	rVV4	4631	5494	0.25%	0.027%
43	17.021	2363	2369	2377	rBV	616515	906558	41.47%	4.517%
44	17.121	2380	2386	2399	rVV	1357397	2025202	92.63%	10.091%
45	17.204	2399	2400	2404	rVB4	2742	2751	0.13%	0.014%
46	17.427	2433	2438	2445	rBV7	4238	8864	0.41%	0.044%
47	17.933	2517	2524	2533	rBV	44483	70010	3.20%	0.349%
48	18.368	2594	2598	2603	rVB4	6649	8216	0.38%	0.041%
49	18.809	2668	2673	2677	rBV7	6244	9316	0.43%	0.046%
50	18.880	2681	2685	2687	rBV4	2468	3335	0.15%	0.017%
51	18.992	2700	2704	2709	rVB3	16601	22180	1.01%	0.111%
52	19.033	2709	2711	2713	rBV2	2094	2427	0.11%	0.012%
53	19.062	2713	2716	2721	rVV	11991	16688	0.76%	0.083%
54	19.109	2722	2724	2728	rVB4	2981	3233	0.15%	0.016%
55	19.227	2740	2744	2749	rBV4	23763	35791	1.64%	0.178%
56	19.433	2772	2779	2788	rBV	1557134	2186253	100.00%	10.894%
57	19.709	2822	2826	2827	rBV3	2795	3549	0.16%	0.018%
58	20.962	3036	3039	3044	rBV5	21010	29715	1.36%	0.148%
59	21.233	3080	3085	3094	rBV	604775	802301	36.70%	3.998%
60	23.309	3431	3438	3452	rBV2	1047360	1984406	90.77%	9.888%
61	23.450	3455	3462	3471	rBV	422531	835030	38.19%	4.161%




Sum of corrected areas: 20068521

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045147.D
Acq On : 11 Apr 2024 22:58
Operator : MA/JU
Sample : P2013-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOMB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

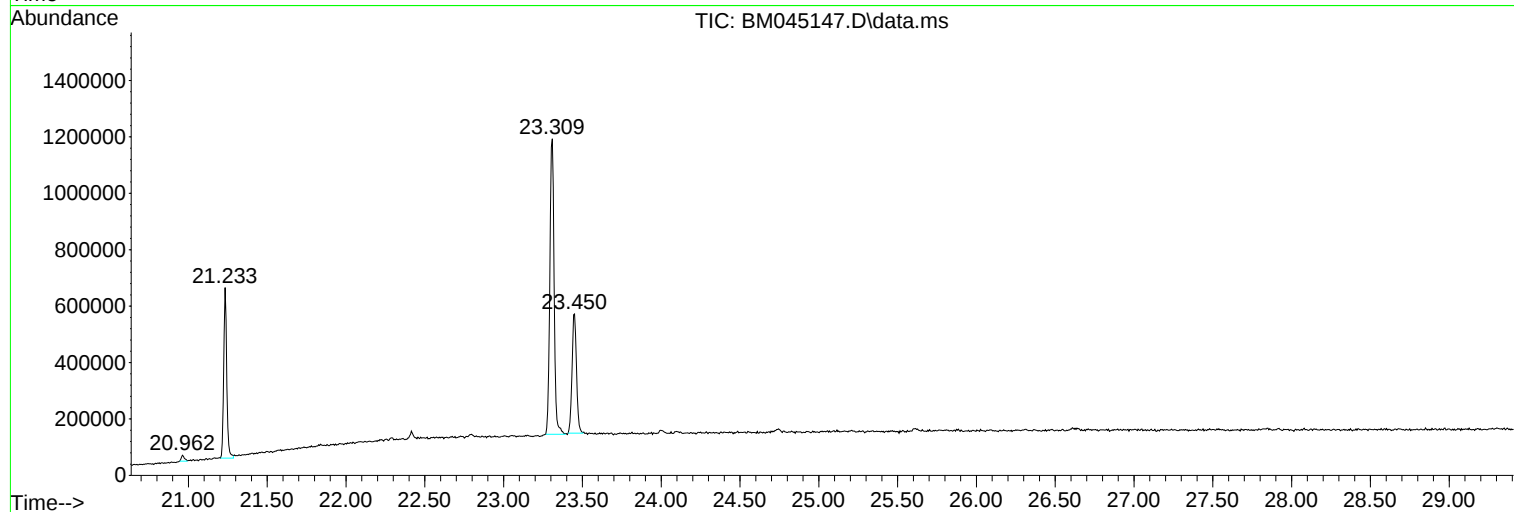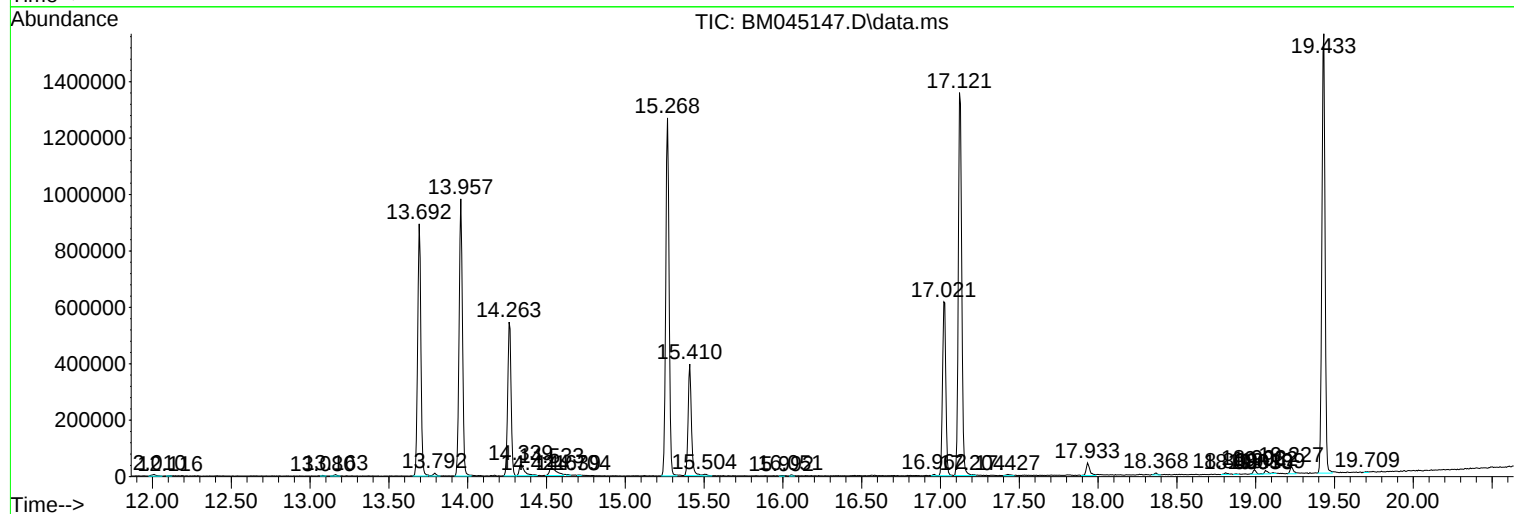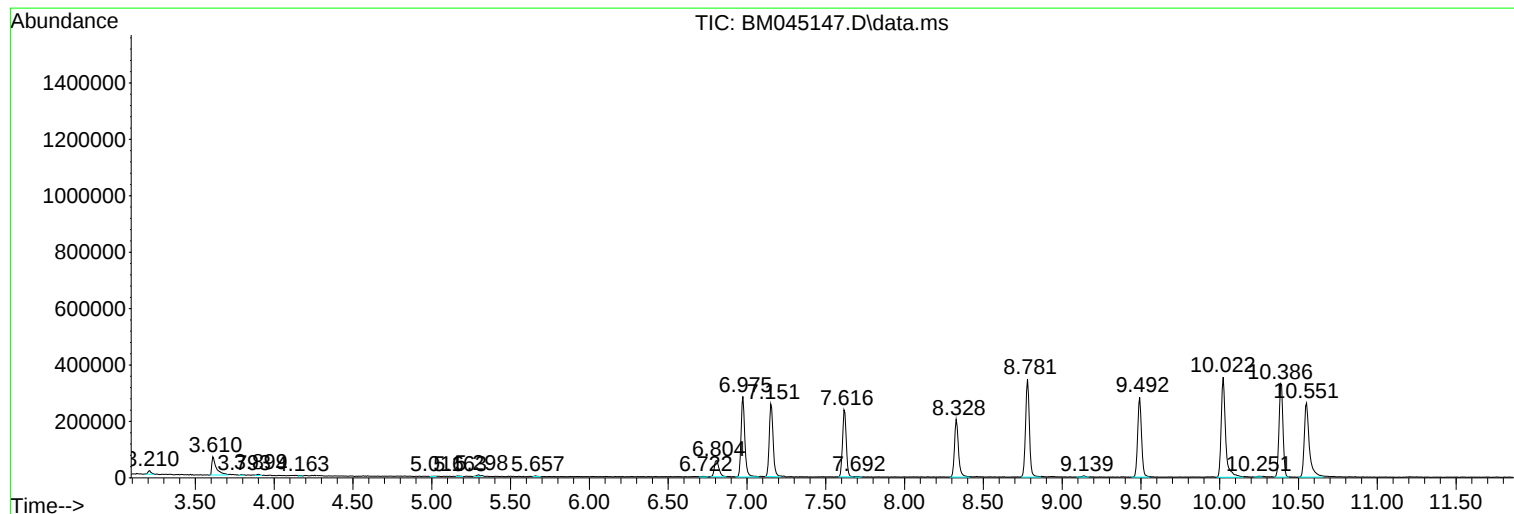

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045147.D
Acq On : 11 Apr 2024 22:58
Operator : MA/JU
Sample : P2013-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOMB7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzoic acid, 2,4-dichloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.339	2.24 ng/ul	90637	Acenaphthene-d10	14.263

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzoic acid, 2,4-dichloro-	190	C7H4Cl2O2	000050-84-0	99
2			Benzoic acid, 2,4-dichloro-	190	C7H4Cl2O2	000050-84-0	98
3			Benzoic acid, 2,3-dichloro-	190	C7H4Cl2O2	000050-45-3	94
4			Benzoic acid, 2,6-dichloro-	190	C7H4Cl2O2	000050-30-6	93
5			Benzoic acid, 2,6-dichloro-	190	C7H4Cl2O2	000050-30-6	93

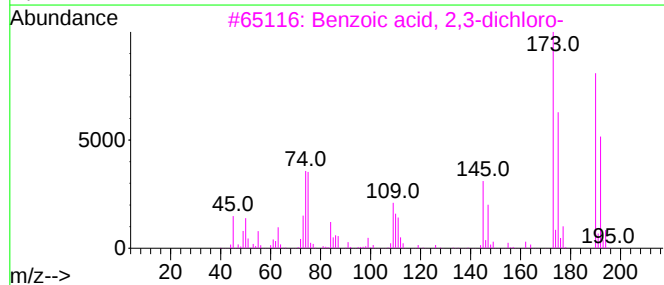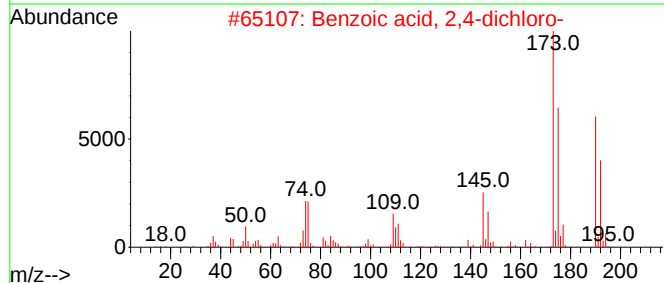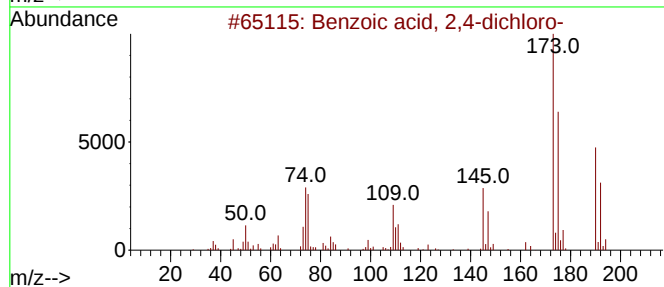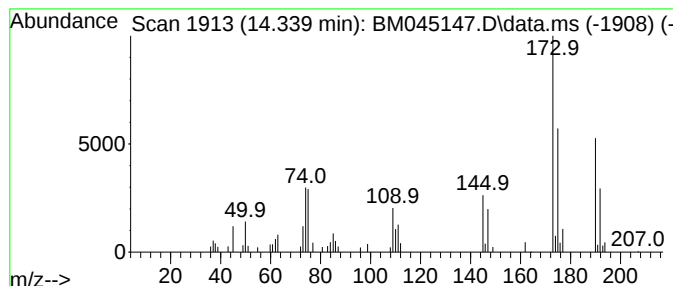

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045147.D
Acq On : 11 Apr 2024 22:58
Operator : MA/JU
Sample : P2013-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzoic acid, 2...	14.339	2.2	ng/u1	90637	3	14.263	807882	20.0