

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045148.D
 Acq On : 11 Apr 2024 23:35
 Operator : MA/JU
 Sample : P2013-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOMB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045148.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	10	14	18	rBV2	17677	21596	0.92%	0.117%
2	3.204	18	20	24	rVB	13790	16988	0.73%	0.092%
3	3.610	86	89	108	rVV	85030	161754	6.91%	0.873%
4	3.734	108	110	112	rVV3	2845	2522	0.11%	0.014%
5	3.757	112	114	118	rVB3	2945	2887	0.12%	0.016%
6	3.898	134	138	141	rVB3	7839	9724	0.42%	0.052%
7	4.393	217	222	231	rVB	61330	94736	4.05%	0.511%
8	5.169	350	354	357	rBV4	2829	3740	0.16%	0.020%
9	5.298	371	376	384	rBV4	7463	16123	0.69%	0.087%
10	5.657	434	437	441	rVB5	3128	3988	0.17%	0.022%
11	5.698	441	444	447	rVB4	1845	2449	0.10%	0.013%
12	6.304	545	547	550	rBV4	1914	2369	0.10%	0.013%
13	6.804	626	632	643	rBV2	63986	123768	5.29%	0.668%
14	6.975	654	661	673	rBV	285287	461278	19.71%	2.490%
15	7.151	684	691	700	rBV	261876	440076	18.80%	2.375%
16	7.616	764	770	777	rBV	227748	369720	15.80%	1.996%
17	8.328	883	891	904	rBV	200591	359395	15.36%	1.940%
18	8.781	960	968	977	rBV	329809	563059	24.06%	3.039%
19	9.139	1023	1029	1033	rVB2	3437	4642	0.20%	0.025%
20	9.492	1082	1089	1106	rBV	265271	463172	19.79%	2.500%
21	10.022	1172	1179	1199	rVV	326273	627921	26.83%	3.389%
22	10.386	1234	1241	1252	rVB	302212	521663	22.29%	2.816%
23	10.551	1261	1269	1286	rBV	271498	600583	25.66%	3.242%
24	12.010	1512	1517	1520	rBV3	4363	6650	0.28%	0.036%
25	12.116	1530	1535	1538	rBV4	1839	2926	0.13%	0.016%
26	13.163	1708	1713	1718	rVB3	3805	6170	0.26%	0.033%
27	13.692	1796	1803	1814	rBV	684219	981545	41.94%	5.298%
28	13.957	1840	1848	1857	rBV	860341	1280382	54.71%	6.911%
29	14.263	1894	1900	1909	rVV	449778	672432	28.73%	3.630%
30	14.539	1940	1947	1957	rBV5	19849	62194	2.66%	0.336%
31	14.710	1973	1976	1979	rBV4	2387	2752	0.12%	0.015%
32	14.833	1989	1997	2009	rBV	16309	46107	1.97%	0.249%
33	14.968	2016	2020	2025	rVB6	1530	2867	0.12%	0.015%
34	15.268	2064	2071	2080	rBV	1020090	1523497	65.09%	8.223%
35	15.409	2089	2095	2106	rBV	281227	415003	17.73%	2.240%
36	15.509	2109	2112	2115	rVB4	2876	3257	0.14%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045148.D
 Acq On : 11 Apr 2024 23:35
 Operator : MA/JU
 Sample : P2013-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOMB9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	16.051	2202	2204	2209	rVB5	2973	3559	0.15%	0.019%
38	16.451	2269	2272	2277	rBV4	1955	2418	0.10%	0.013%
39	16.562	2286	2291	2293	rBV4	2288	2782	0.12%	0.015%
40	16.804	2328	2332	2335	rBV6	2948	4050	0.17%	0.022%
41	16.956	2355	2358	2362	rVB5	2201	2811	0.12%	0.015%
42	17.021	2364	2369	2379	rVV	520514	742138	31.71%	4.006%
43	17.127	2380	2387	2400	rVV	1073102	1636135	69.91%	8.831%
44	17.333	2418	2422	2426	rBV5	1812	2522	0.11%	0.014%
45	17.433	2434	2439	2441	rBV6	3652	5543	0.24%	0.030%
46	17.803	2501	2502	2506	rBV3	2126	2348	0.10%	0.013%
47	17.886	2514	2516	2518	rBV2	2151	2496	0.11%	0.013%
48	17.933	2520	2524	2533	rVV	43560	72352	3.09%	0.391%
49	18.368	2594	2598	2600	rBV4	5394	6682	0.29%	0.036%
50	18.803	2670	2672	2676	rBV5	3846	5973	0.26%	0.032%
51	18.992	2701	2704	2713	rVB4	11411	17295	0.74%	0.093%
52	19.062	2713	2716	2721	rBV	9155	13444	0.57%	0.073%
53	19.227	2740	2744	2751	rBV5	24672	37013	1.58%	0.200%
54	19.374	2767	2769	2772	rBV4	2762	2743	0.12%	0.015%
55	19.427	2772	2778	2789	rVV	1301582	1864521	79.67%	10.064%
56	19.792	2838	2840	2843	rBV2	3670	4445	0.19%	0.024%
57	20.021	2877	2879	2882	rVB3	4563	3500	0.15%	0.019%
58	20.362	2935	2937	2938	rBV2	4398	3846	0.16%	0.021%
59	20.962	3037	3039	3044	rVB5	13141	16021	0.68%	0.086%
60	21.233	3080	3085	3093	rBV	602039	832912	35.59%	4.496%
61	23.309	3430	3438	3454	rBV	1209274	2340429	100.00%	12.633%
62	23.450	3455	3462	3472	rVV	503863	1018818	43.53%	5.499%




Sum of corrected areas: 18526731

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045148.D
Acq On : 11 Apr 2024 23:35
Operator : MA/JU
Sample : P2013-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOMB9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

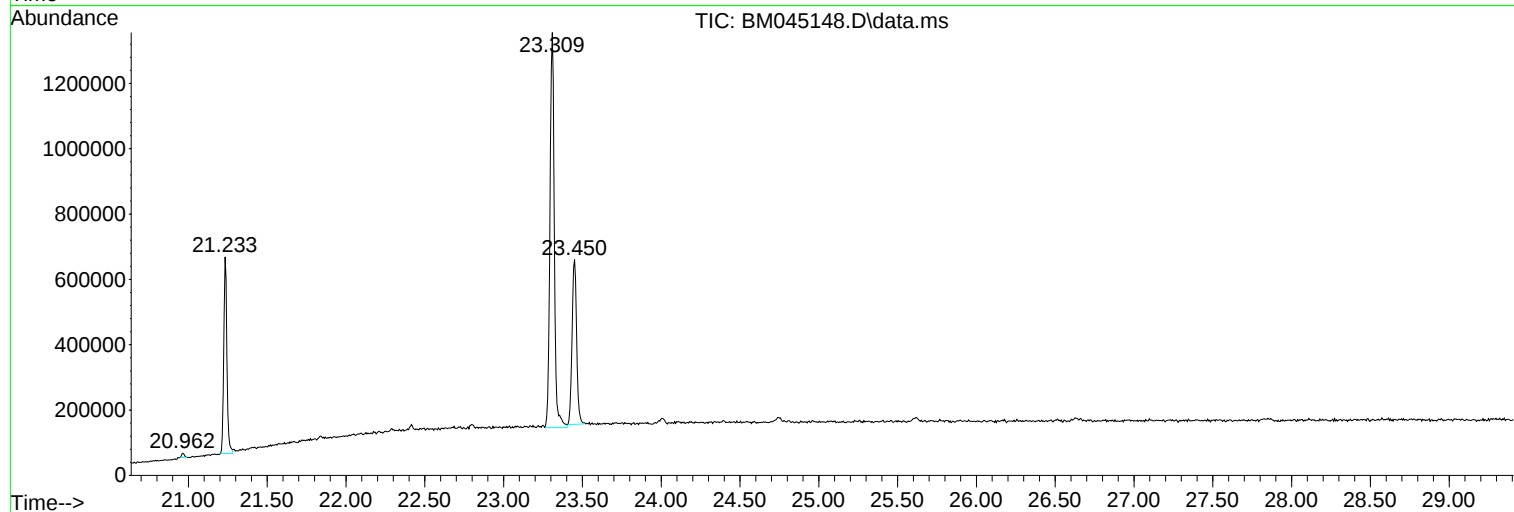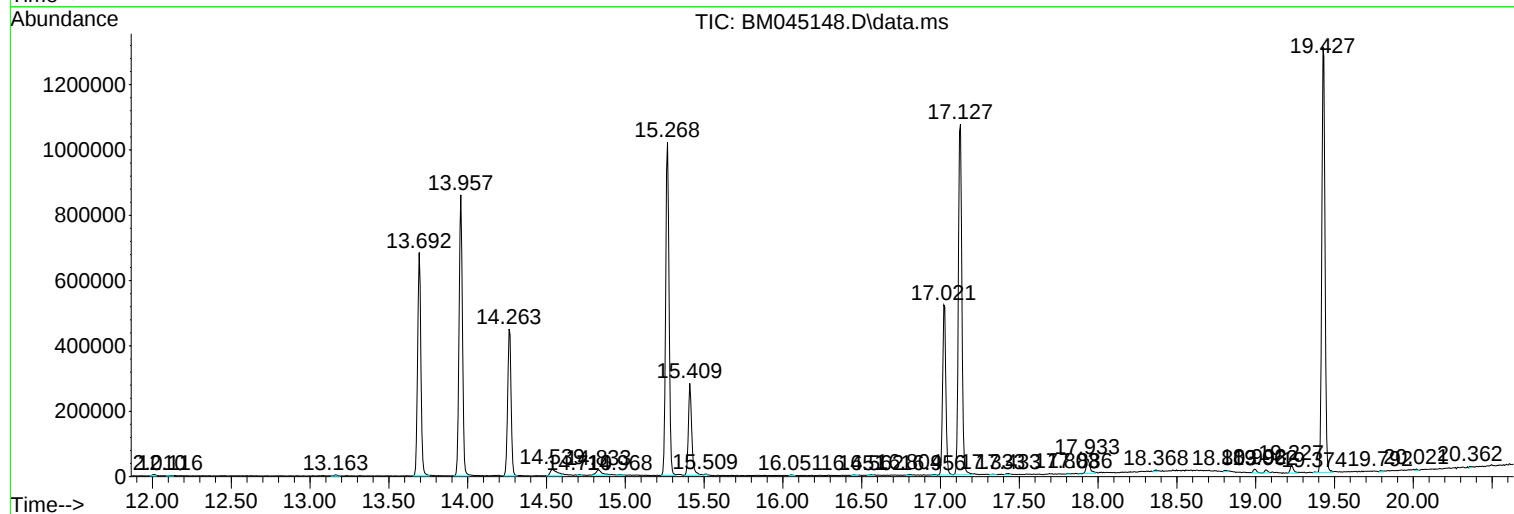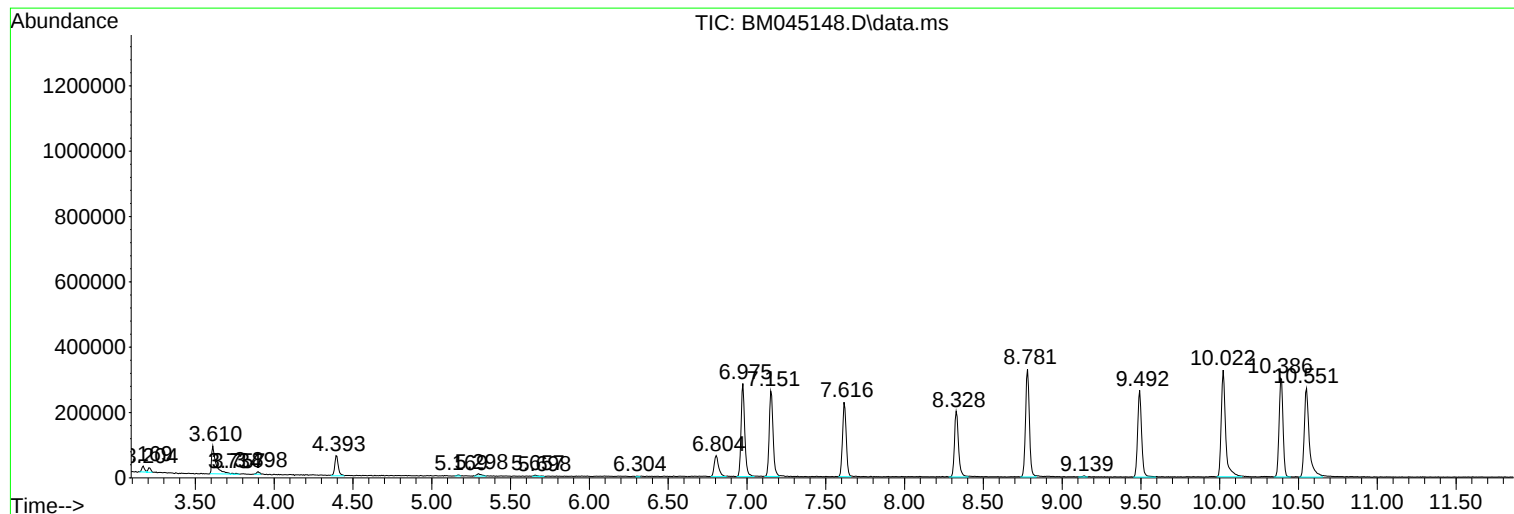

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045148.D
Acq On : 11 Apr 2024 23:35
Operator : MA/JU
Sample : P2013-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MB9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045148.D
Acq On : 11 Apr 2024 23:35
Operator : MA/JU
Sample : P2013-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MB9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc