

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045150.D
 Acq On : 12 Apr 2024 00:47
 Operator : MA/JU
 Sample : P2013-18
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045150.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	10	14	18	rBV2	17951	27312	1.16%	0.129%
2	3.210	18	21	28	rVB	14047	20655	0.88%	0.098%
3	3.610	86	89	102	rBV	63054	129320	5.50%	0.612%
4	3.898	135	138	142	rVB5	5145	6763	0.29%	0.032%
5	4.393	217	222	230	rBV	74296	114571	4.87%	0.542%
6	5.169	351	354	359	rBV4	3306	3392	0.14%	0.016%
7	5.298	371	376	382	rBV4	6606	13691	0.58%	0.065%
8	5.657	433	437	441	rBV5	2458	4273	0.18%	0.020%
9	6.804	626	632	643	rBV	66847	127589	5.43%	0.604%
10	6.975	654	661	672	rBV	272881	448121	19.06%	2.120%
11	7.151	685	691	703	rBV	255700	435314	18.51%	2.060%
12	7.234	703	705	709	rVV3	2374	2429	0.10%	0.011%
13	7.616	762	770	780	rBV	254854	421066	17.91%	1.992%
14	8.328	884	891	906	rBV	211056	378179	16.08%	1.789%
15	8.780	961	968	979	rBV	333939	563130	23.95%	2.664%
16	9.133	1025	1028	1035	rVB4	3036	4298	0.18%	0.020%
17	9.492	1080	1089	1104	rBV	278441	471404	20.05%	2.230%
18	10.022	1173	1179	1198	rBV	332579	643368	27.36%	3.044%
19	10.386	1234	1241	1250	rBV	369797	631325	26.85%	2.987%
20	10.551	1261	1269	1294	rBV	283971	635526	27.02%	3.007%
21	12.016	1513	1518	1525	rVB2	4563	7747	0.33%	0.037%
22	13.080	1694	1699	1702	rVB4	1651	2633	0.11%	0.012%
23	13.163	1707	1713	1719	rBV2	5302	9379	0.40%	0.044%
24	13.692	1796	1803	1821	rVB	833980	1221666	51.95%	5.780%
25	13.957	1841	1848	1860	rBV	978599	1443104	61.37%	6.828%
26	14.262	1893	1900	1910	rBV	619883	917463	39.01%	4.341%
27	14.533	1939	1946	1957	rBV6	23280	78610	3.34%	0.372%
28	14.710	1974	1976	1981	rVB4	2523	3052	0.13%	0.014%
29	15.268	2064	2071	2079	rBV	1247365	1843666	78.40%	8.723%
30	15.409	2089	2095	2109	rBV	378064	571335	24.30%	2.703%
31	15.504	2109	2111	2117	rVB4	4627	6742	0.29%	0.032%
32	16.056	2200	2205	2212	rVB6	4114	5870	0.25%	0.028%
33	16.962	2356	2359	2362	rVB3	3362	4024	0.17%	0.019%
34	17.021	2362	2369	2380	rBV	745087	1078646	45.87%	5.103%
35	17.121	2380	2386	2399	rVV2	1398252	2097104	89.18%	9.922%
36	17.433	2432	2439	2442	rVB6	5078	8022	0.34%	0.038%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045150.D
 Acq On : 12 Apr 2024 00:47
 Operator : MA/JU
 Sample : P2013-18
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	17.698	2480	2484	2490	rVB7	1998	3659	0.16%	0.017%
38	17.809	2500	2503	2508	rVB6	2462	3760	0.16%	0.018%
39	17.933	2520	2524	2531	rBV2	38549	61091	2.60%	0.289%
40	18.021	2536	2539	2542	rVB4	2032	2492	0.11%	0.012%
41	18.368	2595	2598	2600	rVV2	3677	4141	0.18%	0.020%
42	18.815	2669	2674	2676	rBV4	4610	6771	0.29%	0.032%
43	18.868	2680	2683	2687	rBV3	1998	3591	0.15%	0.017%
44	18.939	2691	2695	2698	rBV5	2721	4710	0.20%	0.022%
45	18.992	2700	2704	2709	rVB2	15982	19834	0.84%	0.094%
46	19.068	2713	2717	2721	rBV2	10756	16026	0.68%	0.076%
47	19.227	2740	2744	2752	rBV5	28919	45047	1.92%	0.213%
48	19.386	2768	2771	2772	rBV2	2853	3502	0.15%	0.017%
49	19.433	2772	2779	2787	rVV	1652326	2351642	100.00%	11.126%
50	20.539	2965	2967	2968	rBV2	4512	3944	0.17%	0.019%
51	20.962	3036	3039	3042	rBV4	15095	17099	0.73%	0.081%
52	21.233	3080	3085	3094	rBV	780983	1043615	44.38%	4.938%
53	23.309	3431	3438	3446	rBV	1149340	2113135	89.86%	9.998%
54	23.450	3455	3462	3476	rVB	534089	1051170	44.70%	4.973%




Sum of corrected areas: 21136018

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045150.D
Acq On : 12 Apr 2024 00:47
Operator : MA/JU
Sample : P2013-18
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

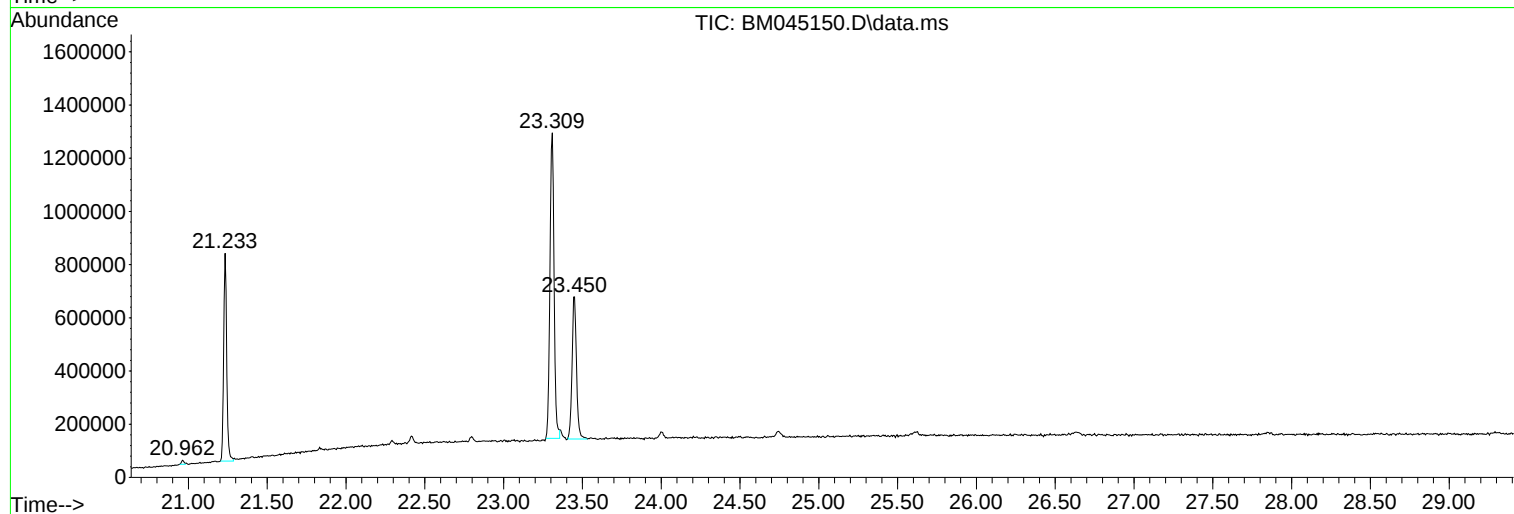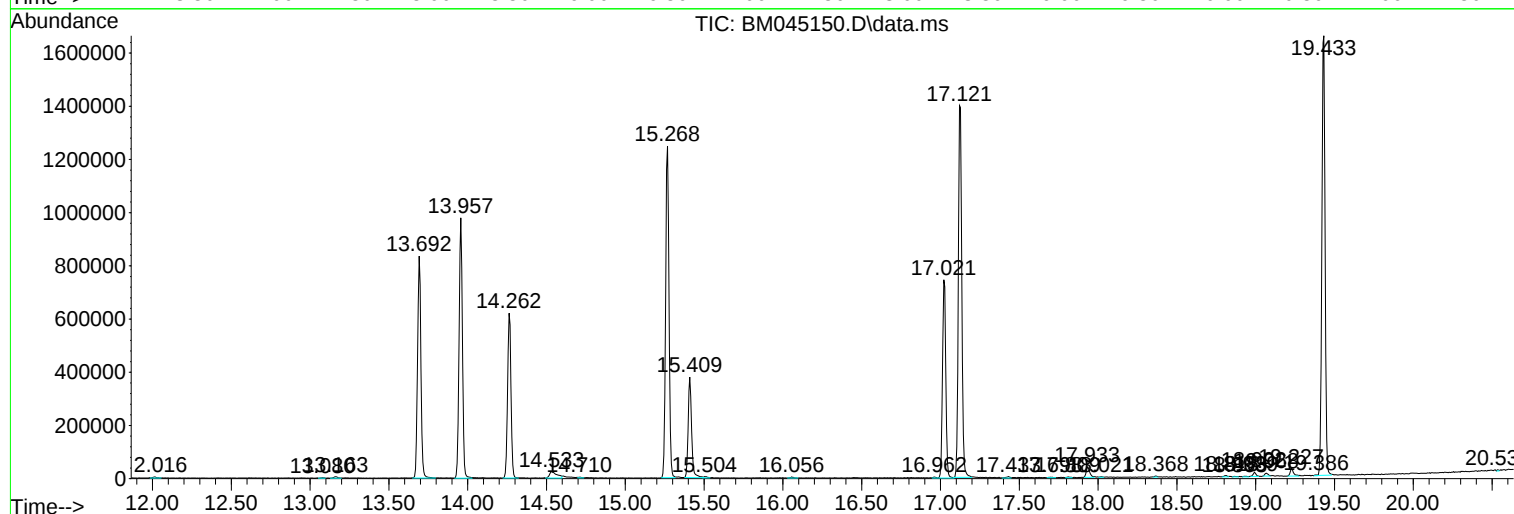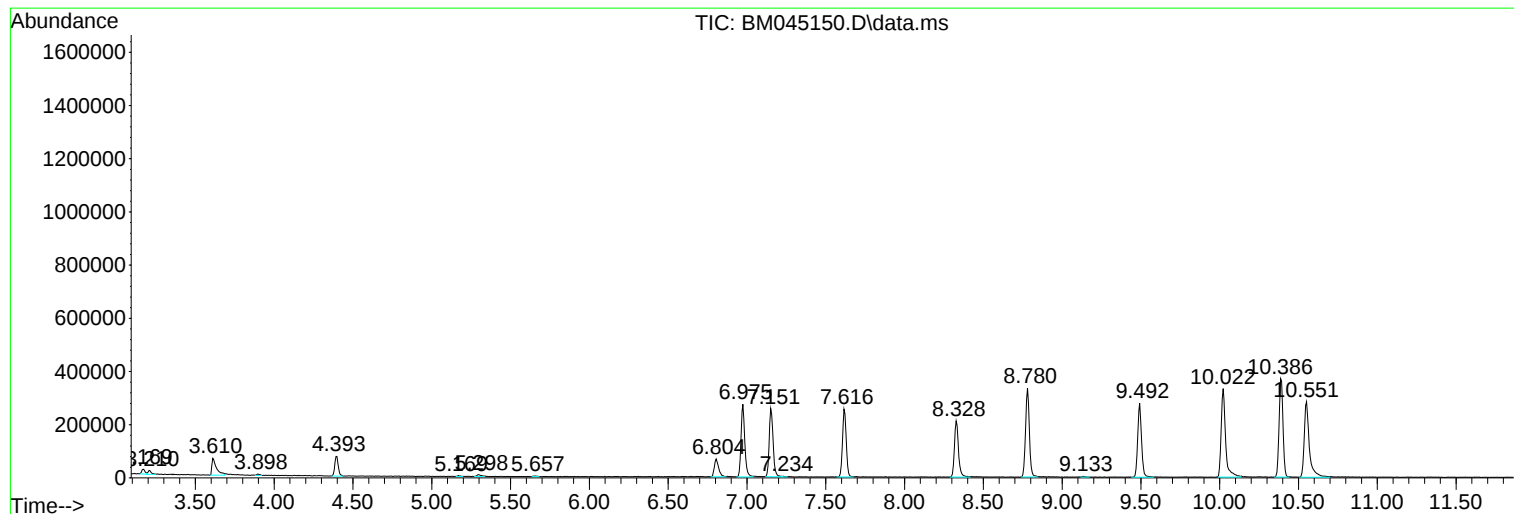

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045150.D
Acq On : 12 Apr 2024 00:47
Operator : MA/JU
Sample : P2013-18
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045150.D
Acq On : 12 Apr 2024 00:47
Operator : MA/JU
Sample : P2013-18
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc