

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045156.D
 Acq On : 12 Apr 2024 05:02
 Operator : MA/JU
 Sample : PB160162BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK162

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045156.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.204	17	20	28	rVB	16068	24293	1.42%	0.140%
2	3.499	68	70	74	rBV4	1536	2220	0.13%	0.013%
3	3.604	84	88	105	rBV	175612	314308	18.41%	1.818%
4	3.904	137	139	141	rVB2	3506	2780	0.16%	0.016%
5	4.057	162	165	167	rVB3	1543	1746	0.10%	0.010%
6	4.751	280	283	287	rBV6	1366	1921	0.11%	0.011%
7	5.328	376	381	384	rVB5	1887	2807	0.16%	0.016%
8	6.004	495	496	500	rBV3	1260	1855	0.11%	0.011%
9	6.798	625	631	643	rBV	225089	408880	23.95%	2.365%
10	6.975	655	661	676	rVB	199344	332355	19.46%	1.922%
11	7.151	685	691	702	rVB	254968	417816	24.47%	2.416%
12	7.616	764	770	782	rVB	210967	345009	20.21%	1.995%
13	8.134	852	858	861	rVB4	1727	2208	0.13%	0.013%
14	8.328	884	891	902	rBV	289021	509078	29.81%	2.944%
15	8.781	960	968	980	rBV	241354	420541	24.63%	2.432%
16	9.492	1082	1089	1100	rBV	204055	362954	21.26%	2.099%
17	10.022	1172	1179	1198	rBV	256917	524797	30.73%	3.035%
18	10.386	1235	1241	1250	rBV	300848	506440	29.66%	2.929%
19	10.551	1261	1269	1288	rBV	233989	561539	32.89%	3.248%
20	11.022	1345	1349	1354	rVB4	1281	1951	0.11%	0.011%
21	11.351	1404	1405	1409	rBV4	1259	1886	0.11%	0.011%
22	11.533	1433	1436	1439	rBV3	1407	1860	0.11%	0.011%
23	12.016	1515	1518	1523	rBV5	2659	4481	0.26%	0.026%
24	12.957	1674	1678	1681	rBV3	1319	2001	0.12%	0.012%
25	13.163	1708	1713	1718	rBV4	3540	5505	0.32%	0.032%
26	13.692	1796	1803	1815	rBV	632844	952548	55.78%	5.509%
27	13.957	1841	1848	1860	rBV	709999	1079065	63.19%	6.240%
28	14.263	1893	1900	1910	rBV	505529	766995	44.92%	4.436%
29	14.504	1936	1941	1967	rBV	121160	398601	23.34%	2.305%
30	14.768	1984	1986	1990	rVB4	1503	1791	0.10%	0.010%
31	14.886	2004	2006	2010	rBV4	1188	1806	0.11%	0.010%
32	15.268	2064	2071	2080	rBV	892715	1371984	80.35%	7.934%
33	15.410	2089	2095	2110	rBV	256239	402171	23.55%	2.326%
34	15.504	2110	2111	2117	rVB5	4619	5476	0.32%	0.032%
35	16.057	2202	2205	2209	rVB5	2738	3111	0.18%	0.018%
36	16.815	2329	2334	2337	rBV5	2008	3605	0.21%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045156.D
Acq On : 12 Apr 2024 05:02
Operator : MA/JU
Sample : PB160162BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK162

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

37	17.021	2363	2369	2378	rBV	643941	924097	54.12%	5.344%
38	17.121	2380	2386	2403	rVB	969337	1512208	88.56%	8.745%
39	17.903	2515	2519	2521	rBV3	2265	2836	0.17%	0.016%
40	17.962	2527	2529	2535	rVB5	2517	3903	0.23%	0.023%
41	18.074	2543	2548	2550	rBV5	1884	3959	0.23%	0.023%
42	18.662	2646	2648	2651	rVB4	2522	2760	0.16%	0.016%
43	18.992	2700	2704	2712	rVB4	10829	16317	0.96%	0.094%
44	19.062	2713	2716	2723	rVV2	6962	11370	0.67%	0.066%
45	19.427	2772	2778	2791	rBV	1170426	1707539	100.00%	9.875%
46	20.227	2913	2914	2915	rBV	4523	1854	0.11%	0.011%
47	21.233	3080	3085	3097	rBV	650097	922753	54.04%	5.336%
48	23.303	3431	3437	3445	rBV	790008	1535052	89.90%	8.878%
49	23.450	3456	3462	3474	rVB	447554	898356	52.61%	5.195%




Sum of corrected areas: 17291388

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045156.D
Acq On : 12 Apr 2024 05:02
Operator : MA/JU
Sample : PB160162BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK162

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

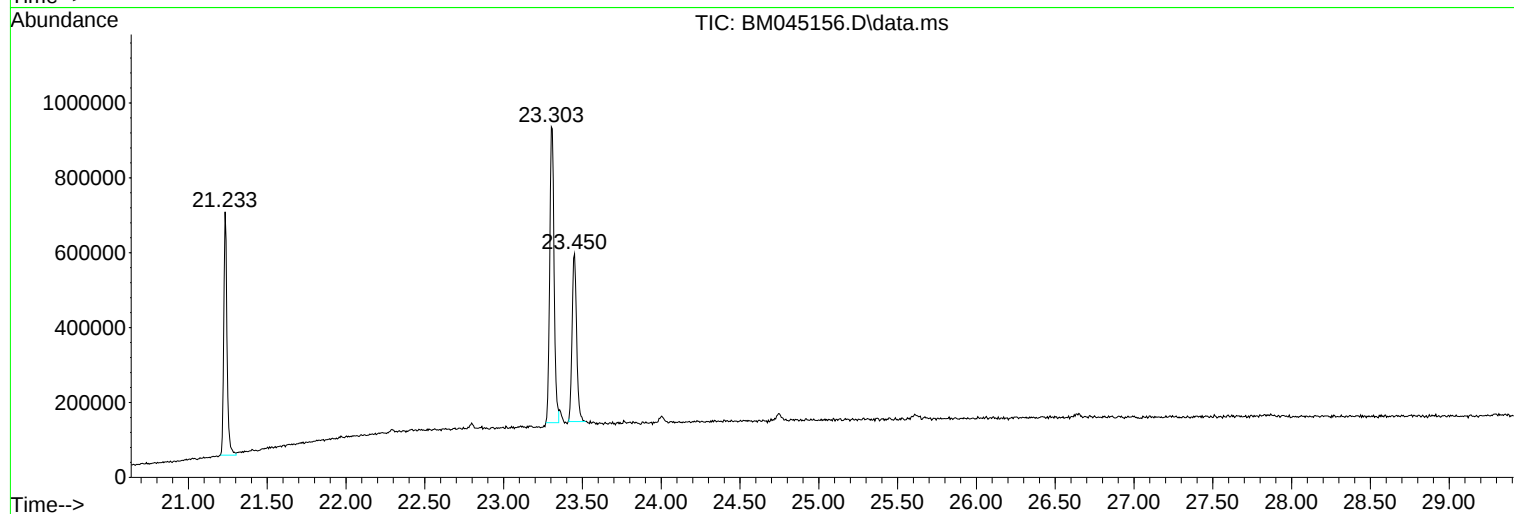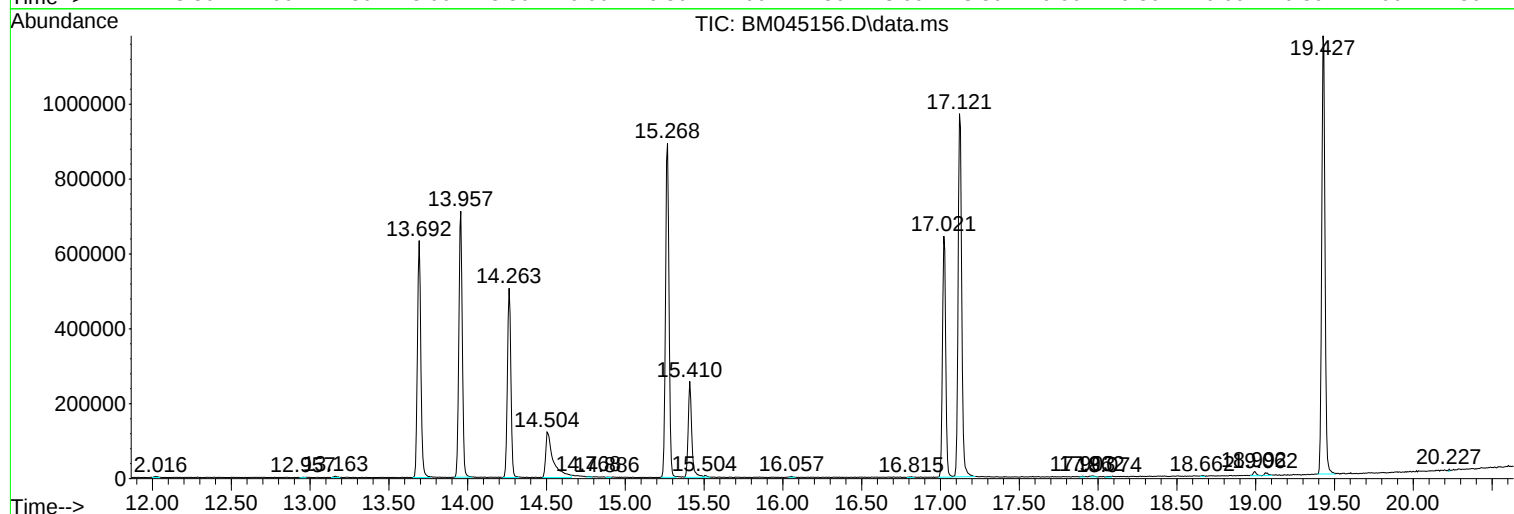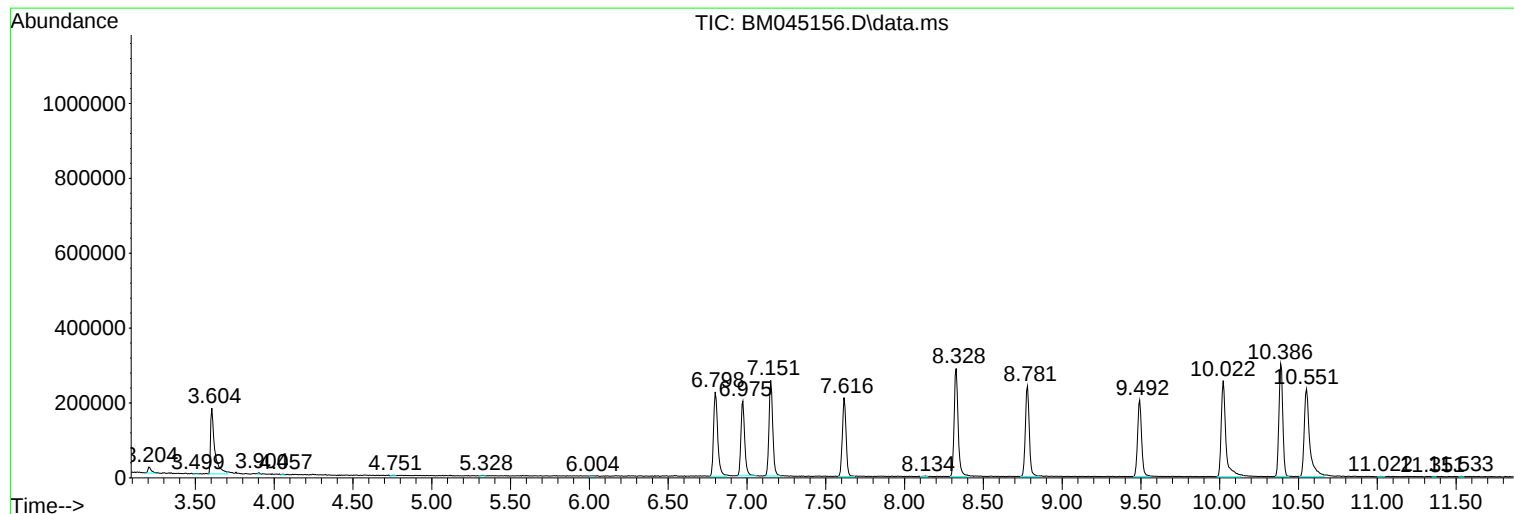

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045156.D
Acq On : 12 Apr 2024 05:02
Operator : MA/JU
Sample : PB160162BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK162

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045156.D
Acq On : 12 Apr 2024 05:02
Operator : MA/JU
Sample : PB160162BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK162

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------