

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045157.D
 Acq On : 12 Apr 2024 05:38
 Operator : MA/JU
 Sample : P2014-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MD6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045157.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.204	17	20	27	rVB2	13114	18599	0.82%	0.093%
2	3.557	78	80	84	rVB4	3051	2747	0.12%	0.014%
3	3.610	87	89	103	rBV	50400	106986	4.69%	0.537%
4	3.799	119	121	126	rVB4	3084	2803	0.12%	0.014%
5	3.893	135	137	141	rVB2	3380	4595	0.20%	0.023%
6	4.451	229	232	237	rBV3	1581	2718	0.12%	0.014%
7	6.804	626	632	645	rVB	50278	101861	4.46%	0.512%
8	6.975	654	661	670	rBV	243039	408853	17.92%	2.053%
9	7.151	684	691	702	rBV	224578	389646	17.08%	1.957%
10	7.616	764	770	782	rBV	245444	396986	17.40%	1.994%
11	8.328	885	891	904	rBV	169400	299446	13.13%	1.504%
12	8.781	961	968	980	rBV	307008	525521	23.04%	2.639%
13	9.133	1025	1028	1034	rBV4	2086	2990	0.13%	0.015%
14	9.492	1081	1089	1099	rBV	243039	425539	18.65%	2.137%
15	10.022	1171	1179	1204	rBV	286399	586169	25.69%	2.944%
16	10.386	1234	1241	1250	rBV	355513	599075	26.26%	3.009%
17	10.551	1262	1269	1288	rBV	239555	564668	24.75%	2.836%
18	11.492	1426	1429	1436	rBV3	1262	3066	0.13%	0.015%
19	12.016	1512	1518	1525	rVB3	4733	9632	0.42%	0.048%
20	13.116	1701	1705	1708	rBV4	1670	2665	0.12%	0.013%
21	13.163	1708	1713	1718	rVB4	5554	8072	0.35%	0.041%
22	13.692	1796	1803	1816	rBV	735980	1088328	47.71%	5.466%
23	13.957	1841	1848	1857	rBV	875025	1315985	57.68%	6.609%
24	14.263	1893	1900	1909	rBV	592796	870513	38.16%	4.372%
25	14.533	1942	1946	1947	rBV3	12731	12955	0.57%	0.065%
26	14.551	1947	1949	1960	rVB7	12025	28424	1.25%	0.143%
27	15.268	2064	2071	2083	rBV	1140353	1697853	74.42%	8.527%
28	15.410	2089	2095	2108	rBV	335673	502651	22.03%	2.524%
29	15.510	2110	2112	2119	rVB5	6564	9019	0.40%	0.045%
30	16.057	2201	2205	2208	rBV3	3357	4105	0.18%	0.021%
31	17.021	2363	2369	2379	rBV	746205	1044973	45.81%	5.248%
32	17.121	2380	2386	2401	rVB2	1304210	1969415	86.33%	9.891%
33	17.433	2434	2439	2440	rBV3	1943	2708	0.12%	0.014%
34	17.933	2520	2524	2532	rBV	36268	61212	2.68%	0.307%
35	18.015	2536	2538	2545	rVB7	2229	4058	0.18%	0.020%
36	18.227	2571	2574	2576	rBV4	2780	3092	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045157.D
 Acq On : 12 Apr 2024 05:38
 Operator : MA/JU
 Sample : P2014-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	18.351	2592	2595	2598	rBV5	2148	3051	0.13%	0.015%
38	18.715	2655	2657	2663	rBV6	3003	4829	0.21%	0.024%
39	18.992	2700	2704	2711	rBV4	14951	21118	0.93%	0.106%
40	19.062	2713	2716	2721	rBV	9918	13230	0.58%	0.066%
41	19.227	2740	2744	2753	rBV4	19588	32812	1.44%	0.165%
42	19.427	2772	2778	2790	rBV	1610011	2281344	100.00%	11.457%
43	19.992	2872	2874	2878	rBV5	3058	3589	0.16%	0.018%
44	20.644	2983	2985	2988	rBV4	5372	6905	0.30%	0.035%
45	20.962	3035	3039	3049	rBV6	31811	60208	2.64%	0.302%
46	21.233	3080	3085	3097	rBV	813426	1087108	47.65%	5.460%
47	23.309	3431	3438	3445	rBV2	1182980	2188562	95.93%	10.991%
48	23.450	3455	3462	3475	rBV	553536	1131059	49.58%	5.680%




Sum of corrected areas: 19911743

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045157.D
Acq On : 12 Apr 2024 05:38
Operator : MA/JU
Sample : P2014-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

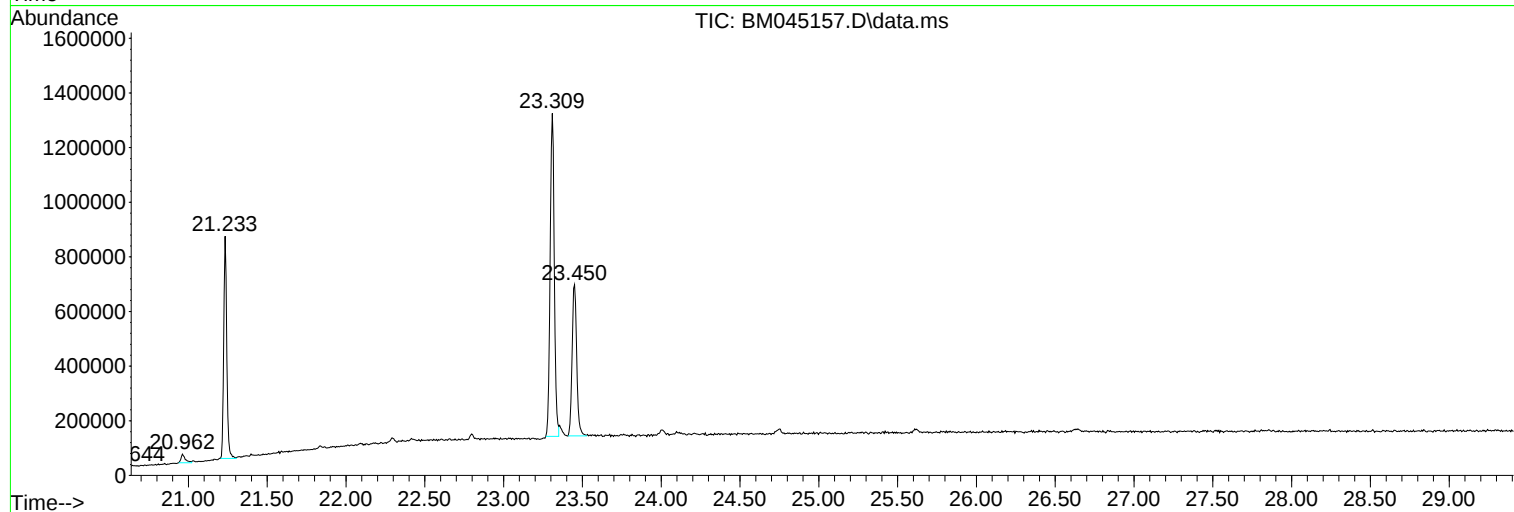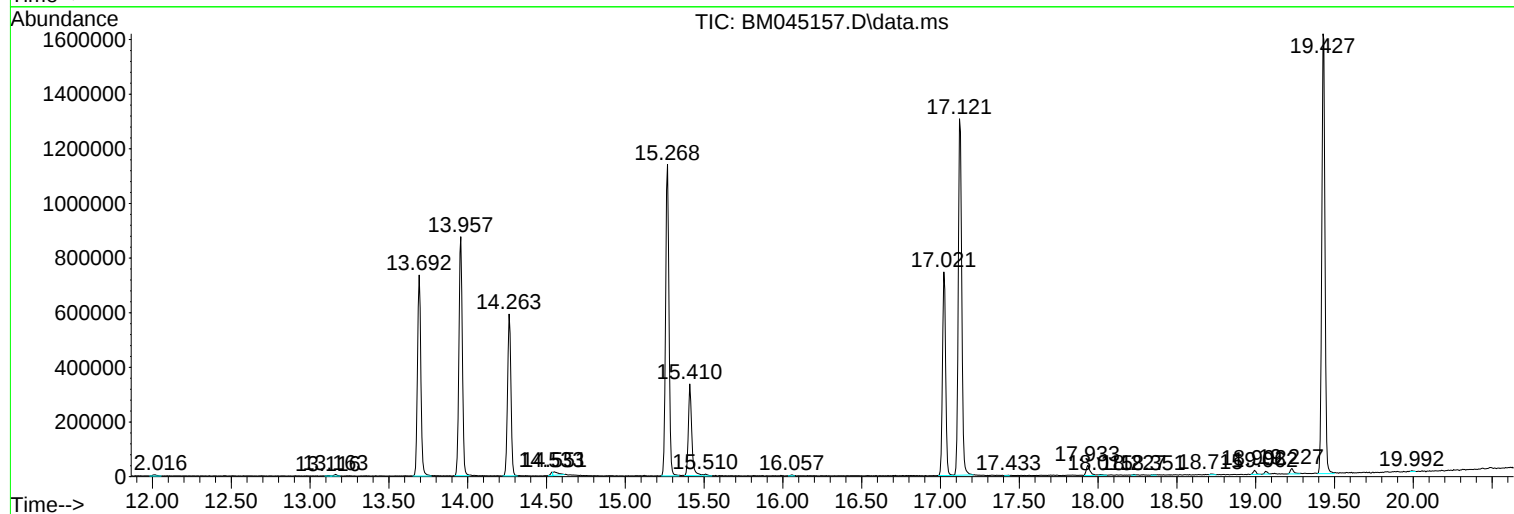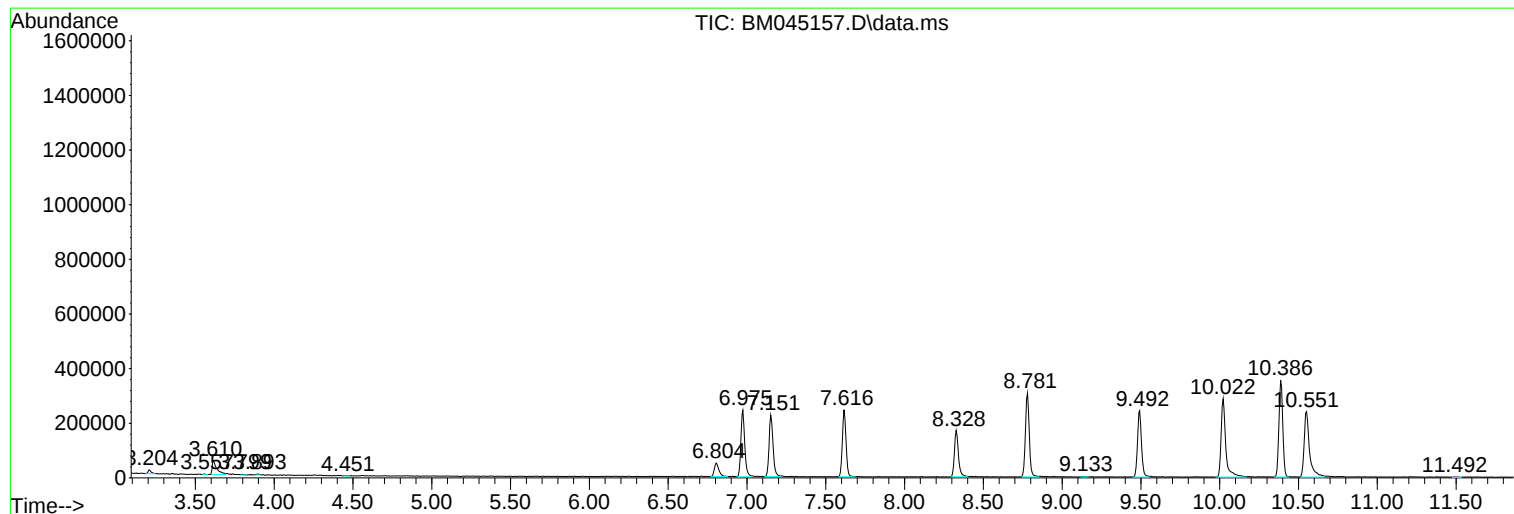

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045157.D
Acq On : 12 Apr 2024 05:38
Operator : MA/JU
Sample : P2014-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045157.D
Acq On : 12 Apr 2024 05:38
Operator : MA/JU
Sample : P2014-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------