

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045162.D
 Acq On : 12 Apr 2024 08:40
 Operator : MA/JU
 Sample : P2014-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOME1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045162.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	17	20	27	rVB	10016	14567	0.77%	0.085%
2	3.510	67	72	73	rBV4	3480	4920	0.26%	0.029%
3	3.610	87	89	105	rBV	48117	105327	5.59%	0.615%
4	3.793	118	120	123	rVB3	2694	2644	0.14%	0.015%
5	3.840	126	128	131	rVV4	2496	2524	0.13%	0.015%
6	3.893	134	137	144	rVB6	3936	7264	0.39%	0.042%
7	4.087	166	170	172	rVB5	2052	2689	0.14%	0.016%
8	4.504	240	241	245	rBV4	1880	2247	0.12%	0.013%
9	4.816	291	294	295	rBV2	1845	2136	0.11%	0.012%
10	5.157	351	352	355	rBV3	1728	2025	0.11%	0.012%
11	5.346	381	384	388	rBV5	1322	2333	0.12%	0.014%
12	6.804	626	632	642	rBV2	49883	98235	5.22%	0.573%
13	6.975	654	661	674	rBV	228986	397890	21.13%	2.322%
14	7.151	684	691	701	rBV	218859	372705	19.79%	2.175%
15	7.616	763	770	778	rBV	217568	353556	18.78%	2.063%
16	8.328	885	891	901	rBV2	164630	295575	15.70%	1.725%
17	8.634	939	943	945	rBV3	2019	2261	0.12%	0.013%
18	8.781	960	968	982	rBV	284129	500807	26.59%	2.922%
19	9.492	1082	1089	1100	rBV	221534	396947	21.08%	2.316%
20	10.022	1172	1179	1200	rBV	273101	558159	29.64%	3.257%
21	10.239	1215	1216	1219	rVB3	2068	1941	0.10%	0.011%
22	10.263	1219	1220	1226	rBV5	1148	1937	0.10%	0.011%
23	10.386	1234	1241	1249	rBV	309038	513130	27.25%	2.994%
24	10.551	1260	1269	1293	rBV	227161	540327	28.69%	3.153%
25	11.204	1377	1380	1382	rBV4	1832	2094	0.11%	0.012%
26	11.939	1502	1505	1510	rVB6	1410	2257	0.12%	0.013%
27	12.010	1514	1517	1522	rVB6	4421	6871	0.36%	0.040%
28	13.157	1704	1712	1717	rBV4	5701	8035	0.43%	0.047%
29	13.692	1796	1803	1818	rBV	686225	1017141	54.01%	5.935%
30	13.957	1841	1848	1858	rBV2	789789	1244292	66.08%	7.261%
31	14.263	1894	1900	1911	rVB	489665	717829	38.12%	4.189%
32	14.545	1943	1948	1956	rBV8	13281	44666	2.37%	0.261%
33	14.710	1973	1976	1981	rVB4	2099	3109	0.17%	0.018%
34	15.080	2036	2039	2043	rBV6	1896	2153	0.11%	0.013%
35	15.263	2064	2070	2085	rBV	1008609	1546350	82.12%	9.024%
36	15.410	2089	2095	2107	rBV	282270	442370	23.49%	2.581%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045162.D
 Acq On : 12 Apr 2024 08:40
 Operator : MA/JU
 Sample : P2014-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOME1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	15.510	2110	2112	2115	rVB4	4635	4694	0.25%	0.027%
38	16.057	2201	2205	2210	rVB5	2859	4686	0.25%	0.027%
39	17.021	2363	2369	2377	rBV	587757	807530	42.88%	4.712%
40	17.121	2380	2386	2400	rBV2	1169537	1752461	93.06%	10.226%
41	17.339	2419	2423	2426	rVB5	1514	2343	0.12%	0.014%
42	17.427	2432	2438	2444	rBV6	5932	9910	0.53%	0.058%
43	17.609	2468	2469	2475	rBV4	1113	1929	0.10%	0.011%
44	17.933	2519	2524	2535	rBV2	36705	61279	3.25%	0.358%
45	18.368	2591	2598	2603	rBV6	8566	10427	0.55%	0.061%
46	18.721	2653	2658	2660	rBV5	1988	2508	0.13%	0.015%
47	18.992	2700	2704	2709	rBV2	11833	15940	0.85%	0.093%
48	19.068	2712	2717	2723	rBV2	8875	17335	0.92%	0.101%
49	19.227	2740	2744	2751	rBV5	15399	23991	1.27%	0.140%
50	19.298	2753	2756	2758	rBV4	1779	2314	0.12%	0.014%
51	19.427	2772	2778	2789	rBV	1323213	1883097	100.00%	10.989%
52	19.662	2816	2818	2821	rBV4	2090	2688	0.14%	0.016%
53	20.962	3036	3039	3045	rBV6	18718	31384	1.67%	0.183%
54	21.233	3080	3085	3093	rBV	517930	731361	38.84%	4.268%
55	23.309	3431	3438	3446	rBV	921135	1749780	92.92%	10.211%
56	23.450	3455	3462	3472	rBV	393659	801610	42.57%	4.678%




Sum of corrected areas: 17136580

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045162.D
Acq On : 12 Apr 2024 08:40
Operator : MA/JU
Sample : P2014-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

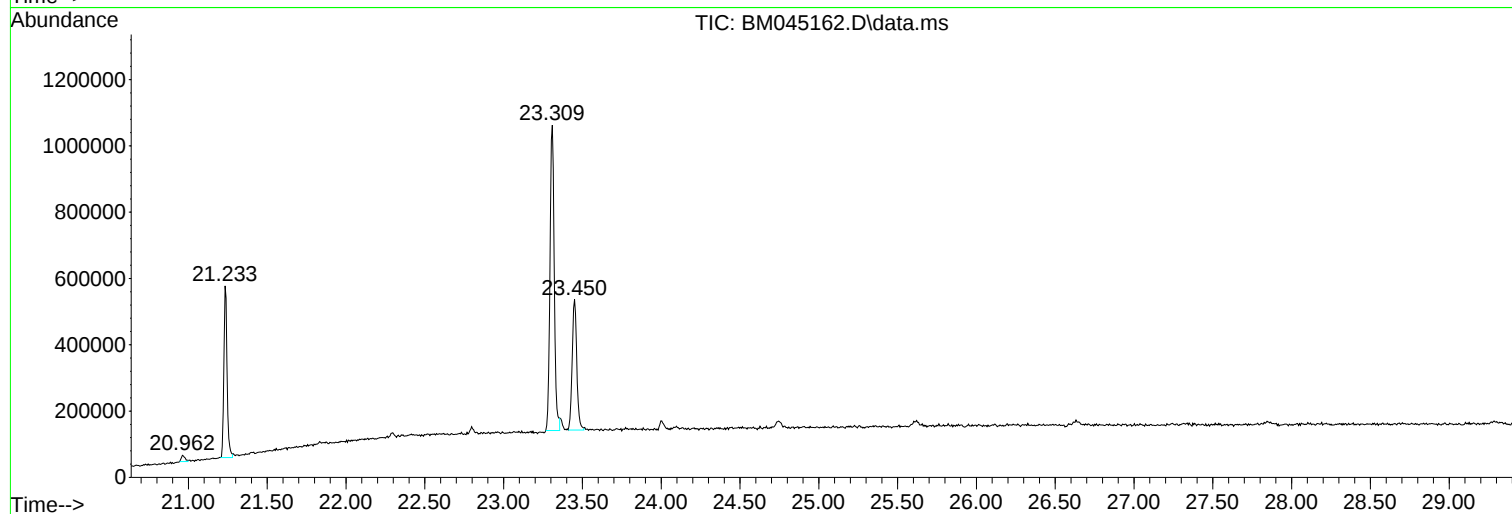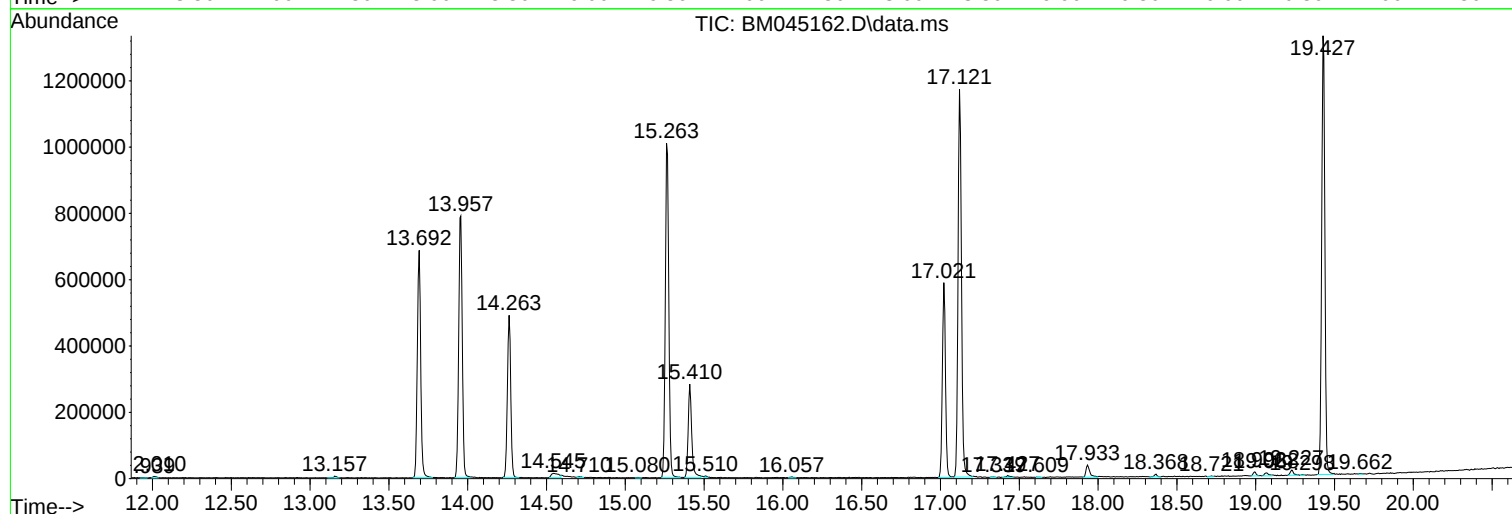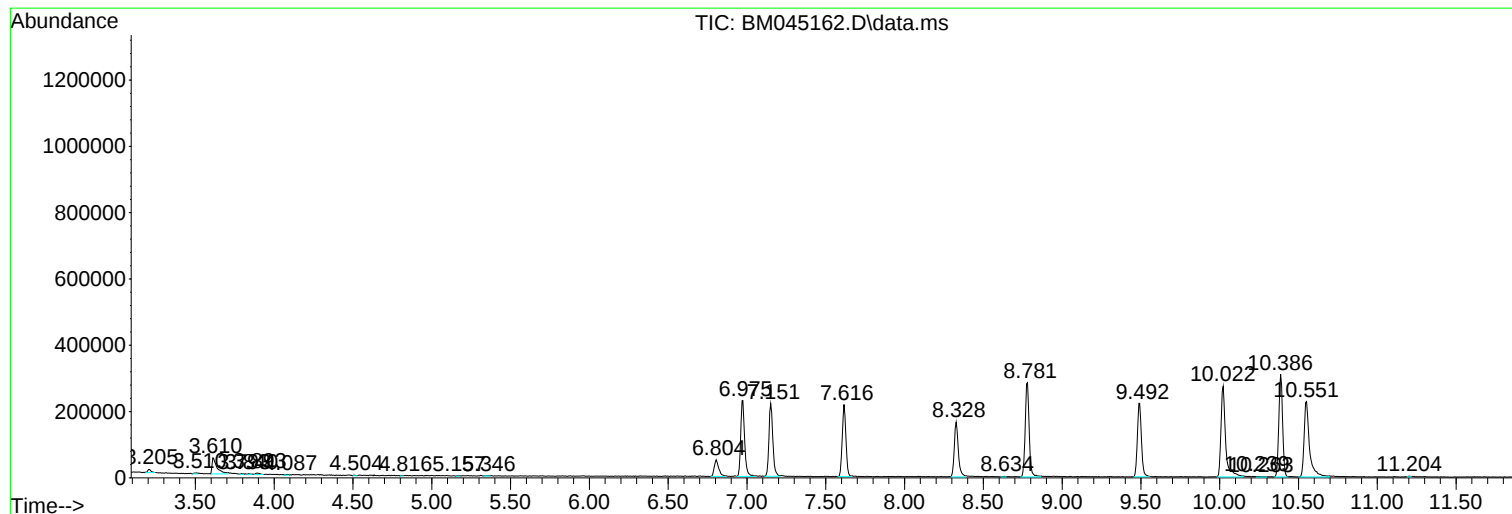

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045162.D
Acq On : 12 Apr 2024 08:40
Operator : MA/JU
Sample : P2014-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045162.D
Acq On : 12 Apr 2024 08:40
Operator : MA/JU
Sample : P2014-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc