

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045165.D
 Acq On : 12 Apr 2024 10:29
 Operator : MA/JU
 Sample : P2014-19
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOME4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045165.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.204	17	20	34	rVB3	11941	23839	0.98%	0.118%
2	3.610	86	89	100	rBV	60000	119975	4.91%	0.596%
3	3.898	136	138	143	rVB5	5716	5547	0.23%	0.028%
4	6.422	564	567	571	rBV4	1711	3154	0.13%	0.016%
5	6.804	626	632	645	rBV	49030	100993	4.13%	0.502%
6	6.975	654	661	671	rBV	248659	416379	17.04%	2.069%
7	7.151	685	691	701	rBV	231431	394852	16.16%	1.962%
8	7.616	763	770	781	rBV	223478	369602	15.13%	1.837%
9	8.328	885	891	906	rBV2	160588	288314	11.80%	1.433%
10	8.775	961	967	981	rBV	303438	533166	21.82%	2.650%
11	9.486	1082	1088	1101	rBV	244551	432313	17.70%	2.148%
12	10.022	1171	1179	1197	rBV	299807	603119	24.69%	2.997%
13	10.386	1234	1241	1250	rBV	324332	547754	22.42%	2.722%
14	10.545	1261	1268	1292	rBV	243588	578007	23.66%	2.872%
15	11.963	1505	1509	1513	rBV5	1677	3066	0.13%	0.015%
16	12.016	1513	1518	1522	rVB4	4180	8079	0.33%	0.040%
17	12.210	1546	1551	1553	rBV3	1295	2467	0.10%	0.012%
18	13.157	1709	1712	1717	rVB5	3757	5372	0.22%	0.027%
19	13.692	1796	1803	1815	rBV	776398	1138658	46.61%	5.659%
20	13.957	1840	1848	1860	rBV	892222	1364834	55.87%	6.783%
21	14.263	1892	1900	1910	rBV	535990	790962	32.38%	3.931%
22	14.357	1910	1916	1919	rBV6	4276	6809	0.28%	0.034%
23	14.545	1942	1948	1950	rBV4	17375	31791	1.30%	0.158%
24	15.268	2063	2071	2080	rBV	1129413	1761318	72.10%	8.753%
25	15.409	2089	2095	2107	rBV	348270	531902	21.77%	2.643%
26	15.504	2109	2111	2116	rVB5	5201	7892	0.32%	0.039%
27	16.057	2201	2205	2208	rBV4	4680	7156	0.29%	0.036%
28	16.456	2270	2273	2277	rBV3	2284	3135	0.13%	0.016%
29	16.809	2327	2333	2335	rBV3	1546	2602	0.11%	0.013%
30	17.021	2362	2369	2379	rBV	698490	941186	38.53%	4.677%
31	17.121	2379	2386	2403	rBV	1341951	2039250	83.47%	10.134%
32	17.439	2433	2440	2444	rBV6	1957	3869	0.16%	0.019%
33	17.933	2519	2524	2532	rBV2	49250	79237	3.24%	0.394%
34	18.797	2668	2671	2675	rBV6	1363	2851	0.12%	0.014%
35	18.992	2700	2704	2708	rBV2	15867	21043	0.86%	0.105%
36	19.068	2713	2717	2720	rBV3	10907	16508	0.68%	0.082%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045165.D
Acq On : 12 Apr 2024 10:29
Operator : MA/JU
Sample : P2014-19
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

37	19.227	2740	2744	2753	rBV3	29098	44907	1.84%	0.223%
38	19.427	2772	2778	2791	rBV	1679166	2371297	97.06%	11.784%
39	20.962	3037	3039	3043	rVB4	13378	16740	0.69%	0.083%
40	21.233	3080	3085	3096	rBV	727028	1003618	41.08%	4.988%
41	23.309	3431	3438	3451	rBV	1296010	2443020	100.00%	12.141%
42	23.450	3455	3462	3473	rVB	533567	1055656	43.21%	5.246%




Sum of corrected areas: 20122239

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045165.D
Acq On : 12 Apr 2024 10:29
Operator : MA/JU
Sample : P2014-19
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

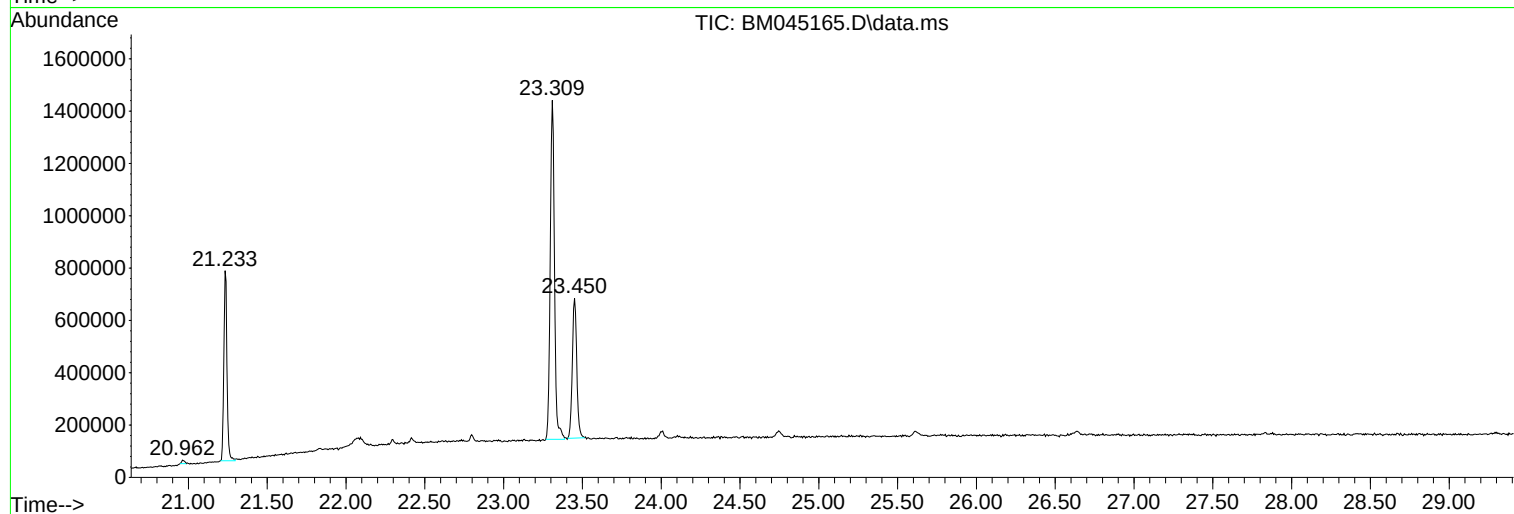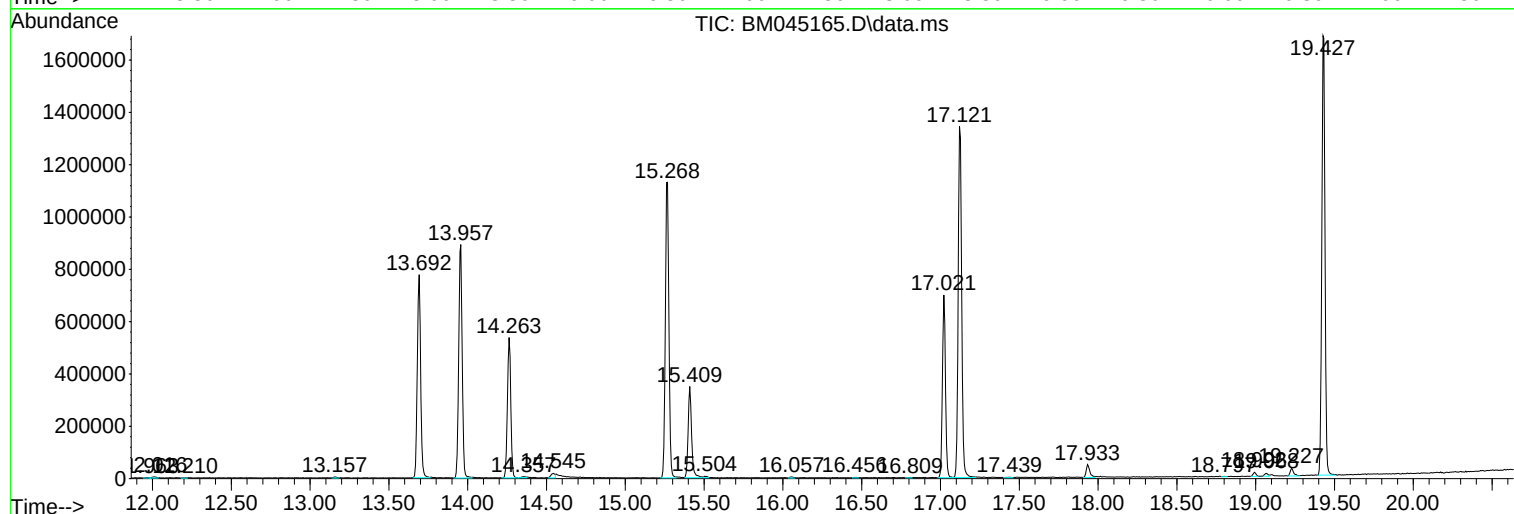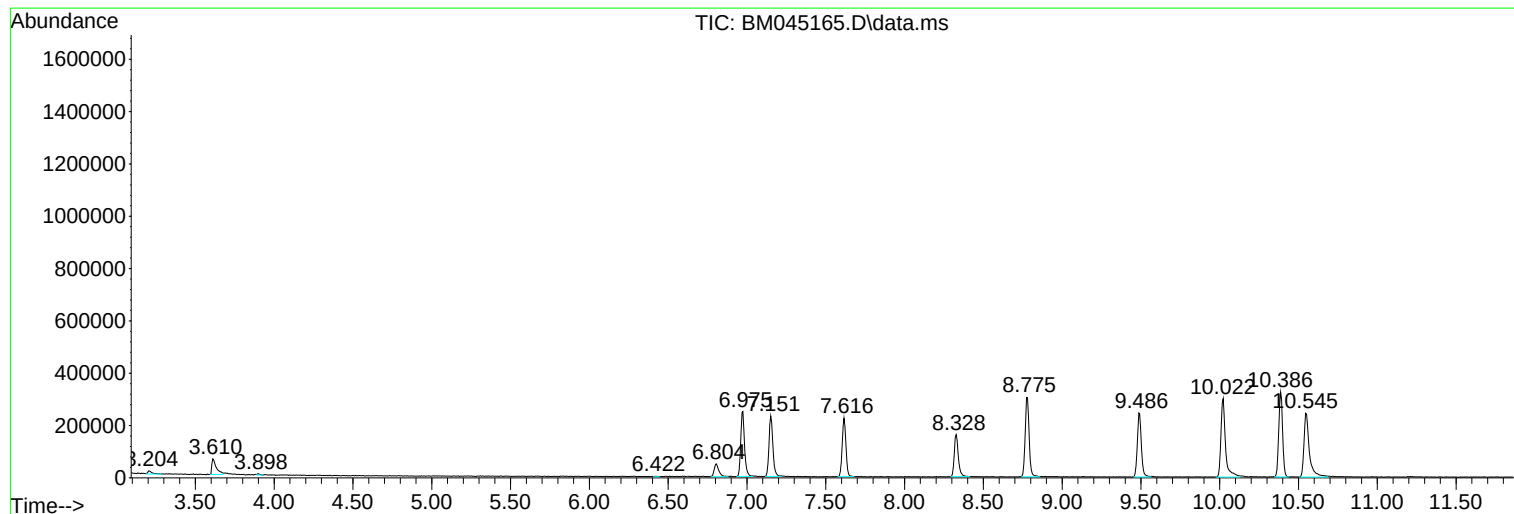

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045165.D
Acq On : 12 Apr 2024 10:29
Operator : MA/JU
Sample : P2014-19
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045165.D
Acq On : 12 Apr 2024 10:29
Operator : MA/JU
Sample : P2014-19
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc