

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045167.D
 Acq On : 12 Apr 2024 11:42
 Operator : MA/JU
 Sample : SP6475
 Misc : SFAM SURROGATE
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SP6475

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045167.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	28	rBV	43360	59372	1.58%	0.163%
2	3.599	83	87	108	rBV	571884	955580	25.51%	2.618%
3	3.899	134	138	142	rVB6	4545	7034	0.19%	0.019%
4	6.798	624	631	650	rBV	695676	1158420	30.92%	3.174%
5	6.975	653	661	674	rVV	578593	926610	24.74%	2.539%
6	7.151	684	691	703	rBV	736038	1166483	31.14%	3.196%
7	7.616	763	770	783	rBV	248492	402635	10.75%	1.103%
8	8.322	883	890	904	rBV	862189	1454016	38.82%	3.983%
9	8.781	960	968	979	rBV	692432	1180679	31.52%	3.235%
10	9.486	1081	1088	1099	rBV	611332	1038153	27.71%	2.844%
11	10.016	1171	1178	1199	rBV	800609	1500241	40.05%	4.110%
12	10.386	1234	1241	1248	rBV	360350	593150	15.83%	1.625%
13	10.545	1258	1268	1290	rBV	791778	1586030	42.34%	4.345%
14	12.004	1511	1516	1522	rBV2	9965	18995	0.51%	0.052%
15	13.692	1796	1803	1816	rBV	1551504	2194495	58.58%	6.012%
16	13.957	1840	1848	1860	rBV	1911919	2781336	74.25%	7.620%
17	14.263	1892	1900	1909	rBV	553054	817128	21.81%	2.239%
18	14.498	1932	1940	1967	rBV	520646	1080606	28.85%	2.960%
19	14.680	1969	1971	1978	rVB6	4939	7863	0.21%	0.022%
20	15.268	2064	2071	2083	rBV	2296427	3306435	88.27%	9.058%
21	15.410	2089	2095	2108	rBV	666848	1022702	27.30%	2.802%
22	15.510	2108	2112	2119	rVB4	11538	18739	0.50%	0.051%
23	16.051	2199	2204	2208	rBV4	5487	7759	0.21%	0.021%
24	17.021	2363	2369	2376	rBV	676929	921534	24.60%	2.525%
25	17.127	2379	2387	2403	rVV	2272485	3450691	92.12%	9.454%
26	18.992	2699	2704	2711	rBV2	23800	33883	0.90%	0.093%
27	19.068	2712	2717	2722	rVB	18493	28537	0.76%	0.078%
28	19.433	2772	2779	2793	rBV	2719598	3745992	100.00%	10.263%
29	21.239	3080	3086	3098	rBV	547310	861877	23.01%	2.361%
30	23.309	3431	3438	3453	rBV2	1729433	3322608	88.70%	9.103%
31	23.450	3456	3462	3475	rVB	433330	851496	22.73%	2.333%




Sum of corrected areas: 36501079

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045167.D
Acq On : 12 Apr 2024 11:42
Operator : MA/JU
Sample : SP6475
Misc : SFAM SURROGATE
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP6475

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

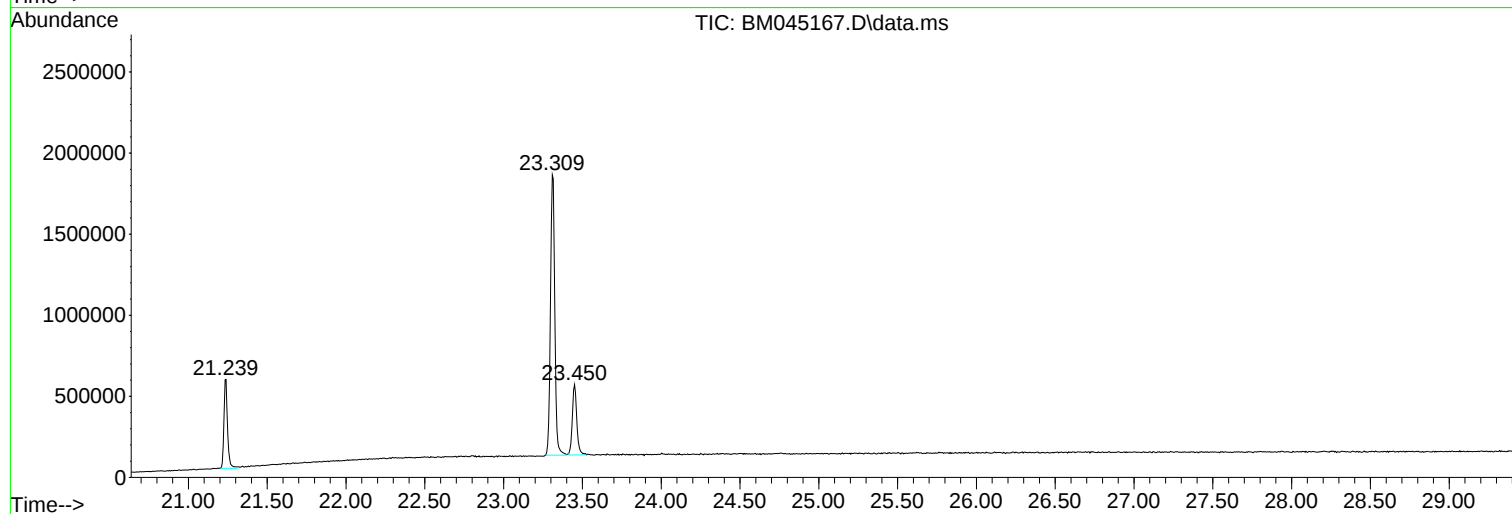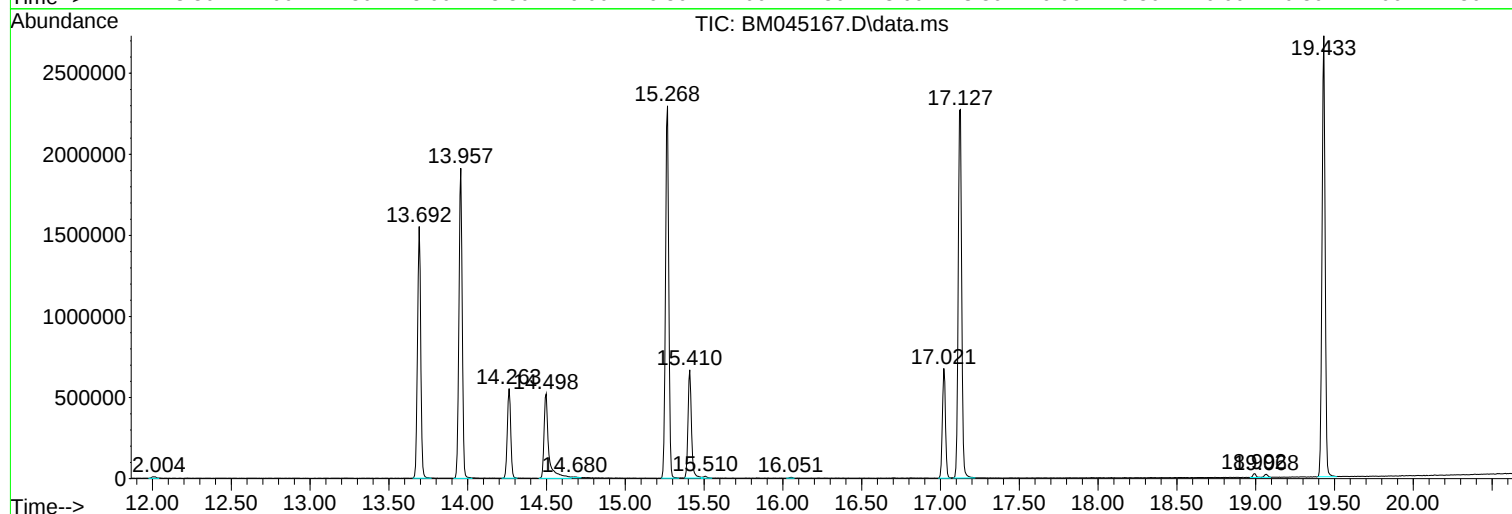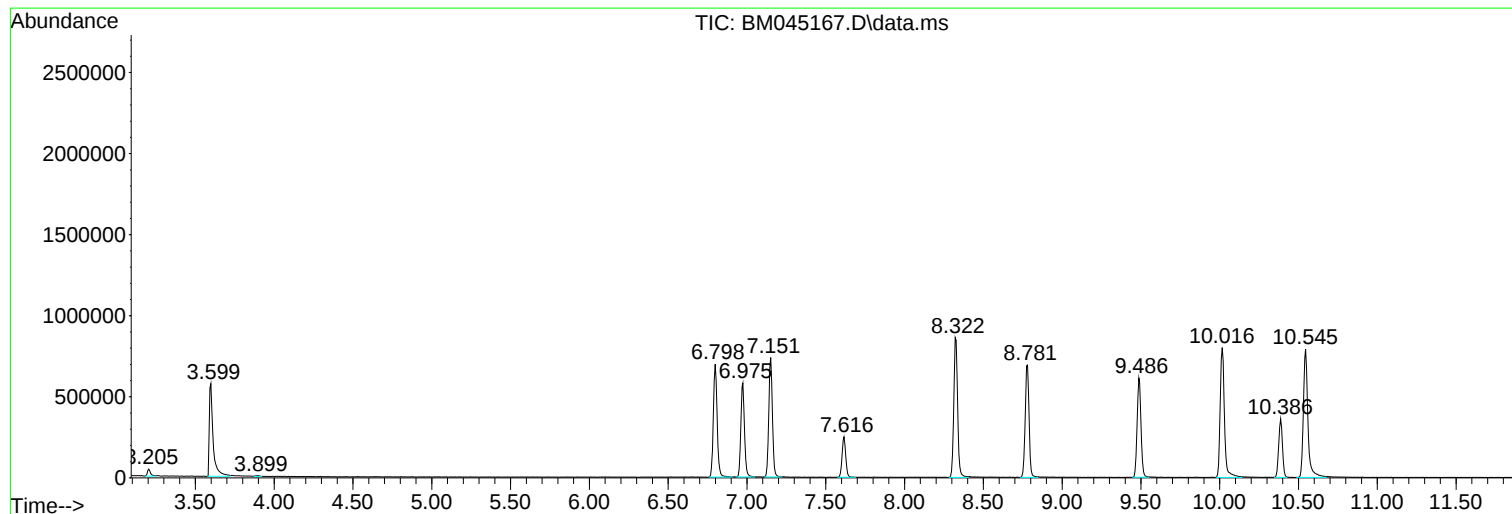

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045167.D
Acq On : 12 Apr 2024 11:42
Operator : MA/JU
Sample : SP6475
Misc : SFAM SURROGATE
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP6475

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045167.D
Acq On : 12 Apr 2024 11:42
Operator : MA/JU
Sample : SP6475
Misc : SFAM SURROGATE
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP6475

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------