

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045170.D
 Acq On : 12 Apr 2024 14:11
 Operator : MA/JU
 Sample : PB160112BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK112

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045170.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	17	21	27	rVB	17024	23821	1.79%	0.174%
2	3.599	84	87	99	rBV	191817	337190	25.31%	2.464%
3	3.899	134	138	140	rBV4	3700	4423	0.33%	0.032%
4	5.204	358	360	363	rVB3	2055	1785	0.13%	0.013%
5	5.551	416	419	420	rVV3	1975	1519	0.11%	0.011%
6	5.875	471	474	475	rBV2	2204	2174	0.16%	0.016%
7	6.051	502	504	505	rVV2	1686	1378	0.10%	0.010%
8	6.304	544	547	551	rBV6	2039	2927	0.22%	0.021%
9	6.334	551	552	555	rVB2	1792	1479	0.11%	0.011%
10	6.410	562	565	566	rBV3	1158	1400	0.11%	0.010%
11	6.798	624	631	645	rBV	239404	433332	32.52%	3.167%
12	6.887	645	646	652	rVB6	3183	3983	0.30%	0.029%
13	6.969	655	660	672	rBV	208080	343766	25.80%	2.512%
14	7.087	678	680	682	rBV2	1636	1389	0.10%	0.010%
15	7.151	685	691	703	rVV	258205	447119	33.56%	3.268%
16	7.275	710	712	717	rVB4	1122	1390	0.10%	0.010%
17	7.345	720	724	728	rBV3	1340	1453	0.11%	0.011%
18	7.616	762	770	778	rBV	210059	345826	25.96%	2.527%
19	7.669	778	779	784	rVV4	1770	2469	0.19%	0.018%
20	7.781	797	798	802	rVB2	1319	1358	0.10%	0.010%
21	7.892	815	817	820	rBV2	1971	1598	0.12%	0.012%
22	8.322	884	890	906	rBV	275797	506526	38.02%	3.702%
23	8.604	934	938	940	rBV4	1400	1483	0.11%	0.011%
24	8.775	959	967	980	rBV	233870	411410	30.88%	3.007%
25	9.016	1004	1008	1011	rVB4	1376	1690	0.13%	0.012%
26	9.428	1074	1078	1081	rVB4	1654	1954	0.15%	0.014%
27	9.486	1081	1088	1101	rBV	195612	350333	26.30%	2.560%
28	9.639	1112	1114	1119	rVB6	1119	1644	0.12%	0.012%
29	10.022	1172	1179	1199	rBV	228598	491341	36.88%	3.591%
30	10.263	1218	1220	1226	rVB6	1283	1962	0.15%	0.014%
31	10.386	1234	1241	1253	rVB	264526	458258	34.40%	3.349%
32	10.551	1261	1269	1285	rBV	201156	493320	37.03%	3.605%
33	11.233	1382	1385	1387	rBV3	1489	1884	0.14%	0.014%
34	11.363	1405	1407	1409	rBV3	1548	1367	0.10%	0.010%
35	11.422	1411	1417	1419	rVB7	1094	1893	0.14%	0.014%
36	12.016	1513	1518	1525	rBV6	3096	5789	0.43%	0.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045170.D
 Acq On : 12 Apr 2024 14:11
 Operator : MA/JU
 Sample : PB160112BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK112

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	12.186	1544	1547	1550	rBV3	1456	2118	0.16%	0.015%
38	12.510	1599	1602	1604	rBV3	1471	1636	0.12%	0.012%
39	13.157	1707	1712	1715	rBV5	2571	2821	0.21%	0.021%
40	13.227	1721	1724	1726	rBV3	1173	1361	0.10%	0.010%

41	13.692	1797	1803	1818	rVB	422307	654612	49.13%	4.784%
42	13.951	1840	1847	1862	rBV	543603	855278	64.19%	6.251%
43	14.174	1883	1885	1887	rBV3	1898	1825	0.14%	0.013%
44	14.263	1893	1900	1913	rBV	372308	554210	41.60%	4.050%
45	14.516	1936	1943	1963	rBV4	68256	250268	18.78%	1.829%

46	14.645	1963	1965	1971	rVB6	3495	5471	0.41%	0.040%
47	14.810	1990	1993	1996	rVB5	1555	1830	0.14%	0.013%
48	15.263	2063	2070	2079	rBV	641962	1005168	75.45%	7.346%
49	15.321	2079	2080	2085	rVB4	3383	2237	0.17%	0.016%
50	15.410	2089	2095	2105	rBV	139689	223890	16.80%	1.636%

51	15.510	2110	2112	2116	rVV3	4254	5086	0.38%	0.037%
52	15.880	2172	2175	2178	rVB3	1447	1672	0.13%	0.012%
53	16.215	2229	2232	2236	rVB3	1237	1519	0.11%	0.011%
54	16.815	2330	2334	2335	rBV2	1663	1579	0.12%	0.012%
55	17.021	2363	2369	2379	rBV	410060	576553	43.27%	4.214%

56	17.121	2379	2386	2402	rBV2	669829	1027706	77.14%	7.511%
57	17.262	2407	2410	2411	rVB3	1809	1530	0.11%	0.011%
58	17.298	2414	2416	2420	rVB5	1459	1437	0.11%	0.011%
59	17.551	2457	2459	2462	rBV4	2318	2841	0.21%	0.021%
60	17.609	2467	2469	2472	rVV3	1514	1974	0.15%	0.014%

61	17.668	2472	2479	2481	rVV7	1551	3298	0.25%	0.024%
62	17.980	2530	2532	2534	rVB3	2124	1784	0.13%	0.013%
63	18.009	2534	2537	2539	rBV3	1756	2502	0.19%	0.018%
64	18.068	2544	2547	2550	rBV5	1295	1344	0.10%	0.010%
65	18.151	2559	2561	2564	rVV3	1646	1940	0.15%	0.014%

66	18.192	2564	2568	2571	rVB4	1650	2455	0.18%	0.018%
67	18.239	2571	2576	2579	rBV6	1569	3418	0.26%	0.025%
68	18.315	2587	2589	2592	rBV3	1451	1484	0.11%	0.011%
69	18.539	2625	2627	2629	rBV3	1733	1610	0.12%	0.012%
70	18.845	2676	2679	2682	rBV5	1491	2542	0.19%	0.019%

71	18.874	2682	2684	2688	rVB5	1740	2089	0.16%	0.015%
72	18.927	2688	2693	2694	rBV4	2625	2795	0.21%	0.020%
73	18.992	2701	2704	2709	rBV3	6910	9238	0.69%	0.068%
74	19.068	2713	2717	2721	rBV3	4976	7917	0.59%	0.058%
75	19.168	2730	2734	2736	rBV5	1400	1901	0.14%	0.014%

76	19.239	2744	2746	2748	rBV3	1712	1573	0.12%	0.011%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045170.D
Acq On : 12 Apr 2024 14:11
Operator : MA/JU
Sample : PB160112BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK112

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

77	19.427	2772	2778	2793	rBV	793560	1133810	85.10%	8.286%
78	21.233	3080	3085	3094	rBV	381971	581959	43.68%	4.253%
79	23.309	3431	3438	3452	rBV2	674420	1332316	100.00%	9.737%
80	23.450	3456	3462	3473	rVB	345437	709973	53.29%	5.189%


Sum of corrected areas: 13683203

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045170.D
Acq On : 12 Apr 2024 14:11
Operator : MA/JU
Sample : PB160112BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK112

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

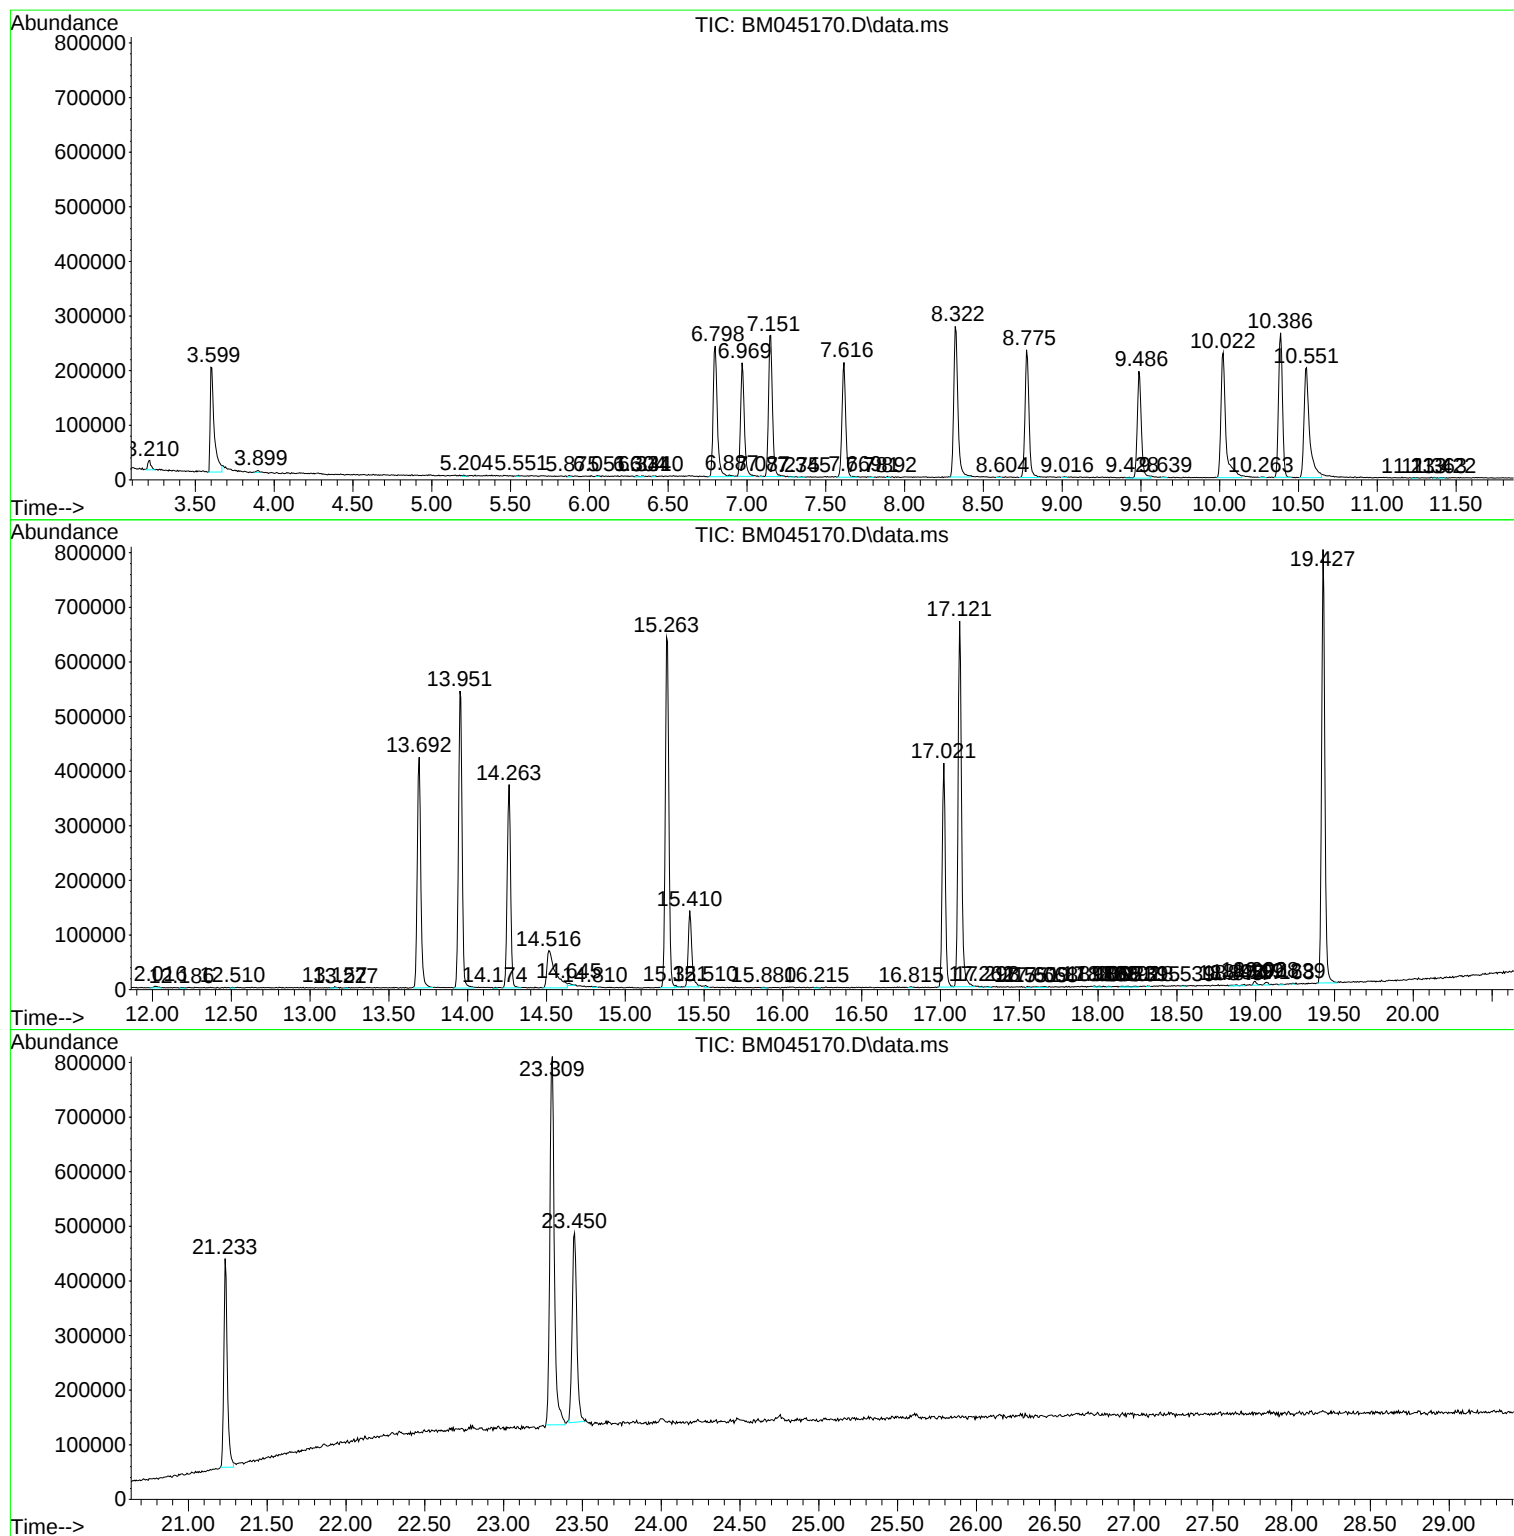

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045170.D
Acq On : 12 Apr 2024 14:11
Operator : MA/JU
Sample : PB160112BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK112

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045170.D
Acq On : 12 Apr 2024 14:11
Operator : MA/JU
Sample : PB160112BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK112

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------