

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045171.D
 Acq On : 12 Apr 2024 14:48
 Operator : MA/JU
 Sample : PB160113BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK113

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045171.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.204	16	20	26	rBV	19566	25682	1.64%	0.156%
2	3.599	85	87	104	rBV	193895	353079	22.53%	2.150%
3	3.822	123	125	129	rVB5	2238	1778	0.11%	0.011%
4	3.963	147	149	152	rVB4	2468	1823	0.12%	0.011%
5	4.099	170	172	175	rBV4	1828	1778	0.11%	0.011%
6	4.269	199	201	204	rBV5	1288	1813	0.12%	0.011%
7	4.387	219	221	224	rBV4	1362	1617	0.10%	0.010%
8	4.957	313	318	319	rBV5	1421	2009	0.13%	0.012%
9	5.198	358	359	362	rBV2	1944	1813	0.12%	0.011%
10	5.245	364	367	370	rBV4	1894	2698	0.17%	0.016%
11	6.257	536	539	540	rBV3	1327	1592	0.10%	0.010%
12	6.428	565	568	570	rBV3	1070	1586	0.10%	0.010%
13	6.492	575	579	581	rBV4	1439	2058	0.13%	0.013%
14	6.651	603	606	608	rVB3	1353	1728	0.11%	0.011%
15	6.681	610	611	614	rVV3	1941	2028	0.13%	0.012%
16	6.798	623	631	647	rBV	250344	456924	29.16%	2.782%
17	6.969	654	660	678	rVB	226344	379937	24.25%	2.313%
18	7.151	682	691	704	rBV	278104	478756	30.55%	2.915%
19	7.310	714	718	720	rVB4	1940	2337	0.15%	0.014%
20	7.363	723	727	729	rVV4	1301	1844	0.12%	0.011%
21	7.616	764	770	780	rVV	208026	345751	22.06%	2.105%
22	7.769	793	796	800	rBV5	1067	1667	0.11%	0.010%
23	8.251	876	878	881	rVB3	1536	1747	0.11%	0.011%
24	8.322	884	890	903	rBV	317264	563332	35.95%	3.430%
25	8.592	932	936	937	rVB4	1599	1943	0.12%	0.012%
26	8.775	959	967	977	rBV	266901	465647	29.72%	2.835%
27	8.886	984	986	989	rVB4	1308	1611	0.10%	0.010%
28	9.345	1061	1064	1067	rBV4	2103	3460	0.22%	0.021%
29	9.380	1067	1070	1072	rVV3	1646	2077	0.13%	0.013%
30	9.428	1075	1078	1081	rVV3	1225	1765	0.11%	0.011%
31	9.486	1081	1088	1103	rVV	217437	388560	24.80%	2.366%
32	10.022	1170	1179	1206	rBV	271560	569900	36.37%	3.470%
33	10.386	1233	1241	1252	rBV	295498	497346	31.74%	3.028%
34	10.545	1261	1268	1288	rBV	279774	636984	40.65%	3.878%
35	10.880	1323	1325	1332	rBB6	1326	2759	0.18%	0.017%
36	11.163	1371	1373	1376	rBV3	1463	1868	0.12%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045171.D
 Acq On : 12 Apr 2024 14:48
 Operator : MA/JU
 Sample : PB160113BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK113

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	11.304	1394	1397	1401	rBV3	1320	1862	0.12%	0.011%
38	11.939	1501	1505	1508	rVB4	1140	1709	0.11%	0.010%
39	12.016	1512	1518	1523	rVV3	3145	6111	0.39%	0.037%
40	12.233	1552	1555	1558	rBV3	1569	1815	0.12%	0.011%
41	13.057	1693	1695	1701	rVB5	1166	1575	0.10%	0.010%
42	13.157	1707	1712	1719	rBV4	3300	5475	0.35%	0.033%
43	13.539	1773	1777	1780	rVB3	1021	1603	0.10%	0.010%
44	13.692	1796	1803	1814	rBV	587237	916886	58.51%	5.582%
45	13.951	1840	1847	1862	rBV	716041	1105086	70.52%	6.728%
46	14.263	1893	1900	1911	rBV	461875	672565	42.92%	4.095%
47	14.510	1936	1942	1962	rBV	108752	348199	22.22%	2.120%
48	14.880	2002	2005	2008	rVB3	1252	1850	0.12%	0.011%
49	15.262	2064	2070	2086	rBV	897045	1345866	85.89%	8.194%
50	15.410	2088	2095	2104	rBV	211781	335849	21.43%	2.045%
51	15.510	2109	2112	2119	rVB6	3457	6080	0.39%	0.037%
52	15.833	2165	2167	2172	rBV4	1462	2167	0.14%	0.013%
53	16.051	2200	2204	2205	rBV4	1717	2056	0.13%	0.013%
54	16.074	2207	2208	2213	rVB4	1518	1986	0.13%	0.012%
55	16.180	2221	2226	2227	rVB3	1447	1886	0.12%	0.011%
56	16.951	2353	2357	2361	rVB6	1872	3066	0.20%	0.019%
57	17.021	2363	2369	2379	rVV	555212	756650	48.29%	4.607%
58	17.121	2379	2386	2399	rVV	983363	1442112	92.03%	8.780%
59	17.445	2439	2441	2445	rVB4	1443	1790	0.11%	0.011%
60	17.709	2483	2486	2488	rBV3	1886	1955	0.12%	0.012%
61	17.951	2524	2527	2528	rBV3	1535	1776	0.11%	0.011%
62	17.968	2528	2530	2533	rVB3	2404	2762	0.18%	0.017%
63	18.821	2673	2675	2677	rBV3	1791	1886	0.12%	0.011%
64	18.992	2700	2704	2709	rBV3	9594	12728	0.81%	0.077%
65	19.062	2713	2716	2720	rBV	7514	10182	0.65%	0.062%
66	19.239	2744	2746	2747	rBV	2196	1662	0.11%	0.010%
67	19.427	2772	2778	2790	rBV	1122184	1566971	100.00%	9.540%
68	19.545	2796	2798	2801	rBV4	2307	3219	0.21%	0.020%
69	19.721	2826	2828	2831	rBV4	2269	2658	0.17%	0.016%
70	21.233	3080	3085	3095	rBV	455150	677060	43.21%	4.122%
71	23.303	3431	3437	3453	rBV2	670756	1326938	84.68%	8.079%
72	23.450	3456	3462	3473	rVB	308117	641633	40.95%	3.906%




Sum of corrected areas: 16424971

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045171.D
Acq On : 12 Apr 2024 14:48
Operator : MA/JU
Sample : PB160113BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK113

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

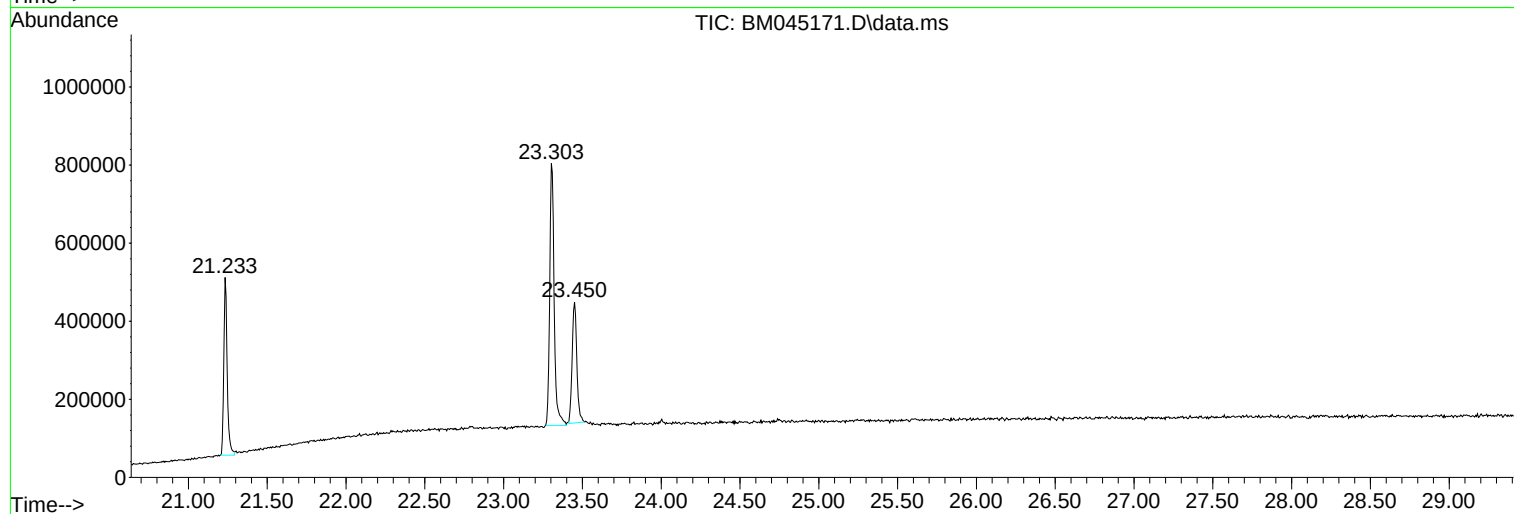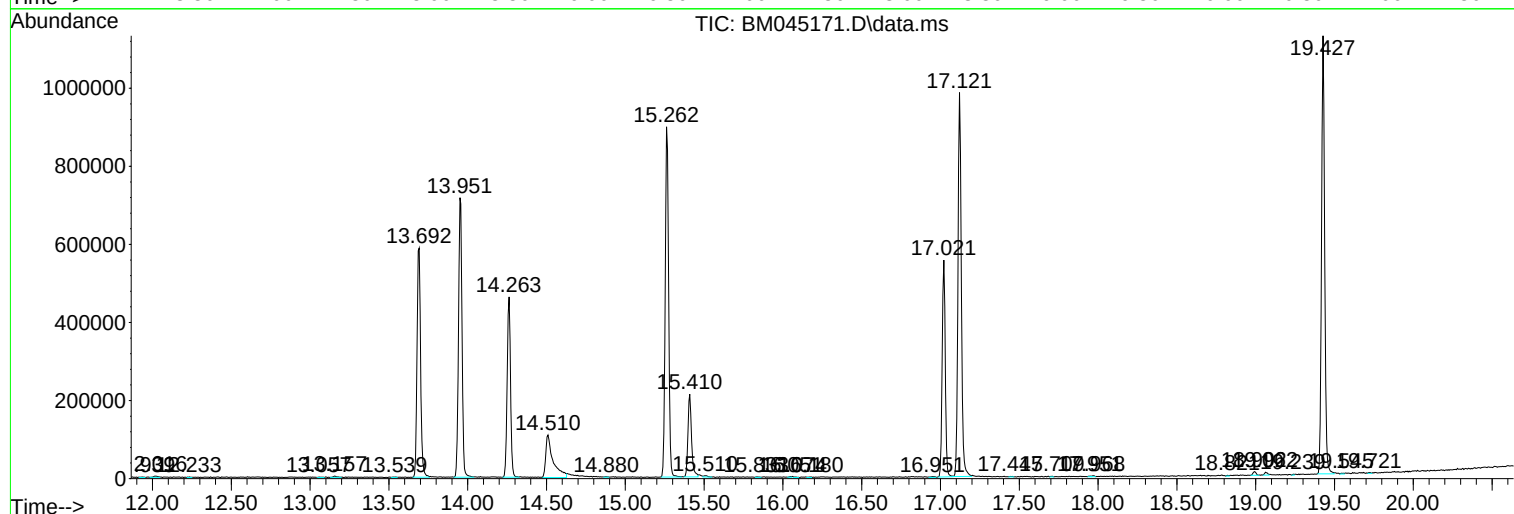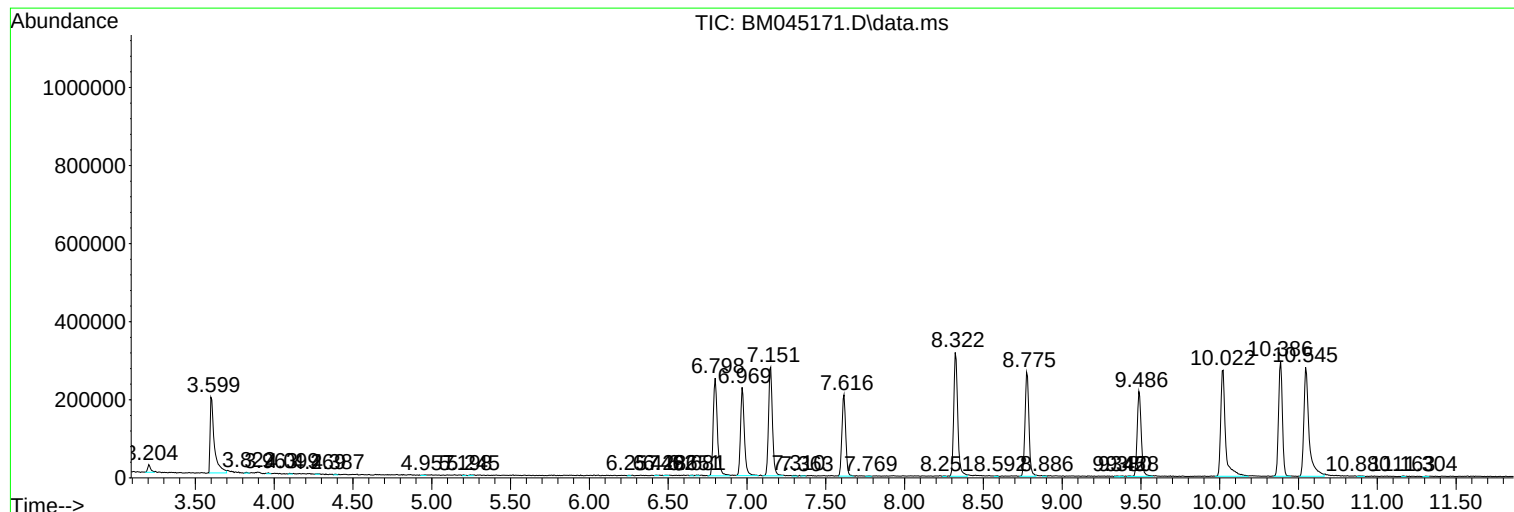

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045171.D
Acq On : 12 Apr 2024 14:48
Operator : MA/JU
Sample : PB160113BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK113

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045171.D
Acq On : 12 Apr 2024 14:48
Operator : MA/JU
Sample : PB160113BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK113

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc