

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045172.D
Acq On : 12 Apr 2024 15:24
Operator : MA/JU
Sample : P2006-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0R44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

Signal : TIC: BM045172.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	17	20	30	rVB2	10329	16699	0.74%	0.086%
2	3.652	92	96	99	rBV4	4657	8197	0.36%	0.042%
3	4.005	154	156	159	rBV3	2132	2573	0.11%	0.013%
4	4.093	169	171	174	rBV3	2873	2399	0.11%	0.012%
5	4.287	202	204	209	rVB6	2197	2593	0.11%	0.013%
6	4.446	229	231	234	rVB4	2206	2466	0.11%	0.013%
7	6.698	611	614	615	rBV3	1958	2323	0.10%	0.012%
8	6.804	625	632	647	rBV2	48582	105004	4.64%	0.540%
9	6.969	654	660	671	rBV	269341	436296	19.26%	2.244%
10	7.151	684	691	699	rBV	235312	407934	18.01%	2.098%
11	7.616	762	770	780	rBV	257880	428464	18.92%	2.204%
12	8.328	884	891	900	rBV	170978	309277	13.66%	1.591%
13	8.775	960	967	980	rBV	327820	550466	24.30%	2.831%
14	9.081	1016	1019	1022	rBV4	1321	2291	0.10%	0.012%
15	9.134	1024	1028	1032	rVB2	7962	11221	0.50%	0.058%
16	9.316	1055	1059	1066	rBV5	1021	2282	0.10%	0.012%
17	9.487	1080	1088	1100	rBV	253483	443433	19.58%	2.281%
18	10.022	1171	1179	1200	rBV	289827	617445	27.26%	3.176%
19	10.386	1234	1241	1253	rVB	359610	606599	26.78%	3.120%
20	10.551	1262	1269	1289	rBV	121779	306919	13.55%	1.579%
21	11.622	1446	1451	1455	rVB5	1477	2761	0.12%	0.014%
22	12.010	1513	1517	1522	rVB5	5012	10180	0.45%	0.052%
23	12.898	1664	1668	1673	rVB6	1895	3342	0.15%	0.017%
24	13.163	1707	1713	1717	rVB4	4745	7613	0.34%	0.039%
25	13.692	1796	1803	1813	rBV	792928	1183955	52.27%	6.089%
26	13.951	1841	1847	1859	rBV2	903179	1351131	59.65%	6.949%
27	14.263	1893	1900	1911	rBV	568964	834729	36.85%	4.293%
28	14.539	1943	1947	1956	rBV6	12479	41038	1.81%	0.211%
29	14.663	1966	1968	1972	rVB5	2416	2789	0.12%	0.014%
30	15.045	2026	2033	2035	rBV4	1745	2755	0.12%	0.014%
31	15.121	2042	2046	2051	rBV6	2836	5243	0.23%	0.027%
32	15.263	2063	2070	2082	rBV	1197479	1800376	79.49%	9.260%
33	15.410	2089	2095	2108	rBV	327563	504299	22.27%	2.594%
34	15.504	2108	2111	2117	rVB7	5241	9726	0.43%	0.050%
35	15.992	2189	2194	2196	rBV5	2404	3088	0.14%	0.016%
36	16.057	2198	2205	2209	rVB4	2800	4728	0.21%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045172.D
 Acq On : 12 Apr 2024 15:24
 Operator : MA/JU
 Sample : P2006-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MC0R44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	16.574	2291	2293	2298	rBV6	1599	2325	0.10%	0.012%
38	17.021	2363	2369	2379	rBV	719749	955784	42.20%	4.916%
39	17.121	2379	2386	2402	rVV2	1366360	2000284	88.32%	10.288%
40	17.498	2444	2450	2454	rBV8	1601	3520	0.16%	0.018%
41	17.592	2464	2466	2472	rVB4	1325	2436	0.11%	0.013%
42	17.933	2516	2524	2535	rBV2	51143	81970	3.62%	0.422%
43	18.139	2556	2559	2564	rBV2	14359	19216	0.85%	0.099%
44	18.362	2593	2597	2601	rBV5	7472	8385	0.37%	0.043%
45	18.480	2614	2617	2620	rBV3	2418	3378	0.15%	0.017%
46	18.662	2644	2648	2650	rBV5	1440	2474	0.11%	0.013%
47	18.874	2680	2684	2685	rVB3	2564	2828	0.12%	0.015%
48	18.904	2685	2689	2690	rBV3	3758	4632	0.20%	0.024%
49	18.992	2700	2704	2710	rBV3	13634	18262	0.81%	0.094%
50	19.068	2713	2717	2721	rBV2	11234	18700	0.83%	0.096%
51	19.168	2730	2734	2736	rVB5	2296	2732	0.12%	0.014%
52	19.227	2740	2744	2750	rBV3	21314	33158	1.46%	0.171%
53	19.380	2767	2770	2772	rBV4	2297	2625	0.12%	0.014%
54	19.427	2772	2778	2789	rBV	1641141	2264921	100.00%	11.649%
55	19.992	2867	2874	2878	rBV8	6717	14872	0.66%	0.076%
56	20.498	2956	2960	2962	rVB5	8931	10696	0.47%	0.055%
57	20.962	3034	3039	3047	rBV3	57001	113465	5.01%	0.584%
58	21.233	3080	3085	3098	rBV	700093	950995	41.99%	4.891%
59	21.398	3111	3113	3119	rBV4	18758	23356	1.03%	0.120%
60	23.309	3431	3438	3445	rBV	1056651	1960749	86.57%	10.085%
61	23.444	3455	3461	3472	rVB	457022	908558	40.11%	4.673%




Sum of corrected areas: 19442955

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045172.D
Acq On : 12 Apr 2024 15:24
Operator : MA/JU
Sample : P2006-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0R44

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

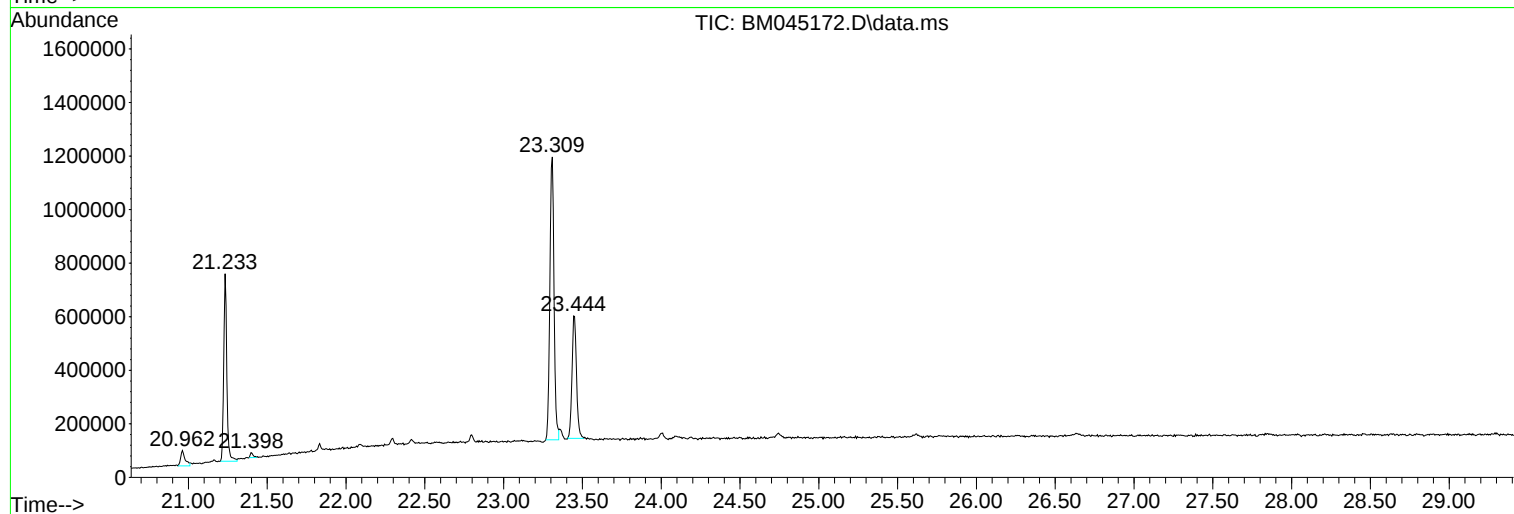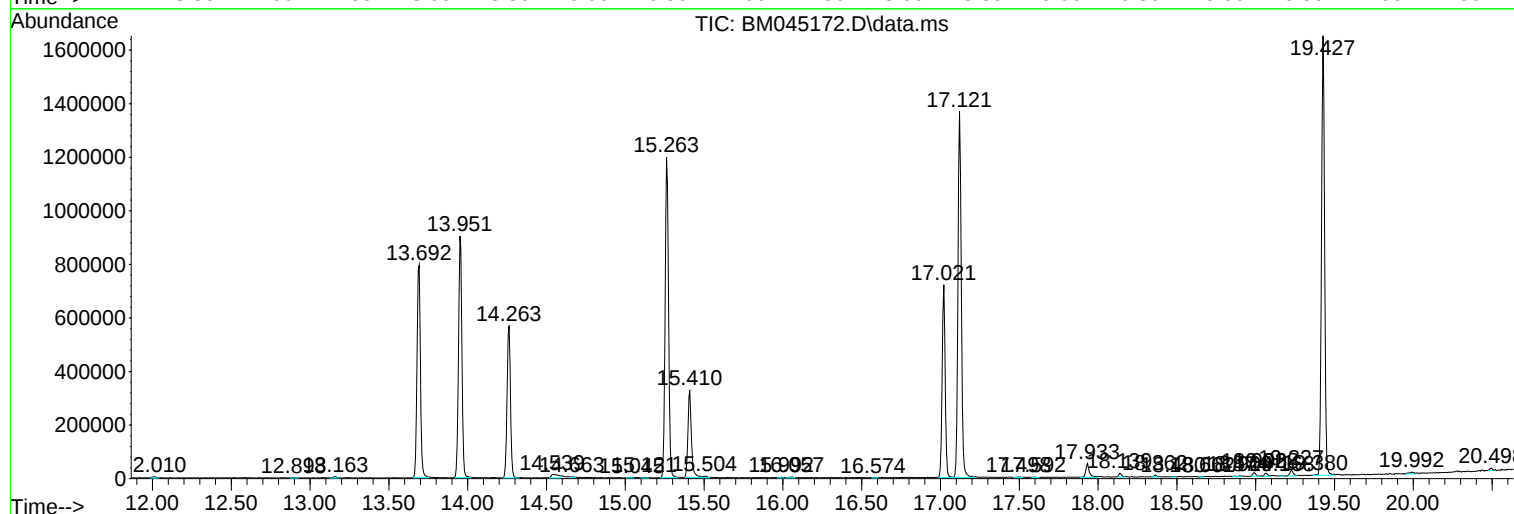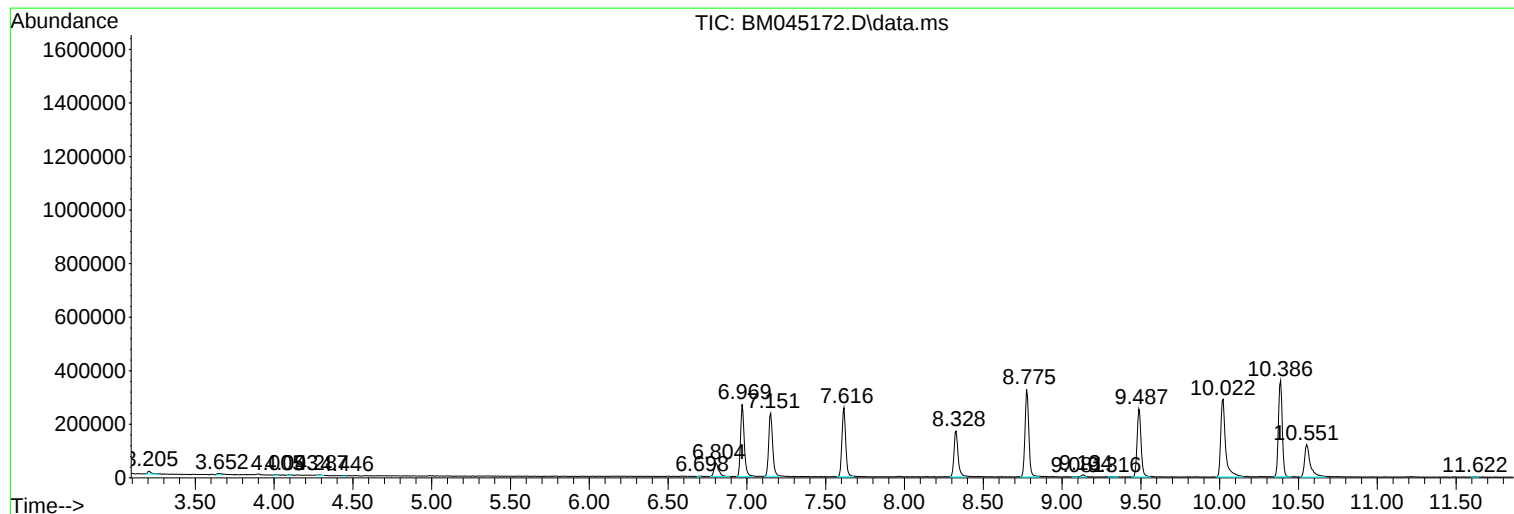

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045172.D
Acq On : 12 Apr 2024 15:24
Operator : MA/JU
Sample : P2006-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MCOR44










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Pentadecafluorooctanoic aci... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.962	2.39 ng/ul	113465	Chrysene-d12	21.233

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	90
2			Ethanol, 2-(tetradecyloxy)-	258	C16H34O2	002136-70-1	81
3			Hexadecyl propyl ether	284	C19H40O	1000406-27-9	81
4			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	76
5			Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	76

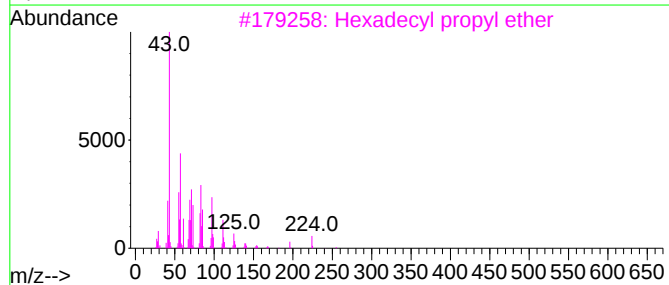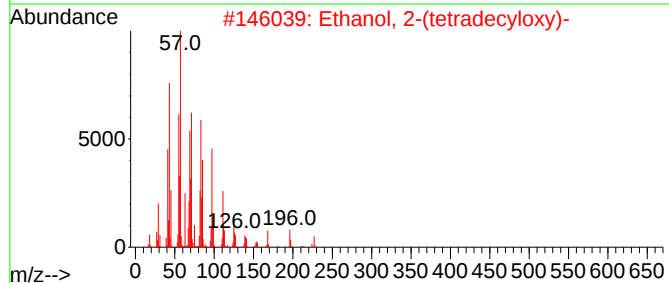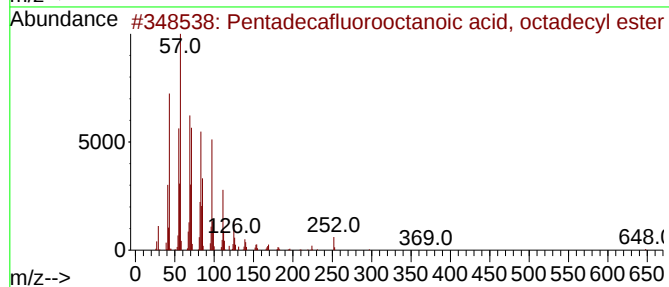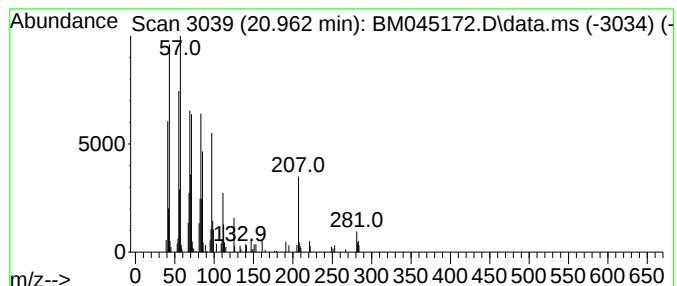

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045172.D
Acq On : 12 Apr 2024 15:24
Operator : MA/JU
Sample : P2006-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0R44

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Pentadecafluoro...	20.962	2.4	ng/u1	113465	5	21.233	950995	20.0