

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045174.D
 Acq On : 12 Apr 2024 16:37
 Operator : MA/JU
 Sample : P2006-03
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MC0R56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045174.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	17	20	25	rVB2	11953	14744	0.72%	0.080%
2	3.575	81	83	85	rBV3	2592	2717	0.13%	0.015%
3	3.616	86	90	104	rBV	42860	94224	4.62%	0.511%
4	3.893	134	137	144	rVB3	3686	5597	0.27%	0.030%
5	4.152	179	181	184	rVV4	1966	2055	0.10%	0.011%
6	4.981	317	322	329	rVB	18960	29000	1.42%	0.157%
7	5.257	367	369	372	rBV4	1703	2193	0.11%	0.012%
8	6.569	589	592	596	rBV5	1788	2819	0.14%	0.015%
9	6.769	622	626	627	rBV4	1580	2222	0.11%	0.012%
10	6.804	627	632	643	rVB	48168	97966	4.81%	0.532%
11	6.969	654	660	674	rBV	261595	427238	20.97%	2.319%
12	7.151	684	691	701	rBV	230656	404546	19.86%	2.195%
13	7.310	716	718	721	rVB3	2341	2040	0.10%	0.011%
14	7.504	747	751	754	rVB5	1750	2121	0.10%	0.012%
15	7.616	762	770	788	rBV	272760	477277	23.43%	2.590%
16	7.863	809	812	815	rBV3	2520	2785	0.14%	0.015%
17	7.969	826	830	834	rVB6	2885	4076	0.20%	0.022%
18	8.322	884	890	904	rBV	169038	313884	15.41%	1.703%
19	8.775	960	967	979	rBV	320414	546909	26.84%	2.968%
20	8.951	994	997	1002	rVV6	1503	2182	0.11%	0.012%
21	9.022	1004	1009	1012	rVB5	1523	2561	0.13%	0.014%
22	9.134	1024	1028	1035	rVB6	2788	4771	0.23%	0.026%
23	9.487	1081	1088	1098	rBV	256075	438260	21.51%	2.378%
24	10.016	1171	1178	1196	rBV	298334	599807	29.44%	3.255%
25	10.145	1198	1200	1207	rVB6	2464	3827	0.19%	0.021%
26	10.386	1233	1241	1247	rBV	373708	639097	31.37%	3.468%
27	10.545	1261	1268	1287	rBV	258725	576215	28.28%	3.127%
28	10.710	1293	1296	1298	rBV3	1678	2111	0.10%	0.011%
29	11.616	1447	1450	1456	rVB5	2455	3746	0.18%	0.020%
30	12.010	1512	1517	1523	rBV5	4391	8241	0.40%	0.045%
31	12.275	1560	1562	1566	rVB4	1460	2038	0.10%	0.011%
32	13.157	1708	1712	1716	rBV4	3146	4246	0.21%	0.023%
33	13.686	1796	1802	1814	rBV	730337	1131868	55.56%	6.142%
34	13.951	1840	1847	1862	rBV	896063	1343671	65.95%	7.292%
35	14.263	1893	1900	1911	rVV	588500	861341	42.28%	4.674%
36	14.345	1911	1914	1918	rVB5	1590	2479	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045174.D
 Acq On : 12 Apr 2024 16:37
 Operator : MA/JU
 Sample : P2006-03
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MC0R56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	14.557	1942	1950	1952	rBV6	11663	25508	1.25%	0.138%
38	14.745	1980	1982	1987	rVB5	2378	3052	0.15%	0.017%
39	14.780	1987	1988	1993	rVB3	1749	2065	0.10%	0.011%
40	15.263	2063	2070	2081	rVV	1160053	1701549	83.52%	9.234%
41	15.410	2089	2095	2104	rBV	295626	462702	22.71%	2.511%
42	15.510	2110	2112	2116	rVB5	5752	5870	0.29%	0.032%
43	16.057	2200	2205	2207	rBV5	3141	3623	0.18%	0.020%
44	16.315	2244	2249	2252	rVB7	1142	2123	0.10%	0.012%
45	17.021	2363	2369	2379	rBV	692491	935364	45.91%	5.076%
46	17.121	2379	2386	2401	rVV	1292706	1887027	92.62%	10.240%
47	17.333	2419	2422	2426	rVB6	1948	2621	0.13%	0.014%
48	17.933	2519	2524	2531	rBV4	21201	36765	1.80%	0.200%
49	18.262	2577	2580	2582	rBV3	1835	2516	0.12%	0.014%
50	18.704	2653	2655	2657	rBV3	1958	2285	0.11%	0.012%
51	18.945	2692	2696	2698	rBV4	1929	2655	0.13%	0.014%
52	18.992	2700	2704	2708	rVV3	12924	17154	0.84%	0.093%
53	19.062	2711	2716	2725	rVV2	10501	16867	0.83%	0.092%
54	19.227	2741	2744	2747	rBV5	11650	15780	0.77%	0.086%
55	19.427	2772	2778	2791	rBV	1488561	2037297	100.00%	11.056%
56	19.756	2832	2834	2836	rBV3	3021	2808	0.14%	0.015%
57	20.186	2905	2907	2909	rBV3	3003	3094	0.15%	0.017%
58	20.956	3036	3038	3044	rBV6	11422	16400	0.80%	0.089%
59	21.233	3080	3085	3095	rBV	554271	780120	38.29%	4.234%
60	23.303	3431	3437	3450	rBV2	858261	1610446	79.05%	8.740%
61	23.444	3455	3461	3476	rVB2	376737	790643	38.81%	4.291%




Sum of corrected areas: 18427208

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045174.D
Acq On : 12 Apr 2024 16:37
Operator : MA/JU
Sample : P2006-03
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0R56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

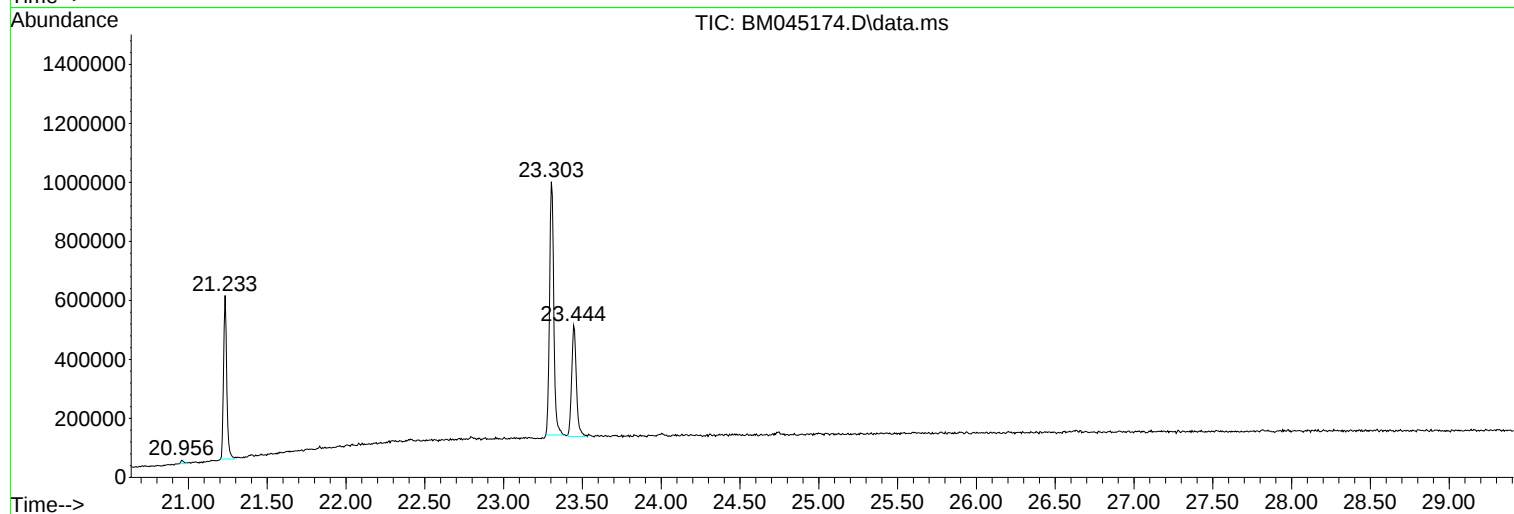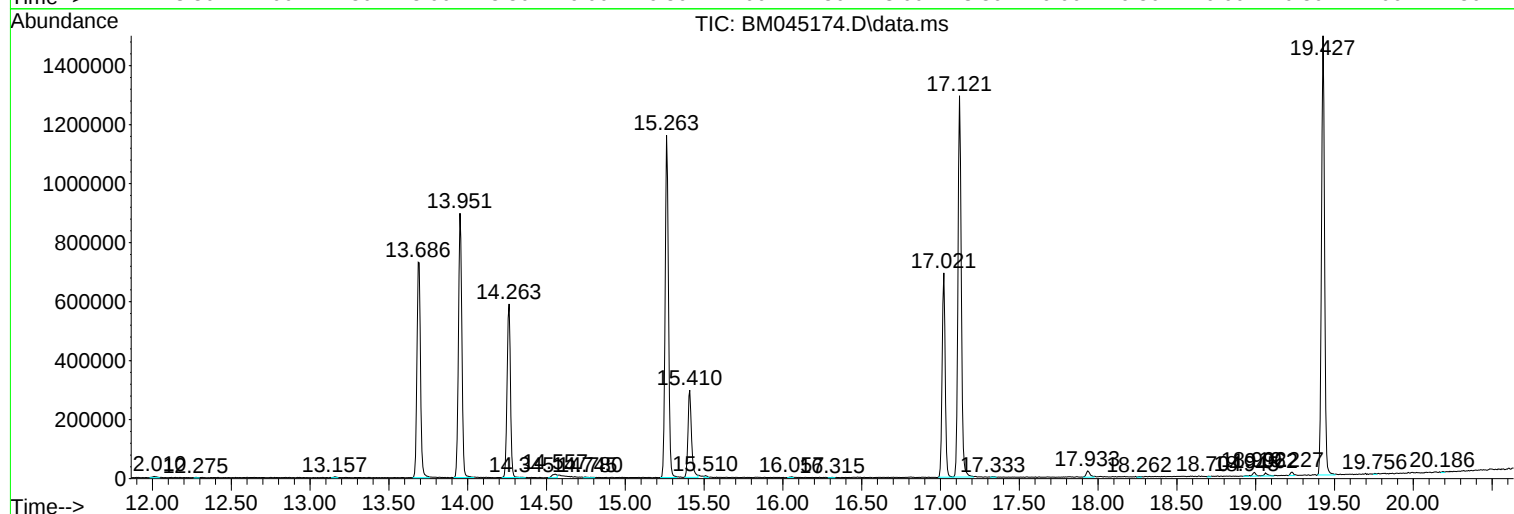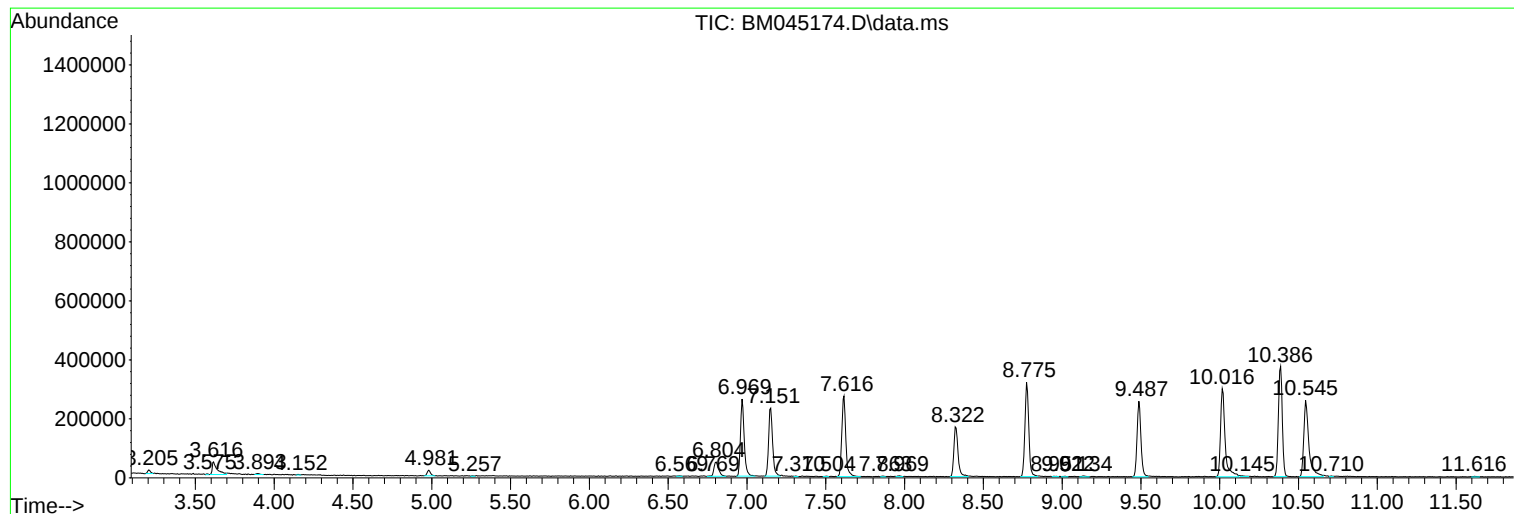

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045174.D
Acq On : 12 Apr 2024 16:37
Operator : MA/JU
Sample : P2006-03
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0R56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045174.D
Acq On : 12 Apr 2024 16:37
Operator : MA/JU
Sample : P2006-03
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0R56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc