

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045175.D
 Acq On : 12 Apr 2024 17:35
 Operator : MA/JU
 Sample : P2006-04
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MC0R63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045175.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	25	rBV3	11864	16701	0.80%	0.092%
2	3.616	87	90	99	rBV	33842	68677	3.30%	0.379%
3	3.893	134	137	143	rVB4	5022	10219	0.49%	0.056%
4	3.999	153	155	159	rBV5	2211	2767	0.13%	0.015%
5	4.881	302	305	308	rBV5	1639	2608	0.13%	0.014%
6	6.387	560	561	568	rBV7	1867	2996	0.14%	0.017%
7	6.510	579	582	585	rVB4	1984	2945	0.14%	0.016%
8	6.804	626	632	642	rBV	36498	73898	3.55%	0.408%
9	6.969	651	660	672	rBV	254377	428247	20.60%	2.364%
10	7.151	685	691	701	rBV	219350	376190	18.09%	2.076%
11	7.616	763	770	779	rBV	268056	439942	21.16%	2.428%
12	7.687	779	782	787	rVB4	3716	4965	0.24%	0.027%
13	7.845	806	809	814	rVV4	1314	2529	0.12%	0.014%
14	8.328	884	891	907	rBV	142291	258619	12.44%	1.427%
15	8.775	961	967	978	rBV	303679	519576	24.99%	2.868%
16	9.128	1026	1027	1033	rVB4	2553	3100	0.15%	0.017%
17	9.486	1081	1088	1099	rBV	235085	417193	20.06%	2.303%
18	10.022	1172	1179	1205	rBV	276680	548367	26.37%	3.027%
19	10.386	1233	1241	1251	rBV	382439	621777	29.90%	3.432%
20	10.545	1260	1268	1291	rBV	231229	550730	26.49%	3.040%
21	11.116	1358	1365	1374	rBV7	7018	12786	0.61%	0.071%
22	11.457	1420	1423	1427	rBV4	1840	2707	0.13%	0.015%
23	12.016	1513	1518	1524	rVB5	4321	7806	0.38%	0.043%
24	12.786	1643	1649	1651	rBV4	1898	2313	0.11%	0.013%
25	13.163	1708	1713	1718	rVB4	4189	6611	0.32%	0.036%
26	13.692	1796	1803	1818	rBV	725794	1073617	51.63%	5.926%
27	13.957	1841	1848	1856	rBV	833838	1245236	59.89%	6.873%
28	14.263	1893	1900	1910	rBV	585377	837873	40.30%	4.625%
29	14.569	1944	1952	1965	rBV10	7653	32404	1.56%	0.179%
30	14.657	1965	1967	1971	rVB4	1822	2118	0.10%	0.012%
31	15.268	2064	2071	2079	rBV	1062101	1619676	77.90%	8.940%
32	15.410	2089	2095	2109	rBV	284972	442273	21.27%	2.441%
33	15.510	2109	2112	2118	rVB6	4528	7857	0.38%	0.043%
34	16.057	2201	2205	2208	rBV3	3046	3384	0.16%	0.019%
35	16.804	2327	2332	2333	rBV3	1792	2224	0.11%	0.012%
36	17.021	2362	2369	2380	rBV	657604	925880	44.53%	5.111%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045175.D
 Acq On : 12 Apr 2024 17:35
 Operator : MA/JU
 Sample : P2006-04
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MC0R63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	17.121	2380	2386	2401	rVV2	1256052	1875796	90.21%	10.354%
38	17.939	2520	2525	2534	rVB6	11696	20585	0.99%	0.114%
39	18.998	2700	2705	2711	rVB4	12519	19508	0.94%	0.108%
40	19.068	2711	2717	2722	rBV3	10675	17433	0.84%	0.096%
41	19.233	2739	2745	2749	rBV8	7126	12636	0.61%	0.070%
42	19.427	2772	2778	2793	rBV	1467447	2079292	100.00%	11.477%
43	19.639	2812	2814	2817	rBV3	2852	2484	0.12%	0.014%
44	19.686	2820	2822	2826	rBV5	2365	2647	0.13%	0.015%
45	20.045	2881	2883	2886	rBV4	3834	4652	0.22%	0.026%
46	20.368	2936	2938	2941	rBV3	3580	4021	0.19%	0.022%
47	20.409	2943	2945	2947	rBV3	3878	3249	0.16%	0.018%
48	21.239	3081	3086	3095	rBV	599968	863634	41.54%	4.767%
49	23.309	3431	3438	3453	rBV2	960542	1819790	87.52%	10.045%
50	23.450	3456	3462	3472	rVB	415896	814384	39.17%	4.495%




Sum of corrected areas: 18116922

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045175.D
Acq On : 12 Apr 2024 17:35
Operator : MA/JU
Sample : P2006-04
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0R63

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

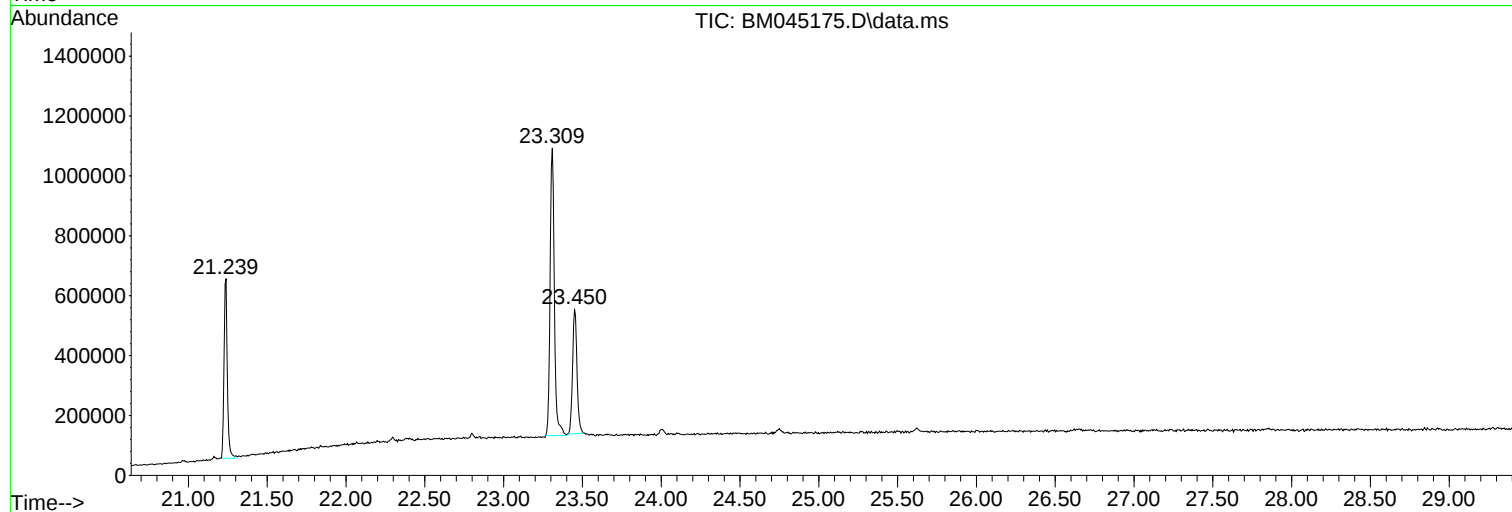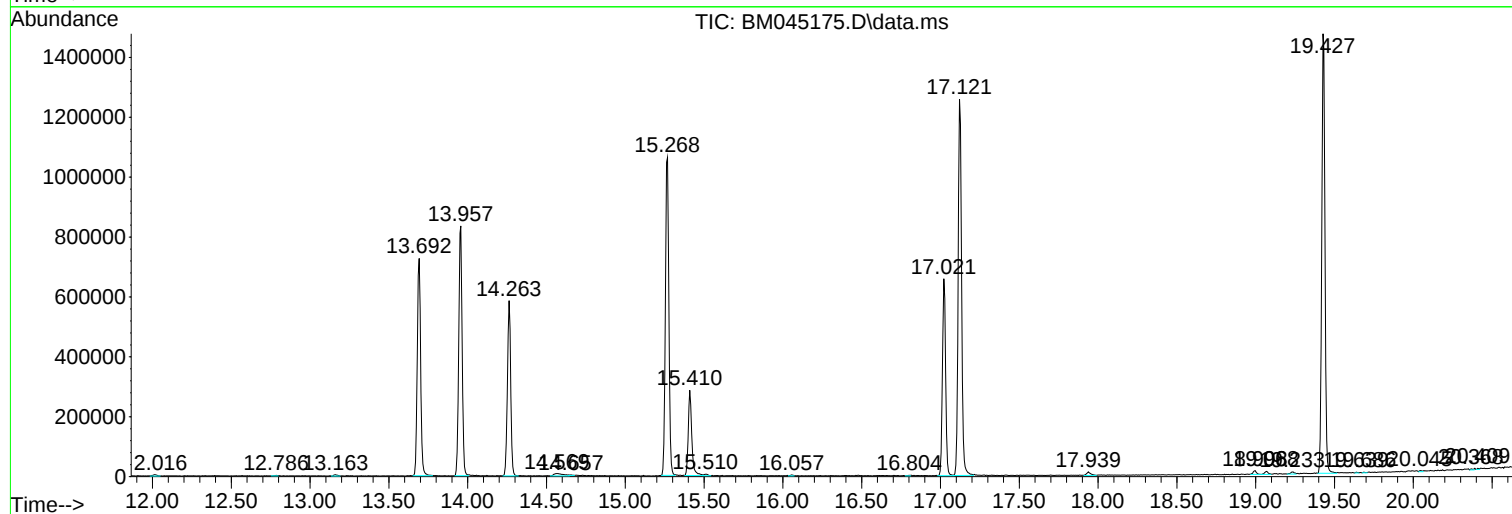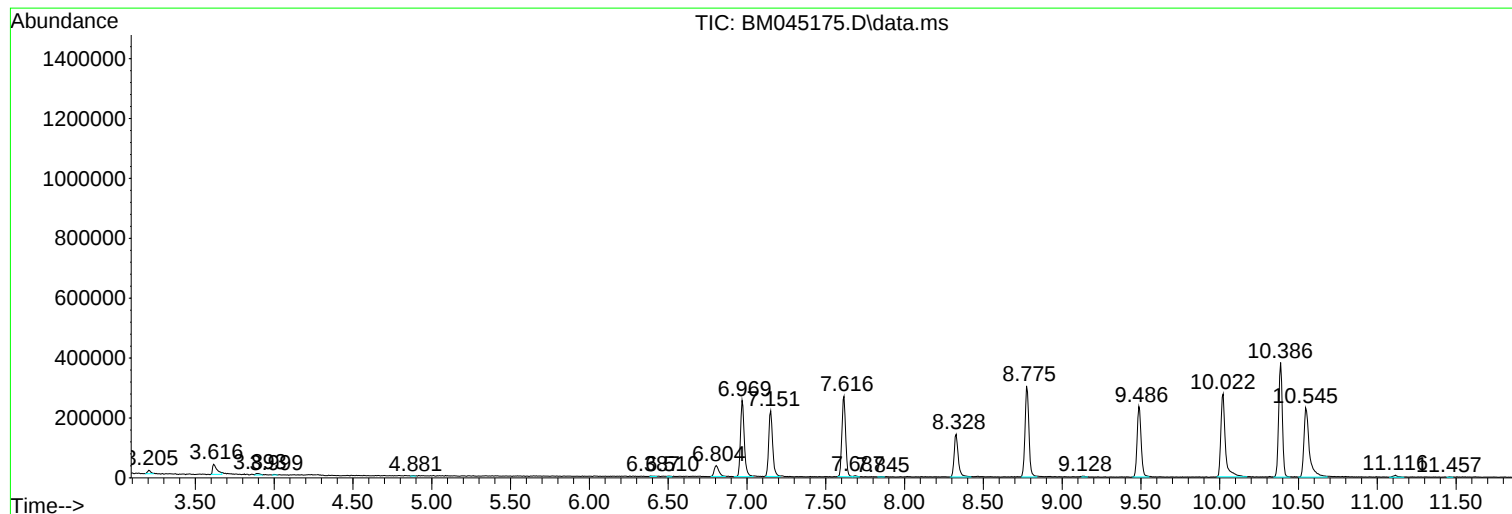

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045175.D
Acq On : 12 Apr 2024 17:35
Operator : MA/JU
Sample : P2006-04
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0R63

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045175.D
Acq On : 12 Apr 2024 17:35
Operator : MA/JU
Sample : P2006-04
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0R63

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc