

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045177.D
 Acq On : 12 Apr 2024 18:48
 Operator : MA/JU
 Sample : P2006-06
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MC0R65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045177.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	17	20	26	rVB2	12732	15711	1.16%	0.118%
2	3.623	88	91	101	rBV	24853	53783	3.97%	0.406%
3	3.893	133	137	140	rBV5	4573	6068	0.45%	0.046%
4	4.517	242	243	246	rBV3	1437	1676	0.12%	0.013%
5	4.740	280	281	282	rBV	2954	1521	0.11%	0.011%
6	4.758	282	284	286	rVB	1613	1433	0.11%	0.011%
7	4.969	319	320	323	rBV3	1774	1824	0.13%	0.014%
8	5.075	335	338	339	rBV3	1204	1416	0.10%	0.011%
9	5.128	345	347	350	rVB2	1825	1427	0.11%	0.011%
10	5.440	397	400	402	rBV3	2185	2195	0.16%	0.017%
11	6.099	508	512	518	rVB6	1755	3667	0.27%	0.028%
12	6.181	523	526	528	rVV3	1455	1653	0.12%	0.012%
13	6.234	532	535	536	rBV2	2325	2051	0.15%	0.015%
14	6.805	626	632	643	rBV	39433	82717	6.11%	0.624%
15	6.969	654	660	674	rBV	234321	392439	28.98%	2.959%
16	7.146	684	690	708	rVB	208120	377233	27.85%	2.844%
17	7.505	747	751	753	rBV4	1274	1605	0.12%	0.012%
18	7.616	763	770	782	rVB	213992	351027	25.92%	2.647%
19	8.075	844	848	851	rBV4	1385	1718	0.13%	0.013%
20	8.328	884	891	902	rBV	136439	251446	18.57%	1.896%
21	8.428	906	908	911	rVV4	1672	2094	0.15%	0.016%
22	8.469	913	915	920	rVB6	1192	1575	0.12%	0.012%
23	8.575	929	933	936	rVB5	2067	2338	0.17%	0.018%
24	8.775	961	967	980	rVV	277065	475161	35.08%	3.583%
25	8.863	980	982	985	rVV4	2909	2873	0.21%	0.022%
26	8.887	985	986	992	rVV5	1947	2931	0.22%	0.022%
27	8.946	994	996	1000	rVB5	1215	1381	0.10%	0.010%
28	9.134	1025	1028	1033	rVB6	2186	3320	0.25%	0.025%
29	9.487	1080	1088	1104	rBV2	219244	380527	28.10%	2.869%
30	9.669	1115	1119	1120	rBV3	1603	1424	0.11%	0.011%
31	9.851	1147	1150	1153	rVB4	2200	2150	0.16%	0.016%
32	10.022	1172	1179	1199	rBV	232487	501243	37.01%	3.779%
33	10.157	1201	1202	1205	rVV3	2574	2168	0.16%	0.016%
34	10.387	1233	1241	1249	rBV	273903	467470	34.52%	3.525%
35	10.551	1261	1269	1292	rBV	179587	446478	32.97%	3.366%
36	10.716	1295	1297	1302	rVV4	2570	3908	0.29%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045177.D
 Acq On : 12 Apr 2024 18:48
 Operator : MA/JU
 Sample : P2006-06
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MC0R65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	10.751	1302	1303	1306	rVV2	2007	2077	0.15%	0.016%
38	10.781	1306	1308	1312	rVB6	1296	1929	0.14%	0.015%
39	10.928	1330	1333	1337	rVB5	1189	1716	0.13%	0.013%
40	11.193	1373	1378	1381	rBV3	1130	1463	0.11%	0.011%

41	11.498	1428	1430	1433	rVB3	1232	1426	0.11%	0.011%
42	11.569	1439	1442	1446	rBV3	1465	2594	0.19%	0.020%
43	11.604	1446	1448	1455	rVB3	1134	2166	0.16%	0.016%
44	11.816	1482	1484	1487	rBV2	1328	1479	0.11%	0.011%
45	12.022	1510	1519	1523	rBV5	2969	6773	0.50%	0.051%

46	12.204	1543	1550	1552	rVB4	1588	2410	0.18%	0.018%
47	13.022	1686	1689	1692	rBV4	971	1530	0.11%	0.012%
48	13.157	1710	1712	1716	rVB4	2860	2998	0.22%	0.023%
49	13.234	1721	1725	1729	rVB5	1256	1804	0.13%	0.014%
50	13.281	1732	1733	1737	rVB3	1480	1449	0.11%	0.011%

51	13.316	1737	1739	1741	rBV2	1715	1447	0.11%	0.011%
52	13.592	1783	1786	1788	rVB2	1453	1611	0.12%	0.012%
53	13.616	1788	1790	1792	rBV	2084	1424	0.11%	0.011%
54	13.687	1796	1802	1820	rVV	516254	794499	58.66%	5.990%
55	13.951	1841	1847	1858	rVV2	690303	1007190	74.37%	7.594%

56	14.169	1881	1884	1889	rBV4	1089	1362	0.10%	0.010%
57	14.263	1893	1900	1907	rBV	382836	558229	41.22%	4.209%
58	14.581	1945	1954	1956	rBV7	6497	13012	0.96%	0.098%
59	14.651	1965	1966	1968	rVB2	2171	1371	0.10%	0.010%
60	14.875	2001	2004	2007	rBV4	911	1380	0.10%	0.010%

61	14.939	2011	2015	2017	rVB3	1485	1557	0.11%	0.012%
62	14.998	2022	2025	2028	rBV4	1493	2007	0.15%	0.015%
63	15.039	2028	2032	2034	rBV3	1335	1483	0.11%	0.011%
64	15.122	2044	2046	2050	rVB4	2161	2316	0.17%	0.017%
65	15.151	2050	2051	2054	rBV3	1267	1441	0.11%	0.011%

66	15.263	2061	2070	2082	rBV	819790	1240511	91.59%	9.353%
67	15.345	2082	2084	2087	rVV4	1840	1866	0.14%	0.014%
68	15.410	2089	2095	2110	rVV	158095	276112	20.39%	2.082%
69	15.504	2110	2111	2118	rVB6	2725	3691	0.27%	0.028%
70	15.769	2154	2156	2158	rBV3	1290	1590	0.12%	0.012%

71	15.845	2168	2169	2172	rBV2	1540	1517	0.11%	0.011%
72	16.057	2202	2205	2208	rVB4	2222	2898	0.21%	0.022%
73	16.310	2247	2248	2253	rVB3	1447	1375	0.10%	0.010%
74	16.769	2323	2326	2327	rBV3	1436	1422	0.10%	0.011%
75	17.022	2363	2369	2380	rBV	370671	533582	39.40%	4.023%

76	17.122	2380	2386	2403	rVV2	811048	1224789	90.43%	9.234%
----	--------	------	------	------	------	--------	---------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045177.D
 Acq On : 12 Apr 2024 18:48
 Operator : MA/JU
 Sample : P2006-06
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MC0R65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

77	17.375	2427	2429	2432	rVB4	2192	2210	0.16%	0.017%
78	17.404	2432	2434	2435	rBV2	2473	1845	0.14%	0.014%
79	17.575	2462	2463	2466	rBV2	1344	1516	0.11%	0.011%
80	17.939	2518	2525	2530	rBV3	12213	22150	1.64%	0.167%
81	18.357	2593	2596	2598	rVV4	1943	2210	0.16%	0.017%
82	18.392	2601	2602	2606	rBV4	1169	1716	0.13%	0.013%
83	18.480	2614	2617	2618	rBV3	1944	1792	0.13%	0.014%
84	18.933	2691	2694	2696	rBV4	1885	2364	0.17%	0.018%
85	18.992	2699	2704	2708	rVV3	6672	10334	0.76%	0.078%
86	19.063	2713	2716	2720	rBV2	5179	7372	0.54%	0.056%
87	19.233	2741	2745	2748	rBV6	4761	6220	0.46%	0.047%
88	19.427	2772	2778	2790	rBV	954608	1259398	92.99%	9.495%
89	20.221	2911	2913	2914	rBV2	3319	1895	0.14%	0.014%
90	21.233	3080	3085	3096	rBV	303279	473145	34.93%	3.567%
91	23.304	3430	3437	3453	rBV	704846	1354380	100.00%	10.212%
92	23.445	3455	3461	3472	rVB2	277646	553518	40.87%	4.173%




Sum of corrected areas: 13263212

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045177.D
Acq On : 12 Apr 2024 18:48
Operator : MA/JU
Sample : P2006-06
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0R65

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

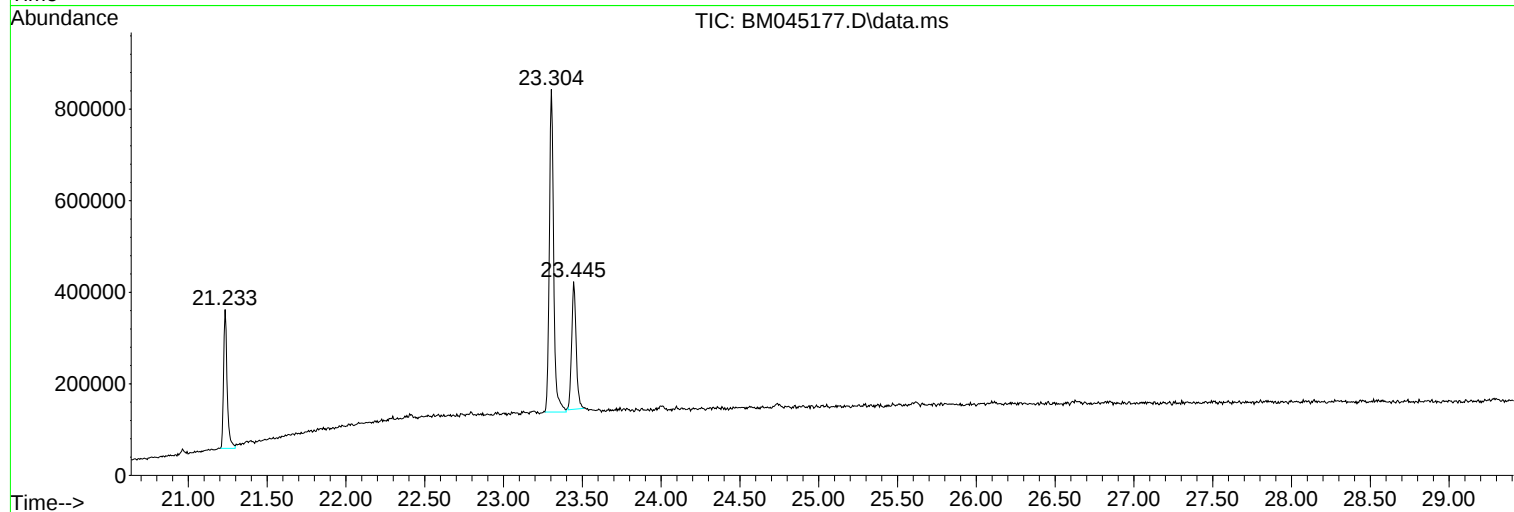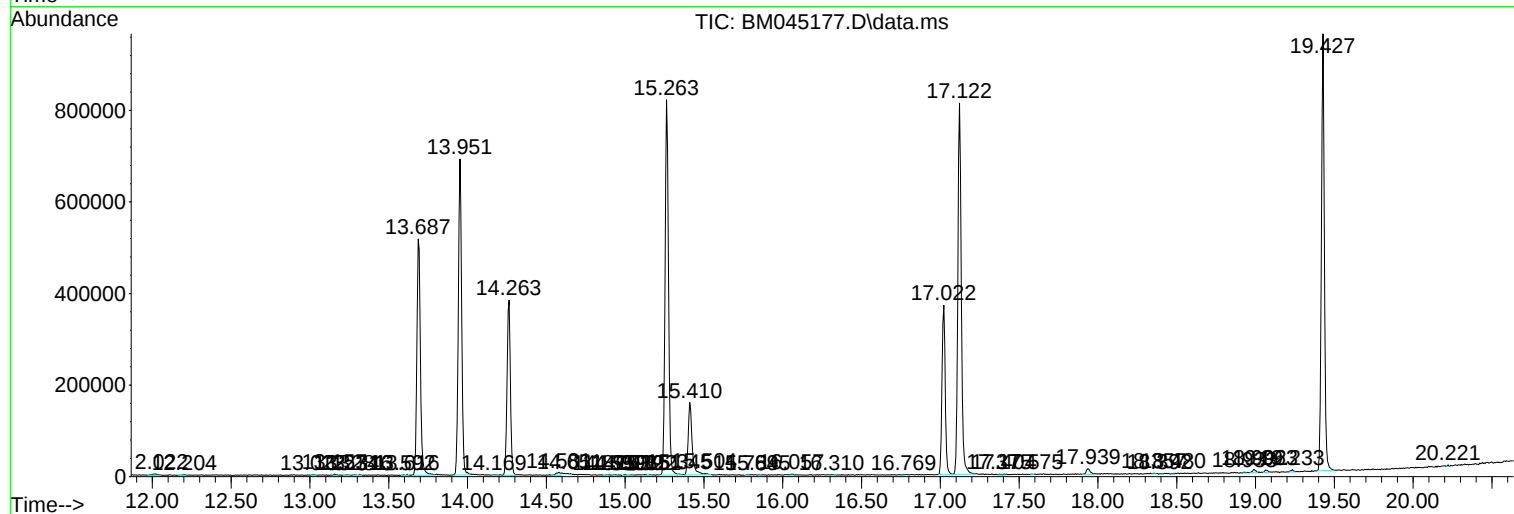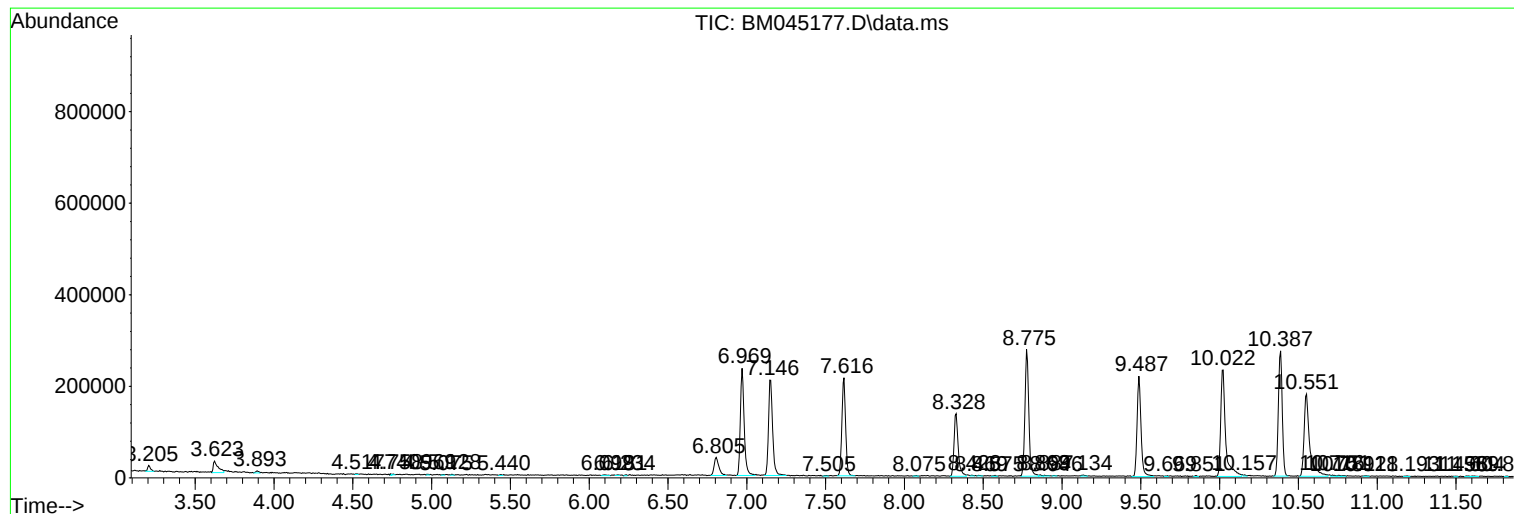

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045177.D
Acq On : 12 Apr 2024 18:48
Operator : MA/JU
Sample : P2006-06
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0R65

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045177.D
Acq On : 12 Apr 2024 18:48
Operator : MA/JU
Sample : P2006-06
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0R65

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc