

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045182.D
 Acq On : 12 Apr 2024 21:50
 Operator : MA/JU
 Sample : P2006-12
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MCORF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045182.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	6	8	12	rVB5	2829	2473	0.15%	0.015%
2	3.205	16	20	25	rBV	12654	15791	0.95%	0.095%
3	3.611	86	89	100	rBV	53696	103871	6.23%	0.625%
4	3.893	134	137	142	rVB6	4308	5575	0.33%	0.034%
5	4.781	286	288	294	rVB7	1982	2119	0.13%	0.013%
6	4.981	317	322	331	rBV	29579	45989	2.76%	0.277%
7	5.528	410	415	416	rBV5	1240	1808	0.11%	0.011%
8	6.340	551	553	558	rVV5	1519	2452	0.15%	0.015%
9	6.422	562	567	570	rBV5	1386	2102	0.13%	0.013%
10	6.799	625	631	640	rBV2	56395	115975	6.95%	0.698%
11	6.881	644	645	650	rVB4	1628	1929	0.12%	0.012%
12	6.969	654	660	673	rBV	295727	483370	28.98%	2.907%
13	7.146	684	690	700	rBV	265976	460479	27.61%	2.770%
14	7.499	744	750	752	rBV6	3213	4536	0.27%	0.027%
15	7.611	760	769	783	rVV	235958	440811	26.43%	2.651%
16	7.958	823	828	836	rVB	24644	43510	2.61%	0.262%
17	8.322	884	890	904	rBV	187984	337741	20.25%	2.031%
18	8.475	911	916	920	rVB6	1561	3088	0.19%	0.019%
19	8.775	960	967	979	rBV	345245	589907	35.37%	3.548%
20	8.857	979	981	985	rVB3	2173	2536	0.15%	0.015%
21	8.987	1000	1003	1005	rVB2	2375	2131	0.13%	0.013%
22	9.087	1017	1020	1023	rBV4	1234	2059	0.12%	0.012%
23	9.128	1025	1027	1034	rVB5	2699	3657	0.22%	0.022%
24	9.175	1034	1035	1040	rVB3	1693	1936	0.12%	0.012%
25	9.487	1080	1088	1100	rVV	278774	479184	28.73%	2.882%
26	9.569	1100	1102	1105	rVB4	1976	1932	0.12%	0.012%
27	10.016	1171	1178	1203	rVV	315710	646529	38.76%	3.889%
28	10.246	1212	1217	1222	rVB5	7895	12219	0.73%	0.073%
29	10.381	1232	1240	1250	rBV	301503	522838	31.35%	3.145%
30	10.546	1262	1268	1288	rVV	225450	534453	32.04%	3.215%
31	10.769	1301	1306	1310	rBV7	2604	4158	0.25%	0.025%
32	11.687	1459	1462	1463	rBV3	1907	1791	0.11%	0.011%
33	12.010	1513	1517	1521	rBV6	4496	7757	0.47%	0.047%
34	12.587	1613	1615	1620	rVB4	1367	1885	0.11%	0.011%
35	13.157	1708	1712	1718	rVB4	3860	7823	0.47%	0.047%
36	13.687	1796	1802	1815	rBV	649979	1002449	60.10%	6.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045182.D
Acq On : 12 Apr 2024 21:50
Operator : MA/JU
Sample : P2006-12
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MCORF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

37	13.775	1815	1817	1822	rVV4	2067	3302	0.20%	0.020%
38	13.951	1839	1847	1859	rBV	869478	1290419	77.37%	7.761%
39	14.151	1877	1881	1885	rBV3	6986	9047	0.54%	0.054%
40	14.257	1893	1899	1910	rVB	435977	667168	40.00%	4.013%
41	14.510	1939	1942	1944	rBV4	2139	2295	0.14%	0.014%
42	14.557	1944	1950	1952	rBV5	8506	14919	0.89%	0.090%
43	14.881	2003	2005	2009	rBV4	1249	2074	0.12%	0.012%
44	15.263	2062	2070	2081	rBV	1023702	1537440	92.18%	9.247%
45	15.410	2089	2095	2106	rBV	240131	400867	24.03%	2.411%
46	15.510	2109	2112	2117	rVB5	4308	6454	0.39%	0.039%
47	15.675	2137	2140	2143	rBV3	1587	2242	0.13%	0.013%
48	15.722	2145	2148	2151	rBV3	2021	2078	0.12%	0.012%
49	15.786	2155	2159	2161	rBV4	1514	1769	0.11%	0.011%
50	15.922	2179	2182	2187	rBV6	1247	2017	0.12%	0.012%
51	16.051	2202	2204	2205	rBV	2422	2517	0.15%	0.015%
52	16.480	2274	2277	2282	rVV4	1709	2746	0.16%	0.017%
53	16.616	2296	2300	2303	rBV4	1346	2289	0.14%	0.014%
54	16.698	2311	2314	2320	rVB5	1616	2643	0.16%	0.016%
55	17.022	2363	2369	2378	rBV	490871	704846	42.26%	4.239%
56	17.122	2378	2386	2401	rBV	1056630	1610579	96.56%	9.687%
57	17.551	2457	2459	2464	rBV5	1883	2844	0.17%	0.017%
58	17.869	2510	2513	2516	rVB5	1470	2130	0.13%	0.013%
59	17.939	2521	2525	2531	rVV5	7775	13227	0.79%	0.080%
60	18.445	2607	2611	2612	rBV3	1637	2031	0.12%	0.012%
61	18.574	2630	2633	2636	rBV5	1380	2482	0.15%	0.015%
62	18.610	2636	2639	2641	rVV3	1910	1896	0.11%	0.011%
63	18.663	2646	2648	2652	rVV5	1524	1761	0.11%	0.011%
64	18.757	2661	2664	2666	rVB4	1501	1682	0.10%	0.010%
65	18.892	2685	2687	2691	rVV3	3303	3028	0.18%	0.018%
66	18.992	2700	2704	2707	rBV4	10113	14003	0.84%	0.084%
67	19.063	2713	2716	2720	rBV2	7713	10457	0.63%	0.063%
68	19.233	2741	2745	2749	rBV6	5351	7101	0.43%	0.043%
69	19.345	2762	2764	2766	rBV3	2532	2183	0.13%	0.013%
70	19.427	2772	2778	2790	rBV	1188740	1667881	100.00%	10.032%
71	19.739	2829	2831	2833	rBV3	2525	2918	0.17%	0.018%
72	21.233	3080	3085	3094	rBV	388836	578827	34.70%	3.481%
73	23.304	3430	3437	3451	rBV2	759809	1504102	90.18%	9.047%
74	23.445	3455	3461	3473	rVB	295820	640861	38.42%	3.855%

Sum of corrected areas: 16625988




Instrument :
BNA_M
ClientSampleId :
MC0RF1

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045182.D
Acq On : 12 Apr 2024 21:50
Operator : MA/JU
Sample : P2006-12
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0RF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

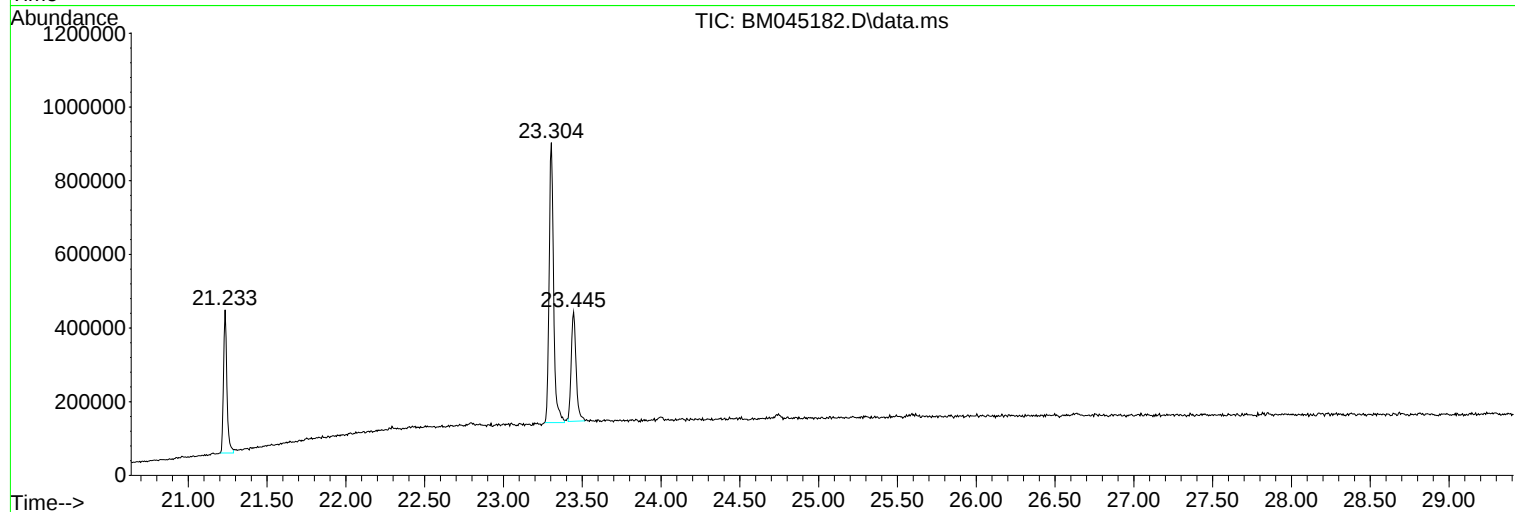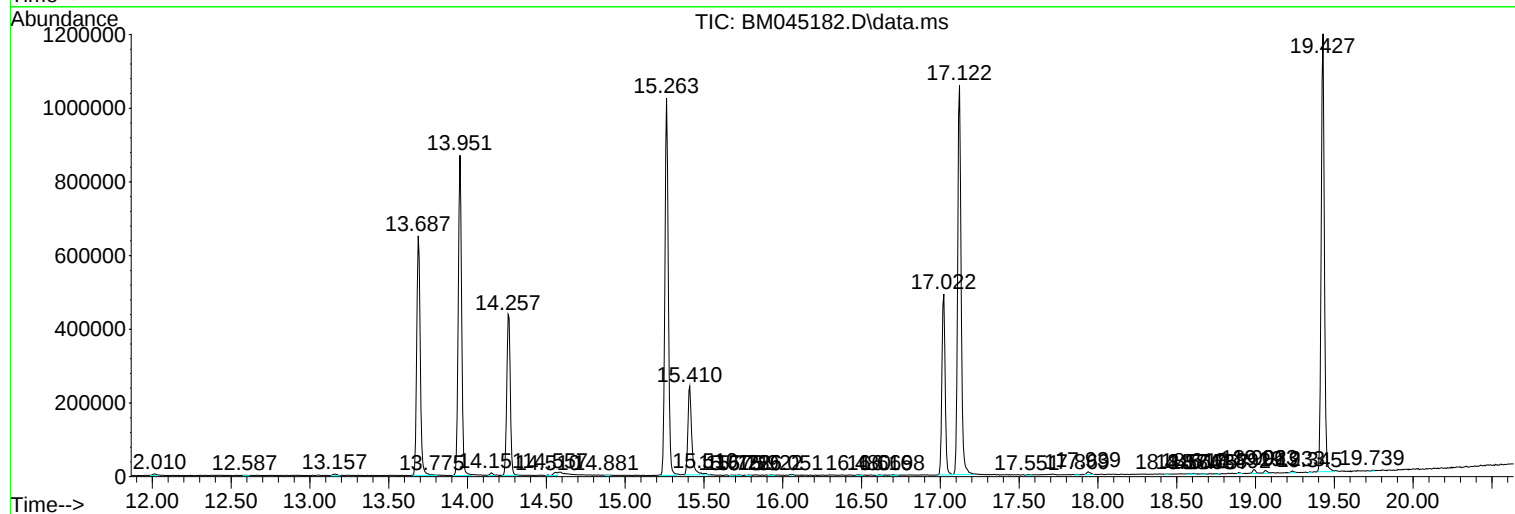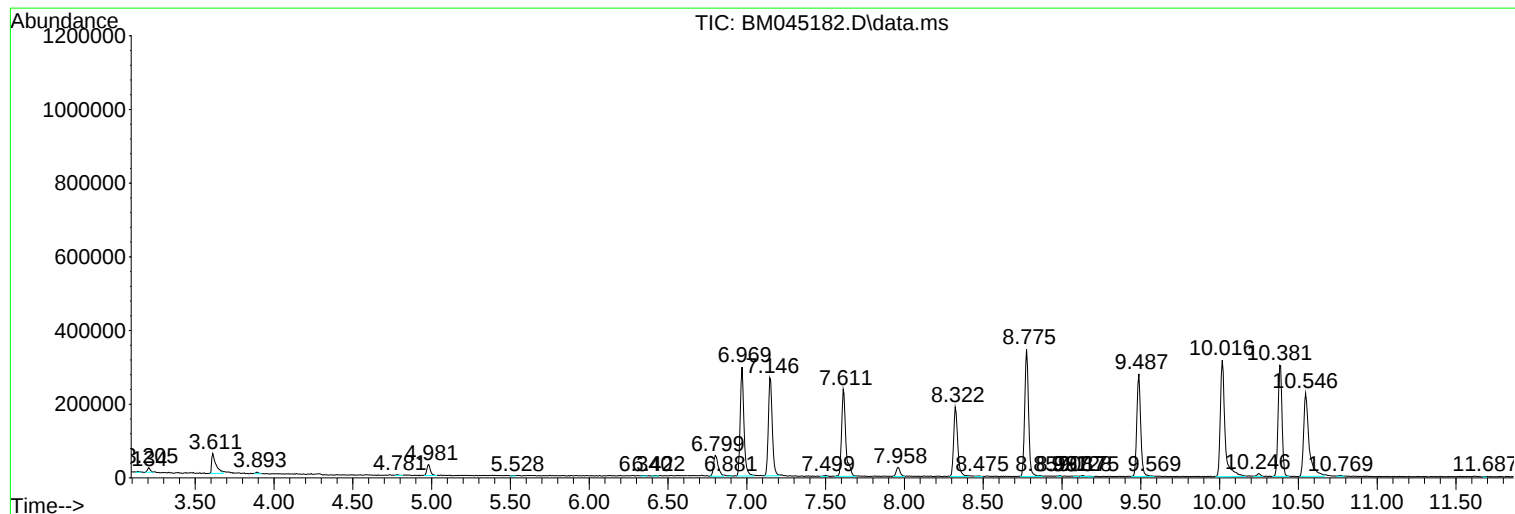

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045182.D
Acq On : 12 Apr 2024 21:50
Operator : MA/JU
Sample : P2006-12
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0RF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045182.D
Acq On : 12 Apr 2024 21:50
Operator : MA/JU
Sample : P2006-12
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MC0RF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------