

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045183.D
 Acq On : 12 Apr 2024 22:27
 Operator : MA/JU
 Sample : P2010-01
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0LZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045183.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.163	10	13	17	rBV3	15108	20230	1.73%	0.172%
2	3.205	17	20	27	rVB2	14667	19138	1.63%	0.163%
3	3.610	85	89	105	rBV	68183	140738	12.02%	1.200%
4	3.899	136	138	140	rVB3	3171	2006	0.17%	0.017%
5	4.999	324	325	329	rVB4	1336	1544	0.13%	0.013%
6	5.110	341	344	346	rVB3	1871	1638	0.14%	0.014%
7	5.246	364	367	368	rBV2	2070	2120	0.18%	0.018%
8	5.299	372	376	377	rVV3	1444	1800	0.15%	0.015%
9	5.340	380	383	386	rVV4	1258	1515	0.13%	0.013%
10	5.616	427	430	433	rBV5	1406	1890	0.16%	0.016%
11	5.740	446	451	463	rBV	26295	53606	4.58%	0.457%
12	6.063	503	506	507	rBV3	1398	1558	0.13%	0.013%
13	6.340	551	553	559	rVB5	1164	1639	0.14%	0.014%
14	6.416	564	566	568	rBV2	1448	1488	0.13%	0.013%
15	6.575	592	593	595	rBV2	2378	1667	0.14%	0.014%
16	6.598	595	597	599	rVV3	1248	1454	0.12%	0.012%
17	6.804	626	632	642	rVV	37710	81645	6.97%	0.696%
18	6.898	646	648	651	rVV2	2021	2192	0.19%	0.019%
19	6.969	653	660	670	rVV	209902	353141	30.16%	3.010%
20	7.057	673	675	679	rVV5	2713	4094	0.35%	0.035%
21	7.151	682	691	700	rVV	106960	197674	16.88%	1.685%
22	7.216	700	702	708	rVV5	3530	5373	0.46%	0.046%
23	7.457	741	743	747	rVB3	1172	1551	0.13%	0.013%
24	7.610	763	769	779	rBV	239707	407875	34.83%	3.477%
25	7.957	825	828	834	rBV6	1649	3250	0.28%	0.028%
26	8.334	886	892	898	rBV2	54221	104987	8.97%	0.895%
27	8.392	898	902	912	rVV	19960	36409	3.11%	0.310%
28	8.469	912	915	919	rVV5	1651	2512	0.21%	0.021%
29	8.581	933	934	937	rVB3	2180	1669	0.14%	0.014%
30	8.775	960	967	978	rBV	236649	418377	35.73%	3.566%
31	9.128	1022	1027	1031	rBV5	2483	4396	0.38%	0.037%
32	9.492	1083	1089	1100	rVV2	40601	77360	6.61%	0.659%
33	9.775	1134	1137	1140	rVB5	1636	2470	0.21%	0.021%
34	9.810	1140	1143	1146	rBV5	1473	1980	0.17%	0.017%
35	10.022	1169	1179	1196	rBV	105273	250053	21.35%	2.132%
36	10.239	1215	1216	1220	rBV4	1852	2189	0.19%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045183.D
 Acq On : 12 Apr 2024 22:27
 Operator : MA/JU
 Sample : P2010-01
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0LZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	10.298	1223	1226	1227	rVV2	2079	2132	0.18%	0.018%
38	10.316	1227	1229	1233	rVV4	2537	3057	0.26%	0.026%
39	10.386	1233	1241	1248	rVV	306083	533920	45.59%	4.551%
40	10.445	1249	1251	1256	rVB5	3422	4431	0.38%	0.038%
41	10.545	1261	1268	1284	rBV	163562	396942	33.90%	3.384%
42	10.751	1301	1303	1304	rVV2	2782	1943	0.17%	0.017%
43	10.763	1304	1305	1309	rVV4	3264	3987	0.34%	0.034%
44	11.110	1361	1364	1368	rVB4	1637	2406	0.21%	0.021%
45	11.763	1471	1475	1479	rBV5	856	1524	0.13%	0.013%
46	12.010	1513	1517	1524	rVV6	3581	8018	0.68%	0.068%
47	12.127	1536	1537	1541	rVV2	1118	1453	0.12%	0.012%
48	12.239	1553	1556	1558	rBV4	1800	1880	0.16%	0.016%
49	12.592	1610	1616	1618	rVB3	1232	2482	0.21%	0.021%
50	13.074	1696	1698	1704	rVB5	1343	2009	0.17%	0.017%
51	13.163	1707	1713	1716	rBV4	4728	7848	0.67%	0.067%
52	13.410	1753	1755	1757	rVB	1846	1445	0.12%	0.012%
53	13.533	1772	1776	1778	rVB4	1480	1540	0.13%	0.013%
54	13.598	1783	1787	1791	rVV5	1250	1663	0.14%	0.014%
55	13.686	1795	1802	1818	rVV	449104	693296	59.20%	5.910%
56	13.810	1822	1823	1826	rVB2	1794	1614	0.14%	0.014%
57	13.857	1826	1831	1833	rBV5	968	1697	0.14%	0.014%
58	13.951	1840	1847	1854	rBV	585627	888315	75.86%	7.572%
59	14.257	1893	1899	1907	rBV	410730	631101	53.89%	5.380%
60	14.610	1952	1959	1961	rBV6	3102	7251	0.62%	0.062%
61	14.669	1966	1969	1971	rVV4	2342	3536	0.30%	0.030%
62	14.716	1975	1977	1982	rVV4	1684	2863	0.24%	0.024%
63	14.763	1982	1985	1989	rVB4	1574	2567	0.22%	0.022%
64	14.851	1997	2000	2002	rBV4	1103	1644	0.14%	0.014%
65	15.039	2028	2032	2033	rBV3	1496	1484	0.13%	0.013%
66	15.074	2037	2038	2043	rVV3	2253	2129	0.18%	0.018%
67	15.121	2043	2046	2052	rVB4	1462	3134	0.27%	0.027%
68	15.263	2064	2070	2084	rBV	684682	1071025	91.46%	9.130%
69	15.421	2093	2097	2108	rBV7	11273	25416	2.17%	0.217%
70	15.504	2108	2111	2112	rVV3	2111	2780	0.24%	0.024%
71	15.516	2112	2113	2117	rVV3	2507	1440	0.12%	0.012%
72	15.574	2121	2123	2127	rVB3	1282	1602	0.14%	0.014%
73	15.627	2131	2132	2136	rBV4	1984	1891	0.16%	0.016%
74	15.739	2148	2151	2155	rVB4	1572	1827	0.16%	0.016%
75	15.768	2155	2156	2160	rBV3	1444	1569	0.13%	0.013%
76	16.063	2201	2206	2209	rVB4	2563	3399	0.29%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045183.D
 Acq On : 12 Apr 2024 22:27
 Operator : MA/JU
 Sample : P2010-01
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0LZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

77	16.315	2246	2249	2250	rBV2	1954	1669	0.14%	0.014%
78	16.480	2274	2277	2280	rBV4	2085	2675	0.23%	0.023%
79	16.810	2329	2333	2337	rBV6	1542	2613	0.22%	0.022%
80	16.957	2355	2358	2361	rBV5	2191	1434	0.12%	0.012%
81	17.021	2361	2369	2379	rBV	407210	597603	51.03%	5.094%
82	17.121	2379	2386	2401	rVV	684432	1083633	92.54%	9.237%
83	17.392	2428	2432	2444	rVV2	15685	31466	2.69%	0.268%
84	17.545	2454	2458	2461	rBV4	966	1521	0.13%	0.013%
85	17.845	2505	2509	2512	rBV6	1572	2000	0.17%	0.017%
86	18.009	2534	2537	2543	rBV3	3759	6309	0.54%	0.054%
87	18.074	2547	2548	2552	rVB4	1642	1446	0.12%	0.012%
88	18.368	2596	2598	2601	rBV3	2603	2151	0.18%	0.018%
89	18.521	2621	2624	2627	rVV3	1242	1555	0.13%	0.013%
90	18.615	2638	2640	2643	rVB3	1572	1611	0.14%	0.014%
91	18.727	2654	2659	2660	rBV3	1614	1547	0.13%	0.013%
92	18.809	2667	2673	2677	rBV7	3388	5863	0.50%	0.050%
93	18.992	2700	2704	2711	rBV5	6497	9468	0.81%	0.081%
94	19.068	2713	2717	2718	rBV2	3609	3724	0.32%	0.032%
95	19.321	2756	2760	2766	rBV3	15714	27680	2.36%	0.236%
96	19.427	2772	2778	2792	rBV	797229	1114578	95.18%	9.501%
97	19.727	2827	2829	2833	rVV3	2142	2228	0.19%	0.019%
98	21.233	3080	3085	3094	rBV	326771	495237	42.29%	4.222%
99	23.303	3430	3437	3453	rBV2	597529	1171024	100.00%	9.982%
100	23.444	3455	3461	3473	rVB	294388	618443	52.81%	5.272%




Sum of corrected areas: 11730966

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045183.D
Acq On : 12 Apr 2024 22:27
Operator : MA/JU
Sample : P2010-01
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0LZ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

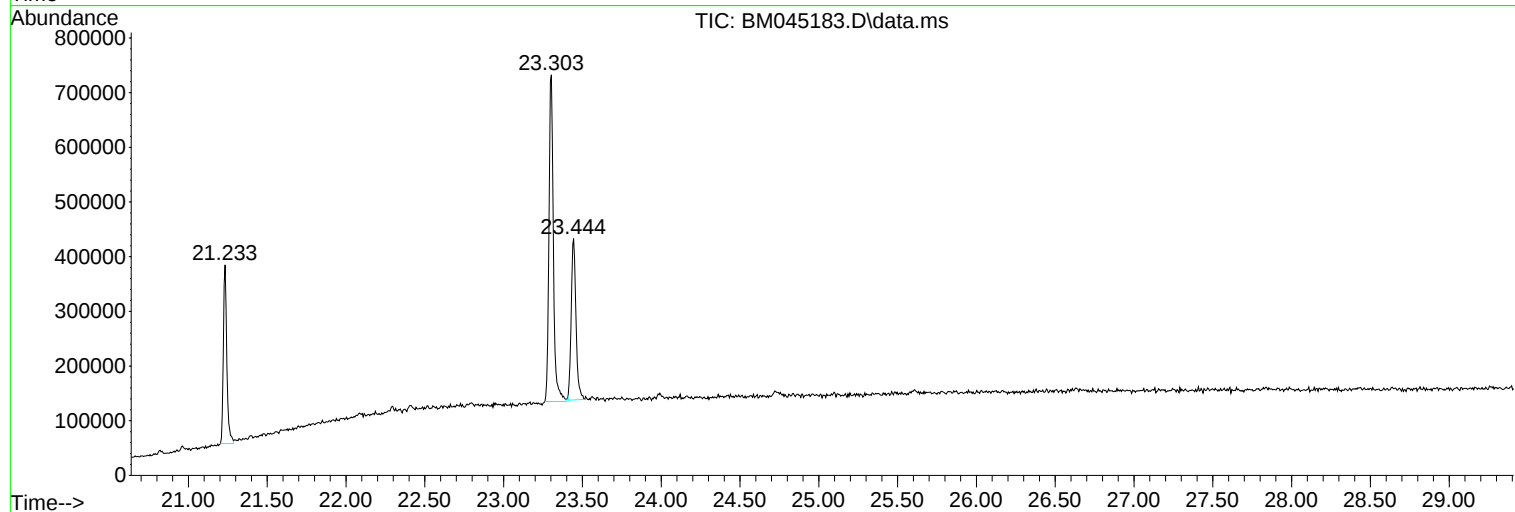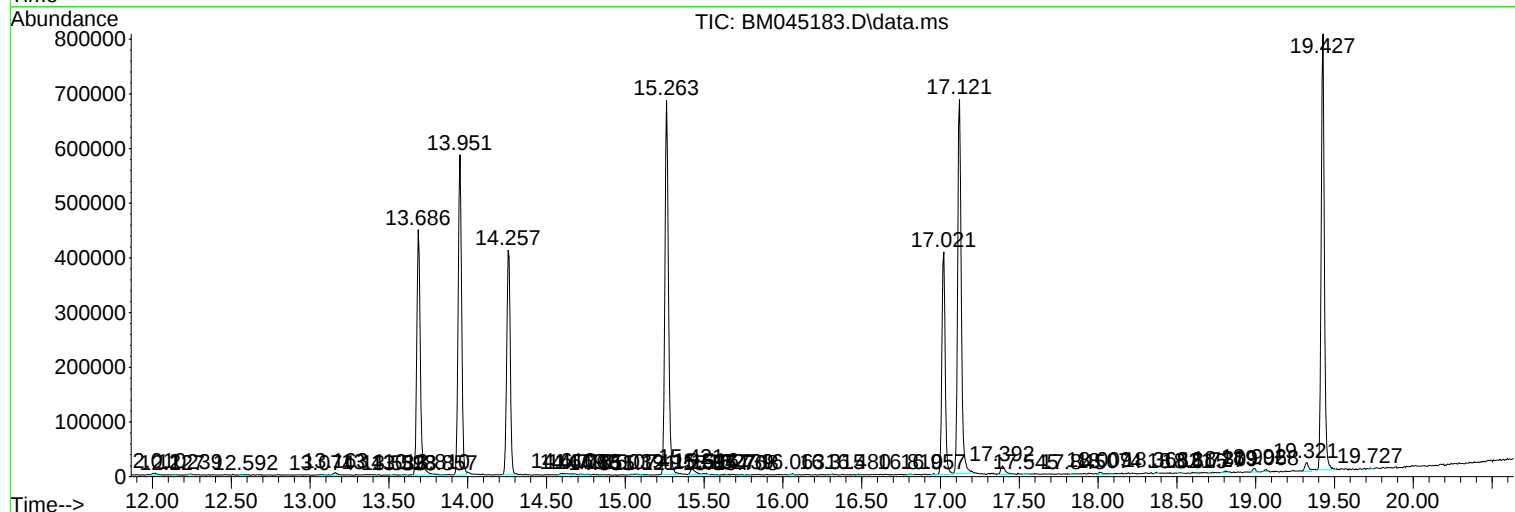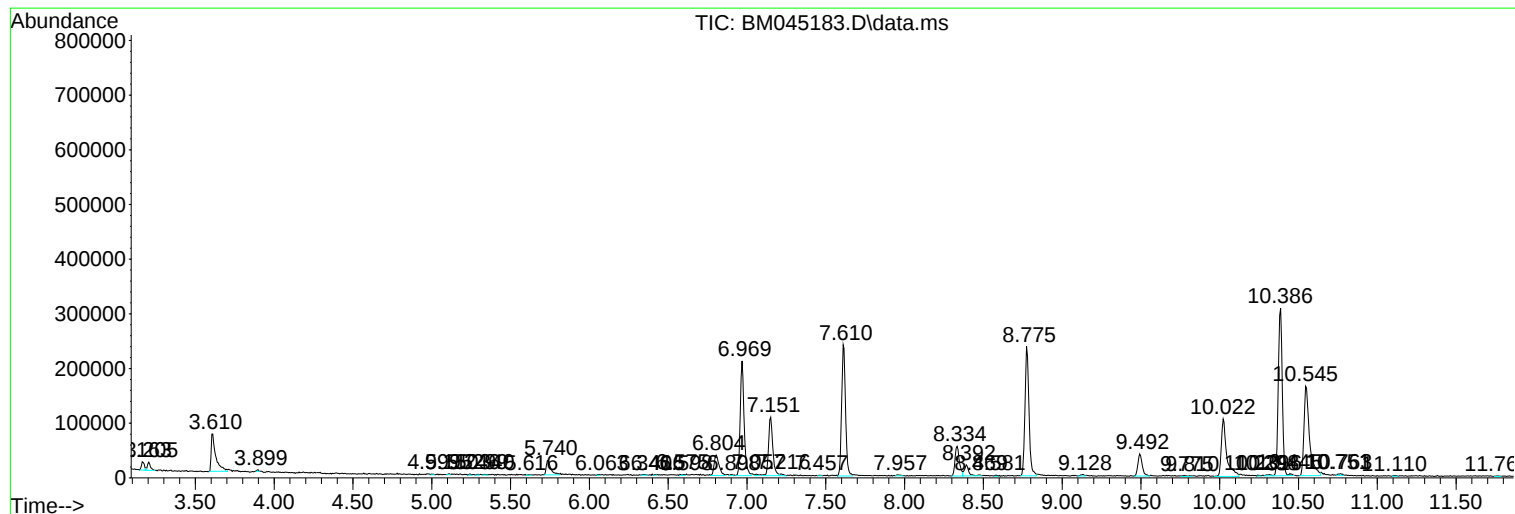

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045183.D
Acq On : 12 Apr 2024 22:27
Operator : MA/JU
Sample : P2010-01
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0LZ9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-butoxy- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.740	2.63 ng/ul	53606	1,4-Dichlorobenzene-d4	7.610

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-butoxy-	118	C6H14O2	000111-76-2	72
2			Ethanol, 2-butoxy-	118	C6H14O2	000111-76-2	72
3			Ethanol, 2-butoxy-	118	C6H14O2	000111-76-2	59
4			Ethanol, 2-butoxy-	118	C6H14O2	000111-76-2	56
5			3-Buten-2-ol	72	C4H8O	000598-32-3	43

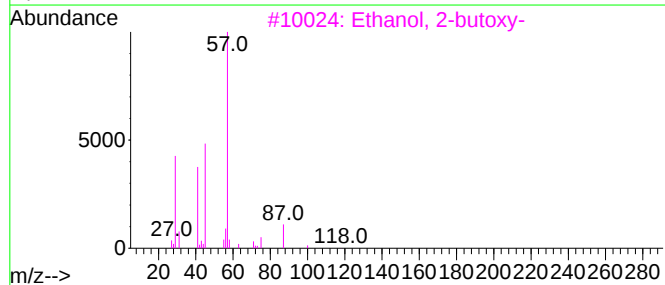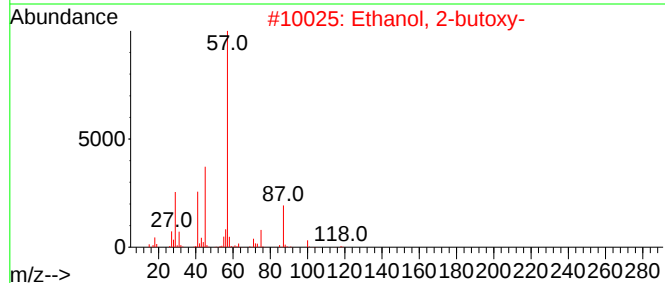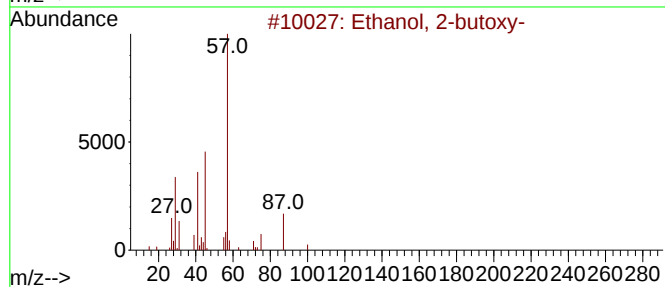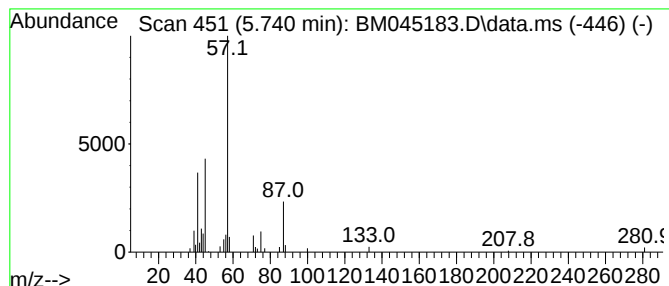

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045183.D
Acq On : 12 Apr 2024 22:27
Operator : MA/JU
Sample : P2010-01
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0LZ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-butoxy-	5.740	2.6	ng/ul	53606	1	7.610	407875	20.0