

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM041124\  
 Data File : BM045187.D  
 Acq On : 13 Apr 2024 02:05  
 Operator : MA/JU  
 Sample : PB160136BL  
 Misc :  
 ALS Vial : 51 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SBLK136

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM040524.MA.M  
 Title : SVOA CALIBRATION

Signal : TIC: BM045187.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.205       | 17            | 20          | 25           | rVB      | 15664          | 18670         | 1.74%           | 0.159%        |
| 2         | 3.599       | 85            | 87          | 106          | rBV      | 168356         | 296069        | 27.65%          | 2.516%        |
| 3         | 4.022       | 157           | 159         | 160          | rBV2     | 3562           | 1996          | 0.19%           | 0.017%        |
| 4         | 5.240       | 365           | 366         | 368          | rVB2     | 2752           | 1329          | 0.12%           | 0.011%        |
| 5         | 5.263       | 368           | 370         | 372          | rBV3     | 1917           | 1829          | 0.17%           | 0.016%        |
| 6         | 5.646       | 433           | 435         | 439          | rBV5     | 1189           | 1584          | 0.15%           | 0.013%        |
| 7         | 5.916       | 478           | 481         | 482          | rBV2     | 1245           | 1307          | 0.12%           | 0.011%        |
| 8         | 6.663       | 606           | 608         | 610          | rBV2     | 1940           | 1945          | 0.18%           | 0.017%        |
| 9         | 6.793       | 624           | 630         | 646          | rBV      | 199351         | 367704        | 34.34%          | 3.124%        |
| 10        | 6.969       | 654           | 660         | 670          | rBV      | 176795         | 288674        | 26.96%          | 2.453%        |
| 11        | 7.146       | 684           | 690         | 704          | rVB      | 226913         | 385372        | 35.99%          | 3.274%        |
| 12        | 7.610       | 763           | 769         | 779          | rBV      | 193644         | 323301        | 30.19%          | 2.747%        |
| 13        | 8.216       | 869           | 872         | 873          | rBV2     | 1757           | 1893          | 0.18%           | 0.016%        |
| 14        | 8.322       | 883           | 890         | 903          | rBV      | 236360         | 429493        | 40.11%          | 3.649%        |
| 15        | 8.775       | 960           | 967         | 980          | rBV      | 198365         | 349951        | 32.68%          | 2.973%        |
| 16        | 9.487       | 1081          | 1088        | 1096         | rBV      | 159677         | 284773        | 26.59%          | 2.420%        |
| 17        | 9.681       | 1119          | 1121        | 1124         | rBV3     | 1125           | 1756          | 0.16%           | 0.015%        |
| 18        | 10.016      | 1170          | 1178        | 1206         | rBV      | 191211         | 428450        | 40.01%          | 3.640%        |
| 19        | 10.381      | 1233          | 1240        | 1248         | rBV      | 249126         | 429842        | 40.14%          | 3.652%        |
| 20        | 10.545      | 1261          | 1268        | 1288         | rBV      | 165416         | 432075        | 40.35%          | 3.671%        |
| 21        | 10.828      | 1313          | 1316        | 1319         | rVB4     | 1617           | 1723          | 0.16%           | 0.015%        |
| 22        | 11.181      | 1374          | 1376        | 1379         | rVB4     | 1360           | 1500          | 0.14%           | 0.013%        |
| 23        | 11.716      | 1464          | 1467        | 1470         | rBV3     | 1251           | 1725          | 0.16%           | 0.015%        |
| 24        | 11.786      | 1477          | 1479        | 1483         | rVB4     | 1055           | 1421          | 0.13%           | 0.012%        |
| 25        | 11.828      | 1483          | 1486        | 1489         | rBV4     | 1540           | 1674          | 0.16%           | 0.014%        |
| 26        | 12.028      | 1515          | 1520        | 1526         | rBV4     | 2831           | 7420          | 0.69%           | 0.063%        |
| 27        | 12.175      | 1543          | 1545        | 1552         | rVB5     | 1150           | 1581          | 0.15%           | 0.013%        |
| 28        | 13.127      | 1701          | 1707        | 1709         | rBV4     | 915            | 1389          | 0.13%           | 0.012%        |
| 29        | 13.686      | 1796          | 1802        | 1815         | rBV      | 343132         | 550048        | 51.37%          | 4.674%        |
| 30        | 13.951      | 1840          | 1847        | 1859         | rBV      | 476624         | 715674        | 66.83%          | 6.081%        |
| 31        | 14.257      | 1893          | 1899        | 1908         | rBV      | 343636         | 510475        | 47.67%          | 4.337%        |
| 32        | 14.521      | 1938          | 1944        | 1962         | rBV3     | 49803          | 187686        | 17.53%          | 1.595%        |
| 33        | 14.716      | 1975          | 1977        | 1980         | rVB4     | 2060           | 1310          | 0.12%           | 0.011%        |
| 34        | 14.827      | 1992          | 1996        | 1998         | rVB4     | 1774           | 1847          | 0.17%           | 0.016%        |
| 35        | 15.263      | 2063          | 2070        | 2083         | rBV      | 557323         | 853601        | 79.71%          | 7.253%        |
| 36        | 15.410      | 2089          | 2095        | 2108         | rBV      | 111966         | 191892        | 17.92%          | 1.630%        |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM041124\  
 Data File : BM045187.D  
 Acq On : 13 Apr 2024 02:05  
 Operator : MA/JU  
 Sample : PB160136BL  
 Misc :  
 ALS Vial : 51 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SBLK136

Integration Parameters: LSCINT.P

Integrator: RTE  
 Smoothing : OFF Filtering: 5  
 Sampling : 1 Min Area: 0.1 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM040524.MA.M  
 Title : SVOA CALIBRATION

|    |        |      |      |      |      |        |         |         |        |
|----|--------|------|------|------|------|--------|---------|---------|--------|
| 37 | 15.768 | 2153 | 2156 | 2158 | rBV4 | 1349   | 1450    | 0.14%   | 0.012% |
| 38 | 16.057 | 2202 | 2205 | 2207 | rVB4 | 1814   | 1930    | 0.18%   | 0.016% |
| 39 | 16.127 | 2213 | 2217 | 2219 | rBV3 | 881    | 1347    | 0.13%   | 0.011% |
| 40 | 16.563 | 2289 | 2291 | 2293 | rVB2 | 1796   | 1519    | 0.14%   | 0.013% |
| 41 | 16.674 | 2307 | 2310 | 2311 | rBV2 | 1709   | 1893    | 0.18%   | 0.016% |
| 42 | 16.763 | 2323 | 2325 | 2328 | rBV3 | 1516   | 1348    | 0.13%   | 0.011% |
| 43 | 17.015 | 2362 | 2368 | 2379 | rBV  | 358074 | 536173  | 50.07%  | 4.556% |
| 44 | 17.121 | 2379 | 2386 | 2397 | rBV  | 562194 | 872140  | 81.45%  | 7.410% |
| 45 | 17.339 | 2419 | 2423 | 2426 | rBV6 | 1571   | 2337    | 0.22%   | 0.020% |
| 46 | 17.439 | 2437 | 2440 | 2443 | rBV4 | 984    | 1362    | 0.13%   | 0.012% |
| 47 | 17.721 | 2486 | 2488 | 2491 | rVB3 | 1716   | 1353    | 0.13%   | 0.011% |
| 48 | 17.968 | 2528 | 2530 | 2534 | rVB5 | 1456   | 1695    | 0.16%   | 0.014% |
| 49 | 18.133 | 2555 | 2558 | 2560 | rBV3 | 1913   | 2083    | 0.19%   | 0.018% |
| 50 | 18.204 | 2568 | 2570 | 2573 | rVB4 | 1294   | 1366    | 0.13%   | 0.012% |
| 51 | 18.239 | 2573 | 2576 | 2577 | rBV3 | 2496   | 1487    | 0.14%   | 0.013% |
| 52 | 18.762 | 2663 | 2665 | 2667 | rBV3 | 1802   | 1806    | 0.17%   | 0.015% |
| 53 | 18.992 | 2700 | 2704 | 2707 | rVB5 | 5893   | 8089    | 0.76%   | 0.069% |
| 54 | 19.062 | 2714 | 2716 | 2721 | rVB4 | 4548   | 4800    | 0.45%   | 0.041% |
| 55 | 19.427 | 2772 | 2778 | 2790 | rBV  | 676860 | 984677  | 91.96%  | 8.366% |
| 56 | 21.233 | 3080 | 3085 | 3096 | rBV  | 338638 | 536774  | 50.13%  | 4.561% |
| 57 | 23.297 | 3431 | 3436 | 3451 | rVB  | 545745 | 1070823 | 100.00% | 9.098% |
| 58 | 23.444 | 3455 | 3461 | 3472 | rVB  | 320576 | 653904  | 61.07%  | 5.556% |




Sum of corrected areas: 11769335

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM041124\  
Data File : BM045187.D  
Acq On : 13 Apr 2024 02:05  
Operator : MA/JU  
Sample : PB160136BL  
Misc :  
ALS Vial : 51 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SBLK136

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM040524.MA.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

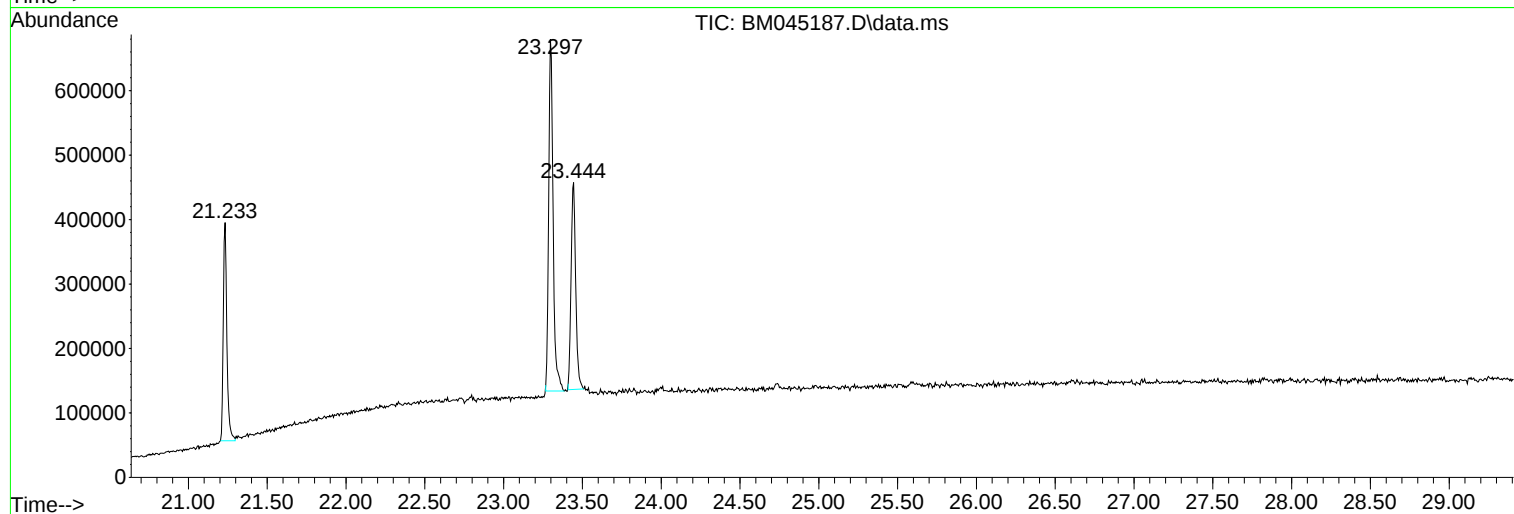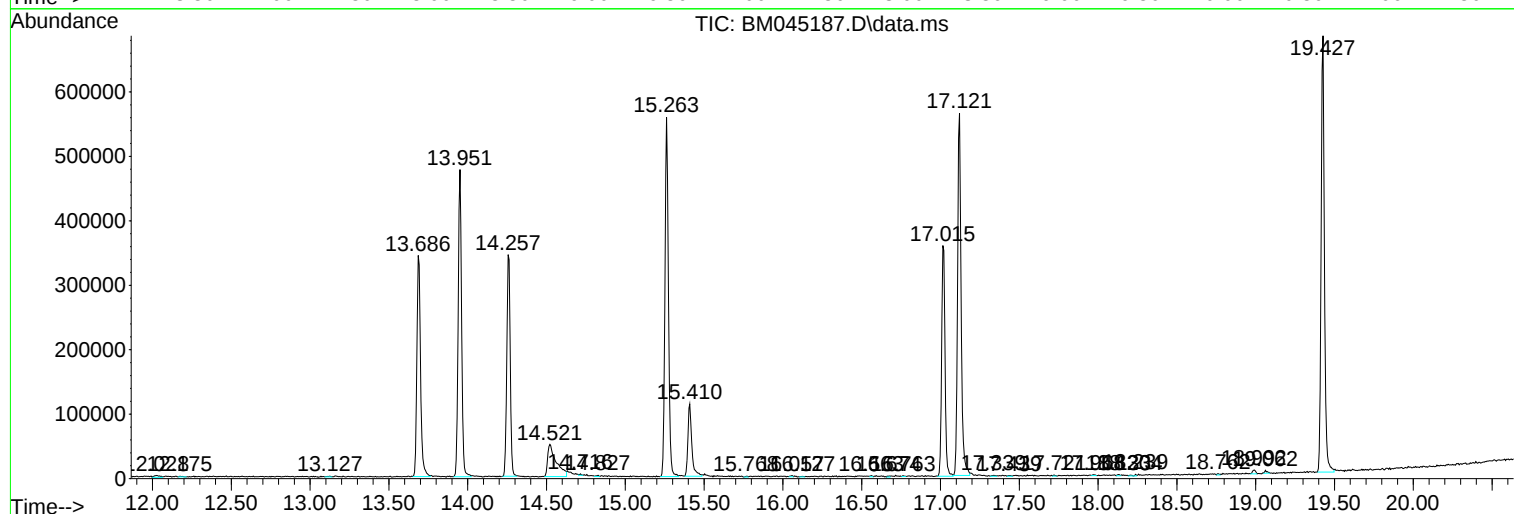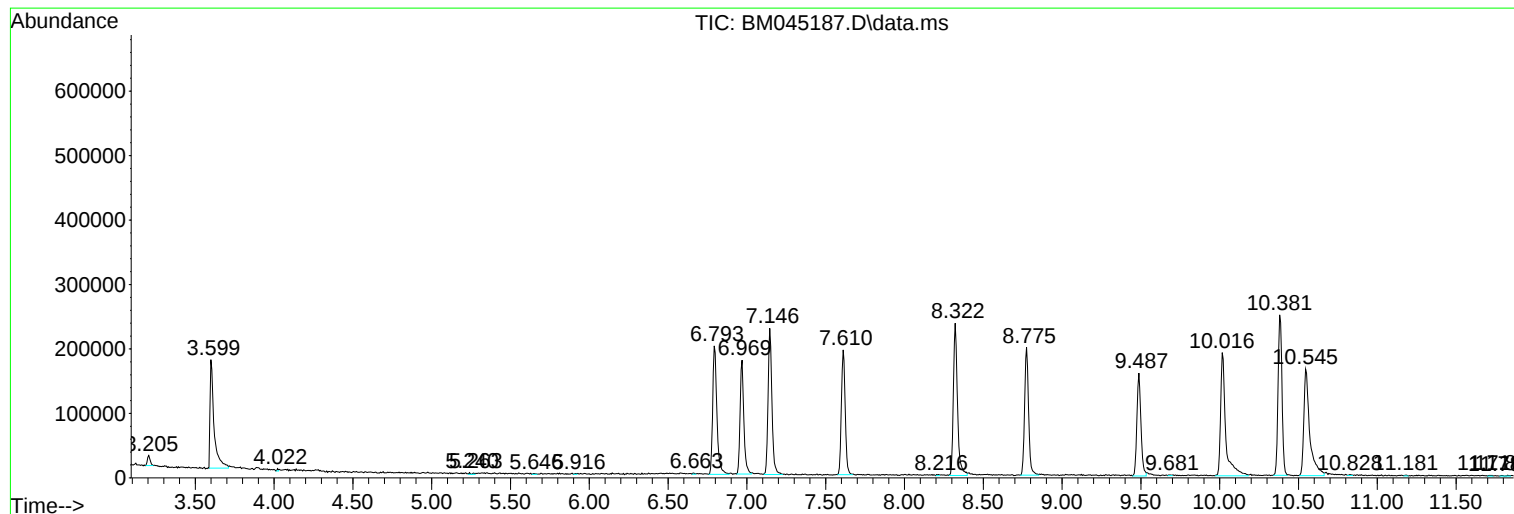

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM041124\  
Data File : BM045187.D  
Acq On : 13 Apr 2024 02:05  
Operator : MA/JU  
Sample : PB160136BL  
Misc :  
ALS Vial : 51 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SBLK136

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM040524.MA.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM041124\  
Data File : BM045187.D  
Acq On : 13 Apr 2024 02:05  
Operator : MA/JU  
Sample : PB160136BL  
Misc :  
ALS Vial : 51 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SBLK136

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM040524.MA.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       | #        | RT Resp Conc          |