

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045189.D
 Acq On : 13 Apr 2024 03:17
 Operator : MA/JU
 Sample : PB160136TB 10X
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLEB097

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045189.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	23	rBV	17793	19029	1.49%	0.129%
2	3.440	59	60	67	rBV6	1881	3481	0.27%	0.024%
3	3.599	84	87	100	rBV	191797	328115	25.63%	2.226%
4	3.893	135	137	140	rVB4	3911	3835	0.30%	0.026%
5	4.010	154	157	158	rBV3	2264	2376	0.19%	0.016%
6	4.069	164	167	169	rBV4	2872	2972	0.23%	0.020%
7	4.363	214	217	220	rBV5	2151	3113	0.24%	0.021%
8	4.399	220	223	224	rVV3	2018	2092	0.16%	0.014%
9	4.434	228	229	232	rBV3	1264	1309	0.10%	0.009%
10	4.499	238	240	243	rBV	1456	1436	0.11%	0.010%
11	4.534	243	246	249	rVV5	1326	1750	0.14%	0.012%
12	4.575	251	253	256	rBV3	1517	2118	0.17%	0.014%
13	4.728	278	279	282	rBV3	1190	1369	0.11%	0.009%
14	6.240	534	536	540	rVB5	2086	1912	0.15%	0.013%
15	6.369	556	558	559	rBV	2084	1717	0.13%	0.012%
16	6.398	561	563	566	rVB4	1570	1835	0.14%	0.012%
17	6.569	590	592	595	rVV4	1491	1464	0.11%	0.010%
18	6.728	617	619	623	rBV5	1200	1693	0.13%	0.011%
19	6.793	623	630	644	rVV	241868	434158	33.92%	2.946%
20	6.969	654	660	669	rBV	217782	354874	27.72%	2.408%
21	7.145	683	690	705	rBV	270854	460234	35.95%	3.123%
22	7.292	714	715	723	rVB7	1855	3076	0.24%	0.021%
23	7.392	730	732	734	rVB2	2661	1884	0.15%	0.013%
24	7.416	734	736	738	rBV2	2004	1828	0.14%	0.012%
25	7.610	762	769	782	rVB	227826	373488	29.18%	2.534%
26	7.981	828	832	836	rVB4	1512	2243	0.18%	0.015%
27	8.045	836	843	846	rBV5	1057	2380	0.19%	0.016%
28	8.322	883	890	904	rBV	293295	535985	41.87%	3.637%
29	8.775	957	967	979	rBV	256993	441077	34.46%	2.993%
30	9.045	1011	1013	1015	rBV	2087	1698	0.13%	0.012%
31	9.092	1017	1021	1024	rVV5	1228	1822	0.14%	0.012%
32	9.181	1034	1036	1041	rVB3	1420	1700	0.13%	0.012%
33	9.486	1081	1088	1097	rBV	202481	359091	28.05%	2.437%
34	9.728	1126	1129	1130	rVV3	1245	1330	0.10%	0.009%
35	10.016	1171	1178	1208	rBV	258138	530808	41.47%	3.602%
36	10.216	1208	1212	1213	rVB4	1543	1857	0.15%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045189.D
 Acq On : 13 Apr 2024 03:17
 Operator : MA/JU
 Sample : PB160136TB 10X
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLEB097

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	10.381	1231	1240	1249	rBV	309633	513117	40.09%	3.482%
38	10.545	1260	1268	1287	rBV	231922	559698	43.72%	3.798%
39	10.686	1291	1292	1294	rVV2	3169	2460	0.19%	0.017%
40	10.704	1294	1295	1301	rVV5	3192	3836	0.30%	0.026%
41	11.298	1393	1396	1399	rVB3	1613	1780	0.14%	0.012%
42	11.769	1473	1476	1479	rBV4	1503	1827	0.14%	0.012%
43	12.016	1512	1518	1519	rVV4	2219	3684	0.29%	0.025%
44	12.686	1630	1632	1638	rBV4	1402	2012	0.16%	0.014%
45	12.827	1652	1656	1657	rBV3	1581	2065	0.16%	0.014%
46	13.069	1695	1697	1700	rVB3	1229	1361	0.11%	0.009%
47	13.098	1700	1702	1703	rBV2	1826	1300	0.10%	0.009%
48	13.151	1708	1711	1722	rVB7	3734	8745	0.68%	0.059%
49	13.222	1722	1723	1726	rBV2	1399	1436	0.11%	0.010%
50	13.686	1792	1802	1815	rBV	507547	775796	60.61%	5.264%
51	13.780	1815	1818	1820	rVB3	1637	2200	0.17%	0.015%
52	13.951	1839	1847	1861	rBV	659161	976955	76.32%	6.629%
53	14.257	1891	1899	1911	rBV	454385	660755	51.62%	4.483%
54	14.363	1914	1917	1918	rBV3	1464	1614	0.13%	0.011%
55	14.510	1936	1942	1963	rBV3	71227	253248	19.78%	1.718%
56	14.716	1975	1977	1979	rVV2	1145	1303	0.10%	0.009%
57	14.739	1979	1981	1983	rVB3	2002	1558	0.12%	0.011%
58	14.798	1989	1991	1994	rVB4	1142	1380	0.11%	0.009%
59	15.263	2063	2070	2081	rBV	783041	1160404	90.65%	7.874%
60	15.333	2081	2082	2084	rVV2	1782	1379	0.11%	0.009%
61	15.404	2088	2094	2106	rBV	158319	266021	20.78%	1.805%
62	15.510	2109	2112	2118	rVB7	3749	6047	0.47%	0.041%
63	15.945	2184	2186	2188	rVV3	1755	1706	0.13%	0.012%
64	15.998	2191	2195	2196	rVV4	1757	1663	0.13%	0.011%
65	16.057	2199	2205	2208	rVV4	1701	4007	0.31%	0.027%
66	16.345	2250	2254	2257	rBV2	1406	1463	0.11%	0.010%
67	16.562	2289	2291	2293	rBV2	1682	1577	0.12%	0.011%
68	16.815	2332	2334	2336	rVB2	1905	1693	0.13%	0.011%
69	16.951	2354	2357	2359	rVV4	1090	1364	0.11%	0.009%
70	17.015	2362	2368	2379	rBV	501958	699238	54.63%	4.745%
71	17.121	2379	2386	2406	rVV	783075	1194153	93.29%	8.103%
72	17.268	2408	2411	2415	rVB3	1494	2233	0.17%	0.015%
73	17.515	2449	2453	2454	rVV2	1518	1438	0.11%	0.010%
74	17.557	2458	2460	2462	rVB2	1546	1322	0.10%	0.009%
75	17.627	2469	2472	2473	rBV2	1664	1648	0.13%	0.011%
76	17.862	2509	2512	2515	rVB4	1672	2244	0.18%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045189.D
 Acq On : 13 Apr 2024 03:17
 Operator : MA/JU
 Sample : PB160136TB 10X
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLEB097

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

77	17.898	2515	2518	2519	rBV2	2025	1697	0.13%	0.012%
78	18.033	2538	2541	2542	rBV3	1360	1514	0.12%	0.010%
79	18.239	2574	2576	2579	rBV4	1290	1556	0.12%	0.011%
80	18.274	2581	2582	2586	rBV2	1214	1517	0.12%	0.010%
81	18.398	2601	2603	2606	rVV4	1230	1587	0.12%	0.011%
82	18.421	2606	2607	2610	rVB3	1674	1431	0.11%	0.010%
83	18.498	2616	2620	2622	rBV4	2504	4036	0.32%	0.027%
84	18.862	2679	2682	2684	rVB4	1488	1611	0.13%	0.011%
85	18.951	2696	2697	2700	rBV3	1212	1325	0.10%	0.009%
86	18.992	2700	2704	2708	rBV5	8435	10652	0.83%	0.072%
87	19.062	2713	2716	2721	rVB5	4357	5882	0.46%	0.040%
88	19.268	2749	2751	2753	rBV3	1907	1837	0.14%	0.012%
89	19.315	2757	2759	2762	rVB4	1818	1656	0.13%	0.011%
90	19.427	2770	2778	2790	rBV	872486	1280060	100.00%	8.686%
91	19.656	2816	2817	2819	rVV2	2376	1417	0.11%	0.010%
92	20.421	2945	2947	2950	rBV4	4753	5566	0.43%	0.038%
93	21.233	3080	3085	3095	rBV	404562	640271	50.02%	4.344%
94	23.303	3431	3437	3450	rBV2	563930	1106115	86.41%	7.505%
95	23.444	3455	3461	3476	rVB	308158	649160	50.71%	4.405%




Sum of corrected areas: 14737769

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045189.D
Acq On : 13 Apr 2024 03:17
Operator : MA/JU
Sample : PB160136TB 10X
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLEB097

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

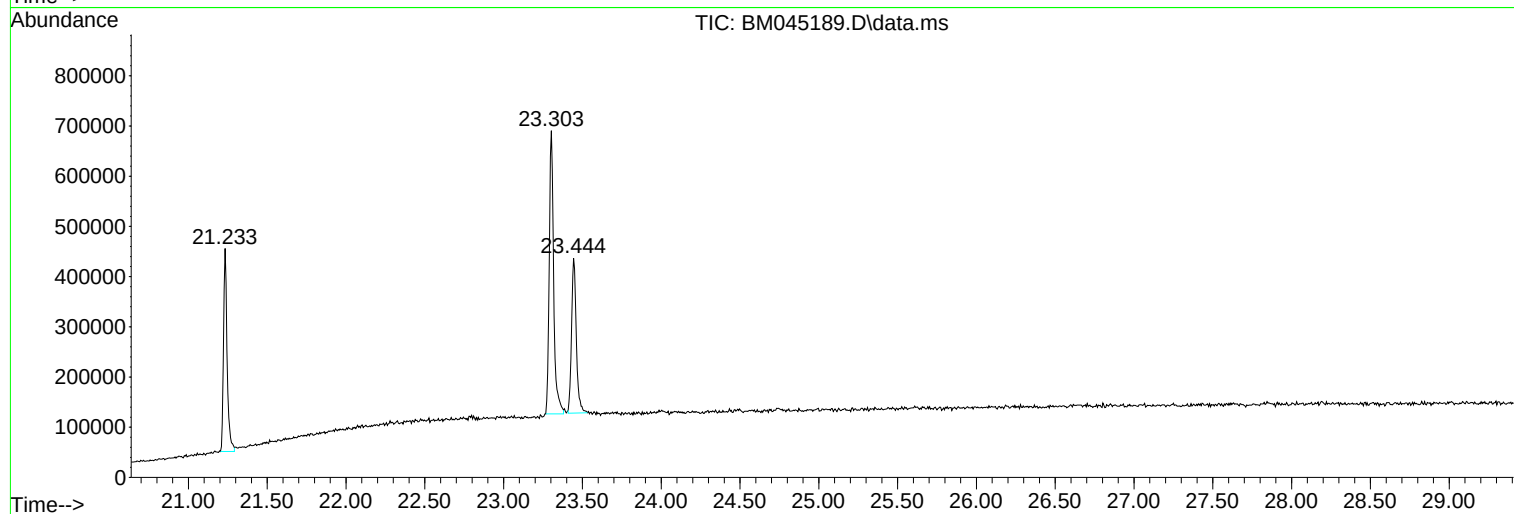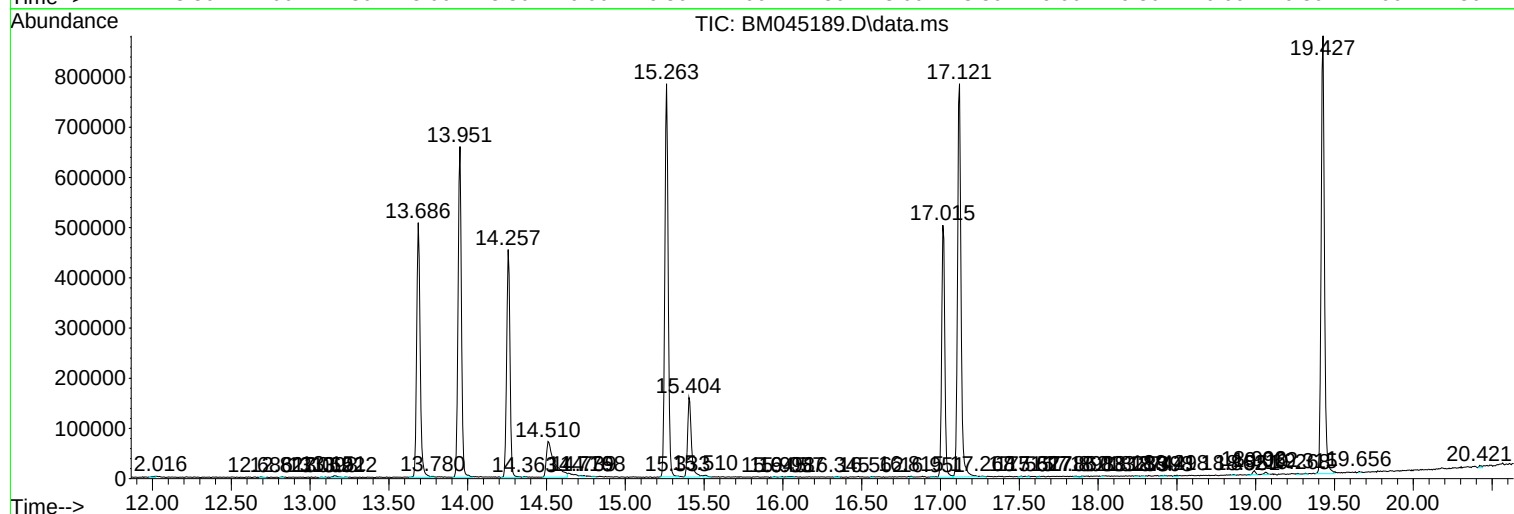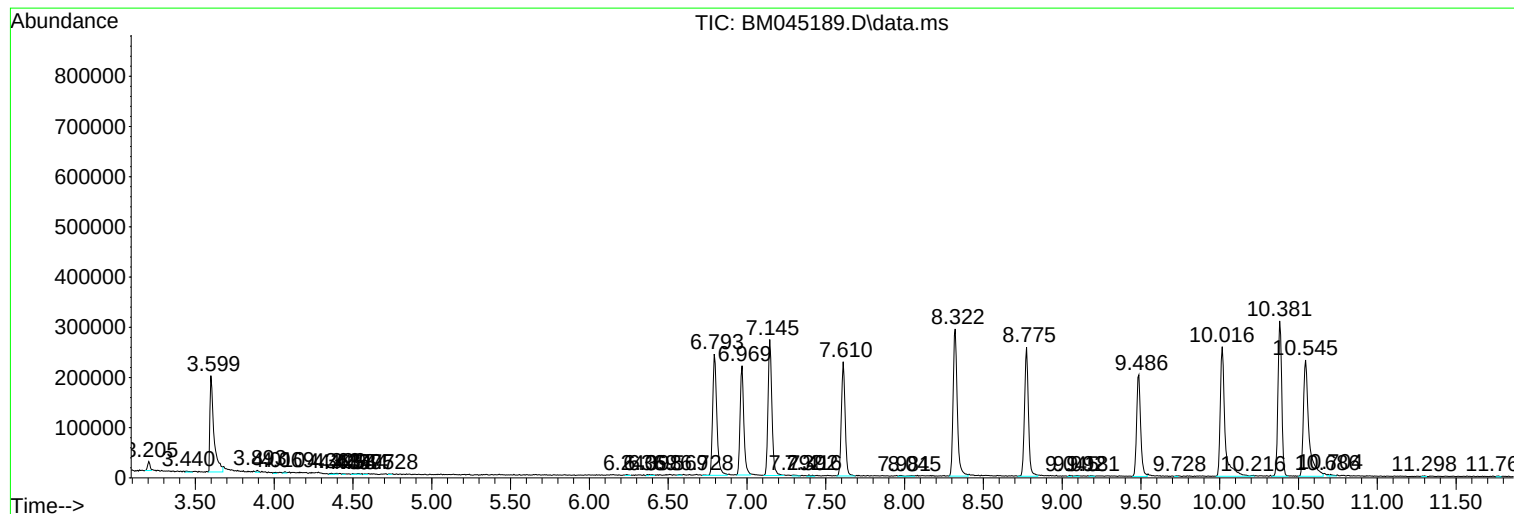

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045189.D
Acq On : 13 Apr 2024 03:17
Operator : MA/JU
Sample : PB160136TB 10X
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLEB097

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045189.D
Acq On : 13 Apr 2024 03:17
Operator : MA/JU
Sample : PB160136TB 10X
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLEB097

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------