

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045193.D
 Acq On : 13 Apr 2024 05:42
 Operator : MA/JU
 Sample : P2014-04
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045193.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	17	20	25	rVB3	14167	17094	0.95%	0.119%
2	3.393	51	52	54	rBV2	2351	2330	0.13%	0.016%
3	3.605	86	88	102	rBV	64855	133010	7.38%	0.922%
4	3.893	133	137	141	rBV5	5863	8758	0.49%	0.061%
5	4.622	260	261	264	rVB3	1940	1937	0.11%	0.013%
6	4.852	297	300	305	rVB6	1444	2343	0.13%	0.016%
7	5.463	400	404	406	rBV4	1451	2378	0.13%	0.016%
8	5.634	430	433	435	rVB3	2059	2285	0.13%	0.016%
9	6.422	563	567	572	rBV4	2022	3388	0.19%	0.023%
10	6.799	624	631	641	rBV	58803	119059	6.61%	0.825%
11	6.969	653	660	673	rBV	216518	370267	20.56%	2.567%
12	7.146	683	690	701	rBV	225532	385817	21.42%	2.675%
13	7.610	763	769	778	rBV	214944	356405	19.79%	2.471%
14	7.687	778	782	787	rVB7	1691	3168	0.18%	0.022%
15	7.810	799	803	808	rVB4	1023	1874	0.10%	0.013%
16	8.322	883	890	901	rBV2	162310	298960	16.60%	2.073%
17	8.769	959	966	978	rBV	253999	455674	25.30%	3.159%
18	9.134	1024	1028	1031	rVB2	3439	4612	0.26%	0.032%
19	9.487	1080	1088	1098	rBV	196283	350468	19.46%	2.430%
20	10.016	1171	1178	1202	rBV	230247	499944	27.76%	3.466%
21	10.381	1232	1240	1250	rBV	274414	471667	26.19%	3.270%
22	10.545	1261	1268	1286	rBV	169666	423055	23.49%	2.933%
23	12.010	1512	1517	1521	rBV4	3534	6049	0.34%	0.042%
24	13.075	1693	1698	1701	rVB4	1376	2236	0.12%	0.016%
25	13.151	1709	1711	1719	rVB4	2540	3781	0.21%	0.026%
26	13.686	1796	1802	1816	rBV	483389	733351	40.71%	5.084%
27	13.951	1839	1847	1858	rBV	616722	960037	53.30%	6.656%
28	14.257	1893	1899	1913	rVV	385360	562505	31.23%	3.900%
29	14.563	1944	1951	1952	rBV4	8695	16083	0.89%	0.112%
30	14.574	1952	1953	1955	rVV2	1925	1816	0.10%	0.013%
31	15.263	2063	2070	2086	rBV	740693	1138724	63.22%	7.895%
32	15.410	2089	2095	2106	rVV	167674	289121	16.05%	2.004%
33	15.504	2110	2111	2118	rVB4	4282	5637	0.31%	0.039%
34	16.427	2265	2268	2271	rBV5	1464	2010	0.11%	0.014%
35	16.533	2284	2286	2289	rBV3	1500	1827	0.10%	0.013%
36	16.804	2328	2332	2336	rBV5	5070	7224	0.40%	0.050%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045193.D
 Acq On : 13 Apr 2024 05:42
 Operator : MA/JU
 Sample : P2014-04
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	16.963	2355	2359	2360	rBV3	2006	1901	0.11%	0.013%
38	17.015	2363	2368	2379	rVV	433866	614664	34.12%	4.261%
39	17.115	2379	2385	2399	rBV2	768405	1200107	66.63%	8.320%
40	17.427	2433	2438	2440	rBV3	3534	4925	0.27%	0.034%
41	17.704	2481	2485	2489	rVB4	2028	2742	0.15%	0.019%
42	17.927	2518	2523	2533	rBV7	16459	29369	1.63%	0.204%
43	18.004	2533	2536	2542	rVV6	3536	5374	0.30%	0.037%
44	18.062	2542	2546	2547	rVV3	1793	2086	0.12%	0.014%
45	18.362	2593	2597	2600	rVV4	2883	3977	0.22%	0.028%
46	18.474	2613	2616	2618	rBV3	2252	2139	0.12%	0.015%
47	18.815	2672	2674	2680	rVB5	2549	3222	0.18%	0.022%
48	18.992	2700	2704	2708	rVB3	9857	12679	0.70%	0.088%
49	19.062	2712	2716	2721	rVV5	7731	10149	0.56%	0.070%
50	19.227	2737	2744	2748	rBV8	7534	13601	0.76%	0.094%
51	19.315	2757	2759	2762	rBV4	2516	2616	0.15%	0.018%
52	19.380	2764	2770	2771	rBV5	3089	4694	0.26%	0.033%
53	19.421	2771	2777	2788	rBV	1026340	1465933	81.38%	10.163%
54	19.733	2829	2830	2833	rBV3	2471	1823	0.10%	0.013%
55	19.815	2839	2844	2847	rBV5	2385	5518	0.31%	0.038%
56	19.921	2858	2862	2864	rBV5	2619	3770	0.21%	0.026%
57	20.133	2896	2898	2900	rBV3	3438	3874	0.22%	0.027%
58	20.968	3036	3040	3044	rBV7	13770	24653	1.37%	0.171%
59	21.233	3079	3085	3094	rBV	451122	674197	37.43%	4.674%
60	23.297	3430	3436	3450	rBV2	953441	1801252	100.00%	12.488%
61	23.439	3454	3460	3473	rVB	451307	883724	49.06%	6.127%




Sum of corrected areas: 14423883

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045193.D
Acq On : 13 Apr 2024 05:42
Operator : MA/JU
Sample : P2014-04
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

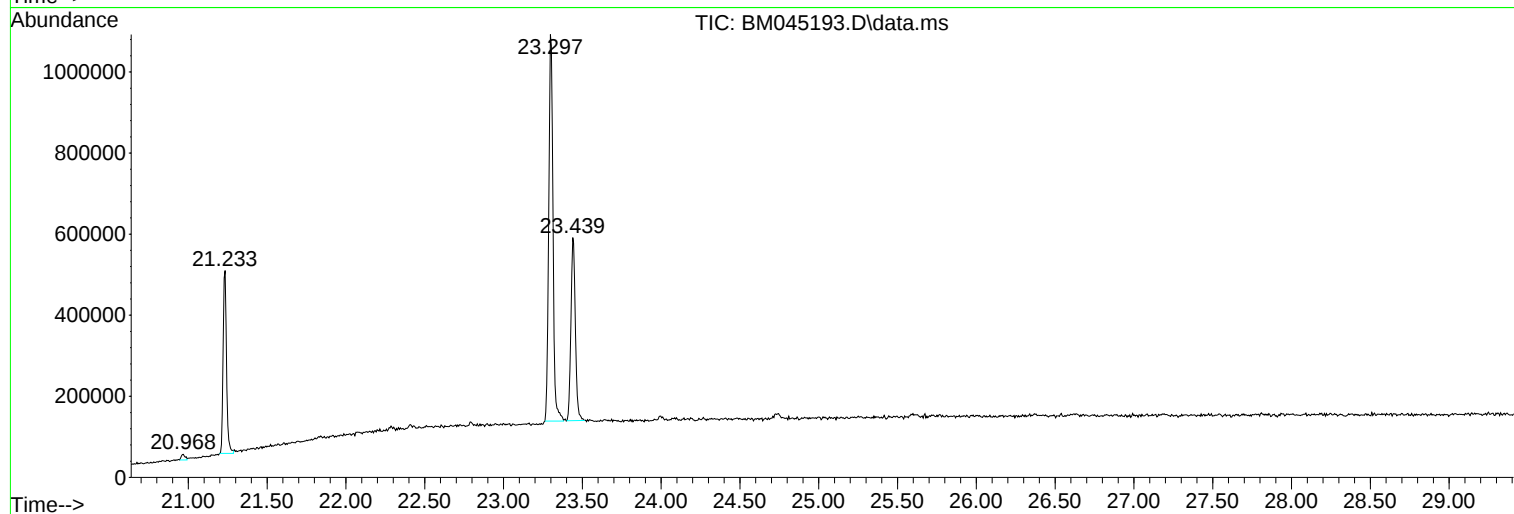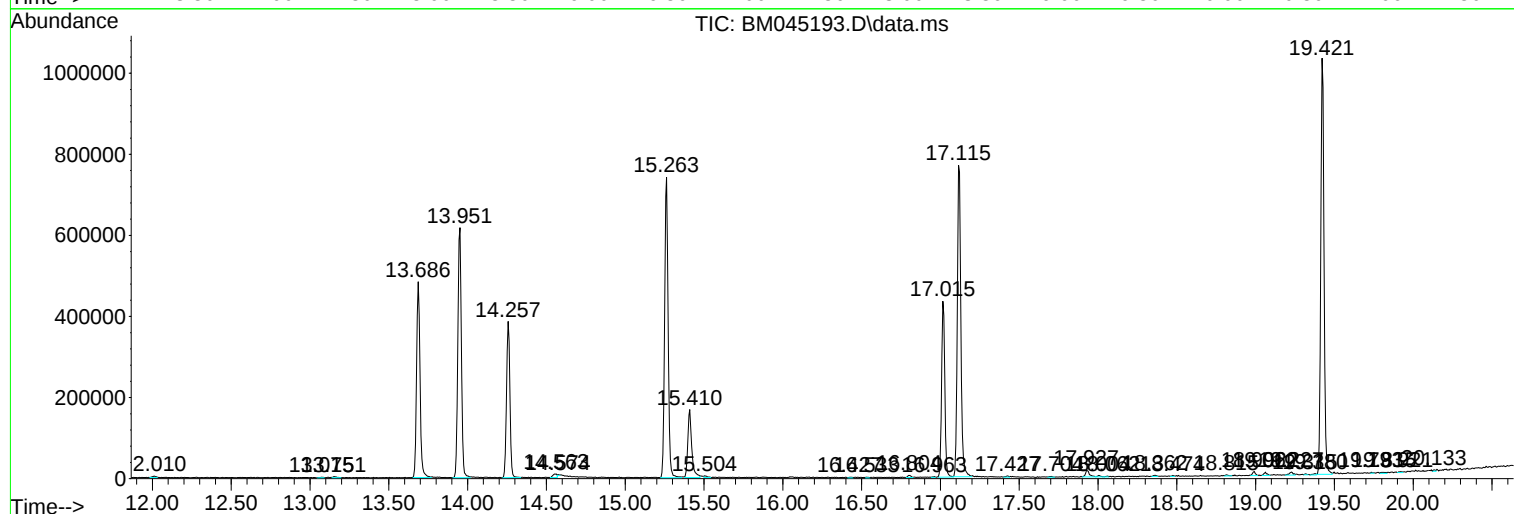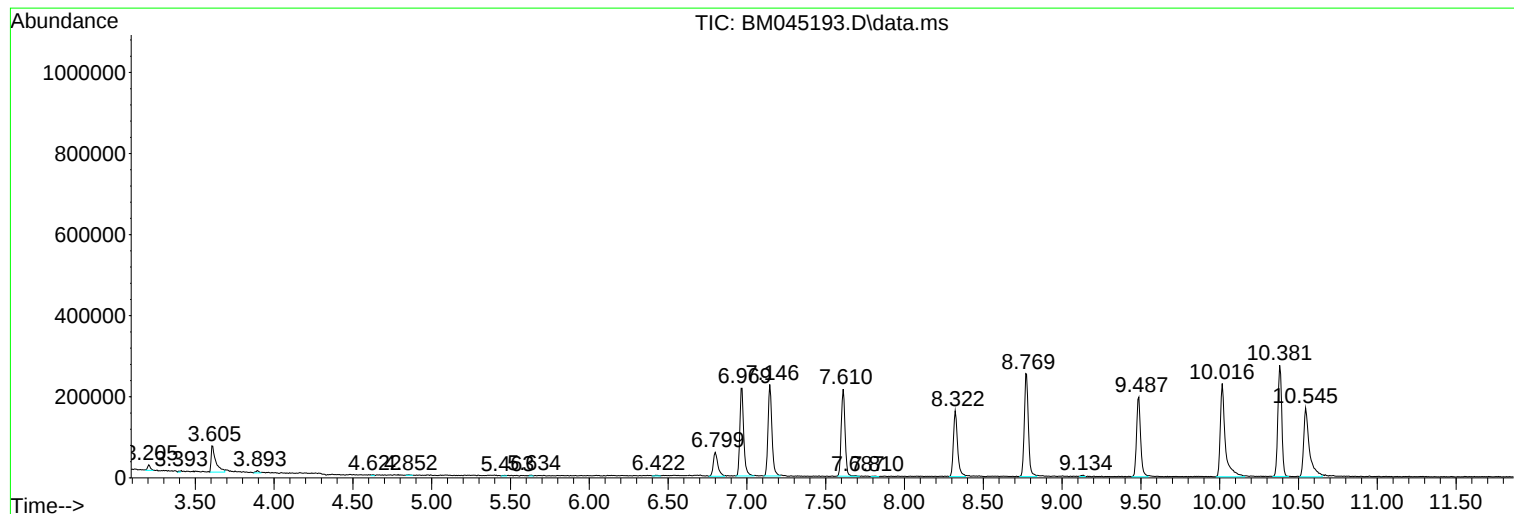

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045193.D
Acq On : 13 Apr 2024 05:42
Operator : MA/JU
Sample : P2014-04
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045193.D
Acq On : 13 Apr 2024 05:42
Operator : MA/JU
Sample : P2014-04
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc