

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045194.D
 Acq On : 13 Apr 2024 06:18
 Operator : MA/JU
 Sample : P2014-05
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045194.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.204	17	20	29	rVB3	12181	19151	1.41%	0.159%
2	3.610	86	89	101	rBV	50032	101157	7.45%	0.839%
3	3.781	116	118	126	rVB7	2566	4016	0.30%	0.033%
4	3.887	134	136	145	rVB8	4134	7882	0.58%	0.065%
5	4.046	161	163	167	rBV5	1501	2383	0.18%	0.020%
6	4.346	212	214	217	rVB2	1769	1616	0.12%	0.013%
7	4.522	243	244	247	rBV2	1282	1516	0.11%	0.013%
8	4.687	269	272	273	rBV3	1713	1595	0.12%	0.013%
9	4.881	302	305	306	rBV3	2279	1911	0.14%	0.016%
10	4.934	312	314	321	rVB5	2523	3863	0.28%	0.032%
11	4.987	321	323	326	rVB3	1743	1746	0.13%	0.014%
12	5.028	329	330	334	rBV4	1814	2013	0.15%	0.017%
13	5.216	361	362	365	rBV3	1648	1908	0.14%	0.016%
14	5.628	430	432	437	rVB5	2000	2585	0.19%	0.021%
15	6.016	496	498	502	rBV4	1405	1528	0.11%	0.013%
16	6.269	539	541	543	rBV3	1140	1395	0.10%	0.012%
17	6.357	553	556	560	rBV5	1545	2226	0.16%	0.018%
18	6.428	566	568	571	rVB5	1928	1599	0.12%	0.013%
19	6.798	626	631	641	rBV	36237	76143	5.61%	0.632%
20	6.969	651	660	671	rBV	186981	321245	23.66%	2.665%
21	7.145	684	690	701	rBV	181751	311765	22.96%	2.586%
22	7.257	708	709	713	rVB2	1806	1922	0.14%	0.016%
23	7.287	713	714	717	rBV3	1699	2140	0.16%	0.018%
24	7.416	732	736	739	rBV6	2145	2956	0.22%	0.025%
25	7.610	762	769	778	rBV	223330	370269	27.27%	3.072%
26	8.322	884	890	902	rBV	108494	207444	15.28%	1.721%
27	8.775	960	967	979	rBV	216543	389639	28.70%	3.232%
28	8.992	1001	1004	1005	rBV3	1080	1362	0.10%	0.011%
29	9.128	1023	1027	1032	rVB7	2488	3406	0.25%	0.028%
30	9.333	1060	1062	1064	rBV2	1596	1359	0.10%	0.011%
31	9.386	1069	1071	1076	rVV4	1134	1469	0.11%	0.012%
32	9.486	1082	1088	1099	rBV	165896	295627	21.77%	2.452%
33	9.616	1107	1110	1115	rVB4	1288	1760	0.13%	0.015%
34	10.016	1172	1178	1203	rBV2	177277	406841	29.96%	3.375%
35	10.216	1209	1212	1216	rVB5	1793	2398	0.18%	0.020%
36	10.380	1233	1240	1249	rBV	285778	487038	35.87%	4.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045194.D
 Acq On : 13 Apr 2024 06:18
 Operator : MA/JU
 Sample : P2014-05
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	10.545	1262	1268	1289	rBV	138837	364649	26.86%	3.025%
38	10.992	1342	1344	1349	rBV4	1379	1416	0.10%	0.012%
39	11.057	1353	1355	1358	rVB2	1254	1484	0.11%	0.012%
40	11.469	1420	1425	1428	rBV5	1119	1475	0.11%	0.012%
41	11.551	1434	1439	1444	rVB5	1450	3085	0.23%	0.026%
42	12.022	1513	1519	1527	rVB6	3474	6578	0.48%	0.055%
43	13.157	1709	1712	1715	rBV3	2552	3399	0.25%	0.028%
44	13.645	1791	1795	1796	rBV2	1155	1490	0.11%	0.012%
45	13.686	1796	1802	1819	rVV	370969	570186	41.99%	4.730%
46	13.951	1839	1847	1858	rBV2	509516	777259	57.24%	6.448%
47	14.257	1892	1899	1909	rBV	391191	561403	41.35%	4.657%
48	14.586	1950	1955	1960	rBV7	4344	11970	0.88%	0.099%
49	14.710	1975	1976	1981	rVV4	937	1643	0.12%	0.014%
50	14.910	2008	2010	2013	rBV2	1610	1770	0.13%	0.015%
51	15.262	2064	2070	2084	rBV	585617	931975	68.64%	7.731%
52	15.410	2090	2095	2106	rBV	119395	215259	15.85%	1.786%
53	15.504	2109	2111	2113	rVV2	3620	3621	0.27%	0.030%
54	15.527	2113	2115	2118	rVB2	1864	1769	0.13%	0.015%
55	15.662	2134	2138	2140	rBV3	1207	1414	0.10%	0.012%
56	16.145	2217	2220	2224	rVB3	1087	1943	0.14%	0.016%
57	16.245	2235	2237	2239	rBV2	1745	1776	0.13%	0.015%
58	16.698	2312	2314	2318	rVB4	1567	2276	0.17%	0.019%
59	16.962	2356	2359	2362	rVB4	1898	2559	0.19%	0.021%
60	17.015	2362	2368	2379	rBV	394766	576183	42.43%	4.780%
61	17.121	2379	2386	2402	rVV	631539	986966	72.69%	8.187%
62	17.333	2419	2422	2426	rVB6	1763	2451	0.18%	0.020%
63	17.562	2459	2461	2465	rVB4	1156	1484	0.11%	0.012%
64	17.703	2483	2485	2489	rBV4	2414	2435	0.18%	0.020%
65	17.933	2519	2524	2530	rBV5	7293	12696	0.94%	0.105%
66	18.056	2543	2545	2549	rBV4	1294	2150	0.16%	0.018%
67	18.233	2572	2575	2576	rBV3	1460	1358	0.10%	0.011%
68	18.274	2579	2582	2583	rBV3	1946	2079	0.15%	0.017%
69	18.327	2588	2591	2592	rBV2	1364	1639	0.12%	0.014%
70	18.351	2594	2595	2600	rBV5	1087	1538	0.11%	0.013%
71	18.615	2636	2640	2641	rBV4	1386	1848	0.14%	0.015%
72	18.627	2641	2642	2646	rVB4	2010	1694	0.12%	0.014%
73	18.662	2646	2648	2650	rBV2	1424	1420	0.10%	0.012%
74	18.845	2677	2679	2680	rBV	2305	1503	0.11%	0.012%
75	18.939	2692	2695	2696	rBV3	1708	1614	0.12%	0.013%
76	18.992	2699	2704	2707	rVV7	5386	8151	0.60%	0.068%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045194.D
Acq On : 13 Apr 2024 06:18
Operator : MA/JU
Sample : P2014-05
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

77	19.068	2709	2717	2721	rBV3	5394	11601	0.85%	0.096%
78	19.192	2737	2738	2741	rBV	1478	1504	0.11%	0.012%
79	19.233	2741	2745	2747	rBV4	4629	5807	0.43%	0.048%
80	19.427	2772	2778	2789	rBV	797517	1139022	83.89%	9.449%
81	20.021	2877	2879	2881	rBV3	2663	1494	0.11%	0.012%
82	20.962	3035	3039	3040	rBV4	9953	12525	0.92%	0.104%
83	21.233	3079	3085	3094	rBV	400000	623388	45.91%	5.171%
84	23.297	3430	3436	3447	rBV	708401	1357812	100.00%	11.264%
85	23.444	3454	3461	3473	rVB	386940	779282	57.39%	6.464%




Sum of corrected areas: 12054916

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045194.D
Acq On : 13 Apr 2024 06:18
Operator : MA/JU
Sample : P2014-05
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

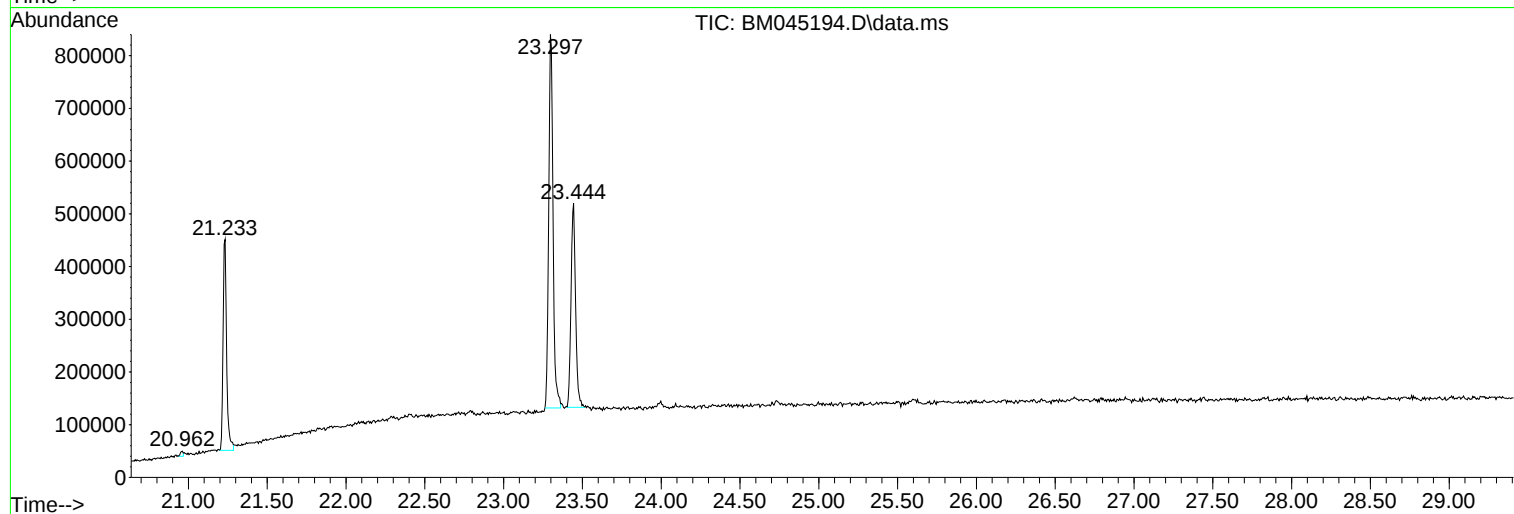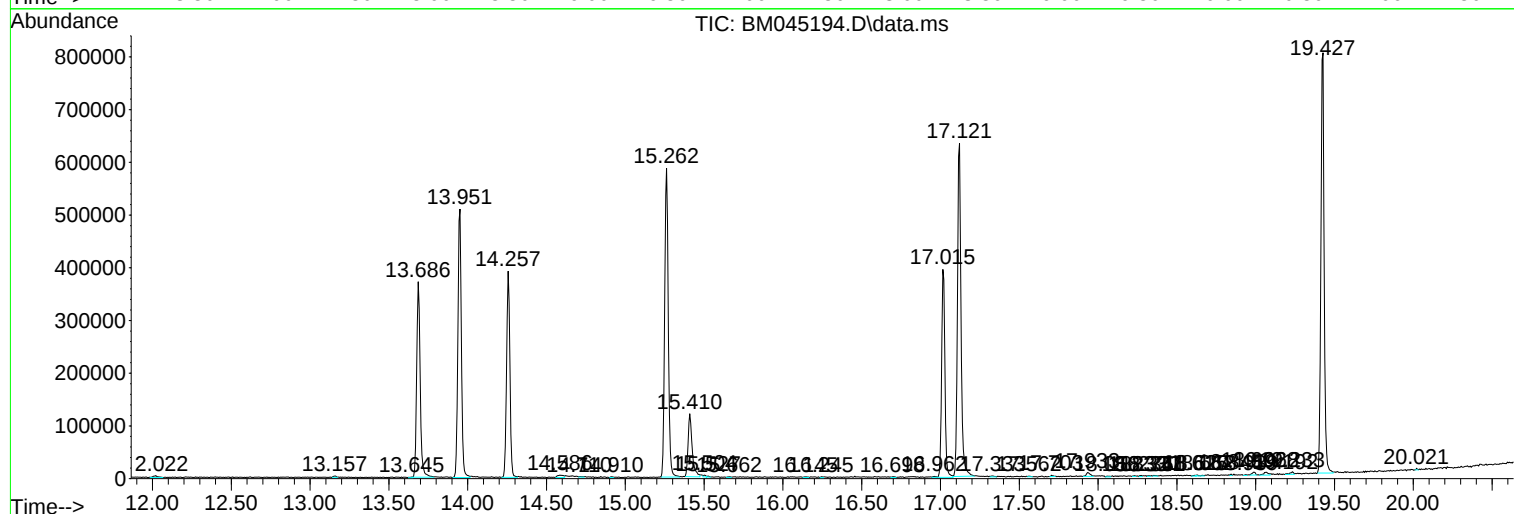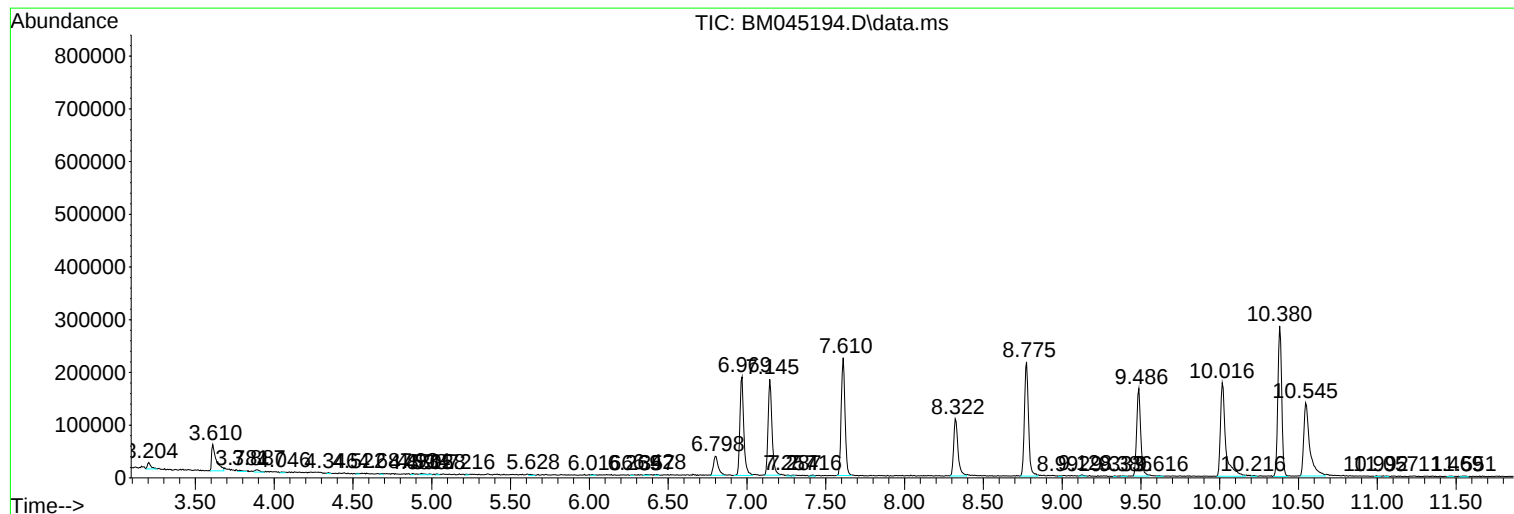

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045194.D
Acq On : 13 Apr 2024 06:18
Operator : MA/JU
Sample : P2014-05
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045194.D
Acq On : 13 Apr 2024 06:18
Operator : MA/JU
Sample : P2014-05
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------