

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045197.D
 Acq On : 13 Apr 2024 08:06
 Operator : MA/JU
 Sample : P2014-20
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOME5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045197.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.204	16	20	27	rVV3	8683	14358	1.43%	0.136%
2	3.604	86	88	99	rBV	52142	99702	9.91%	0.946%
3	3.852	128	130	133	rVB4	2625	1616	0.16%	0.015%
4	3.893	135	137	143	rVB7	3742	5222	0.52%	0.050%
5	4.134	175	178	179	rVB2	1803	1369	0.14%	0.013%
6	4.157	179	182	185	rBV3	1980	2313	0.23%	0.022%
7	4.216	191	192	194	rVB	2108	1252	0.12%	0.012%
8	4.240	194	196	198	rBV3	1527	1449	0.14%	0.014%
9	5.028	329	330	334	rVB3	1403	1360	0.14%	0.013%
10	5.122	345	346	349	rVB3	1763	1167	0.12%	0.011%
11	5.146	349	350	354	rBV3	1367	1718	0.17%	0.016%
12	5.198	357	359	363	rVB4	985	1253	0.12%	0.012%
13	5.363	385	387	389	rVB3	1823	1284	0.13%	0.012%
14	5.540	413	417	419	rVB3	1685	1870	0.19%	0.018%
15	5.851	468	470	474	rVB5	1677	1661	0.17%	0.016%
16	5.893	474	477	479	rBV4	1237	1409	0.14%	0.013%
17	6.293	543	545	548	rBV2	1721	2004	0.20%	0.019%
18	6.322	548	550	553	rBV4	1417	1625	0.16%	0.015%
19	6.463	570	574	575	rBV3	1024	1345	0.13%	0.013%
20	6.610	598	599	601	rVV2	2074	1217	0.12%	0.012%
21	6.798	626	631	641	rVV2	36982	79679	7.92%	0.756%
22	6.963	653	659	674	rBV	197432	340047	33.81%	3.226%
23	7.069	676	677	679	rVV2	1400	1188	0.12%	0.011%
24	7.145	683	690	701	rVV	195346	338576	33.66%	3.212%
25	7.222	701	703	706	rVB3	3591	3005	0.30%	0.029%
26	7.334	721	722	726	rVB3	1614	1354	0.13%	0.013%
27	7.457	740	743	744	rBV3	1522	1269	0.13%	0.012%
28	7.498	747	750	752	rBV4	1269	1429	0.14%	0.014%
29	7.551	757	759	763	rVV4	1260	1627	0.16%	0.015%
30	7.610	763	769	781	rVV	167600	275197	27.36%	2.611%
31	7.739	788	791	794	rVB5	1063	1552	0.15%	0.015%
32	7.781	794	798	801	rBV4	1422	2012	0.20%	0.019%
33	7.922	819	822	826	rVV5	1105	2060	0.20%	0.020%
34	8.216	869	872	875	rVB4	1659	2089	0.21%	0.020%
35	8.245	875	877	880	rBV2	1462	1606	0.16%	0.015%
36	8.322	884	890	903	rBV2	129801	238124	23.67%	2.259%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045197.D
 Acq On : 13 Apr 2024 08:06
 Operator : MA/JU
 Sample : P2014-20
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOME5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	8.710	954	956	959	rBV3	1120	1231	0.12%	0.012%
38	8.775	959	967	977	rBV	224793	398439	39.61%	3.780%
39	8.886	985	986	988	rVB2	1885	1235	0.12%	0.012%
40	8.916	990	991	994	rBV2	1740	1310	0.13%	0.012%
41	8.992	1003	1004	1008	rBV3	1169	1303	0.13%	0.012%
42	9.228	1040	1044	1048	rBV4	1075	2169	0.22%	0.021%
43	9.392	1069	1072	1075	rVB4	1032	1230	0.12%	0.012%
44	9.486	1081	1088	1102	rBV	174530	312268	31.05%	2.962%
45	9.663	1116	1118	1121	rVB3	1347	1239	0.12%	0.012%
46	10.016	1171	1178	1202	rVV	202203	436968	43.44%	4.145%
47	10.222	1209	1213	1218	rVB6	1011	1770	0.18%	0.017%
48	10.380	1233	1240	1251	rVV	216338	358918	35.68%	3.405%
49	10.545	1261	1268	1286	rBV	142211	351282	34.92%	3.332%
50	10.657	1286	1287	1288	rVV	4000	2150	0.21%	0.020%
51	10.680	1290	1291	1296	rVV3	2993	3565	0.35%	0.034%
52	10.851	1318	1320	1323	rVB3	1260	1347	0.13%	0.013%
53	10.904	1323	1329	1332	rBV5	1417	3011	0.30%	0.029%
54	11.227	1378	1384	1386	rBV6	931	1529	0.15%	0.015%
55	11.327	1399	1401	1403	rVB3	1444	1201	0.12%	0.011%
56	11.416	1412	1416	1420	rBV3	849	1229	0.12%	0.012%
57	11.733	1467	1470	1472	rVB3	1208	1506	0.15%	0.014%
58	11.798	1478	1481	1484	rBV2	959	1737	0.17%	0.016%
59	11.951	1500	1507	1513	rBV3	9510	20863	2.07%	0.198%
60	12.004	1513	1516	1524	rVB6	3569	6978	0.69%	0.066%
61	12.863	1660	1662	1668	rBV4	1379	2957	0.29%	0.028%
62	13.145	1709	1710	1715	rBV4	1297	1572	0.16%	0.015%
63	13.233	1721	1725	1726	rBV3	1352	1616	0.16%	0.015%
64	13.416	1753	1756	1759	rVB3	1007	1467	0.15%	0.014%
65	13.686	1796	1802	1816	rVV	416699	646061	64.23%	6.129%
66	13.951	1840	1847	1857	rBV	561228	850074	84.51%	8.064%
67	14.257	1891	1899	1907	rBV	294412	430513	42.80%	4.084%
68	14.386	1916	1921	1922	rBV3	1348	1737	0.17%	0.016%
69	14.592	1951	1956	1957	rBV4	3895	5720	0.57%	0.054%
70	14.910	2009	2010	2014	rBV3	1330	1495	0.15%	0.014%
71	15.027	2024	2030	2031	rBV2	1541	1918	0.19%	0.018%
72	15.163	2050	2053	2056	rVB2	928	1183	0.12%	0.011%
73	15.263	2063	2070	2082	rBV	655007	1005854	100.00%	9.542%
74	15.410	2089	2095	2109	rBV	113840	201837	20.07%	1.915%
75	15.515	2111	2113	2119	rVB4	3134	3429	0.34%	0.033%
76	15.957	2186	2188	2191	rBV2	1477	1478	0.15%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045197.D
 Acq On : 13 Apr 2024 08:06
 Operator : MA/JU
 Sample : P2014-20
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOME5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

77	16.051	2202	2204	2207	rBV2	1761	1908	0.19%	0.018%
78	16.168	2220	2224	2226	rBV3	1341	1714	0.17%	0.016%
79	16.274	2239	2242	2245	rBV2	1233	1449	0.14%	0.014%
80	16.327	2248	2251	2256	rVB5	1148	1771	0.18%	0.017%
81	16.709	2313	2316	2319	rBV3	1489	1477	0.15%	0.014%
82	17.015	2363	2368	2379	rBV	298246	424869	42.24%	4.030%
83	17.115	2379	2385	2398	rVV	620790	972545	96.69%	9.226%
84	17.227	2402	2404	2406	rVB2	1617	1443	0.14%	0.014%
85	17.451	2438	2442	2446	rBV4	982	1746	0.17%	0.017%
86	17.704	2481	2485	2486	rBV2	1671	2099	0.21%	0.020%
87	17.762	2494	2495	2497	rBV2	1598	1204	0.12%	0.011%
88	17.792	2497	2500	2505	rVB4	1136	1796	0.18%	0.017%
89	17.933	2520	2524	2533	rBV7	10851	21940	2.18%	0.208%
90	18.080	2547	2549	2552	rBV2	1245	1182	0.12%	0.011%
91	18.574	2632	2633	2636	rBV2	1405	1233	0.12%	0.012%
92	18.992	2700	2704	2709	rBV6	5146	8255	0.82%	0.078%
93	19.062	2712	2716	2719	rBV3	5958	8504	0.85%	0.081%
94	19.233	2740	2745	2751	rBV8	5959	12639	1.26%	0.120%
95	19.374	2768	2769	2772	rVV2	2659	1728	0.17%	0.016%
96	19.421	2772	2777	2790	rVV	673366	968909	96.33%	9.191%
97	20.956	3036	3038	3041	rBV4	6327	8207	0.82%	0.078%
98	21.233	3080	3085	3094	rBV	217676	339714	33.77%	3.223%
99	23.303	3430	3437	3449	rBV	412874	874731	86.96%	8.298%
100	23.444	3455	3461	3472	rVB	174234	370944	36.88%	3.519%




Sum of corrected areas: 10541404

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045197.D
Acq On : 13 Apr 2024 08:06
Operator : MA/JU
Sample : P2014-20
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

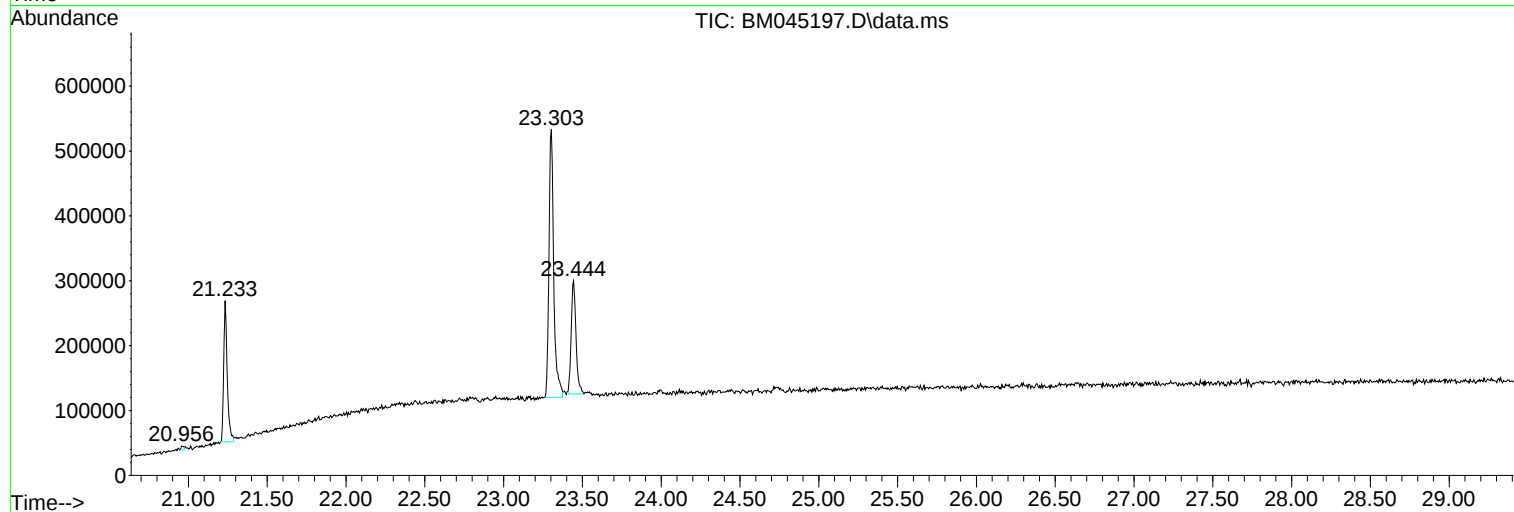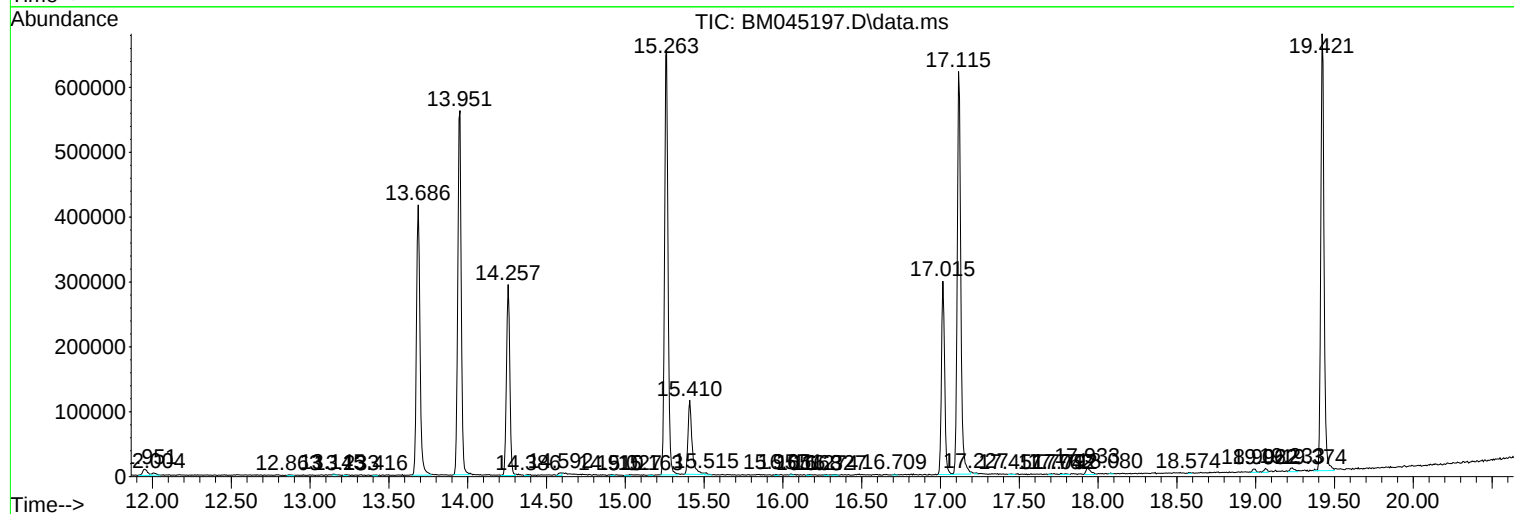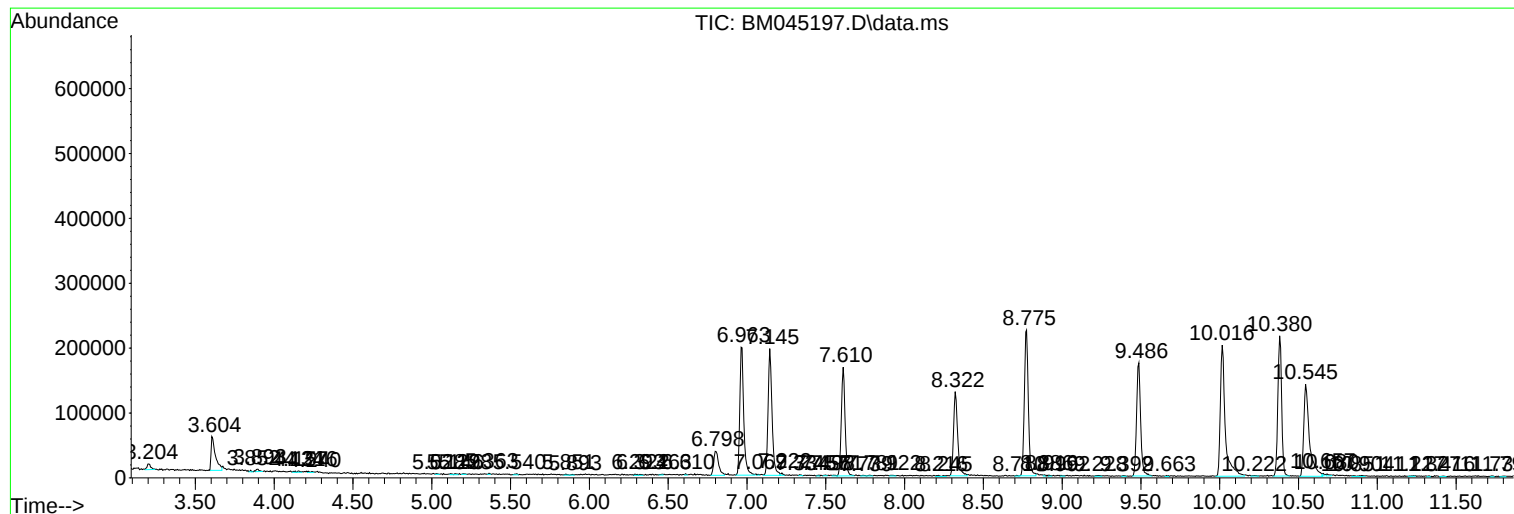

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045197.D
Acq On : 13 Apr 2024 08:06
Operator : MA/JU
Sample : P2014-20
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045197.D
Acq On : 13 Apr 2024 08:06
Operator : MA/JU
Sample : P2014-20
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------