

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045200.D
 Acq On : 13 Apr 2024 09:54
 Operator : MA/JU
 Sample : P2014-09
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045200.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	26	rBV2	12928	19060	1.15%	0.120%
2	3.605	86	88	104	rBV	56808	130488	7.91%	0.822%
3	3.893	133	137	141	rBV4	5247	8126	0.49%	0.051%
4	4.334	209	212	213	rBV3	2167	2098	0.13%	0.013%
5	4.381	218	220	225	rBV4	1742	2633	0.16%	0.017%
6	5.628	428	432	434	rVB4	1462	1937	0.12%	0.012%
7	6.052	502	504	507	rBV3	1458	1750	0.11%	0.011%
8	6.305	543	547	552	rBV5	1440	2571	0.16%	0.016%
9	6.799	626	631	643	rBV	49350	101296	6.14%	0.638%
10	6.964	651	659	671	rBV	251409	431000	26.12%	2.715%
11	7.146	683	690	699	rBV	238336	412836	25.02%	2.600%
12	7.211	699	701	706	rVB6	4133	5839	0.35%	0.037%
13	7.611	763	769	779	rBV	249933	414891	25.14%	2.613%
14	8.322	881	890	902	rBV	164321	306194	18.55%	1.929%
15	8.769	960	966	977	rBV	300548	526699	31.92%	3.317%
16	8.928	992	993	1000	rVB7	2759	3914	0.24%	0.025%
17	9.128	1021	1027	1032	rVB6	2939	5892	0.36%	0.037%
18	9.481	1081	1087	1105	rBV	229229	408815	24.77%	2.575%
19	10.016	1171	1178	1192	rBV	266269	549040	33.27%	3.458%
20	10.381	1231	1240	1249	rBV	342142	577424	34.99%	3.637%
21	10.540	1259	1267	1290	rBV	230540	546495	33.12%	3.442%
22	10.969	1339	1340	1344	rBV5	1559	1751	0.11%	0.011%
23	11.222	1380	1383	1388	rVB6	1837	3213	0.19%	0.020%
24	12.004	1513	1516	1521	rVB3	3249	6060	0.37%	0.038%
25	12.398	1580	1583	1587	rBV3	1256	1863	0.11%	0.012%
26	13.157	1708	1712	1717	rVB5	4556	7909	0.48%	0.050%
27	13.687	1793	1802	1816	rBV	626867	960755	58.22%	6.051%
28	13.945	1839	1846	1860	rBV2	799543	1196769	72.52%	7.538%
29	14.257	1892	1899	1914	rVB	499603	724566	43.91%	4.564%
30	14.569	1945	1952	1955	rBV6	8553	17252	1.05%	0.109%
31	14.628	1960	1962	1965	rVV4	3360	4516	0.27%	0.028%
32	14.675	1968	1970	1973	rVB4	2235	1763	0.11%	0.011%
33	15.057	2034	2035	2039	rVB3	1907	1899	0.12%	0.012%
34	15.204	2056	2060	2061	rBV3	1259	1704	0.10%	0.011%
35	15.257	2061	2069	2083	rVV	947586	1469467	89.05%	9.255%
36	15.404	2089	2094	2109	rBV	200521	328633	19.91%	2.070%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
 Data File : BM045200.D
 Acq On : 13 Apr 2024 09:54
 Operator : MA/JU
 Sample : P2014-09
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	15.663	2134	2138	2140	rBV5	1710	2261	0.14%	0.014%
38	16.057	2200	2205	2208	rBV4	2943	5235	0.32%	0.033%
39	16.692	2310	2313	2314	rBV	1839	1779	0.11%	0.011%
40	16.875	2341	2344	2350	rBV5	2612	4108	0.25%	0.026%
41	17.016	2362	2368	2378	rBV	556648	769408	46.62%	4.846%
42	17.116	2378	2385	2401	rVV2	1016381	1548325	93.82%	9.752%
43	17.222	2401	2403	2409	rVB5	2073	2768	0.17%	0.017%
44	17.445	2440	2441	2446	rBV3	1788	2380	0.14%	0.015%
45	17.775	2494	2497	2500	rBV4	1477	1683	0.10%	0.011%
46	17.833	2500	2507	2509	rBV4	1300	2589	0.16%	0.016%
47	17.933	2517	2524	2532	rBV7	10669	20037	1.21%	0.126%
48	18.010	2536	2537	2540	rVB2	2068	1845	0.11%	0.012%
49	18.339	2590	2593	2598	rBV6	1582	2442	0.15%	0.015%
50	18.498	2615	2620	2621	rBV4	2933	4102	0.25%	0.026%
51	18.986	2699	2703	2707	rBV3	9091	12895	0.78%	0.081%
52	19.063	2713	2716	2721	rVB	7524	10157	0.62%	0.064%
53	19.122	2725	2726	2729	rBV4	2959	3572	0.22%	0.022%
54	19.233	2740	2745	2748	rBV7	4595	6976	0.42%	0.044%
55	19.374	2767	2769	2771	rBV3	2495	2430	0.15%	0.015%
56	19.422	2771	2777	2791	rBV	1181982	1650240	100.00%	10.394%
57	19.557	2798	2800	2802	rBV3	2274	1747	0.11%	0.011%
58	19.639	2812	2814	2817	rVB4	2822	2454	0.15%	0.015%
59	20.122	2894	2896	2897	rBV2	3867	2668	0.16%	0.017%
60	20.421	2945	2947	2948	rBV2	3680	2801	0.17%	0.018%
61	20.969	3036	3040	3046	rBV6	11205	20524	1.24%	0.129%
62	21.233	3079	3085	3094	rBV	391655	616965	37.39%	3.886%
63	23.298	3430	3436	3450	rBV2	679116	1359869	82.40%	8.565%
64	23.439	3455	3460	3474	rVB	305200	627402	38.02%	3.952%




Sum of corrected areas: 15876780

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045200.D
Acq On : 13 Apr 2024 09:54
Operator : MA/JU
Sample : P2014-09
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MD5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

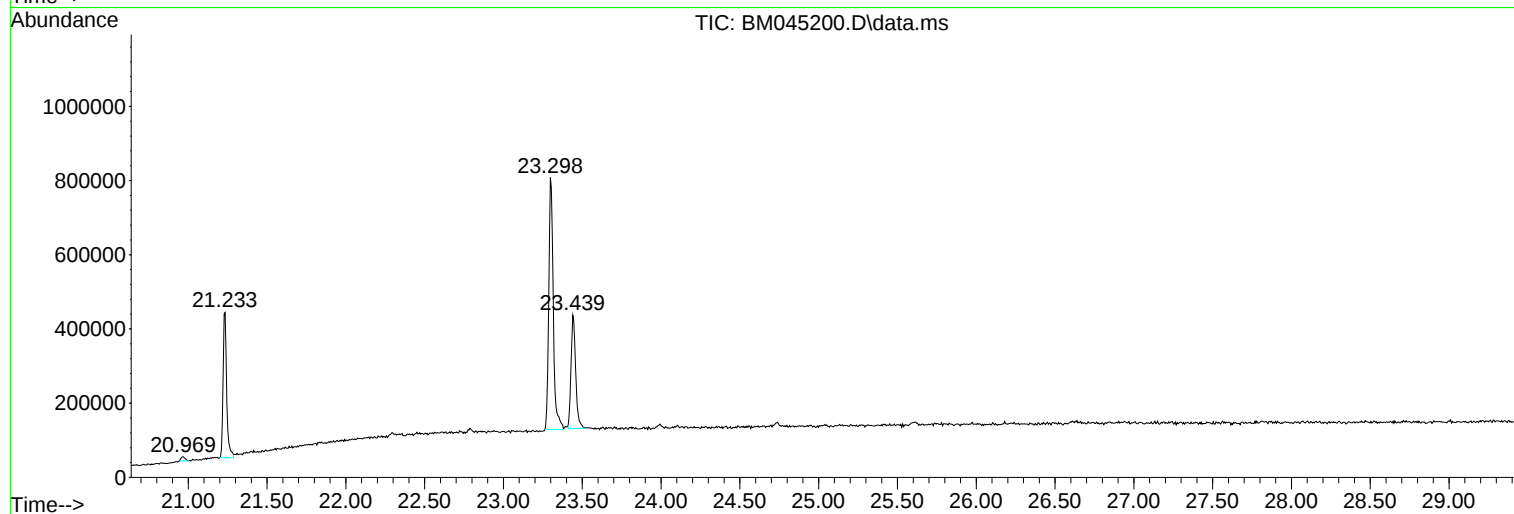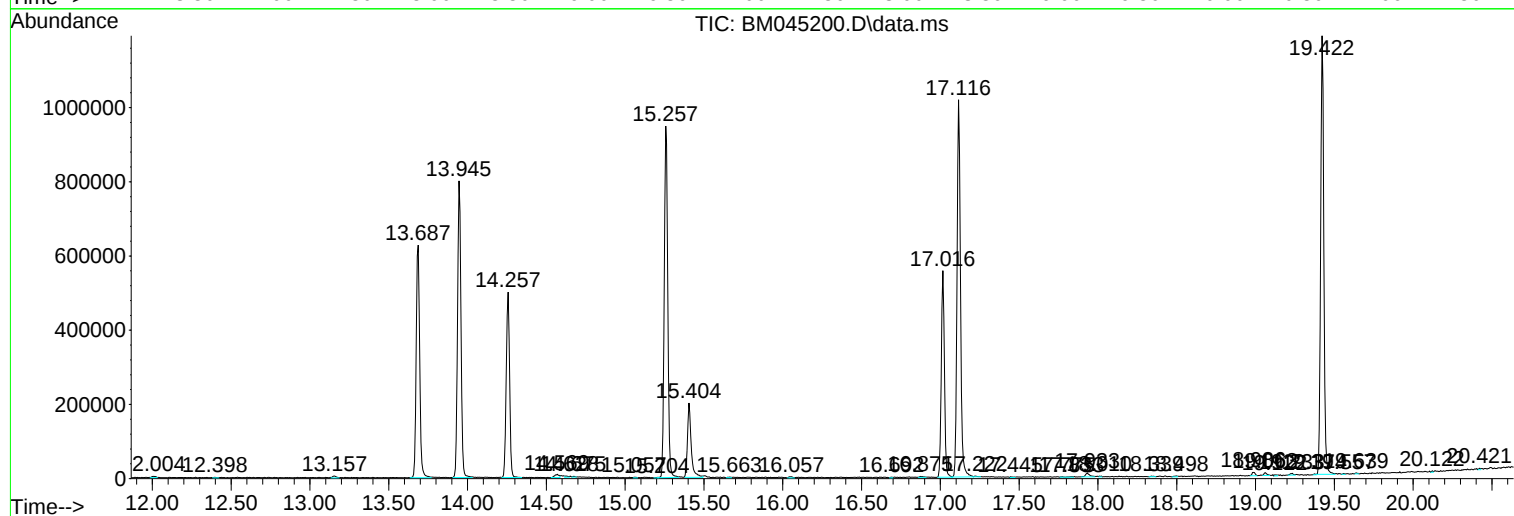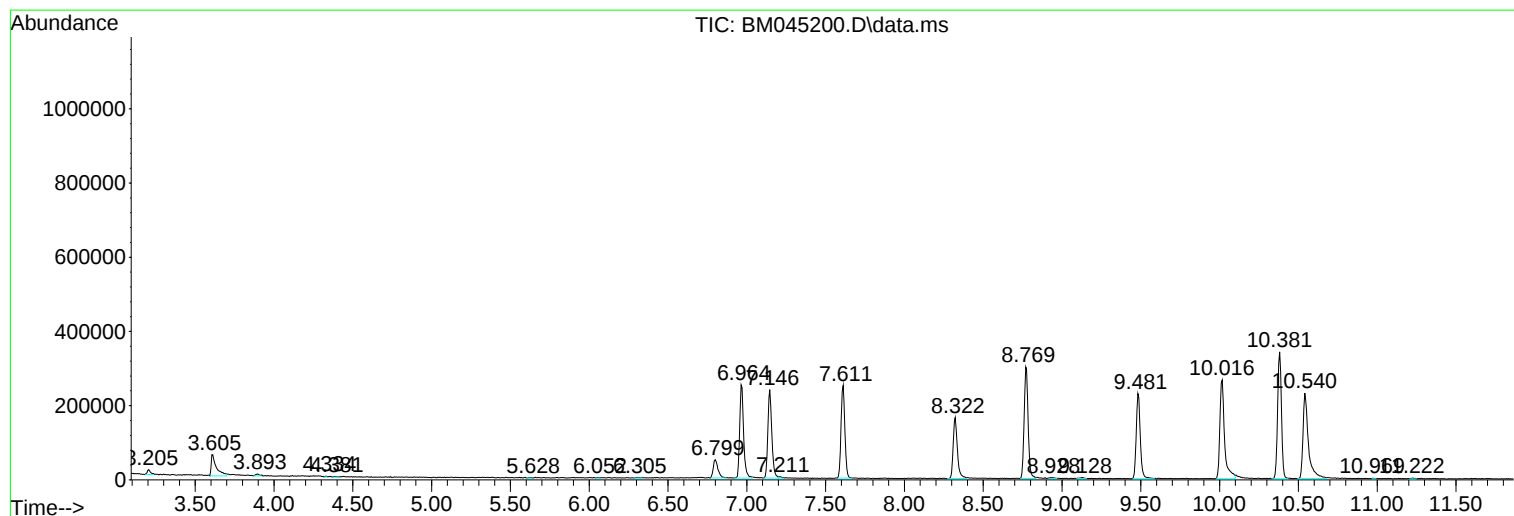

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045200.D
Acq On : 13 Apr 2024 09:54
Operator : MA/JU
Sample : P2014-09
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MD5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045200.D
Acq On : 13 Apr 2024 09:54
Operator : MA/JU
Sample : P2014-09
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MD5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc