
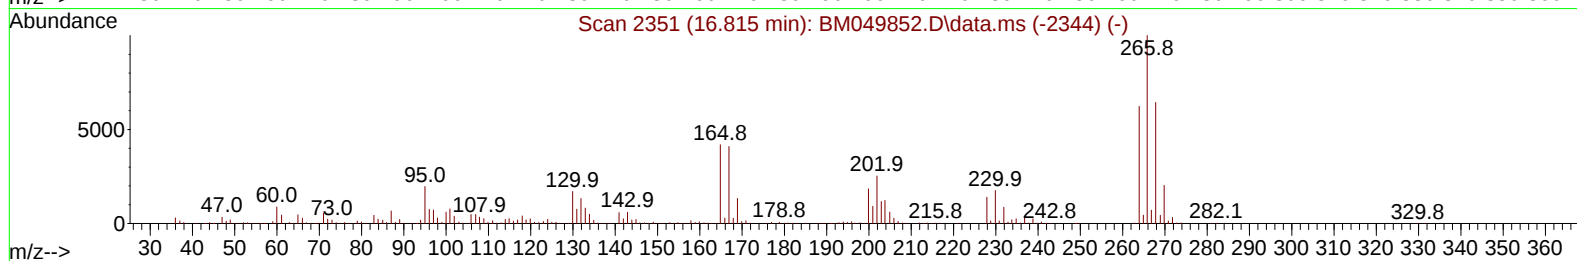
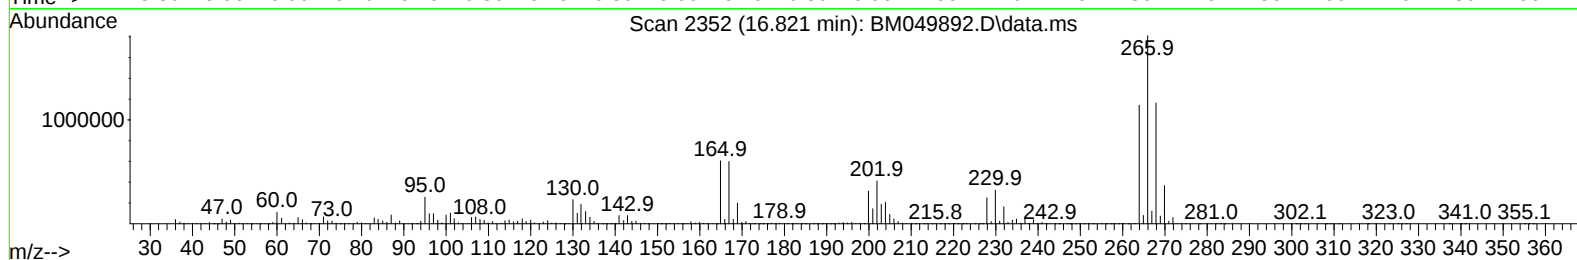


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041125\
Data File : BM049892.D
Acq On : 11 Apr 2025 08:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 11:40:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

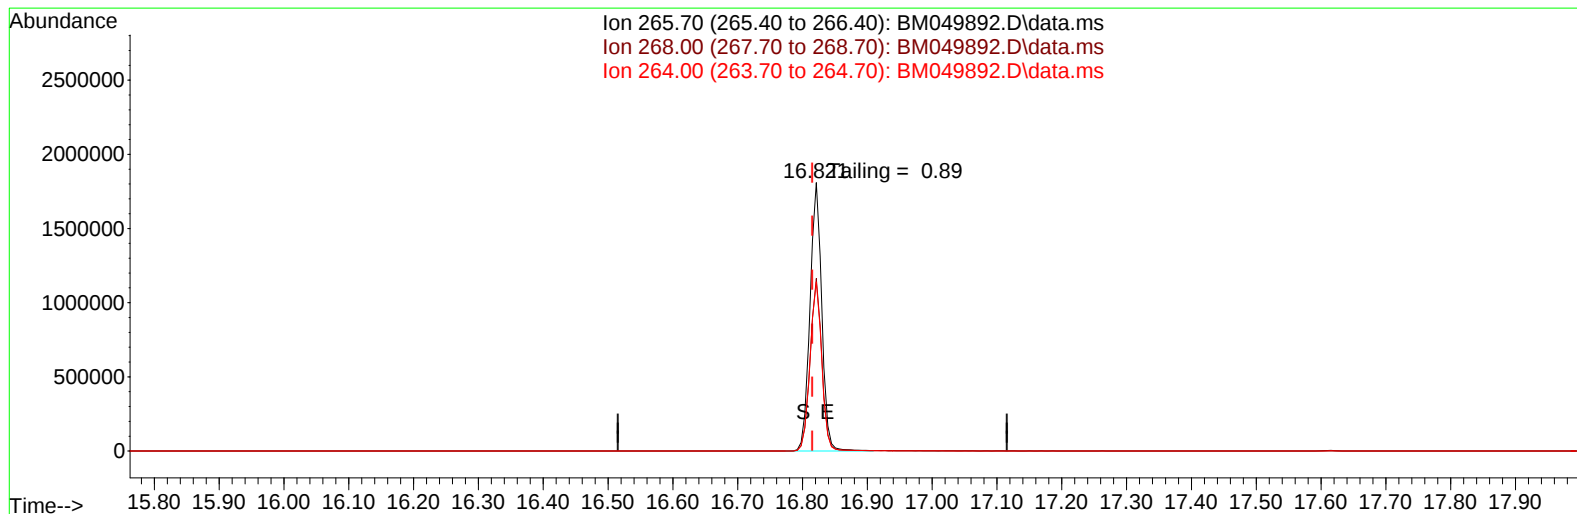

TIC: BM049892.D\data.ms

(70) Pentachlorophenol (C)




16.821min (+ 0.006) 669887.62 ng

response 2252497

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	64.26
264.00	62.30	63.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041125\
Data File : BM049892.D
Acq On : 11 Apr 2025 08:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 11:40:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

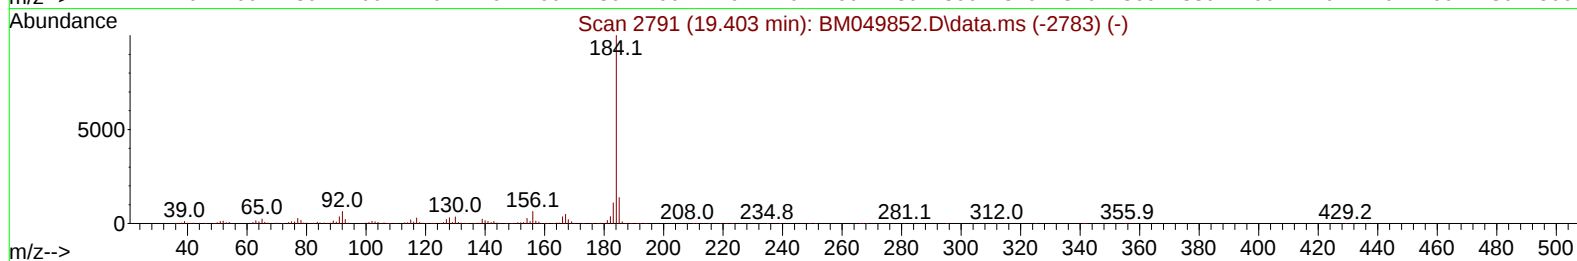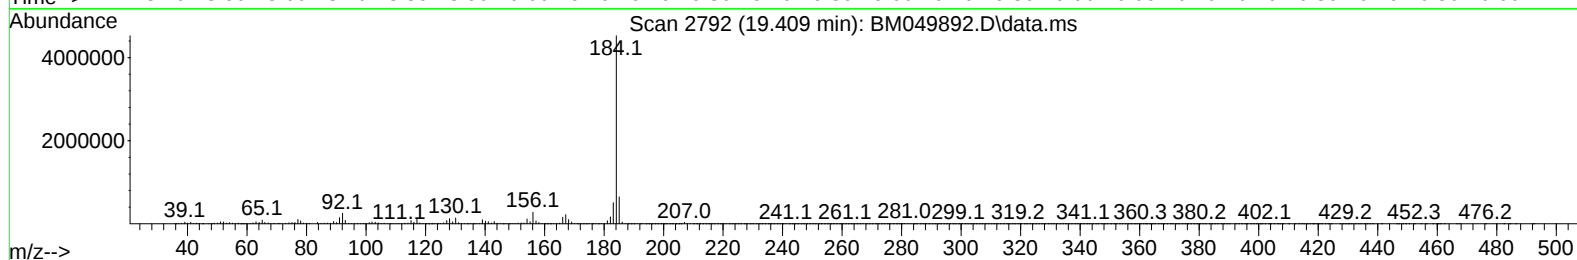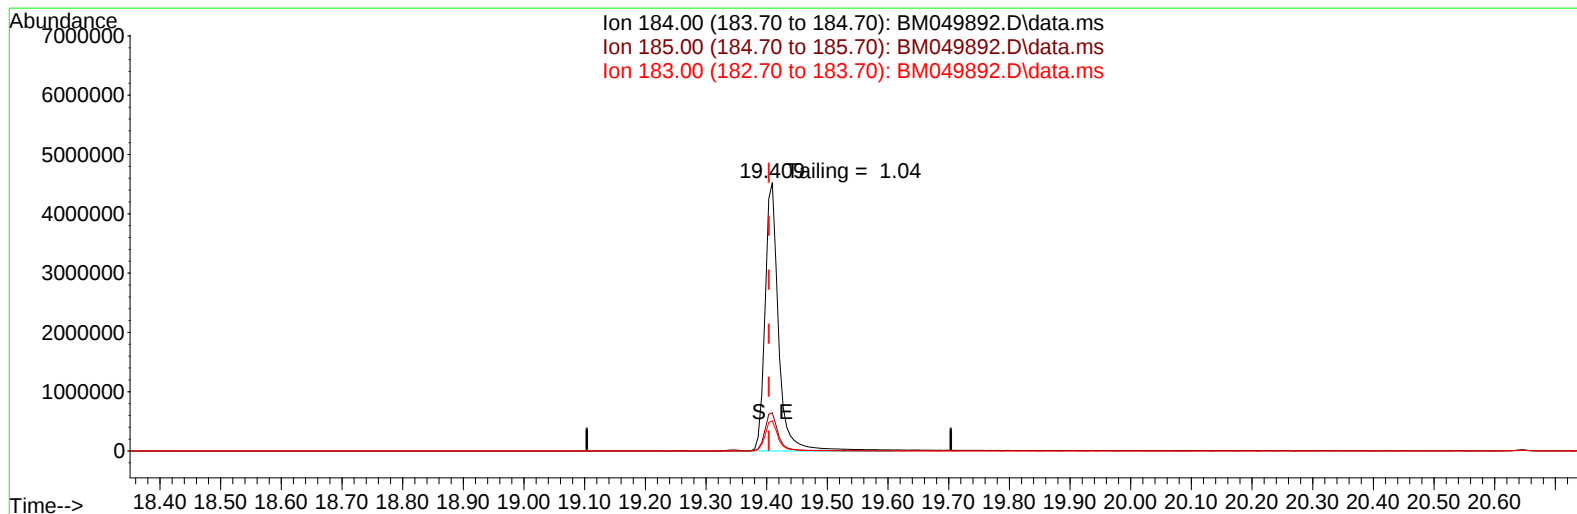

TIC: BM049892.D\data.ms

(77) Benzidine

19.409min (+ 0.006) 1373999.43 ng m

response 7145396

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.29
183.00	11.00	11.21
0.00	0.00	0.00