


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041125\
Data File : BM049892.D
Acq On : 11 Apr 2025 08:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 09 04:00:55 2025

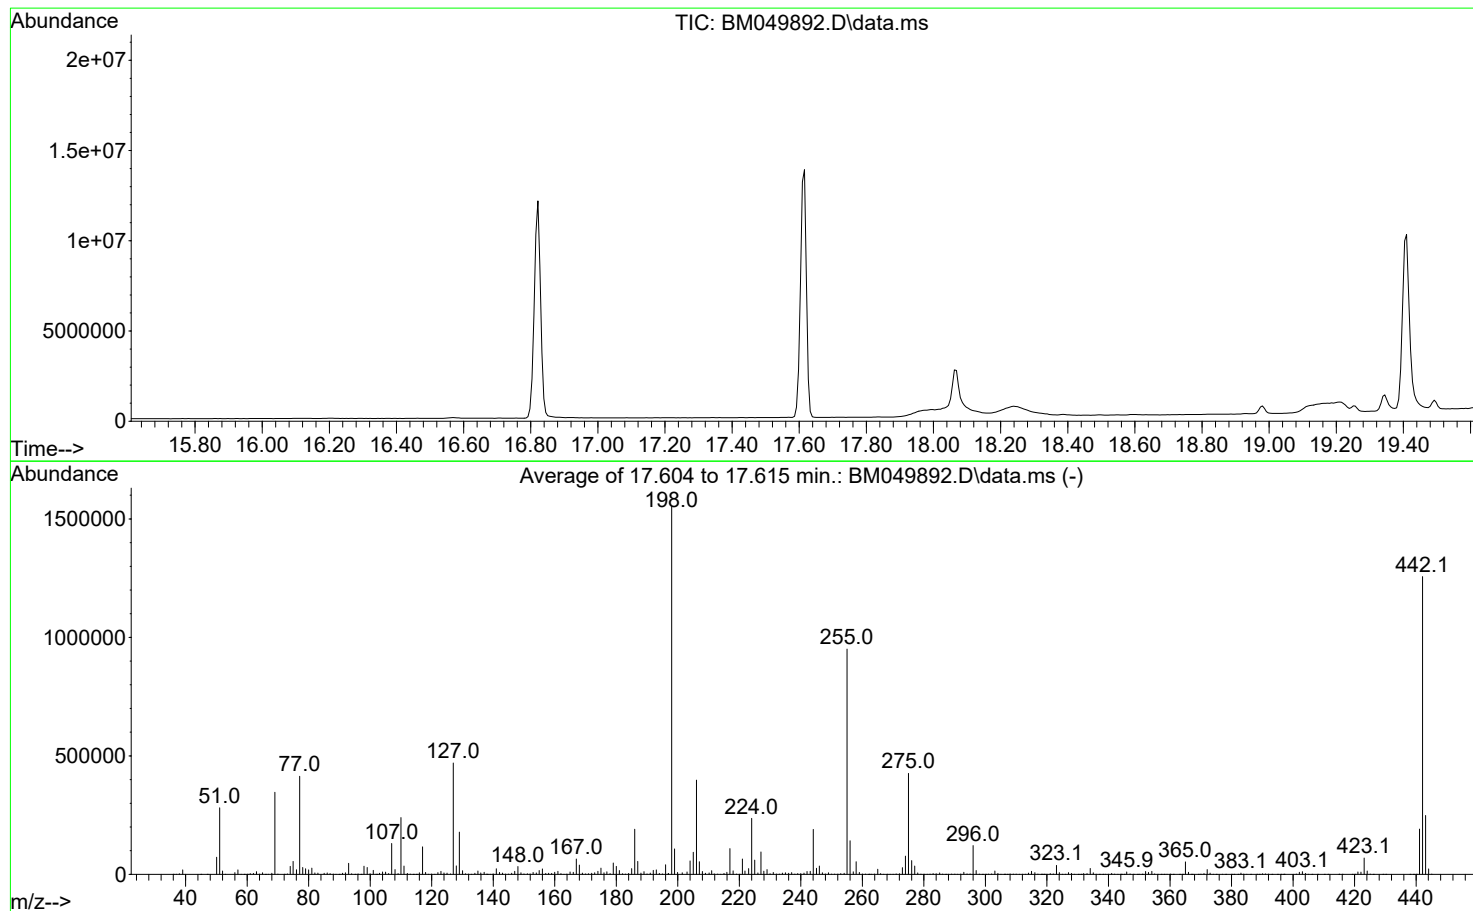

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.1	280907	PASS
68	69	0.00	2	1.4	4829	PASS
69	198	0.00	100	22.3	346715	PASS
70	69	0.00	2	0.4	1340	PASS
127	198	10	80	30.3	470187	PASS
197	198	0.00	2	0.3	4040	PASS
198	198	100	100	100.0	1552401	PASS
199	198	5	9	6.9	107322	PASS
275	198	10	60	27.4	426133	PASS
365	198	1	100	3.4	52747	PASS
441	198	0.01	100	12.3	190805	PASS
442	442	50	100	100.0	1256491	PASS
443	442	15	24	19.8	248232	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/11/2025	BNA_M	<u>BM049892.D</u>
Compound Name	Response	Retention Time
DDT	4858322	20.645
DDD	79976	20.256
DDE	3552	19.698
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
83528	4941850	1.69

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041125\
Data File : BM049892.D
Acq On : 11 Apr 2025 08:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 11 11:40:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

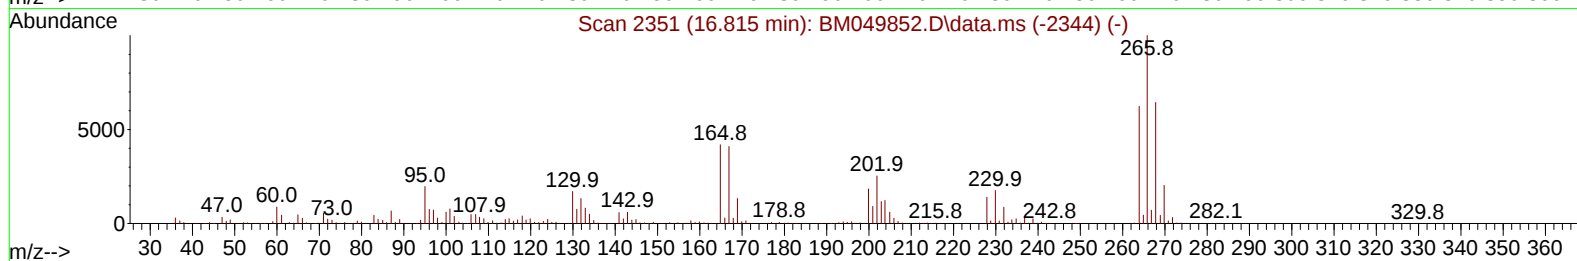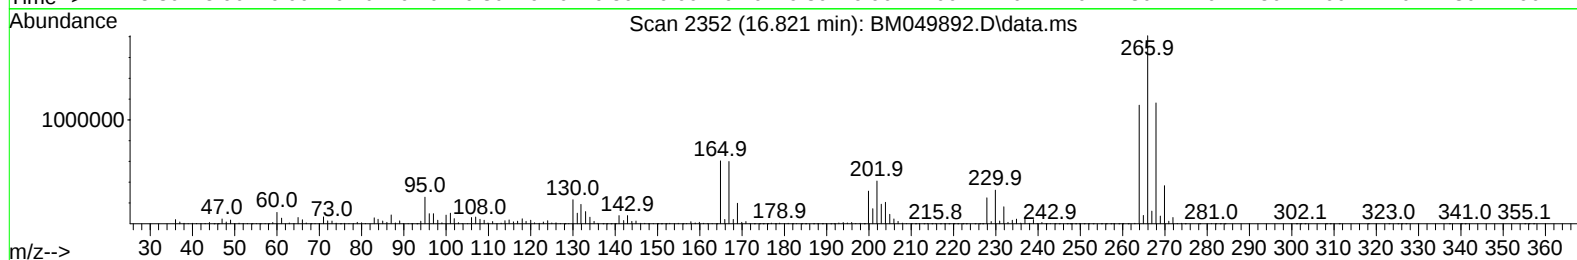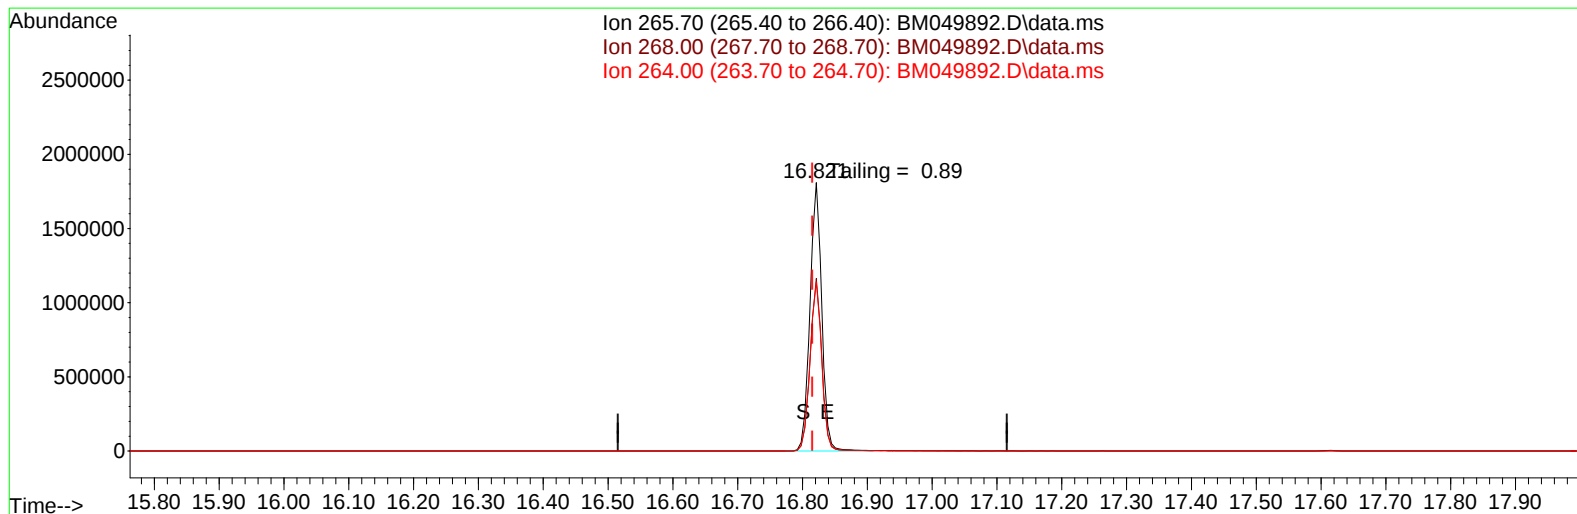

TIC: BM049892.D\data.ms

(70) Pentachlorophenol (C)

16.821min (+ 0.006) 669887.62 ng




response 2252497

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	64.26
264.00	62.30	63.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041125\
Data File : BM049892.D
Acq On : 11 Apr 2025 08:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 11 11:40:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

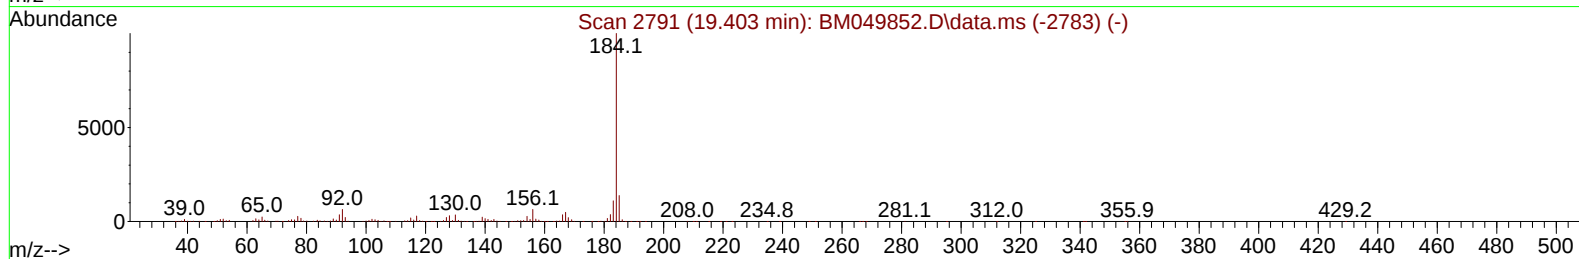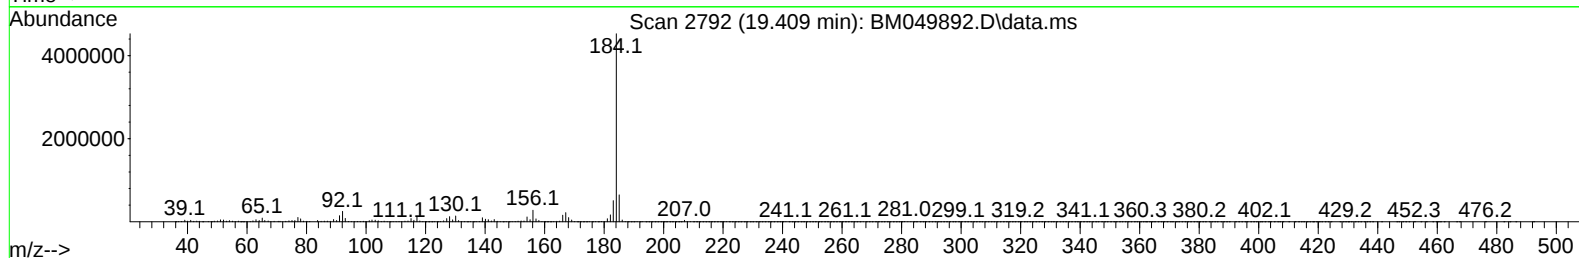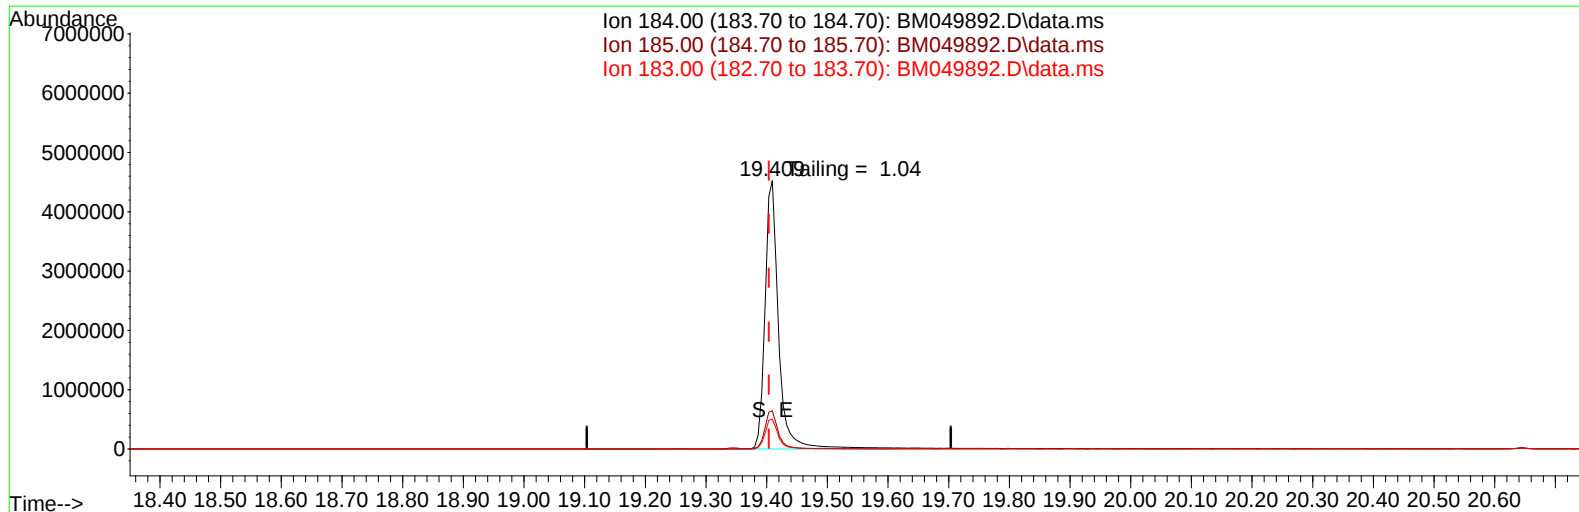

TIC: BM049892.D\data.ms

(77) Benzidine

19.409min (+ 0.006) 1373999.43 ng m

response 7145396

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.29
183.00	11.00	11.21
0.00	0.00	0.00