

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041425\
 Data File : BM049916.D
 Acq On : 14 Apr 2025 16:29
 Operator : RC/JU
 Sample : Q1760-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TP-17

Quant Time: Apr 14 19:36:17 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 09 04:00:55 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	414370	20.000	ng	-0.01
21) Naphthalene-d8	10.563	136	1440095	20.000	ng	-0.01
39) Acenaphthene-d10	14.416	164	941798	20.000	ng	0.00
64) Phenanthrene-d10	17.157	188	1863593	20.000	ng	0.00
76) Chrysene-d12	21.392	240	1839515	20.000	ng	-0.01
86) Perylene-d12	24.391	264	1894785	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.357	112	2712832	111.171	ng	0.00
7) Phenol-d6	6.951	99	2990682	98.504	ng	0.00
23) Nitrobenzene-d5	8.928	82	2207847	85.372	ng	0.00
42) 2,4,6-Tribromophenol	15.904	330	1880734	137.292	ng	0.00
45) 2-Fluorobiphenyl	13.033	172	5874109	84.576	ng	-0.01
79) Terphenyl-d14	19.786	244	9699231	98.813	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041425\
Data File : BM049916.D
Acq On : 14 Apr 2025 16:29
Operator : RC/JU
Sample : Q1760-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-17

Quant Time: Apr 14 19:36:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

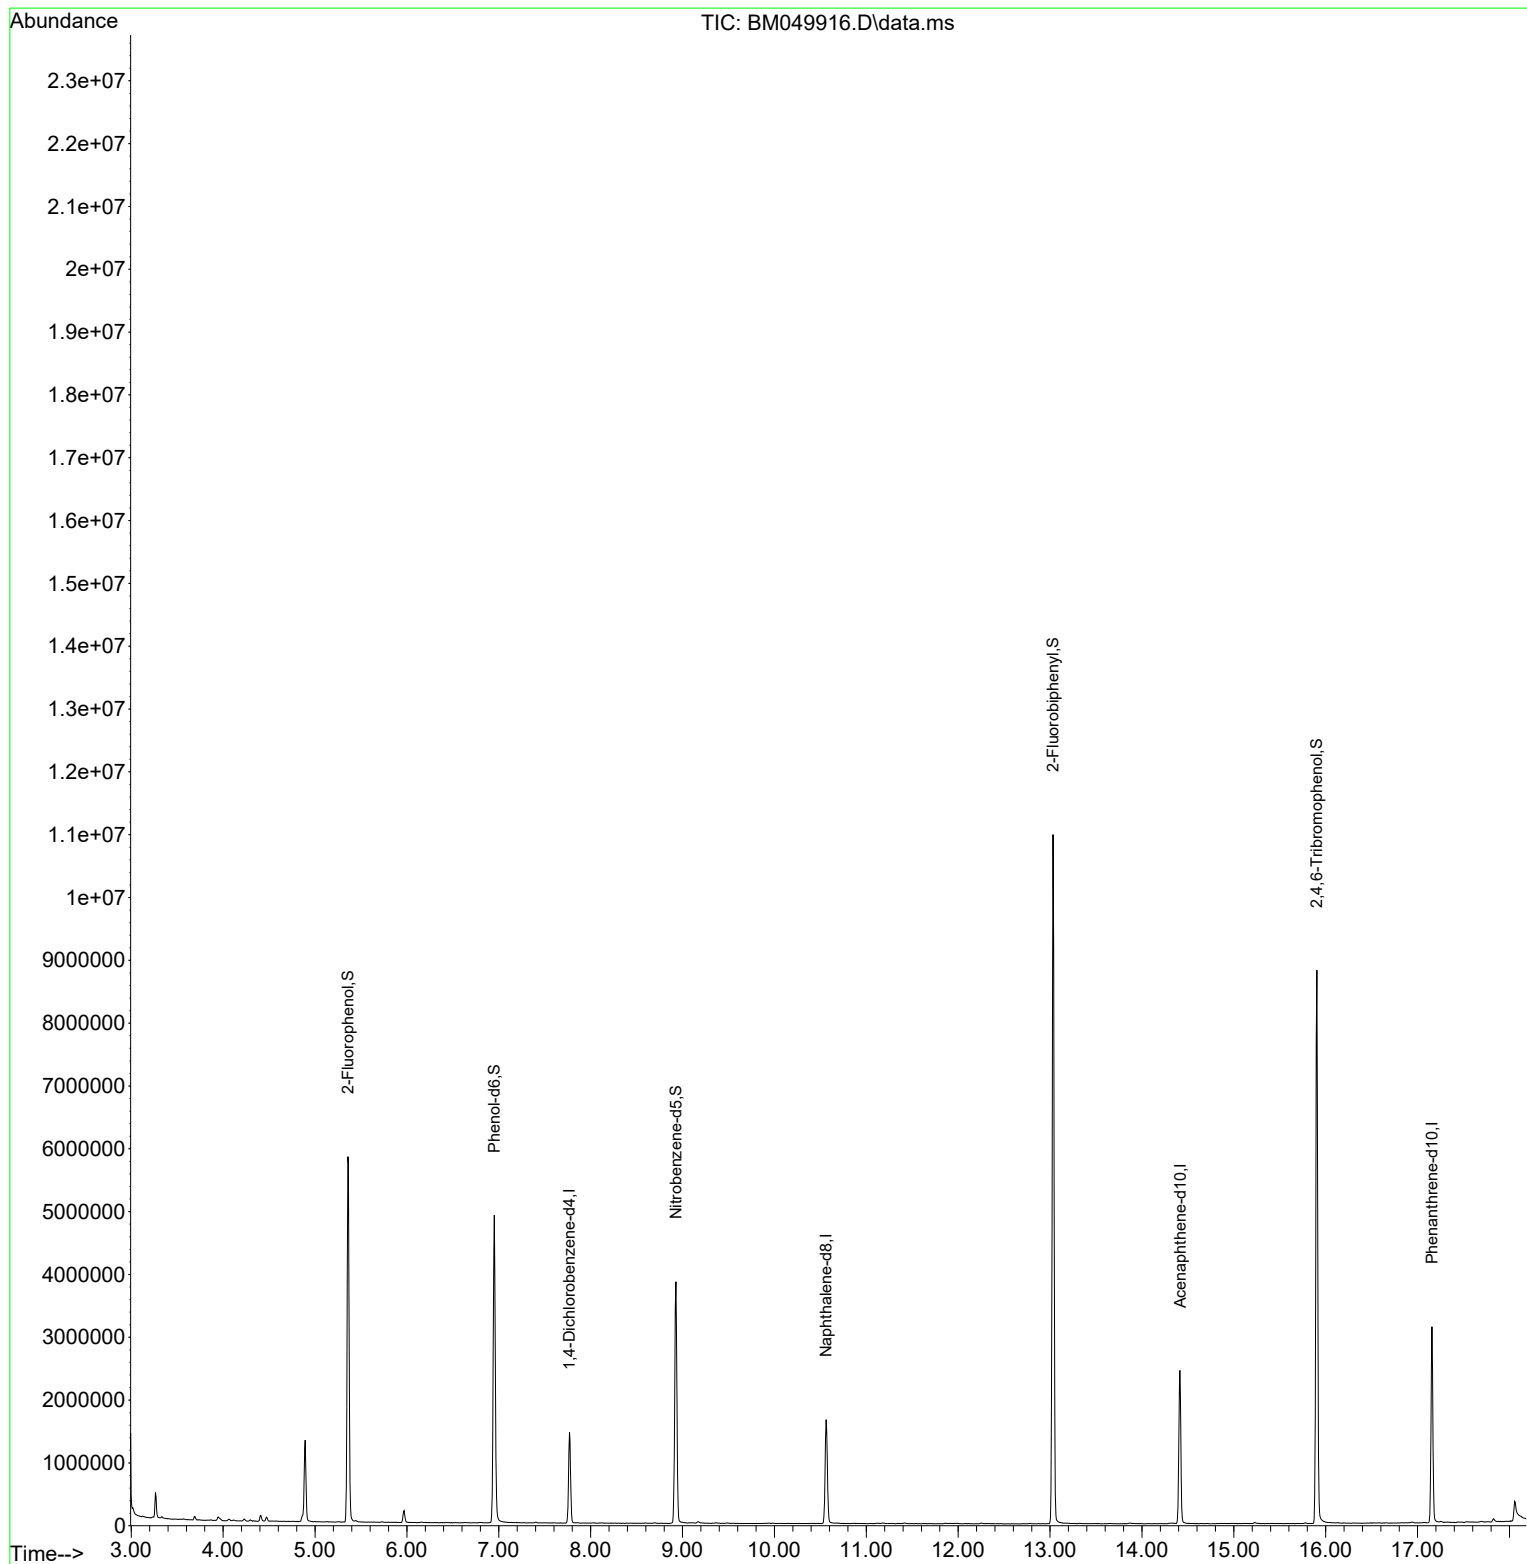

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041425\
Data File : BM049916.D
Acq On : 14 Apr 2025 16:29
Operator : RC/JU
Sample : Q1760-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-17

Quant Time: Apr 14 19:36:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

