

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041425\
 Data File : BM049917.D
 Acq On : 14 Apr 2025 17:08
 Operator : RC/JU
 Sample : Q1760-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TP-15

Quant Time: Apr 14 19:03:34 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 09 04:00:55 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	428027	20.000	ng	-0.01
21) Naphthalene-d8	10.563	136	1481991	20.000	ng	-0.01
39) Acenaphthene-d10	14.416	164	965248	20.000	ng	0.00
64) Phenanthrene-d10	17.157	188	1916547	20.000	ng	0.00
76) Chrysene-d12	21.392	240	1860704	20.000	ng	-0.01
86) Perylene-d12	24.391	264	1898093	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.363	112	2865308	113.673	ng	0.00
7) Phenol-d6	6.951	99	3190911	101.746	ng	0.00
23) Nitrobenzene-d5	8.928	82	2297797	86.339	ng	0.00
42) 2,4,6-Tribromophenol	15.904	330	1966244	140.047	ng	0.00
45) 2-Fluorobiphenyl	13.033	172	6086253	85.502	ng	-0.01
79) Terphenyl-d14	19.786	244	10391110	104.656	ng	0.00
Target Compounds						
31) Naphthalene	10.616	128	235573	3.094	ng	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041425\
Data File : BM049917.D
Acq On : 14 Apr 2025 17:08
Operator : RC/JU
Sample : Q1760-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-15

Quant Time: Apr 14 19:03:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

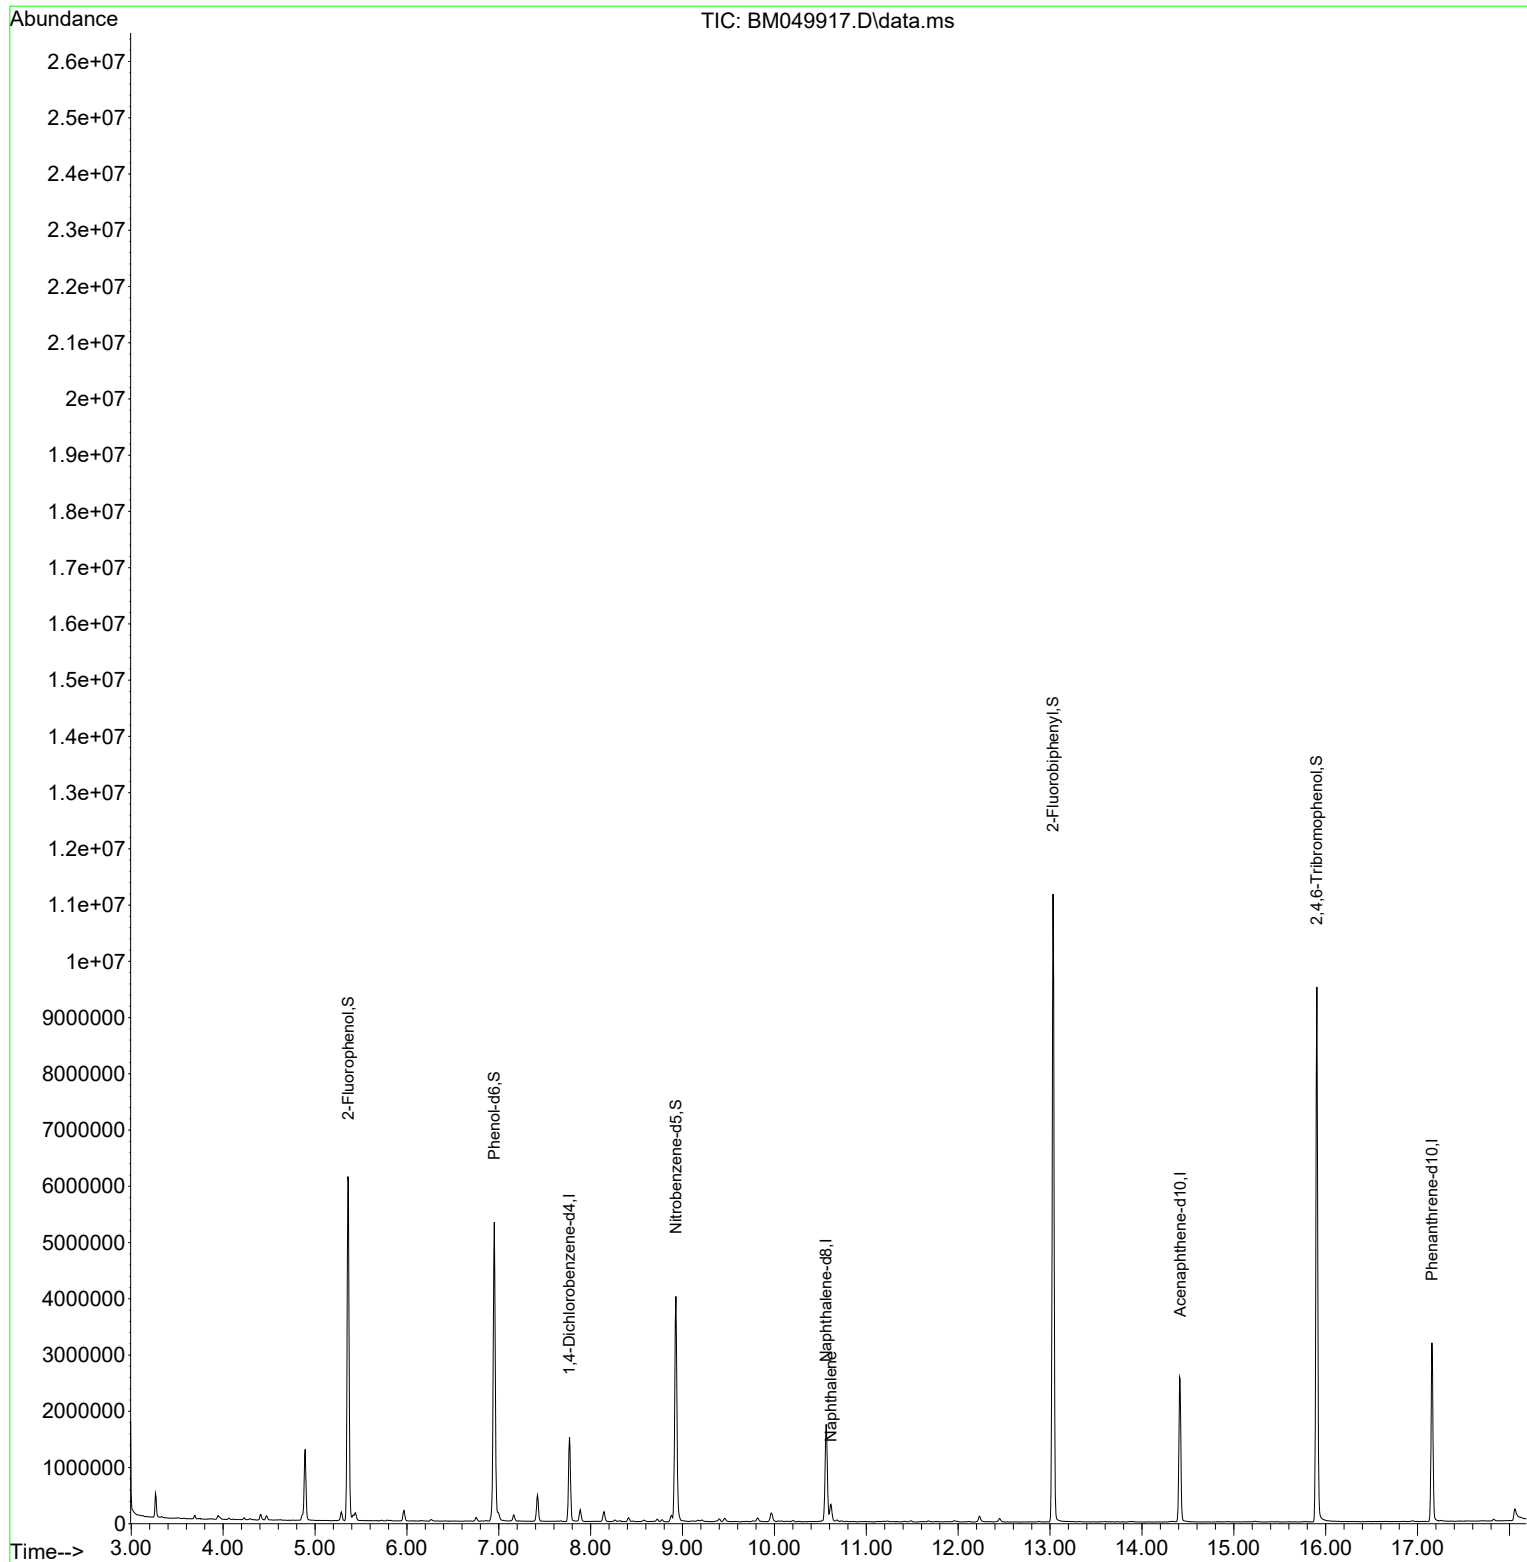

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041425\
Data File : BM049917.D
Acq On : 14 Apr 2025 17:08
Operator : RC/JU
Sample : Q1760-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-15

Quant Time: Apr 14 19:03:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

