

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041425\
 Data File : BM049918.D
 Acq On : 14 Apr 2025 17:48
 Operator : RC/JU
 Sample : Q1760-05DL 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TP-15DL

Quant Time: Apr 15 04:27:48 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 09 04:00:55 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	372955	20.000	ng	-0.01
21) Naphthalene-d8	10.563	136	1313910	20.000	ng	-0.01
39) Acenaphthene-d10	14.410	164	877744	20.000	ng	-0.01
64) Phenanthrene-d10	17.157	188	1740077	20.000	ng	0.00
76) Chrysene-d12	21.392	240	1790517	20.000	ng	-0.01
86) Perylene-d12	24.386	264	1938740	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.357	112	392648	17.877	ng	0.00
7) Phenol-d6	6.945	99	643141	23.535	ng	0.00
23) Nitrobenzene-d5	8.928	82	397550	16.849	ng	0.00
42) 2,4,6-Tribromophenol	15.904	330	141229	11.062	ng	0.00
45) 2-Fluorobiphenyl	13.033	172	1061320	16.396	ng	-0.01
79) Terphenyl-d14	19.780	244	1646261	17.231	ng	-0.01
Target Compounds						
						Qvalue
31) Naphthalene	10.616	128	1475583	21.856	ng	98
37) 2-Methylnaphthalene	12.227	142	1253263	26.347	ng	100
38) 1-Methylnaphthalene	12.451	142	495029	10.682	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041425\
Data File : BM049918.D
Acq On : 14 Apr 2025 17:48
Operator : RC/JU
Sample : Q1760-05DL 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-15DL

Quant Time: Apr 15 04:27:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

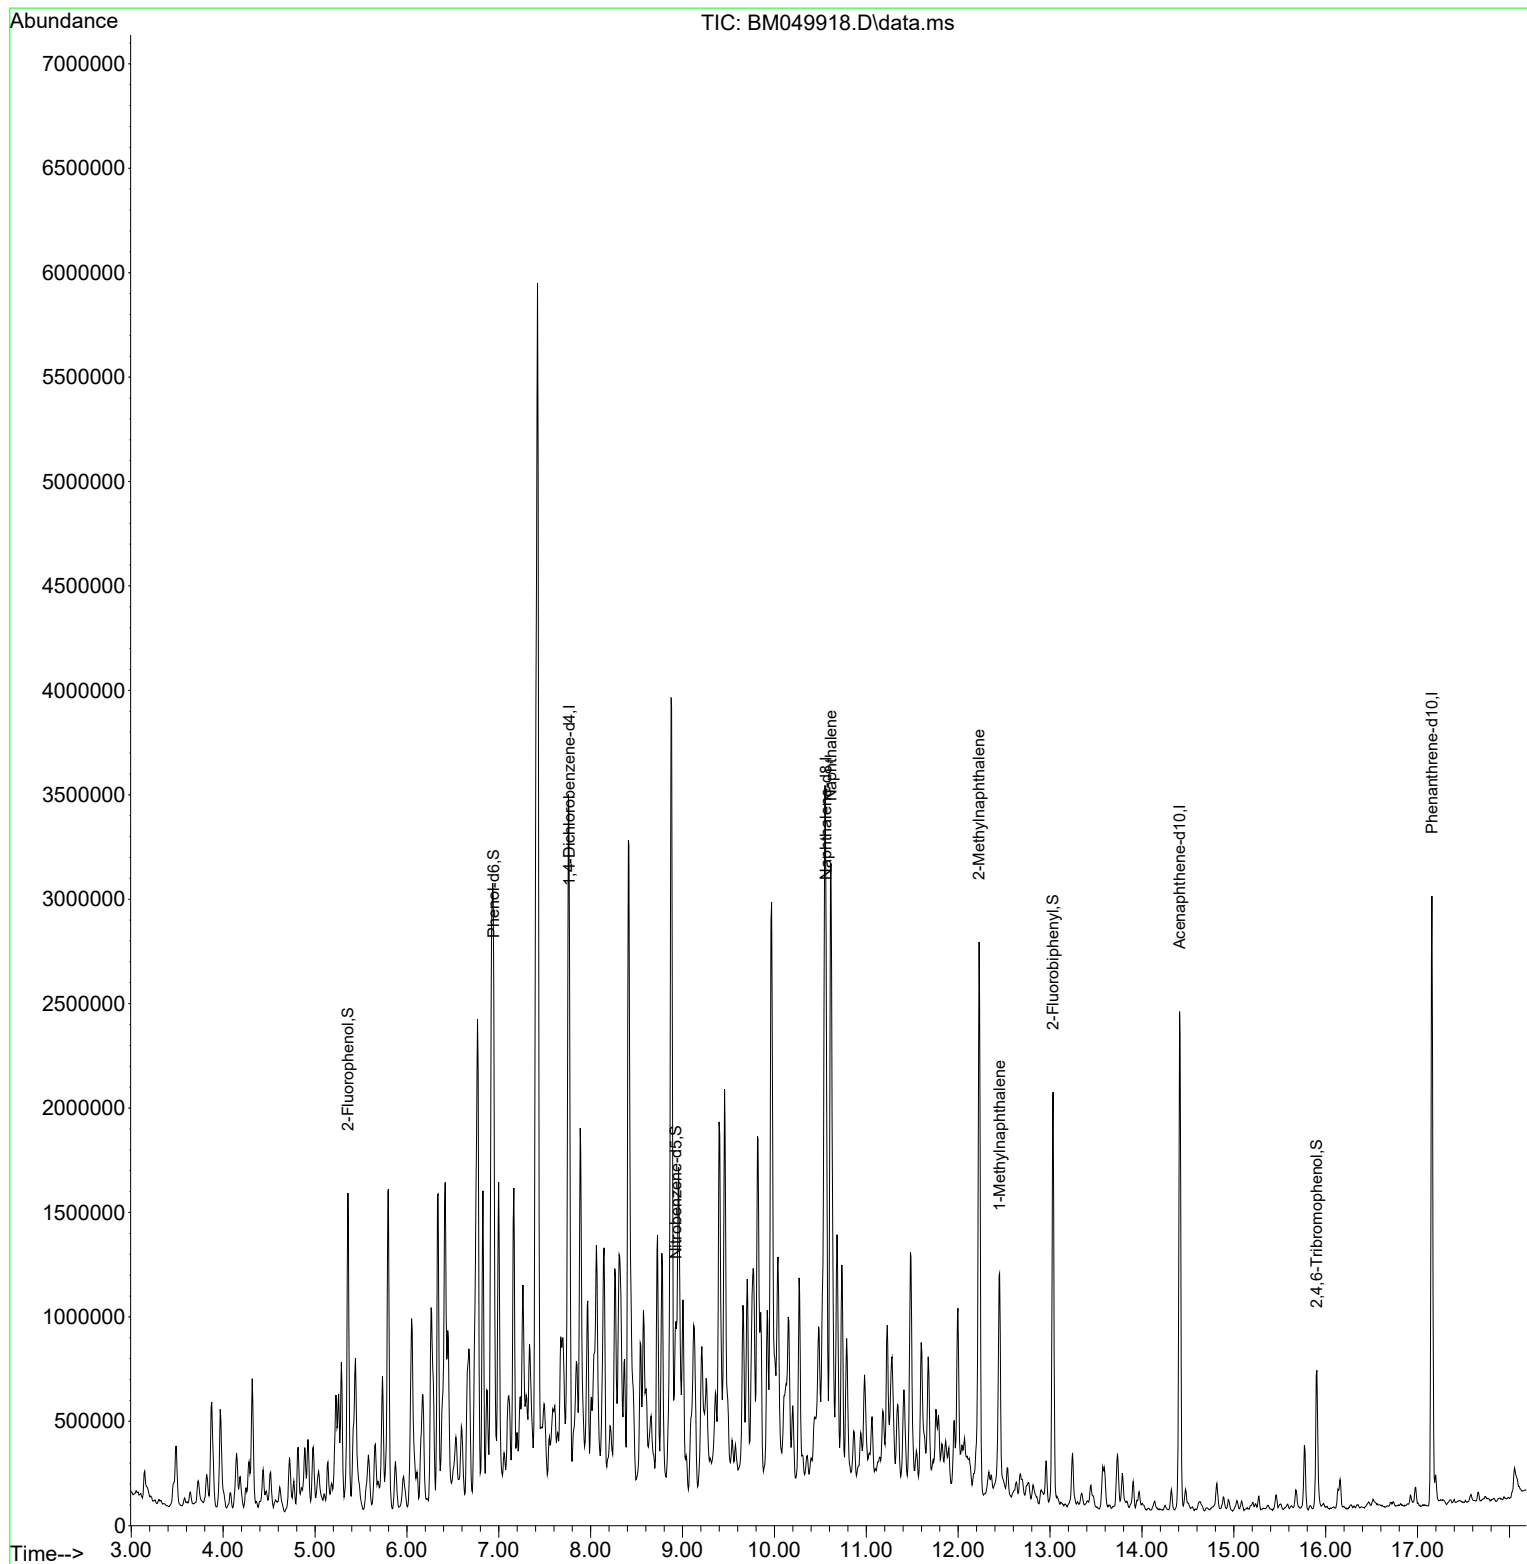

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041425\
Data File : BM049918.D
Acq On : 14 Apr 2025 17:48
Operator : RC/JU
Sample : Q1760-05DL 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-15DL

Quant Time: Apr 15 04:27:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

