


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041425\
Data File : BM049909.D
Acq On : 14 Apr 2025 11:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 09 04:00:55 2025

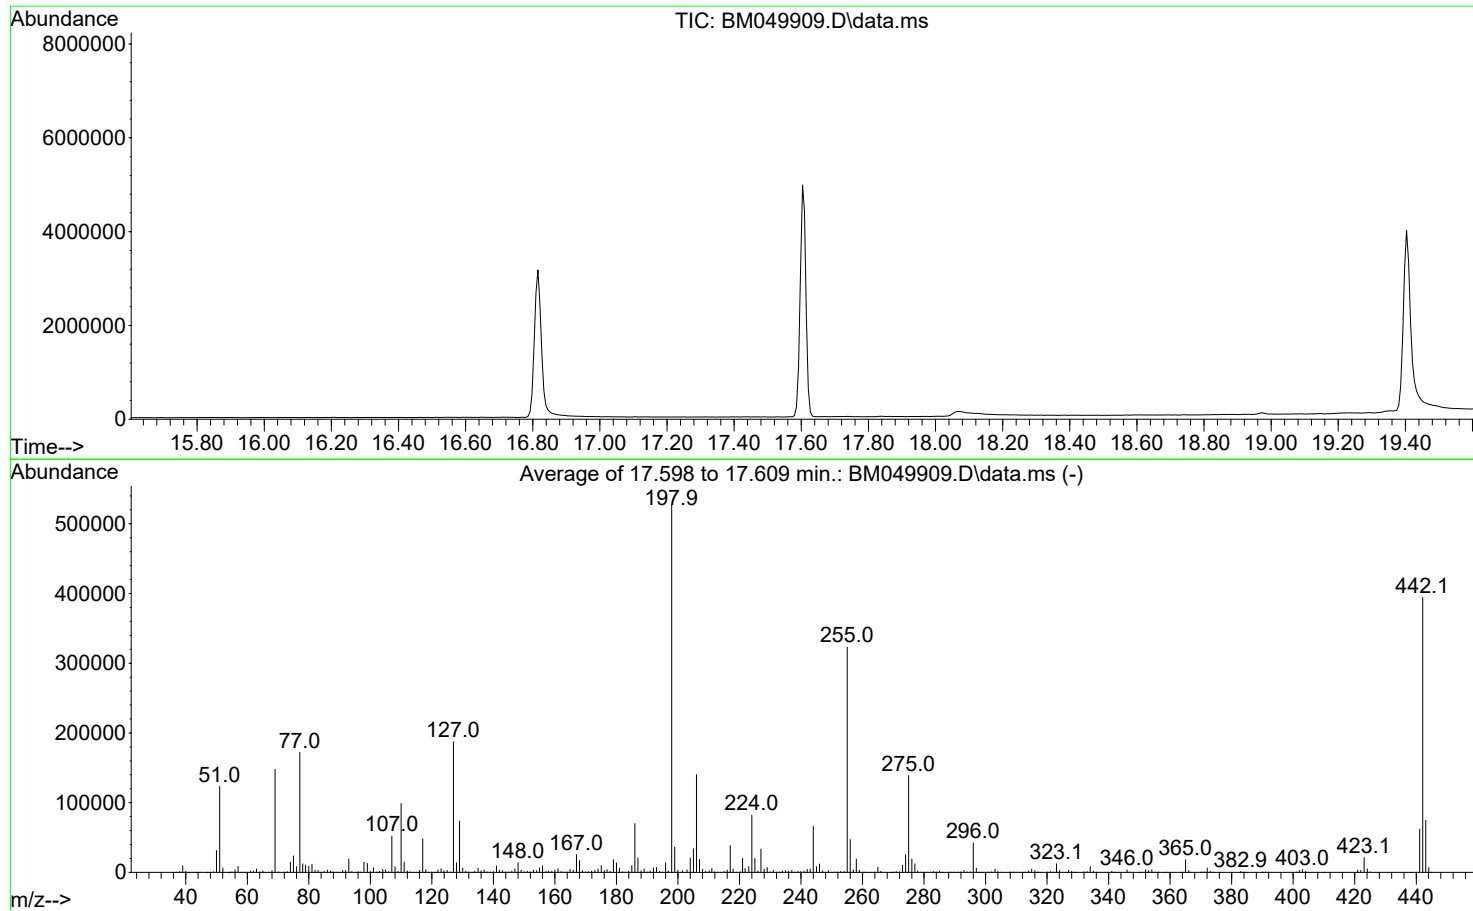

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.4	123208	PASS
68	69	0.00	2	1.6	2434	PASS
69	198	0.00	100	28.1	148078	PASS
70	69	0.00	2	0.5	726	PASS
127	198	10	80	35.5	187371	PASS
197	198	0.00	2	0.4	2163	PASS
198	198	100	100	100.0	527637	PASS
199	198	5	9	6.9	36296	PASS
275	198	10	60	26.3	138843	PASS
365	198	1	100	3.4	18137	PASS
441	198	0.01	100	11.7	61968	PASS
442	442	50	100	100.0	394261	PASS
443	442	15	24	19.0	74853	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/14/2025	BNA_M	<u>BM049909.D</u>
Compound Name	Response	Retention Time
DDT	1838455	20.639
DDD	27396	20.25
DDE	1181	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28577	1867032	1.53

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041425\
Data File : BM049909.D
Acq On : 14 Apr 2025 11:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 14 13:33:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

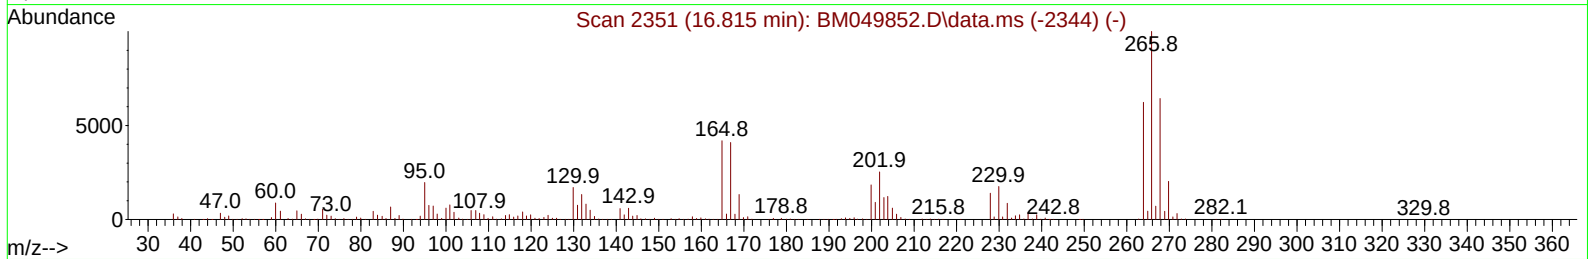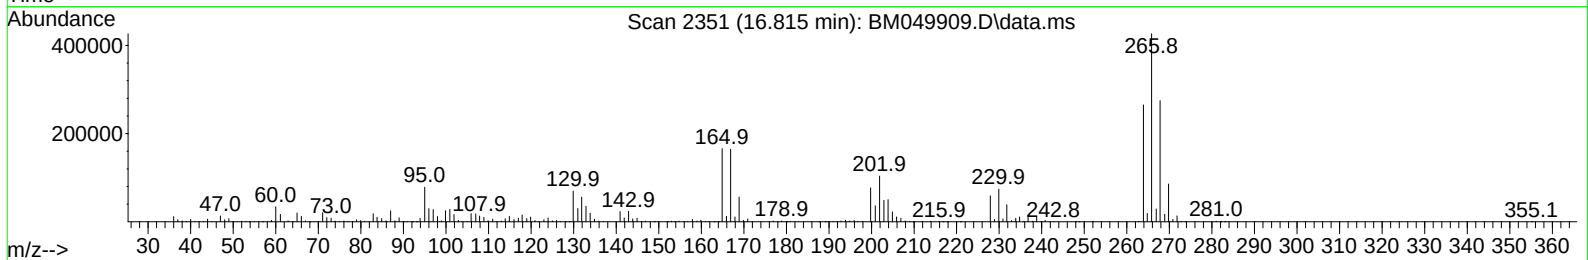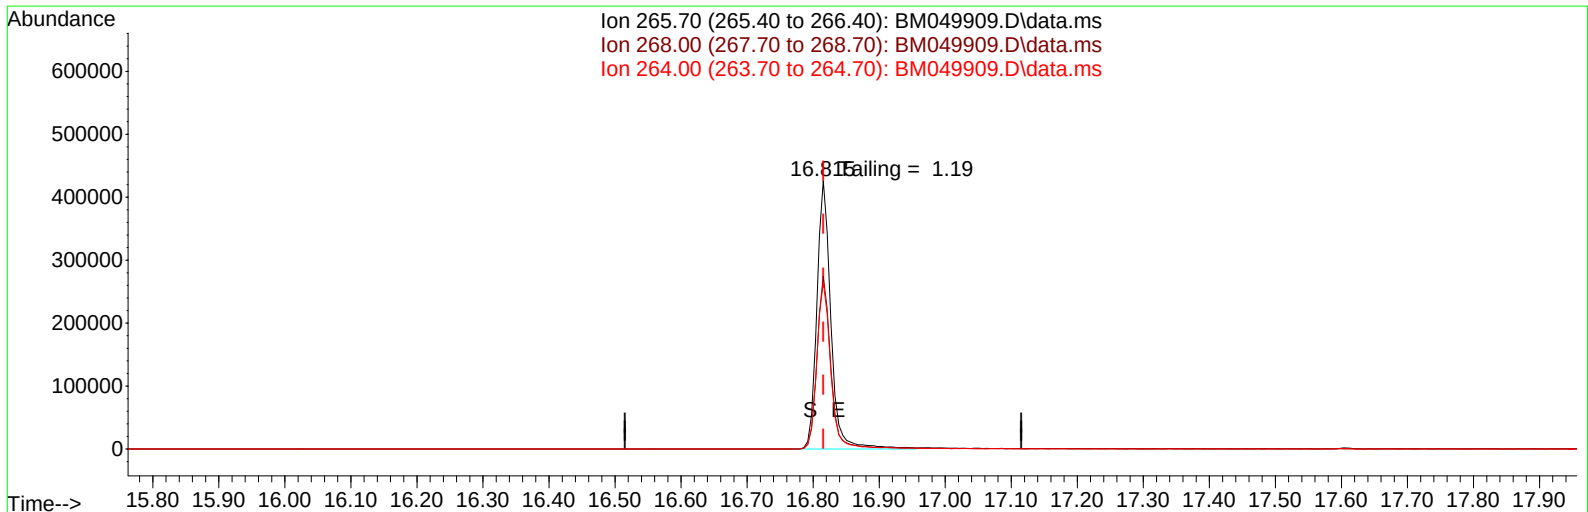

TIC: BM049909.D\data.ms

(70) Pentachlorophenol (C)

16.815min (-0.000) 254292.86 ng




response 630700

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	64.41
264.00	62.30	62.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041425\
Data File : BM049909.D
Acq On : 14 Apr 2025 11:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 14 13:33:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

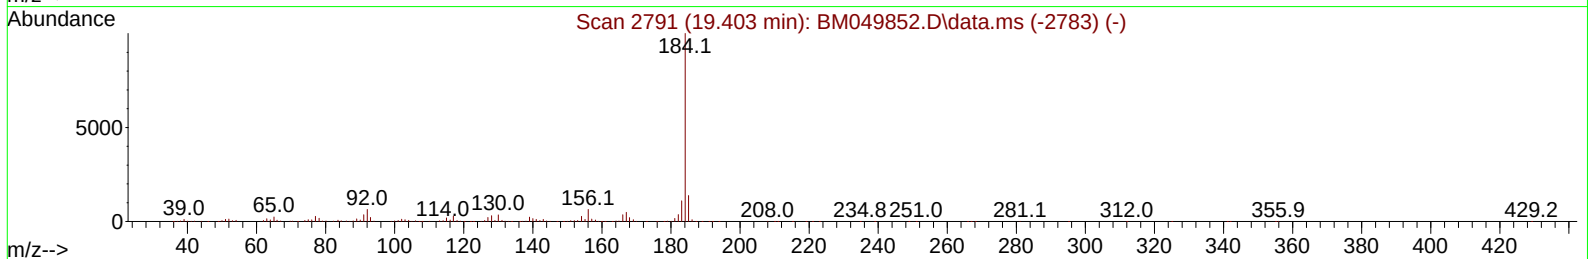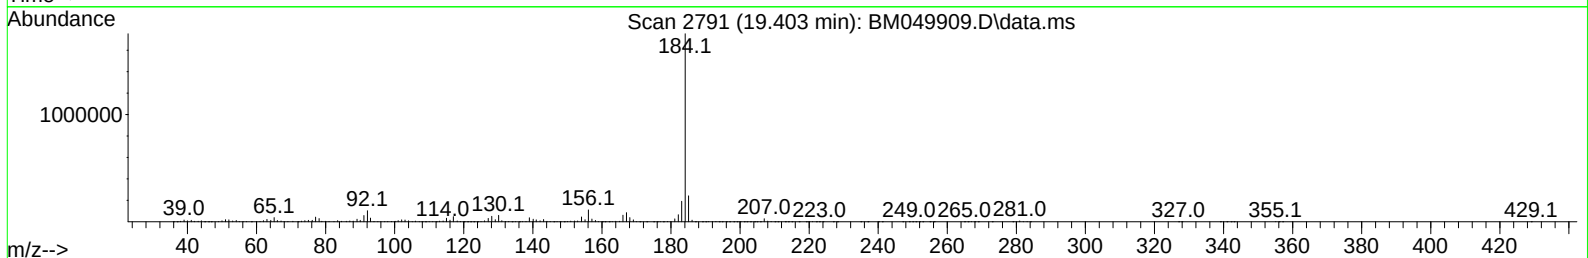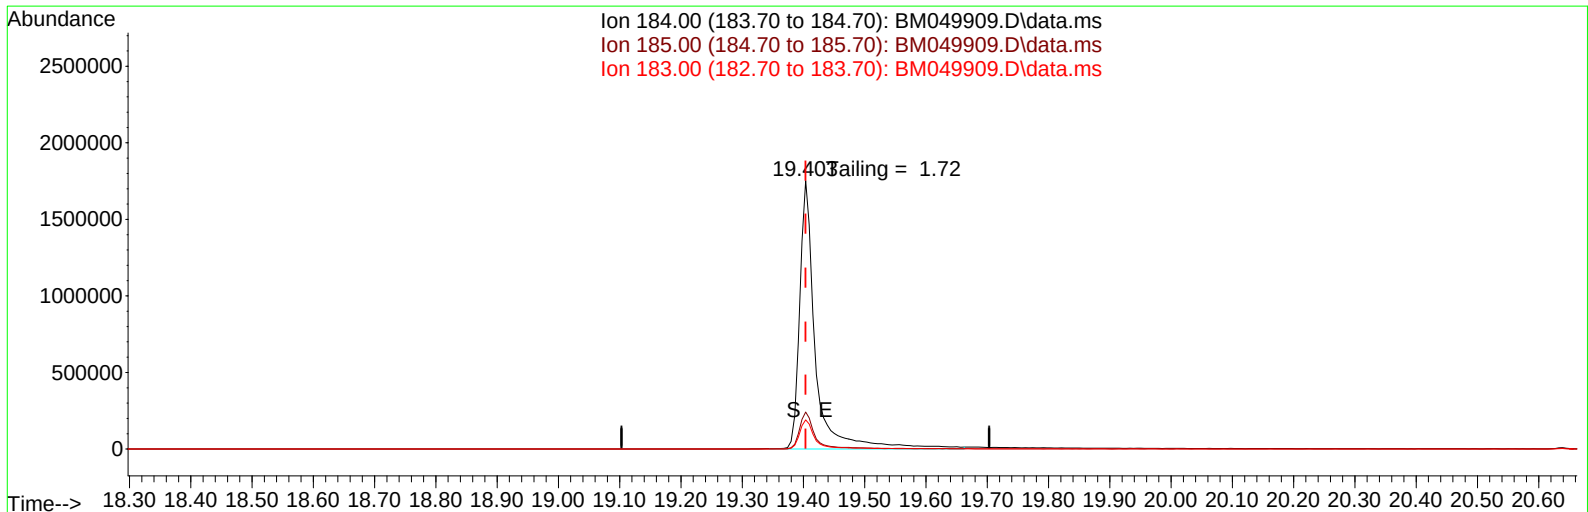

TIC: BM049909.D\data.ms

(77) Benzidine

19.403min (-0.000) 101434.92 ng

response 3159652

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.80
183.00	11.00	10.89
0.00	0.00	0.00