



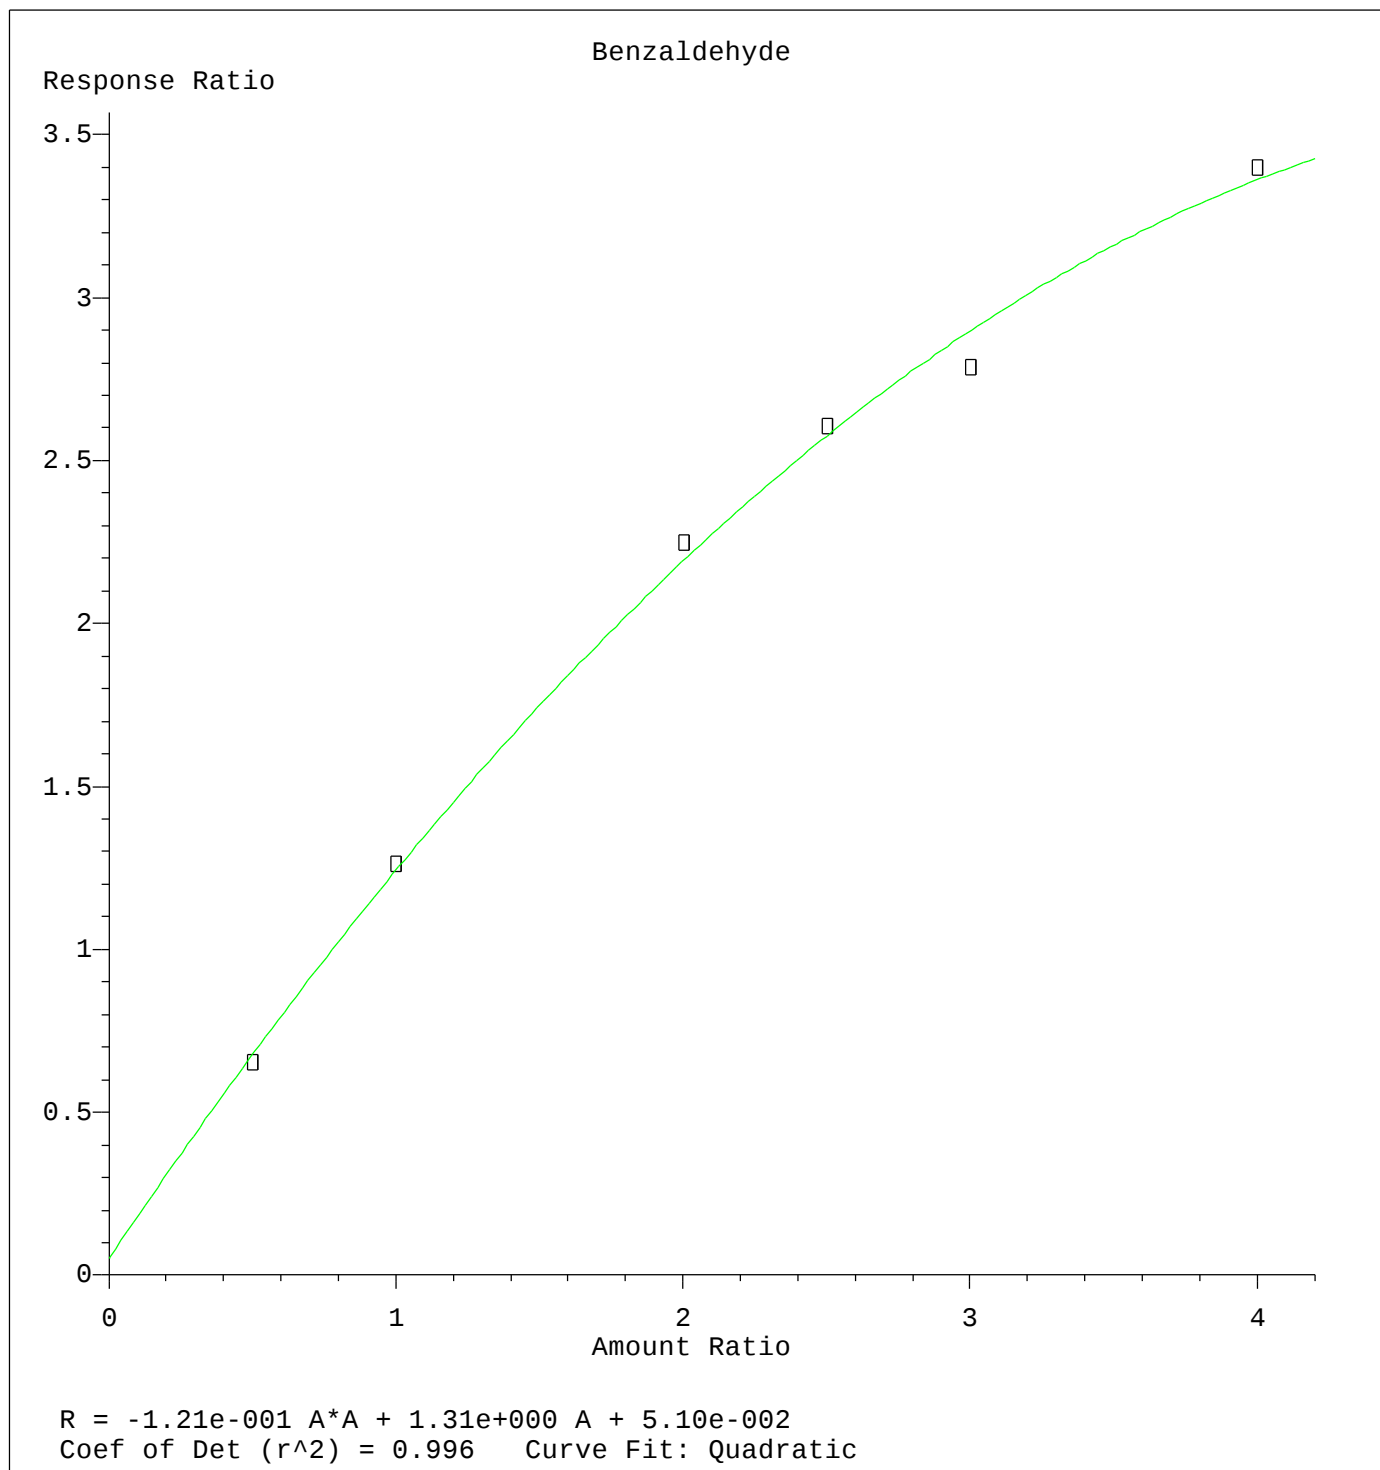


Method Name: Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM041519.M  
Calibration Table Last Updated: Mon Apr 15 16:16:29 2019

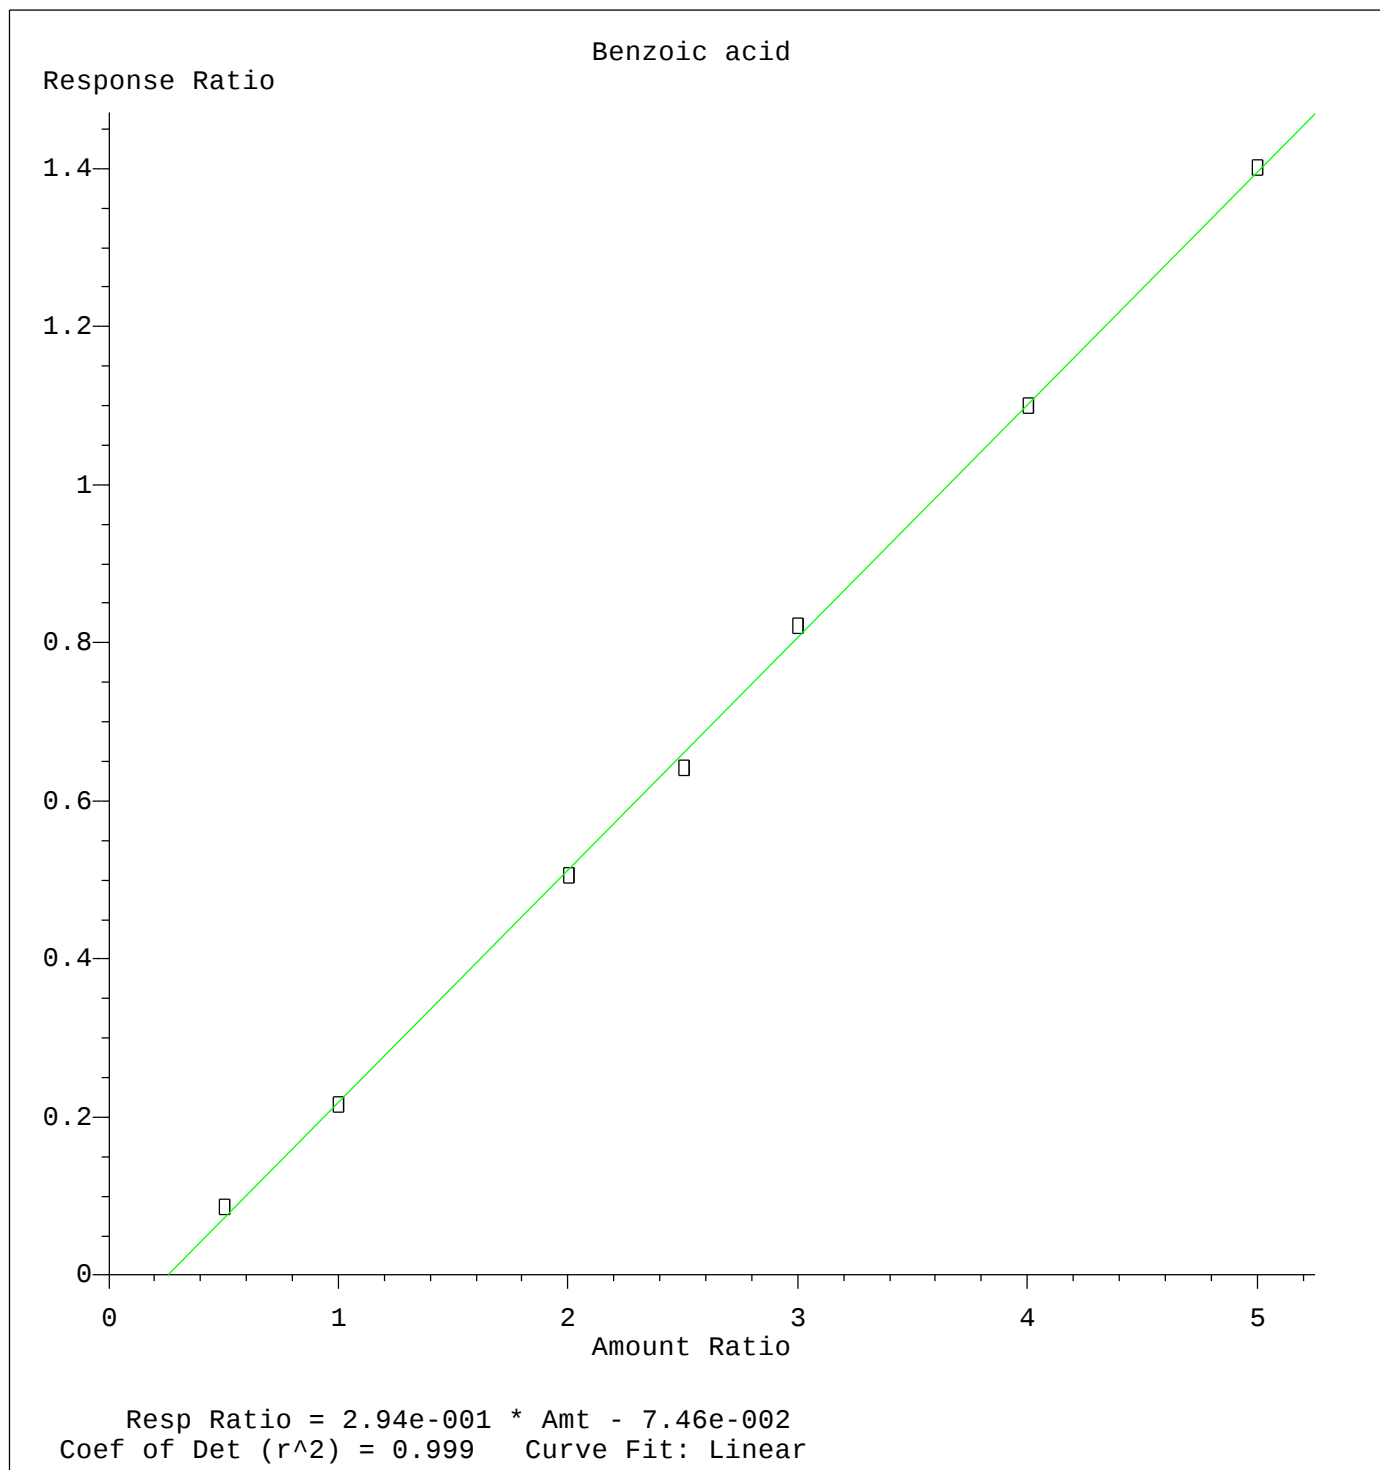

Method Name: Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM041519.M  
Calibration Table Last Updated: Mon Apr 15 16:16:29 2019

# Hexachlorocyclopentadiene

Response Ratio

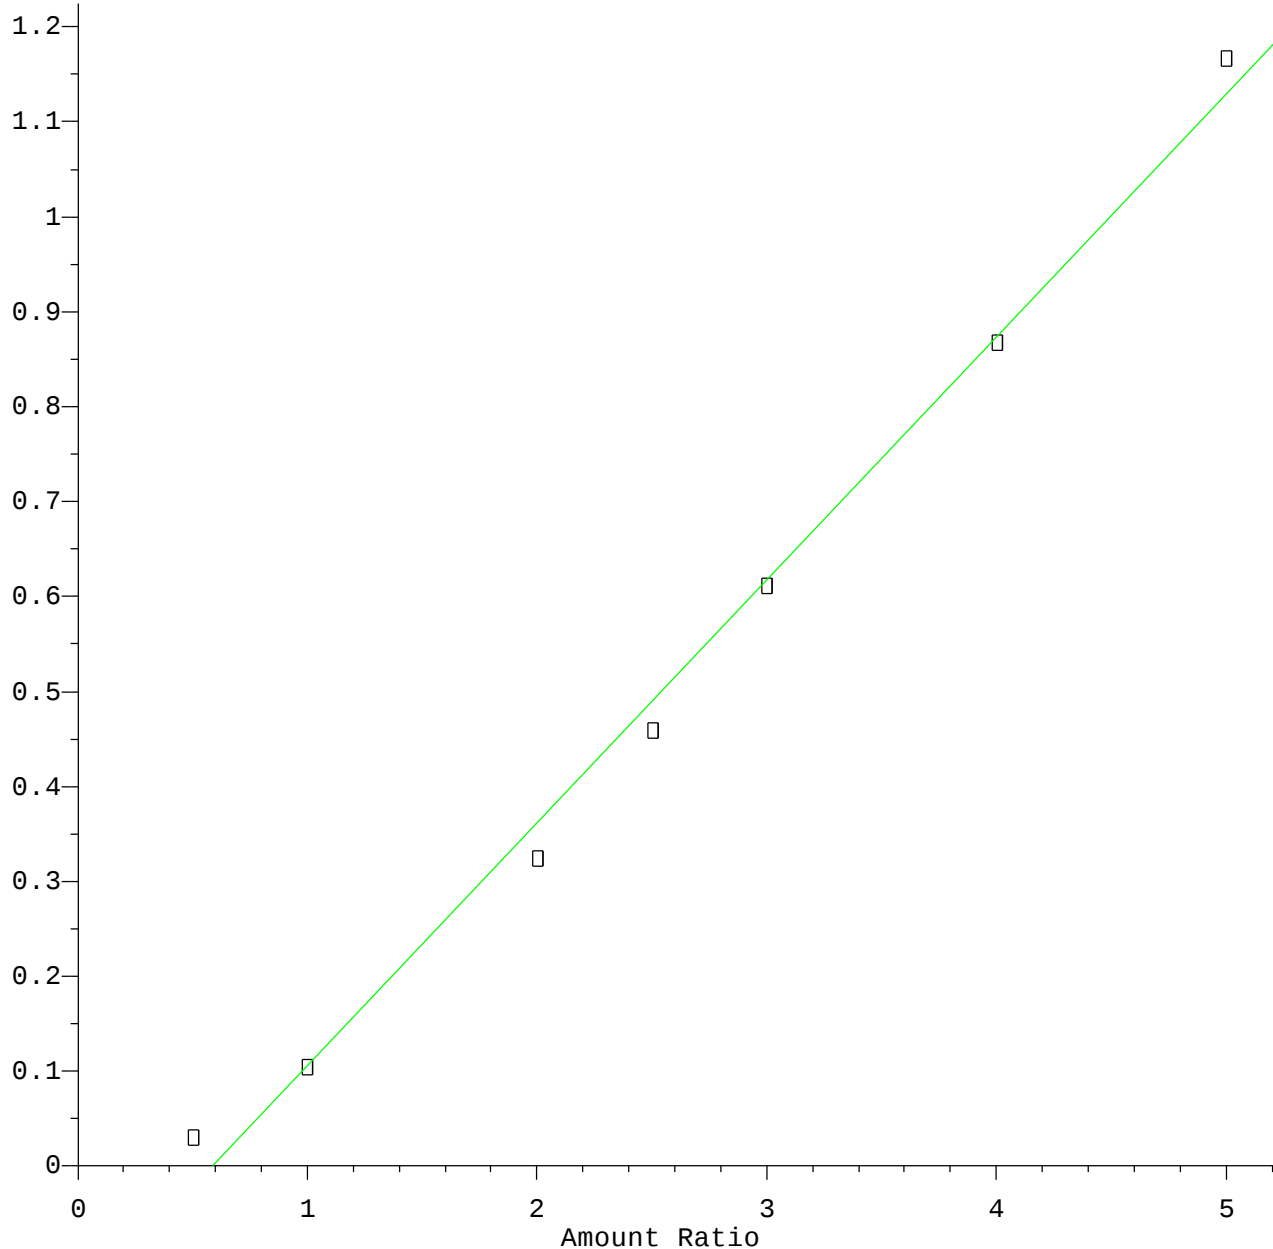


Resp Ratio =  $2.56 \times 10^{-1} \times \text{Amt} - 1.49 \times 10^{-1}$   
Coef of Det ( $r^2$ ) = 0.993    Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM041519.M  
Calibration Table Last Updated: Mon Apr 15 16:16:29 2019

# 2,4-Dinitrophenol

Response Ratio

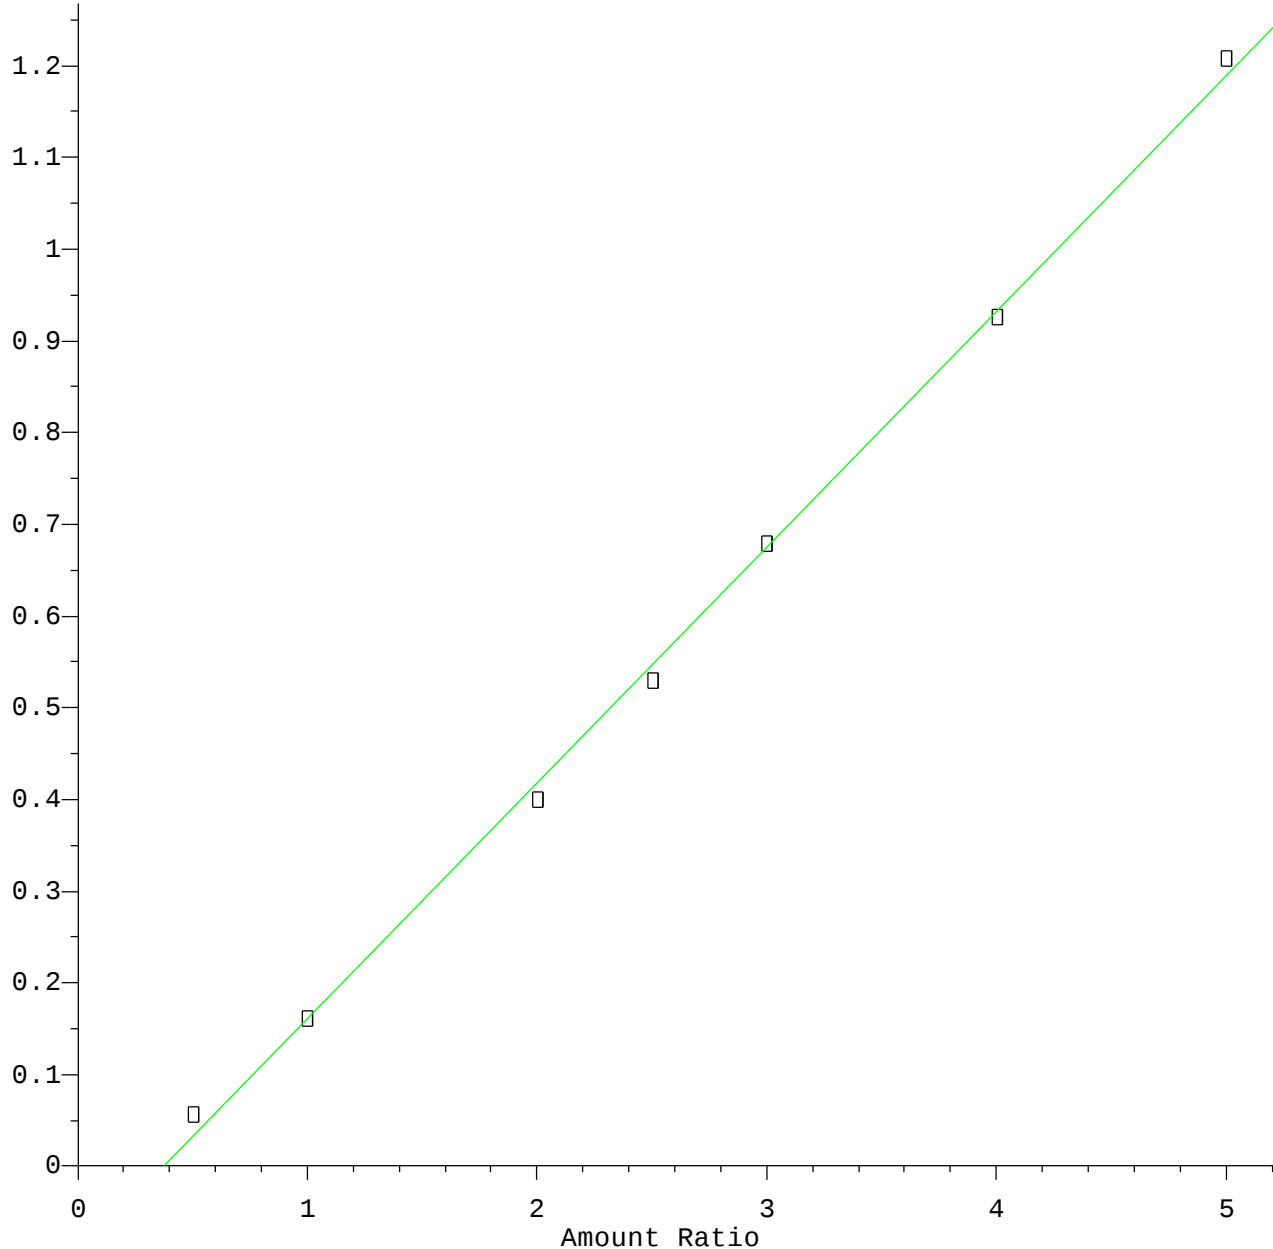


Resp Ratio =  $2.57 \times 10^{-1} \times \text{Amt} - 9.61 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.998    Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM041519.M  
Calibration Table Last Updated: Mon Apr 15 16:16:29 2019

# 4-Nitrophenol

Response Ratio

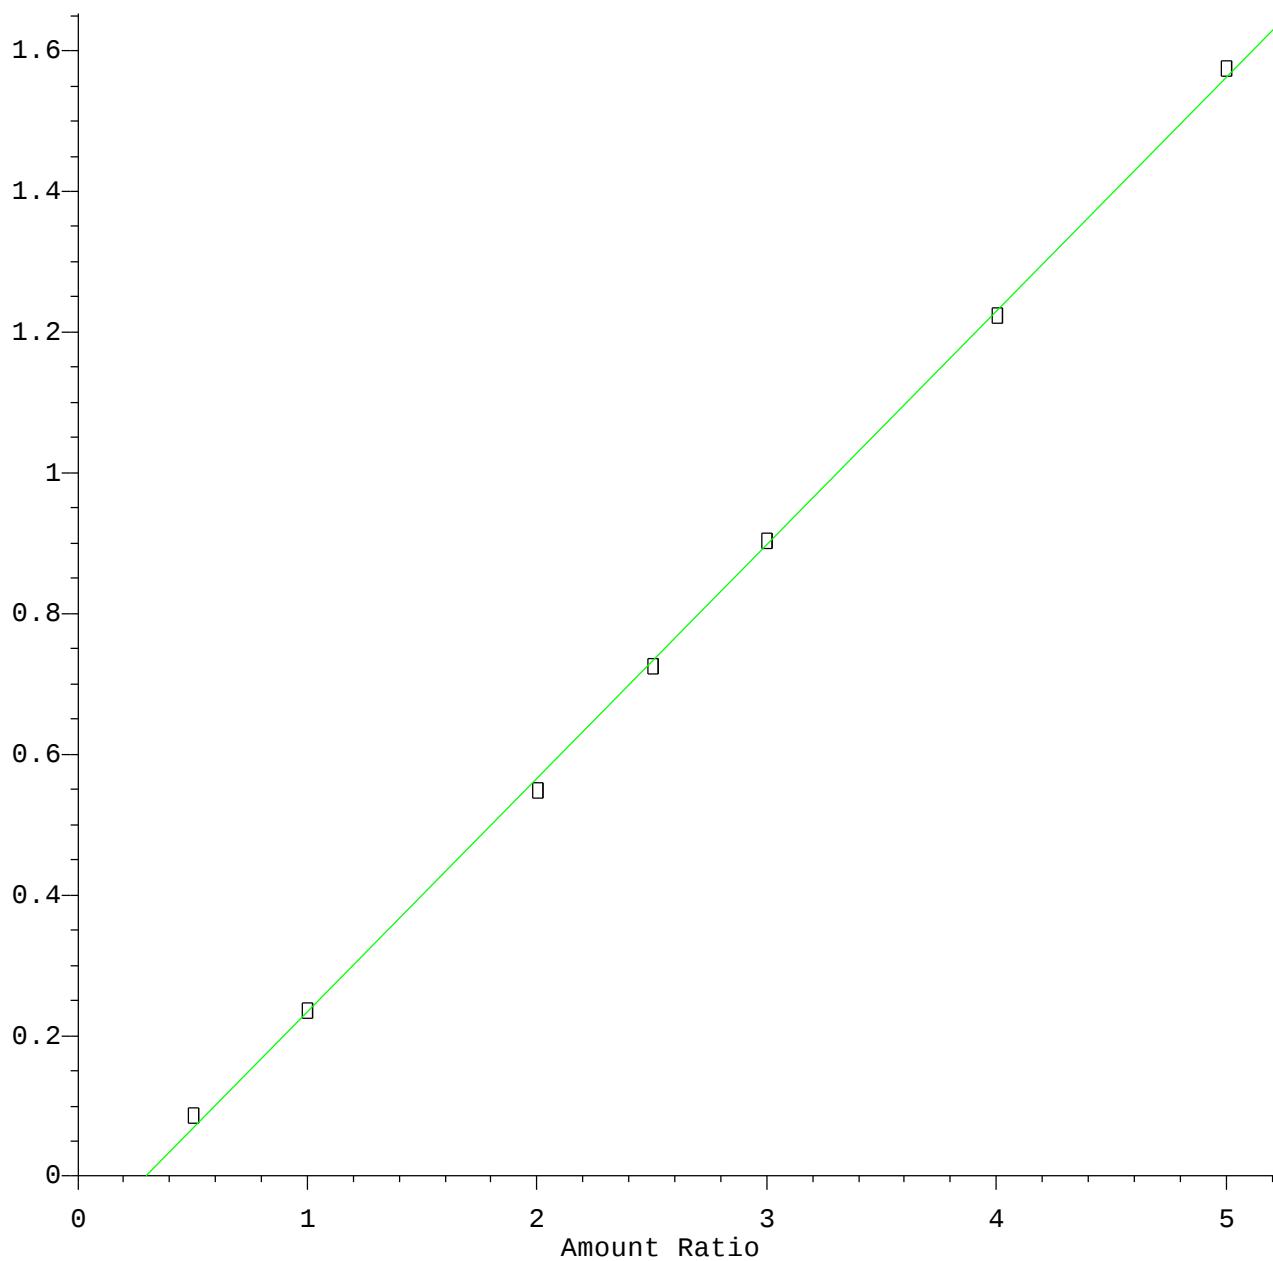

Resp Ratio = 3.32e-001 \* Amt - 9.72e-002  
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM041519.M  
Calibration Table Last Updated: Mon Apr 15 16:16:29 2019