
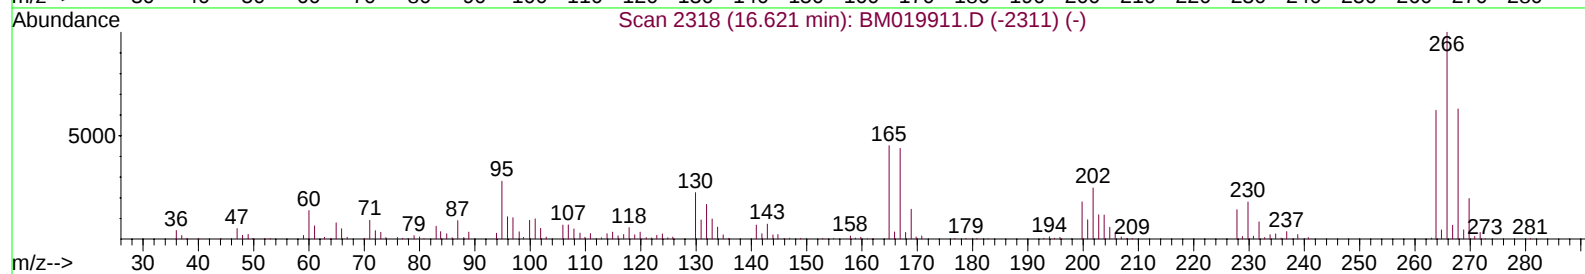
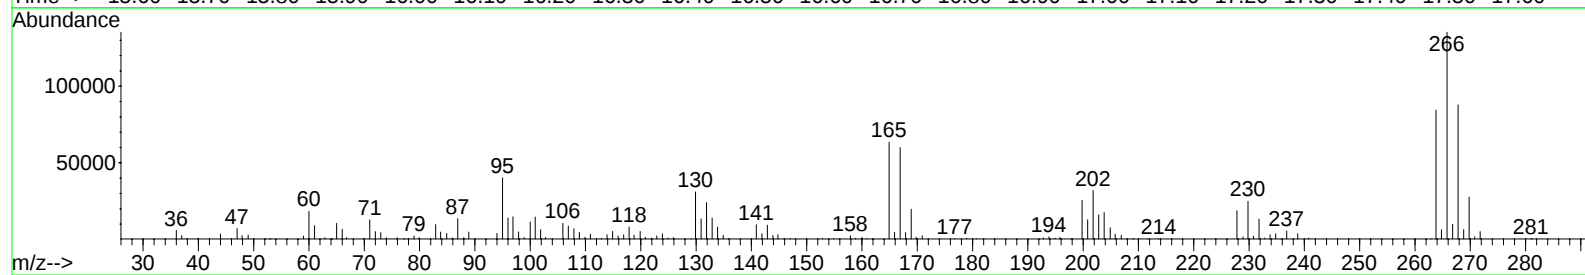


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM041519\
Data File : BM019908.D
Acq On : 15 Apr 2019 10:37
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 17:49:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 15 16:16:29 2019
Response via : Initial Calibration

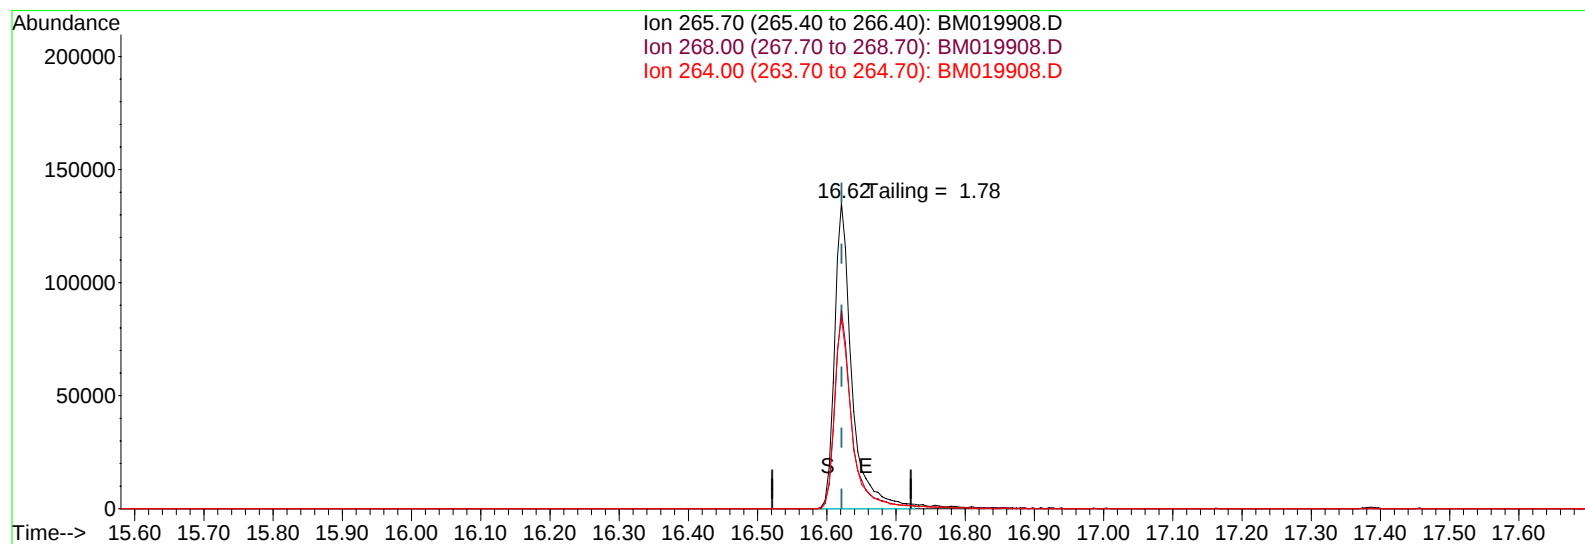

TIC: BM019908.D

(70) Pentachlorophenol (C)




16.621min (-0.000) 0.00ng

response 231145

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	64.96
264.00	62.30	62.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM041519\
 Data File : BM019908.D
 Acq On : 15 Apr 2019 10:37
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 17:49:45 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 15 16:16:29 2019
 Response via : Initial Calibration

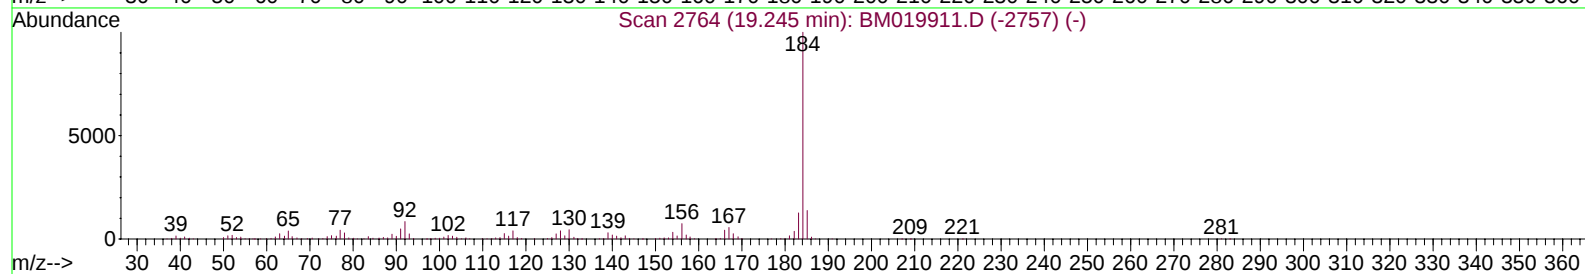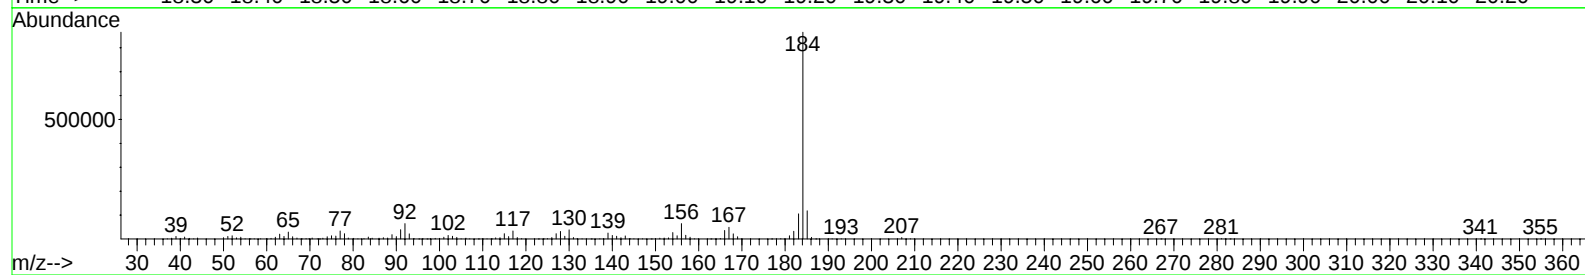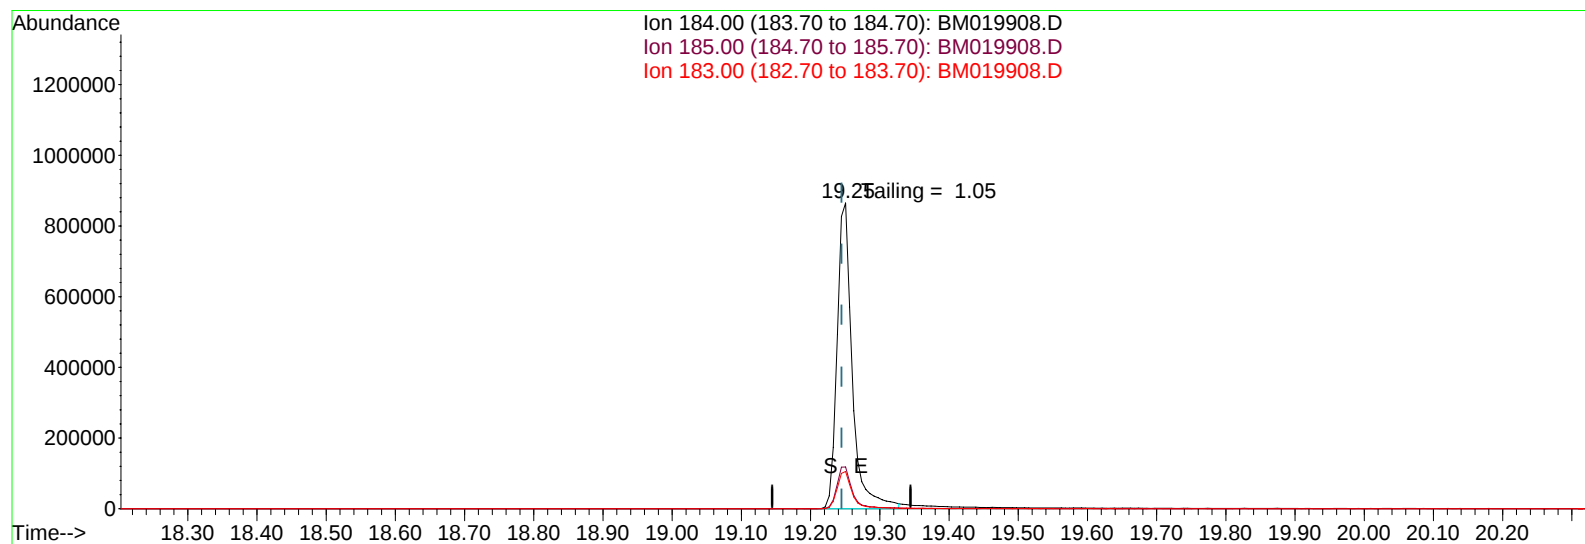

TIC: BM019908.D

(77) Benzidine

19.250min (+0.006) 0.00ng

response 1309864

Ion	Exp%	Act%
184.00	100	100
185.00	13.80	13.65
183.00	12.60	12.17
0.00	0.00	0.00