


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041519\
 Data File : BM019908.D
 Acq On : 15 Apr 2019 10:37
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 15 16:16:29 2019

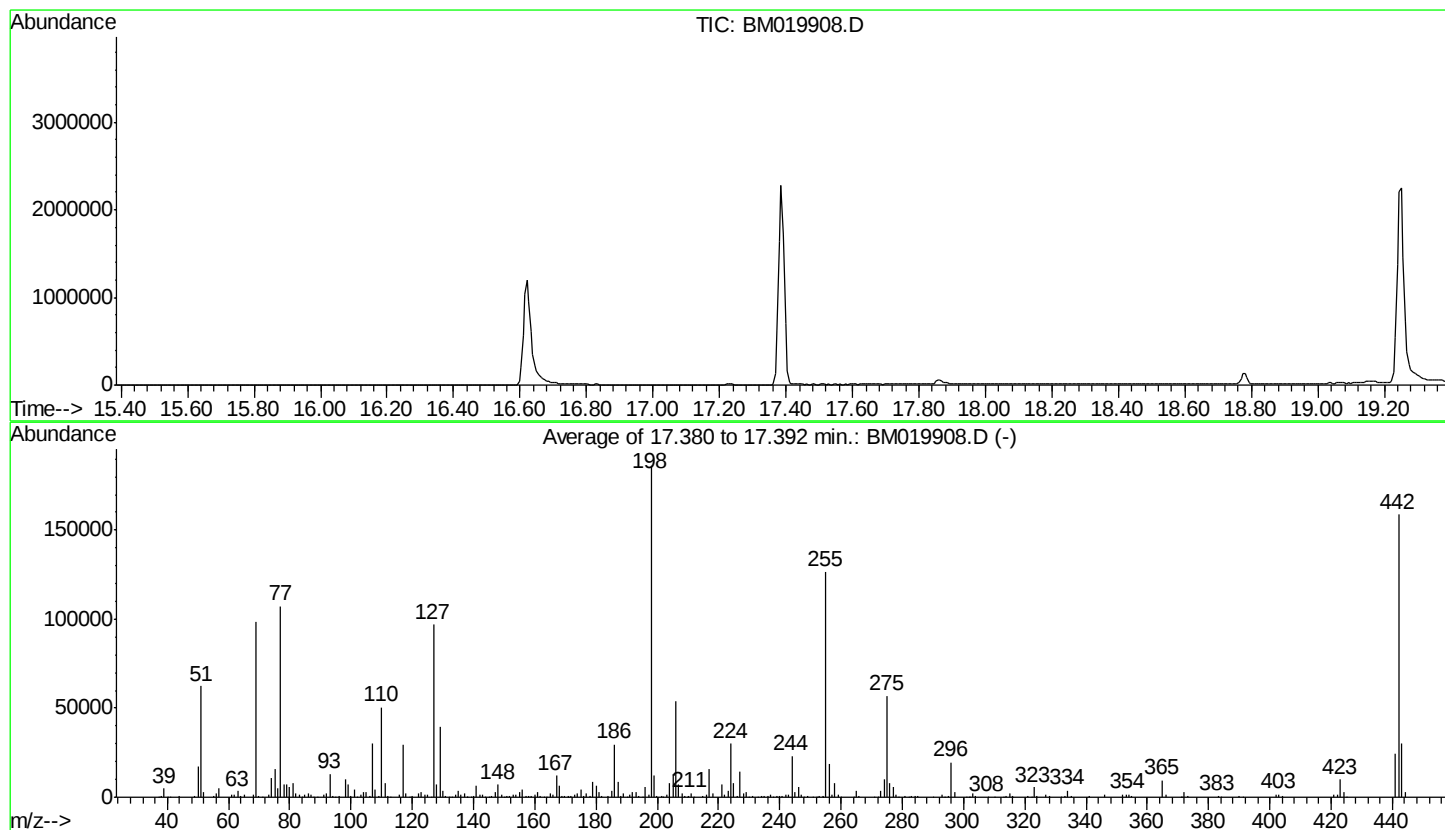

AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	62309	PASS
68	69	0.00	2	1.8	1767	PASS
69	198	0.00	100	52.9	98533	PASS
70	69	0.00	2	0.6	564	PASS
127	198	10	80	52.0	96770	PASS
197	198	0.00	2	0.7	1325	PASS
198	198	100	100	100.0	186218	PASS
199	198	5	9	6.8	12575	PASS
275	198	10	60	30.5	56880	PASS
365	198	1	100	5.1	9571	PASS
441	198	0.01	100	13.0	24292	PASS
442	198	50	100	85.2	158722	PASS
443	442	15	24	18.9	30024	PASS